

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 02/27/2002 Time: 12:02:26

Sample: AE01333
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 2/27/02 12:02 Ended: 2/27/02 12:02 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		104		5.0

Comments for Sample AE01333 - Analysis \$GCMS

Westchester Dept. of Labs & Research
User: Vinci, David L
Date: 02-27-2002 Time: 12:02:36

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB1902\1333.D
 Acq On : 19 Feb 2002 4:15 pm
 Sample : gc/ms scan 1/18
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Feb 21 14:31 2002

Vial: 7
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Feb 13 11:43:23 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0208

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.33	152	242393	20.00	ug/l	-0.02
10) Naphthalene-d8	15.97	136	921517	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.29	164	476214	20.00	ug/l	-0.03
29) Phenanthrene-d10	25.74	188	642900	20.00	ug/l	-0.03
38) Chrysene-d12	33.80	240	379335	20.00	ug/l	-0.05
44) Perylene-d12	38.08	264	245103	20.00	ug/l	-0.05

System Monitoring Compounds

37) 2,4-DDD	30.81	235	33568	5.20	ug/mL	0.32
Spiked Amount	5.000		Recovery	=	104.00%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	16.03	128	402	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.
25) Diethylphthalate	22.75	149	202	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#) = qualifier out of range (m) = manual integration

1333.D GCMS0208.M Thu Feb 21 14:32:03 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\FEB1902\1333.D
 Acq On : 19 Feb 2002 4:15 pm
 Sample : gc/ms scan 1/18
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Feb 21 14:31 2002

Vial: 7
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0208.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Feb 13 11:43:23 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0208

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	0.00	178	0	N.D.		
34) Anthracene	0.00	178	0	N.D.		
35) Di-n-butylphthalate	27.70	149	9700	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.80	228	837	N.D.		
42) Bis(2-ethylhexyl)phthalate	34.01	149	1907	N.D.		
43) Chrysene	33.80	228	837	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	38.07	252	858	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

 (#) = qualifier out of range (m) = manual integration

1333.D GCMS0208.M

Thu Feb 21 14:32:07 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\FEB1902\1333.D
Acq On : 19 Feb 2002 4:15 pm
Sample : gc/ms scan 1/18
Misc :
MS Integration Params: GOOFY.P
Quant Time: Feb 21 14:31 2002

Vial: 7
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0208.RES

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Feb 13 11:43:23 2002
Response via : Initial Calibration

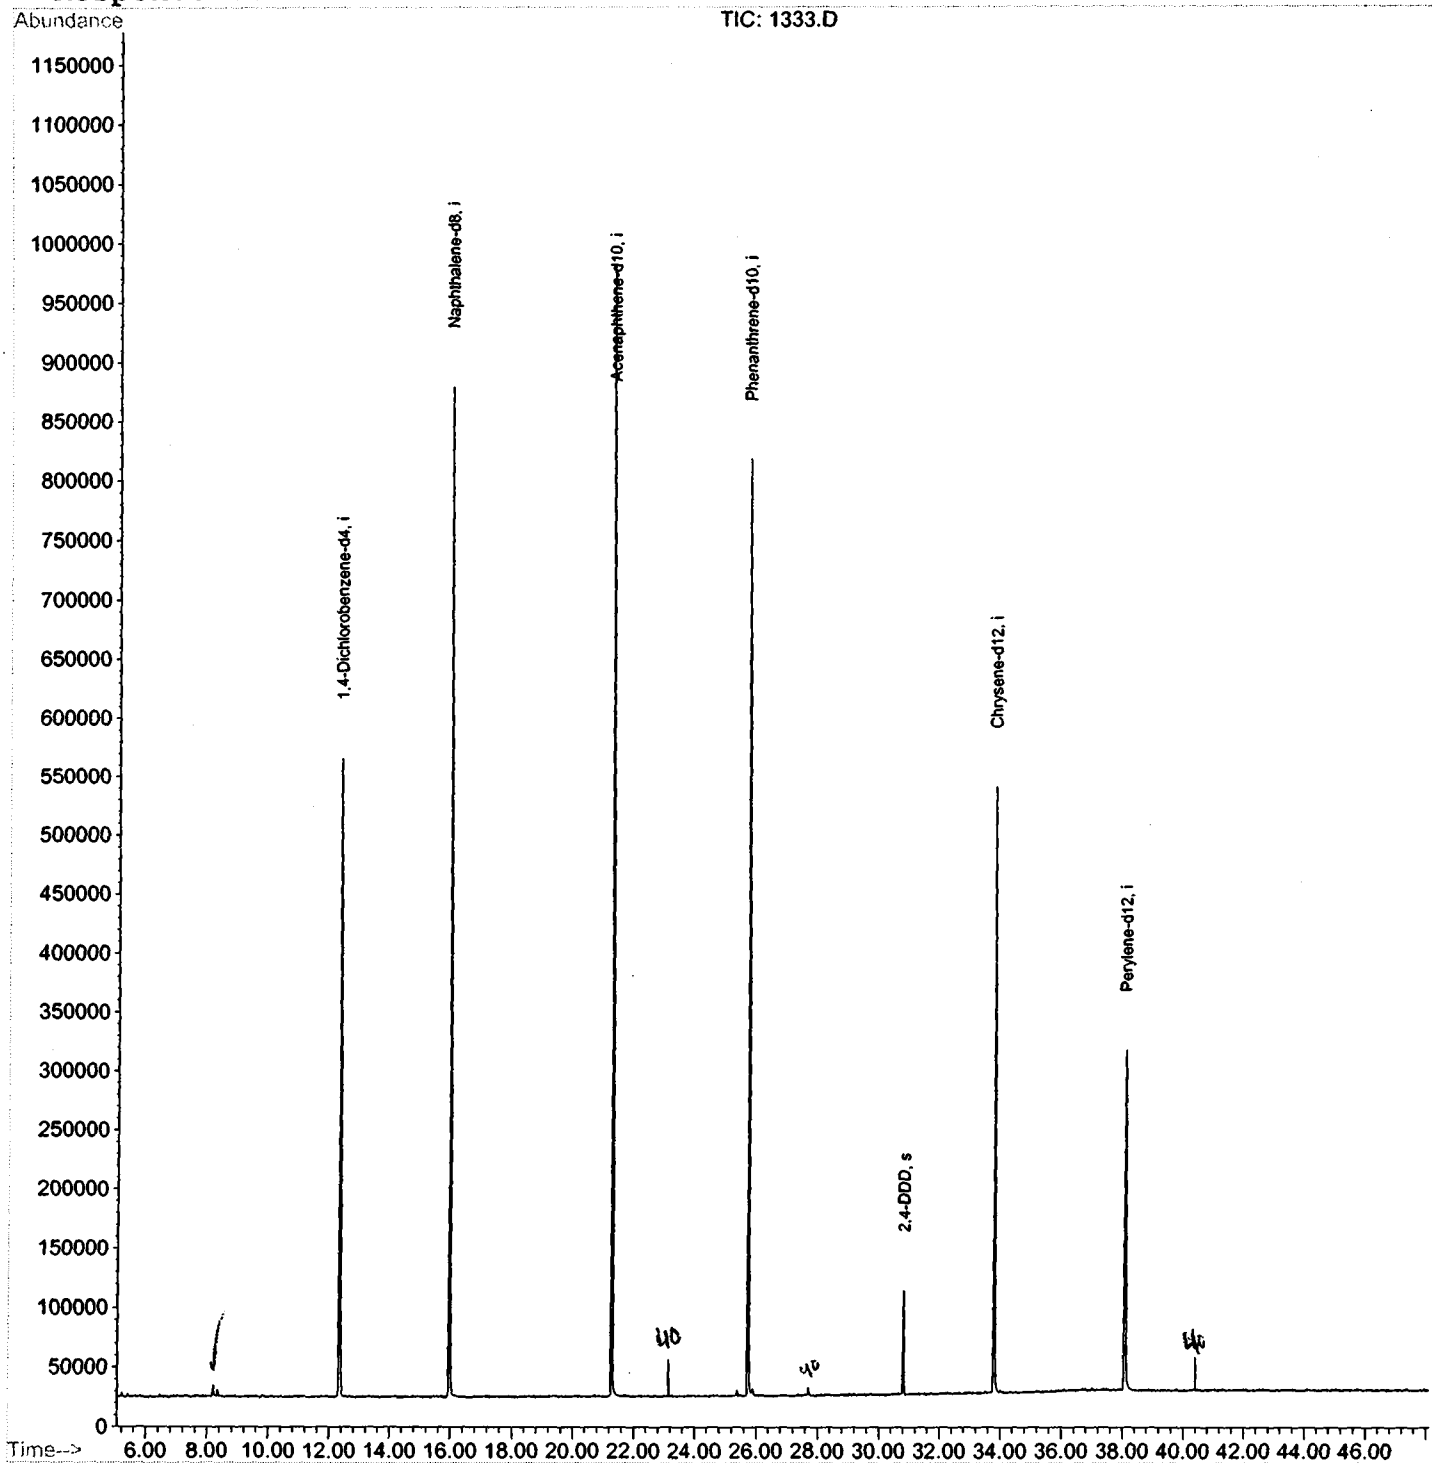

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\FEB1902\1333.D

Acq On : 19 Feb 2002 4:15 pm

Sample : gc/ms scan 1/18

Misc :

MS Integration Params: LSCINT.P

Vial: 7

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.204	341	344	349	rBV2	10469	24920	1.32%	0.279%
2	12.335	788	794	804	rBV	540700	1344926	71.02%	15.039%
3	15.970	1184	1190	1205	rBV	854029	1771542	93.55%	19.809%
4	21.286	1763	1769	1777	rBV	956080	1893726	100.00%	21.175%
5	25.738	2248	2254	2264	rBV2	791132	1708402	90.21%	19.103%
6	30.815	2802	2807	2813	rVB	87824	174266	9.20%	1.949%
7	33.798	3126	3132	3142	rBV2	512762	1150894	60.77%	12.869%
8	38.076	3590	3598	3613	rBV2	287647	874363	46.17%	9.777%




Sum of corrected areas: 8943039

1333.D GCMS0208.M

Thu Feb 21 15:26:25 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\FEB1902\1333.D
 Operator : 209 GALOS
 Acquired : 19 Feb 2002 4:15 pm using AcqMethod GCMS0208
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 1/18
 Misc Info :
 Vial Number: 7
 Quant File :GCMS0208.RES (RTE Integrator)

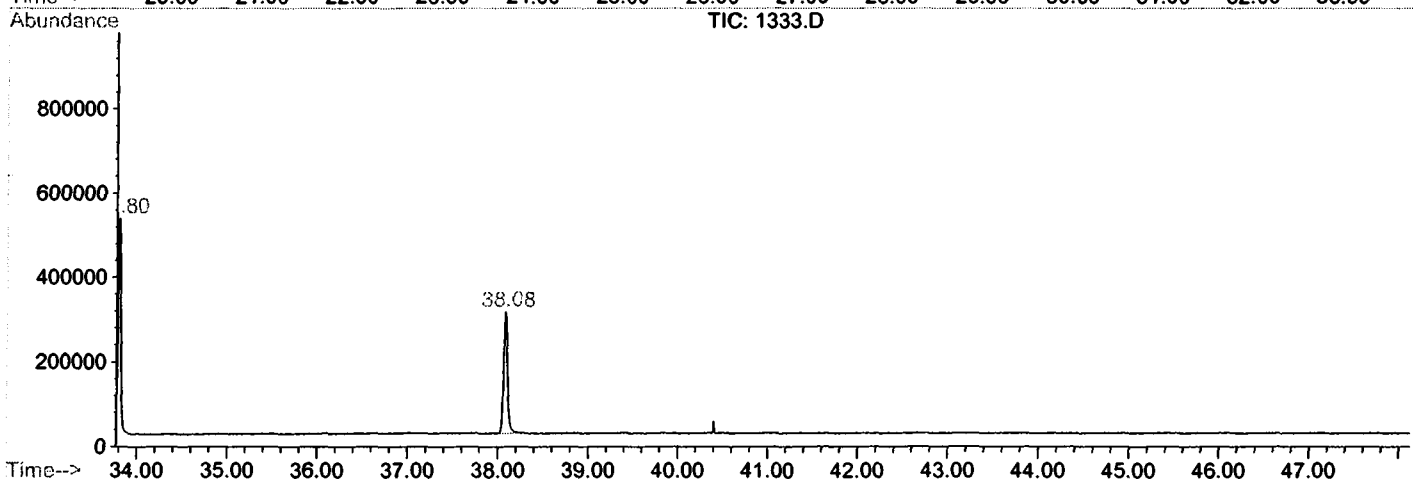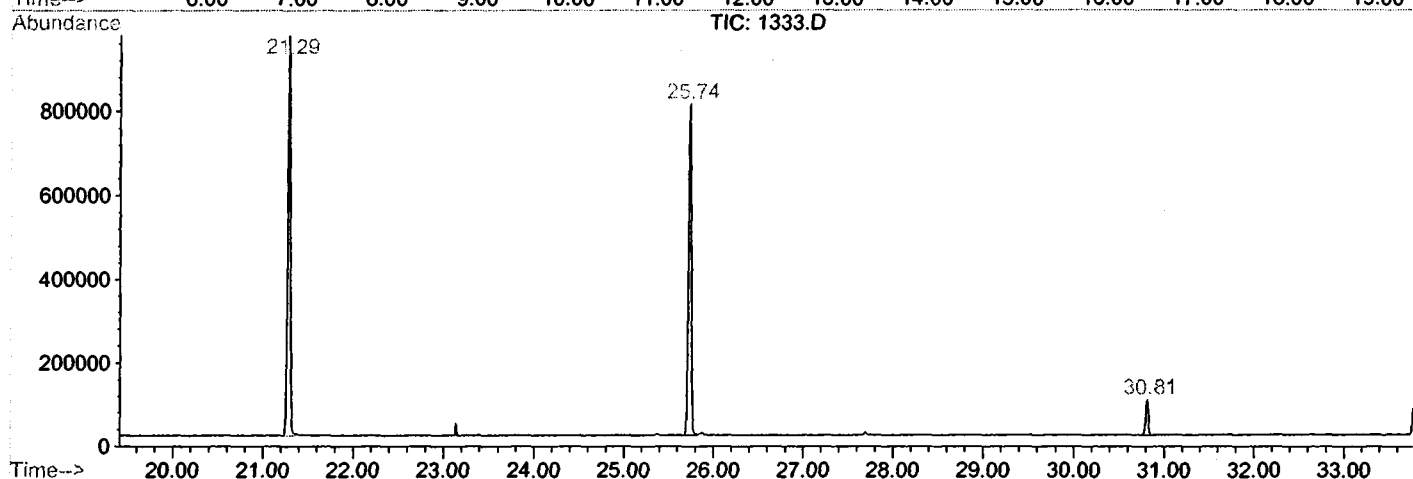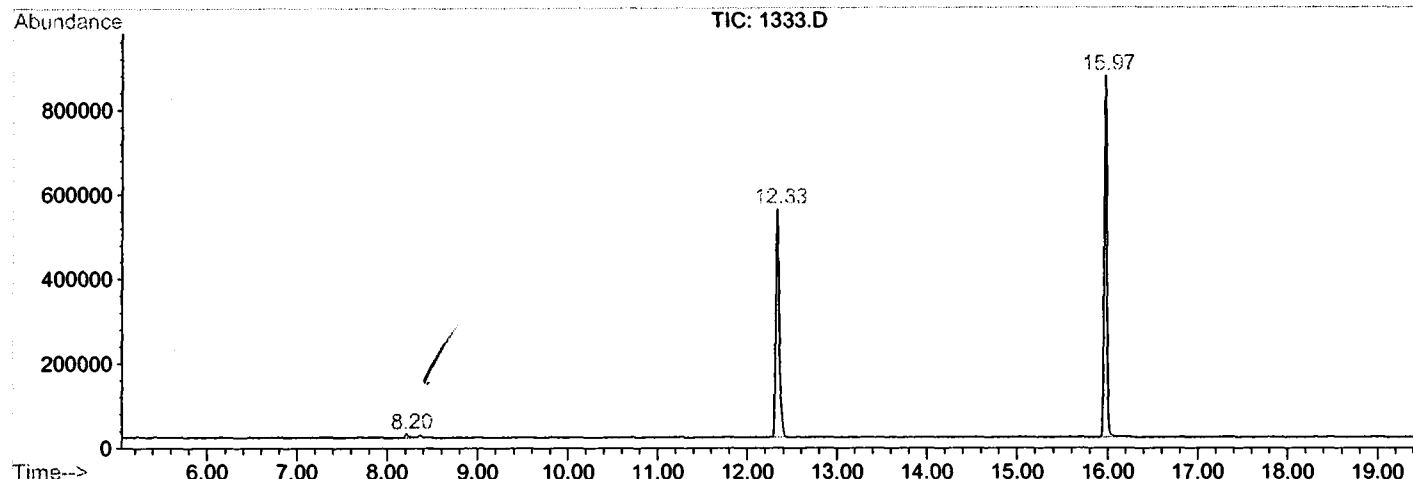

1333.D GCMS0208.M

Thu Feb 21 15:26:31 2002

Library Search Compound

Data File : C:\HPCHEM\1\DATA\FEB1902\1333.D
Acq On : 19 Feb 2002 4:15 pm
Sample : gc/ms scan 1/18
Misc :
MS Integration Params: LSCINT.P


Vial: 7
Operator: 209 GALOS
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 N-Ethylformamide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.20	0.37 ug/l	24920	1,4-Dichlorobenzene-d4	12.33

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			N-Ethylformamide	73	C3H7NO	000627-45-2	5
2			1,3-Dioxolane	74	C3H6O2	000646-06-0	4
3			1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	4
4			Formamide, N,N-dimethyl-	73	C3H7NO	000068-12-2	4

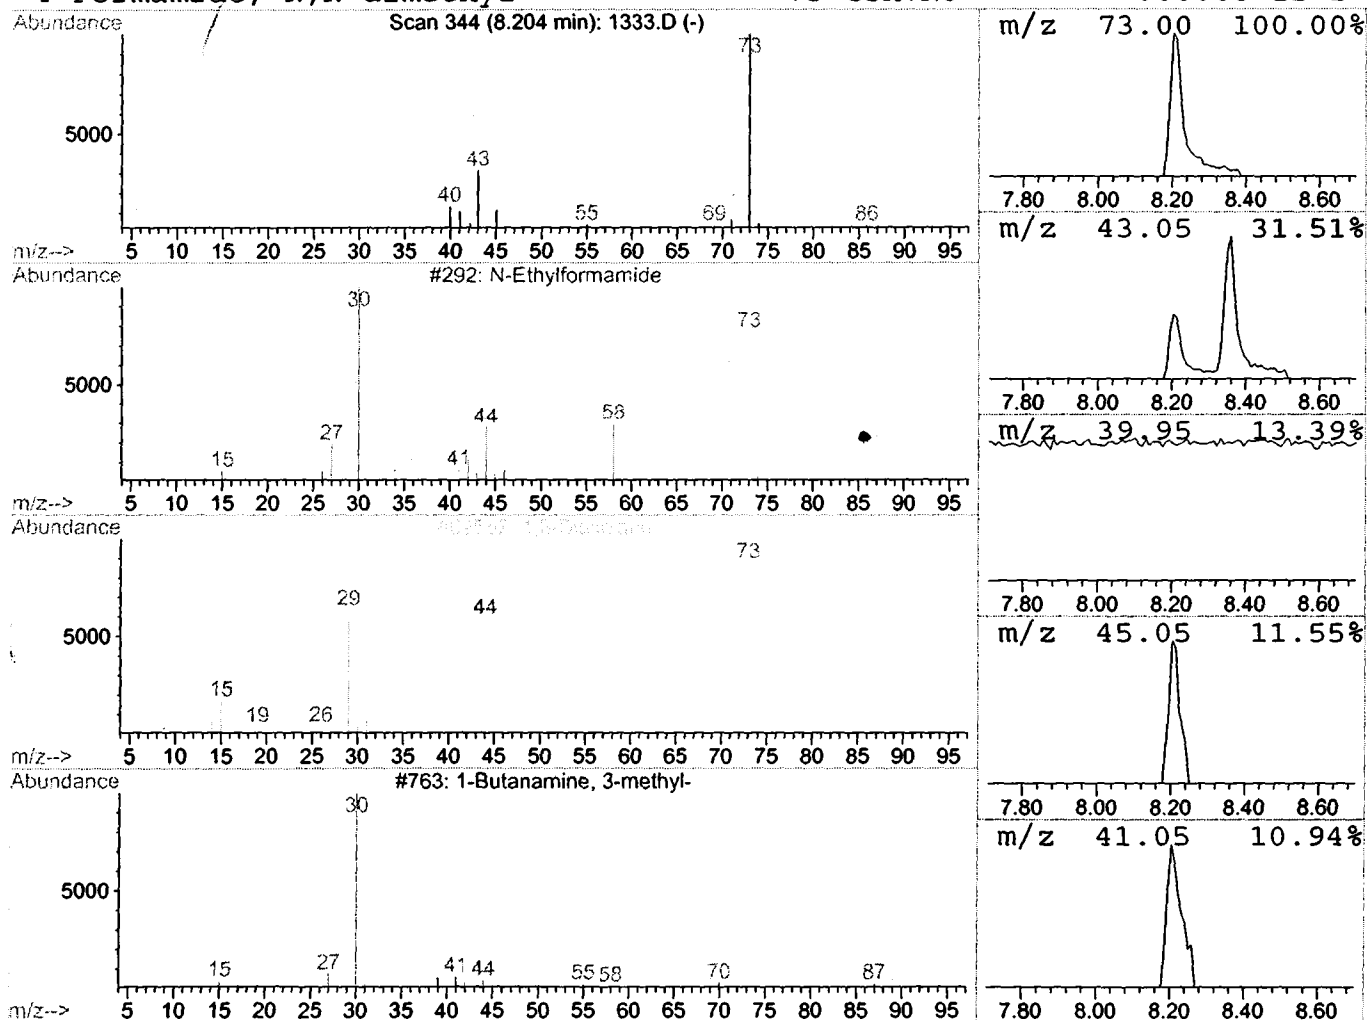

Tentatively Identified Compound (LSC) summary

Operator ID: 209 GALOS Date Acquired: 19 Feb 2002 4:15 pm
Data File: C:\HPCHEM\1\DATA\FEB1902\1333.D
Name: gc/ms scan 1/18
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0208.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
N-Ethylformamide	8.20	0.4	ug/l	24920	ISTD01	12.33	1344930	20.0

1333.D GCMS0208.M Thu Feb 21 15:26:39 2002