

User: Fakhouri, Morgan
 Westchester Dept. of Labs & Research
 Date: 12/11/2001 Time: 11:03:21

Sample: AD27547
 Analysis: \$LP525 Organic Extractables
 Units: ug
 Started: 11/16/01 10:58 Ended: 12/5/01 10:58 Analyst: MF
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result
1	DFTPP		passes
2	ENDRIN		14.8
3	DDT		16.6

DFTPP

Data File : C:\MSDCHEM\1\DATA\121001B\DFTPP.D

Acq On : 10 Dec 2001 4:37 pm

Sample : dftpp +ddt+end

Misc :

MS Integration Params: BENZO.P

Vial: 1

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)

Title : Quantitation For Method 525.2

Spectrum Information: Scan 869

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.9	167296	PASS
68	69	0.00	2	1.3	2798	PASS
69	198	0.00	100	34.3	221952	PASS
70	69	0.00	2	0.3	611	PASS
127	198	10	80	49.5	319744	PASS
197	198	0.00	2	0.5	2984	PASS
198	198	50	100	100.0	646336	PASS
199	198	5	9	6.7	43624	PASS
275	198	10	60	17.2	110920	PASS
365	198	1	100	1.2	7875	PASS
441	443	0.01	100	73.0	71272	PASS
442	198	50	100	72.8	470784	PASS
443	442	15	24	20.7	97680	PASS

DFTPP.D 120501.M

Tue Dec 11 08:36:44 2001

Area Percent Report

Date File : C:\MSDCHEM\1\DATA\121001B\DFTPP.D
 Acq On : 10 Dec 2001 4:37 pm
 Sample : dftpp +ddt+end
 Misc :
 MS Integration Params: BENZO.P

Vial: 1
 Operator: McLean
 Inst : Instrumen
 Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)
 Title : Quantitation For Method 525.2
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 2500 Area counts
 Start Thrs: 0.15 Max Peaks: 10
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	28.602	1376	1381	1386	rM 4	272187	733821	10.76%	9.169%
2	29.654	1493	1497	1501	rM 6	191544	447402	6.56%	5.590%
3	30.234	1554	1561	1570	rM 2	2554427	6822072	100.00%	85.241%

Sum of corrected areas: 8003295

Andreas
= 14.8

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\121001B\DDT.D

Acq On : 10 Dec 2001 5:16 pm

Sample :

Misc :

MS Integration Params: BENZO.P

Vial: 2

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)

Title : Quantitation For Method 525.2

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 2500 Area counts

Start Thrs: 0.15

Max Peaks: 10

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	26.715	1164	1173	1188	rM	27375	142272	5.98%	4.986%
2	27.441	1244	1253	1269	rM	102643	331717	13.94%	11.624%
3	29.264	1449	1454	1463	rM	1036337	2379706	100.00%	83.390%

Sum of corrected areas: 2853695

DDT
16.6

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\121001B\DFTPP.D
 Acq On : 10 Dec 2001 4:37 pm
 Sample : dftpp +ddt+end
 Misc :
 MS Integration Params: BENZO.P

Vial: 1
 Operator: McLean
 Inst : Instrumen
 Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)
 Title : Quantitation For Method 525.2
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 2500 Area counts
 Start Thrs: 0.15 Max Peaks: 10
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	30.234	1555	1561	1570	rM 2	2542538	6710469	100.00%	100.000%

Sum of corrected areas: 6710469

*no Andrus
BD*

Data File : C:\MSDCHEM\1\DATA\121001B\DFTPP.D

Vial: 1

Acq On : 10 Dec 2001 4:37 pm

Operator: McLean

Sample : dftpp +ddt+end

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Dec 17 9:43 2001


Quant Results File: 120501.RES

Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)

Title : Quantitation For Method 525.2

Last Update : Mon Dec 17 09:20:49 2001

Response via : Initial Calibration

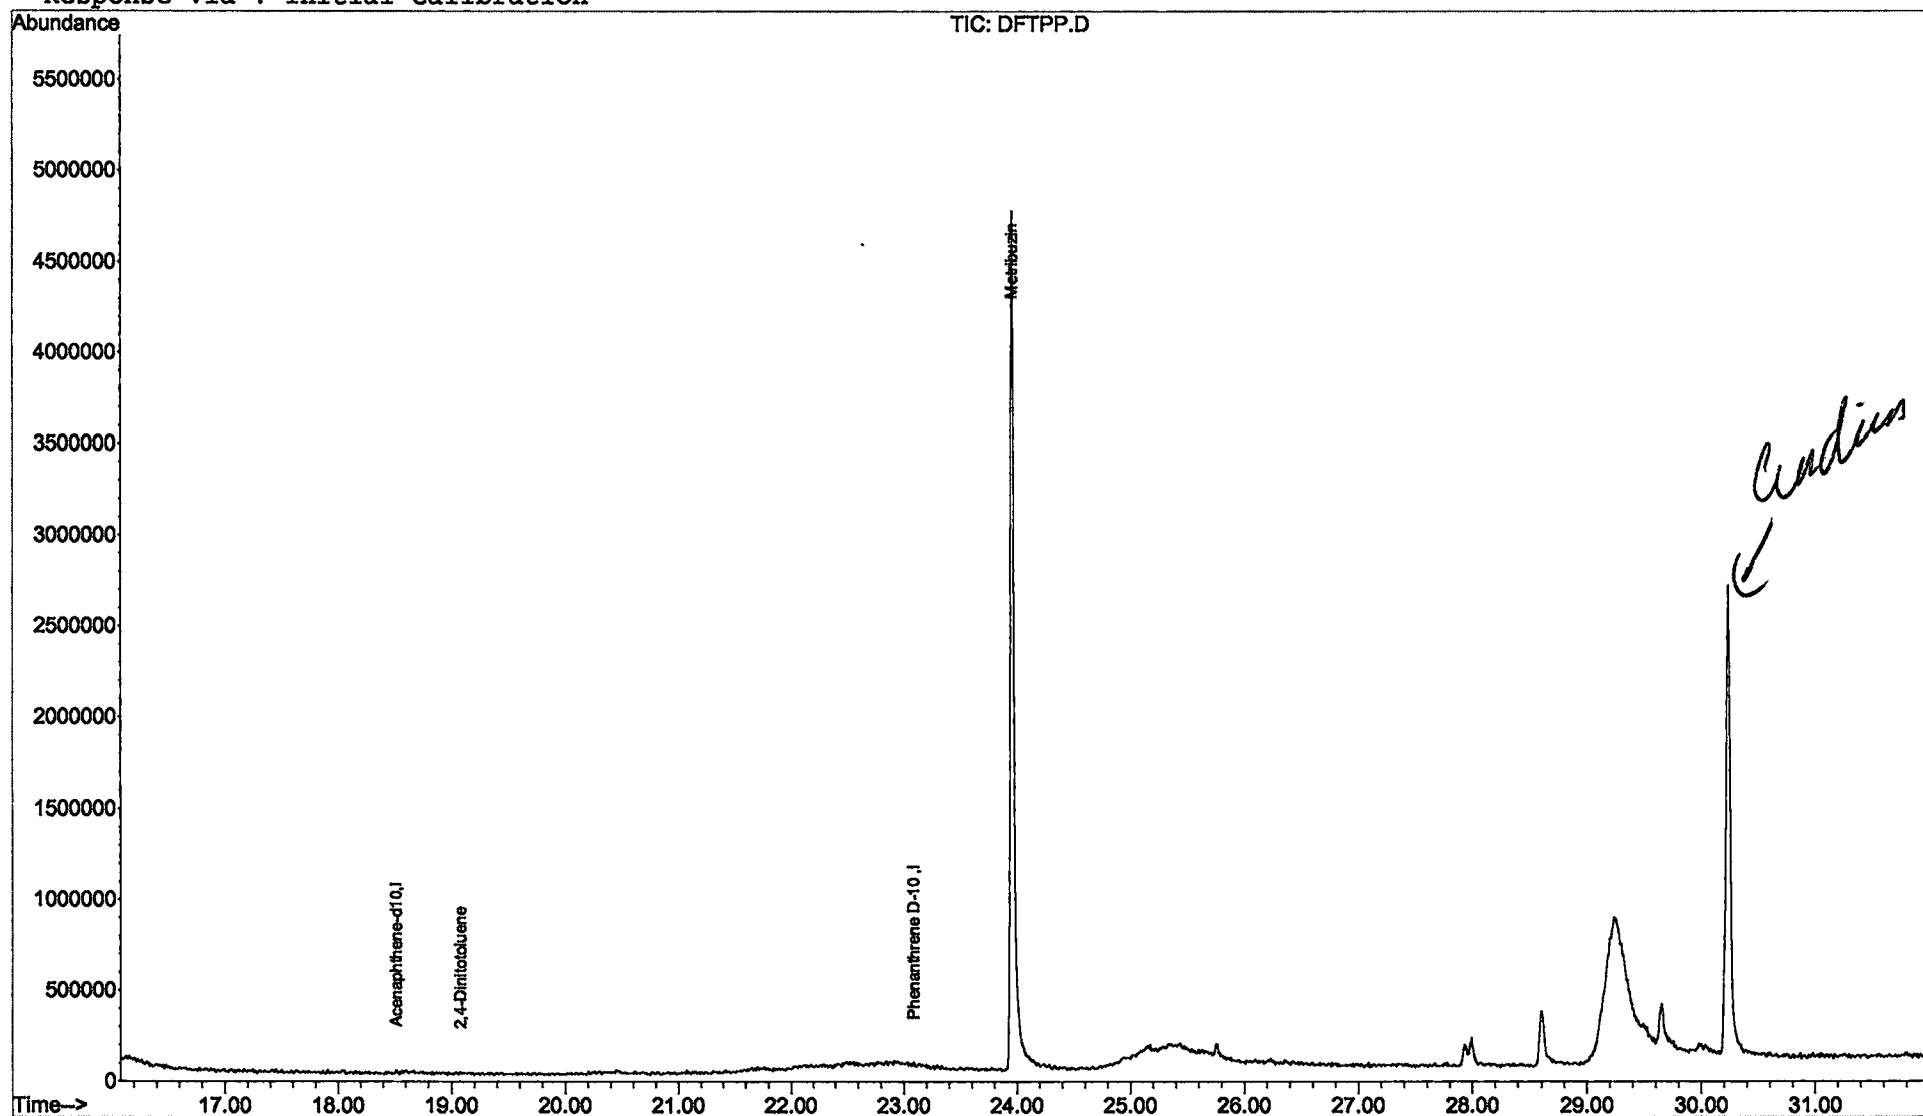

DFTPP

Data File : C:\MSDCHEM\1\DATA\120501\DFTP.D
 Acq On : 5 Dec 2001 8:39 pm
 Sample : con
 Misc :
 MS Integration Params: BENZO.P

Vial: 8
 Operator: McLean
 Inst : Instrumen
 Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)
 Title : Quantitation For Method 525.2

Spectrum Information: Scan 868

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.0	257408	PASS
68	69	0.00	2	1.2	4127	PASS
69	198	0.00	100	32.5	334592	PASS
70	69	0.00	2	0.3	905	PASS
127	198	10	80	50.0	514816	PASS
197	198	0.00	2	0.0	0	PASS
198	198	50	100	100.0	1029376	PASS
199	198	5	9	6.4	65576	PASS
275	198	10	60	17.9	184704	PASS
365	198	1	100	1.5	15907	PASS
441	443	0.01	100	76.4	104504	PASS
442	198	50	100	72.0	740672	PASS
443	442	15	24	18.5	136832	PASS

DFTP.D 120501.M Tue Dec 11 09:24:45 2001

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\120501\DFTP.D
 Acq On : 5 Dec 2001 8:39 pm
 Sample : con
 Misc :
 MS Integration Params: BENZO.P

Vial: 8
 Operator: McLean
 Inst : Instrumen
 Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)
 Title : Quantitation For Method 525.2
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 2500 Area counts
 Start Thrs: 0.15 Max Peaks: 10
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	27.985	1309	1313	1318	rM 2	4355887	8024324	100.00%	87.808%
2	28.384	1354	1357	1360	rM	229665	436692	5.44%	4.779%
3	28.584	1374	1379	1381	rM 2	300032	677485	8.44%	7.414%

Sum of corrected areas: 9138501

Endian
12.2%

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\120501\DFTPP.D

Acq On : 5 Dec 2001 12:21 pm

Sample : dftpp +ddt+end

Misc :

MS Integration Params: BENZO.P

Vial: 1

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)

Title : Quantitation For Method 525.2

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 2500 Area counts

Start Thrs: 0.15

Max Peaks: 10

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	29.255	1447	1453	1458	rM	6602509	11722848	100.00%	86.757%
2	30.216	1553	1559	1565	rM 4	673652	1789416	15.26%	13.243%

Sum of corrected areas: 13512264