

User: Bohlk, Ted
 Westchester Dept. of Labs & Research
 Date: 01/10/2002 Time: 09:55:46

Sample: AD27491
 Analysis: SLP525 Organic Extractables
 Units: ug
 Started: 12/6/01 09:52 Ended: 12/6/01 09:52 Analyst: TB
 Page: 1

	Component Name	Viol	Result
1	DFTPP		PASSED
2	ENDRIN		20
3	DDT		46

DFTPP

Data File : C:\MSDCHEM\1\DATA\120601\DFTPP.D

Acq On : 6 Dec 2001 4:02 pm

Sample : dftpp +ddt+end

Misc :

MS Integration Params: BENZO.P

Vial: 1

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080102.M (RTE Integrator)

Title : Quantitation For Method 508gcscan



Spectrum Information: Scan 868

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	282816	PASS
68	69	0.00	2	1.4	4623	PASS
69	198	0.00	100	34.9	335552	PASS
70	69	0.00	2	0.6	2155	PASS
127	198	10	80	52.5	505216	PASS
197	198	0.00	2	0.3	2800	PASS
198	198	50	100	100.0	961984	PASS
199	198	5	9	5.8	55744	PASS
275	198	10	60	16.9	162176	PASS
365	198	1	100	1.9	18104	PASS
441	443	0.01	100	75.0	92472	PASS
442	198	50	100	61.8	594496	PASS
443	442	15	24	20.7	123216	PASS

DFTPP.D 5080102.M

Thu Jan 10 09:02:51 2002

File : C:\MSDCHEM\1\DATA\120601\DFTPP.D
 Operator : McLean
 Acquired : 6 Dec 2001 4:02 pm using AcqMethod BIG3
 Instrument : Instrumen
 Sample Name: dftpp +ddt+end
 Misc Info :
 Vial Number: 1

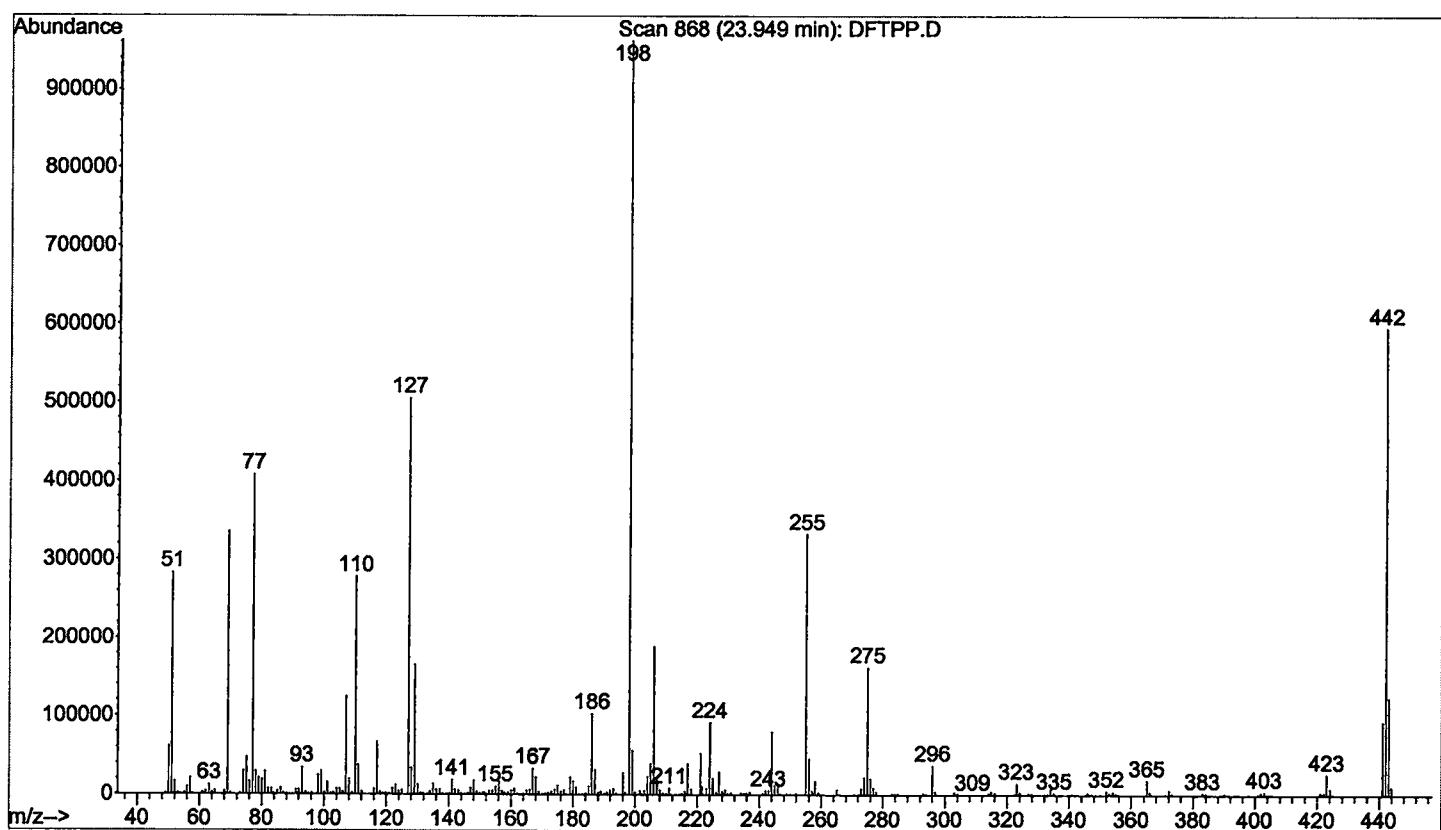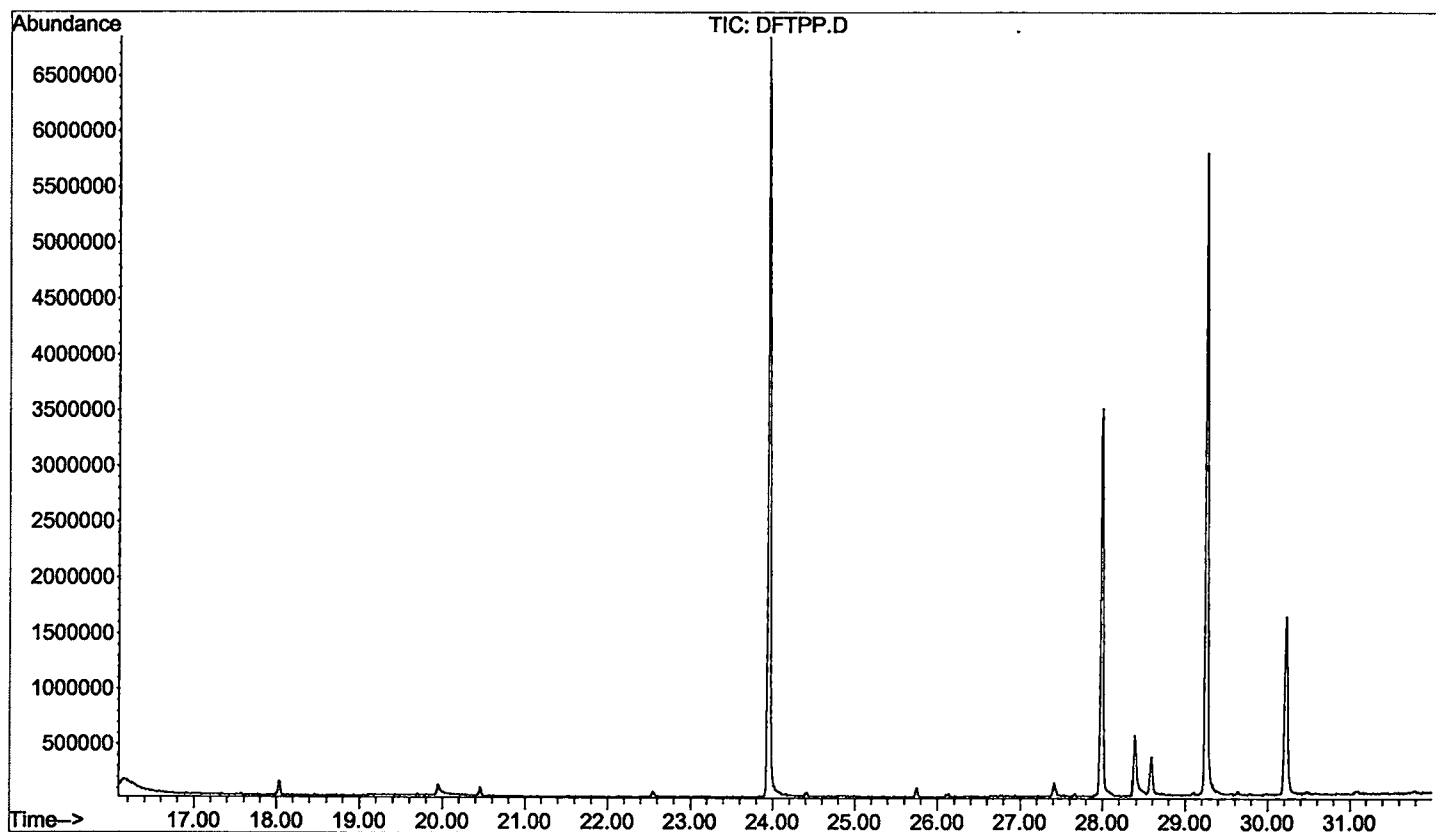

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\120601\DFTPP.D

Acq On : 6 Dec 2001 4:02 pm

Sample : dftpp +ddt+end

Misc :

MS Integration Params: BENZO.P

Vial: 1

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080102.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 2500 Area counts

Start Thrs: 0.15

Max Peaks: 10

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	27.994	1308	1314	1323	rM 2	3480683	7039767	100.00%	79.948%
2	28.384	1354	1357	1361	rM	472239	949339	13.49%	10.781%
3	28.593	1374	1380	1385	rM 3	341147	816360	11.60%	9.271%

Sum of corrected areas: 8805466

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\120601\DFTPP.D

Acq On : 6 Dec 2001 4:02 pm

Sample : dftpp +ddt+end

Misc :

MS Integration Params: BENZO.P

Vial: 1

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080102.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 2500 Area counts

Start Thrs: 0.15

Max Peaks: 10

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	29.255	1445	1453	1466	rM	5747200	11210326	100.00%	74.512%
2	30.225	1555	1560	1566	rM 2	1559147	3834666	34.21%	25.488%

Sum of corrected areas: 15044992