

User: Bohlk, Ted  
 Westchester Dept. of Labs & Research  
 Date: 01/10/2002 Time: 09:04:26

Sample: AD27548  
 Analysis: \$525 Organic Chemicals - 525.2  
 Units: ug  
 Started: 11/19/01 09:03 Ended: 12/6/01 09:03 Analyst: TB  
 Result source: manual entry  
 Page: 1

|    | Component Name                 | Vol | Result    | Qualifier | MDL  |
|----|--------------------------------|-----|-----------|-----------|------|
| 1  | Hexachlorocyclopentadiene      |     | < MDL     |           | 0.10 |
| 2  | Hexachlorobenzene              |     | < MDL     |           | 0.10 |
| 3  | Simazine                       |     | < MDL     |           | 0.40 |
| 4  | Atrazine                       |     | < MDL     |           | 0.20 |
| 5  | Alachlor                       |     | < MDL     |           | 0.20 |
| 6  | bis(2-Ethylhexyl)adipate       |     | < MDL     |           | 0.60 |
| 7  | bis(2-Ethylhexyl)phthalate     |     | 1.3 - 0.4 |           | 0.60 |
| 8  | Benzo(a)pyrene                 |     | < MDL     |           | 0.20 |
| 9  | EPTC                           |     | < MDL     |           | 1.0  |
| 10 | 2,6-Dinitrotoluene             |     | < MDL     |           | 2.0  |
| 11 | 2,4-Dinitrotoluene             |     | < MDL     |           | 2.0  |
| 12 | Mollinate                      |     | < MDL     |           | 0.90 |
| 13 | Terbacil                       |     | < MDL     |           | 2.0  |
| 14 | Acetochlor                     |     | < MDL     |           | 2.0  |
| 15 | Metribuzin                     |     | < MDL     |           | 0.15 |
| 16 | Metolachlor                    |     | < MDL     |           | 0.75 |
| 17 | Butachlor                      |     | < MDL     |           | 0.40 |
| 18 | 4,4-DDE                        |     | < MDL     |           | 0.80 |
| 19 | Surr_1,3-Dimethyl-2-nitrobenze |     | 3.9       |           | 1.0  |
| 20 | Surr_Triphenyl phosphate       |     | 6.2       |           | 1.0  |
| 21 | Surr_Perylene-d12              |     | 4.4       |           | 1.0  |

## Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\120601\27548.D

Acq On : 7 Dec 2001 9:10 am

Sample : 11/19 sample

Misc :

MS Integration Params: BENZO.P

Quant Time: Dec 07 09:47:31 2001

Vial: 23

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 120501.RES

Quant Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)

Title : Quantitation For Method 525.2

Last Update : Thu Dec 06 10:31:04 2001

Response via : Initial Calibration

DataAcq Meth : 120501

| Internal Standards   | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|----------------------|-------|------|----------|------|-------|----------|
| 1) Acenaphthene-d10  | 18.32 | 164  | 6859667  | 5.00 | ug/L  | 0.00     |
| 9) Phenanthrene D-10 | 22.65 | 188  | 9745229  | 5.00 | ug/L  | 0.00     |
| 20) Chrysene D-12    | 30.42 | 240  | 6532536  | 5.00 | ug/L  | 0.00     |

## System Monitoring Compounds

|                               |       |     |          |      |         |      |
|-------------------------------|-------|-----|----------|------|---------|------|
| 2) 1,3-Dimethyl-2-nitrobenzen | 13.23 | 134 | 1414564  | 3.88 | ug/L    | 0.00 |
| Spiked Amount                 | 5.000 |     | Recovery | =    | 77.60%  |      |
| 19) Triphenyl Phosphate surr  | 29.69 | 326 | 2090145  | 6.19 | ug/L    | 0.00 |
| Spiked Amount                 | 5.000 |     | Recovery | =    | 123.80% |      |
| 21) Perylene D-12 surr        | 34.44 | 264 | 4012743  | 4.38 | ug/L    | 0.00 |
| Spiked Amount                 | 5.000 |     | Recovery | =    | 87.60%  |      |

## Target Compounds

|                                |       |     |         |           | Qvalue |    |
|--------------------------------|-------|-----|---------|-----------|--------|----|
| 3) Hexachlorocyclopentadiene   | 0.00  | 237 | 0       | N.D.      |        |    |
| 4) Hexachlorobenzene           | 21.51 | 284 | 12289   | 0.02 ug/L | #      | 76 |
| 5) EPTC                        | 0.00  | 128 | 0       | N.D.      |        |    |
| 6) 2,6-Dinitrotoluene          | 17.93 | 165 | 182964  | 0.91 ug/L | #      | 36 |
| 7) 2,4-Dinitrotoluene          | 0.00  | 165 | 0       | N.D.      | d      |    |
| 8) Molinate                    | 19.23 | 126 | 6694    | 0.01 ug/L | #      | 1  |
| 10) Simazine                   | 0.00  | 201 | 0       | N.D.      |        |    |
| 11) Atrazine                   | 0.00  | 200 | 0       | N.D.      |        |    |
| 12) Alachlor                   | 23.98 | 160 | 5647    | 0.02 ug/L | #      | 1  |
| 13) Terbacil                   | 0.00  | 161 | 0       | N.D.      | d      |    |
| 14) Acetochlor                 | 0.00  | 146 | 0       | N.D.      |        |    |
| 15) Metribuzin                 | 0.00  | 198 | 0       | N.D.      |        |    |
| 16) Metolachlor                | 0.00  | 162 | 0       | N.D.      |        |    |
| 17) Butachlor                  | 0.00  | 160 | 0       | N.D.      | d      |    |
| 18) 4,4'-DDE                   | 0.00  | 246 | 0       | N.D.      | d      |    |
| 22) Bis (2-Ethylhexyl) adipate | 29.62 | 129 | 30128   | 0.14 ug/L | #      | 1  |
| 23) Bis (2-Ethylhexyl) phthala | 31.06 | 149 | 1904838 | 1.29 ug/L |        | 96 |
| 24) Benzo (a) pyrene           | 0.00  | 252 | 0       | N.D.      | d      |    |

(#) = qualifier out of range (m) = manual integration

27548.D 5080102.M

Thu Jan 10 08:49:23 2002

Page 1

Data File : C:\MSDCHEM\1\DATA\120601\27548.D

Vial: 23

Acq On : 7 Dec 2001 9:10 am

Operator: McLean

Sample : 11/19 sample

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Jan 10 8:49 2002


Quant Results File: 120501.RES

Method : C:\MSDCHEM\1\5973N\5080102.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Wed Jan 09 14:35:53 2002

Response via : Initial Calibration

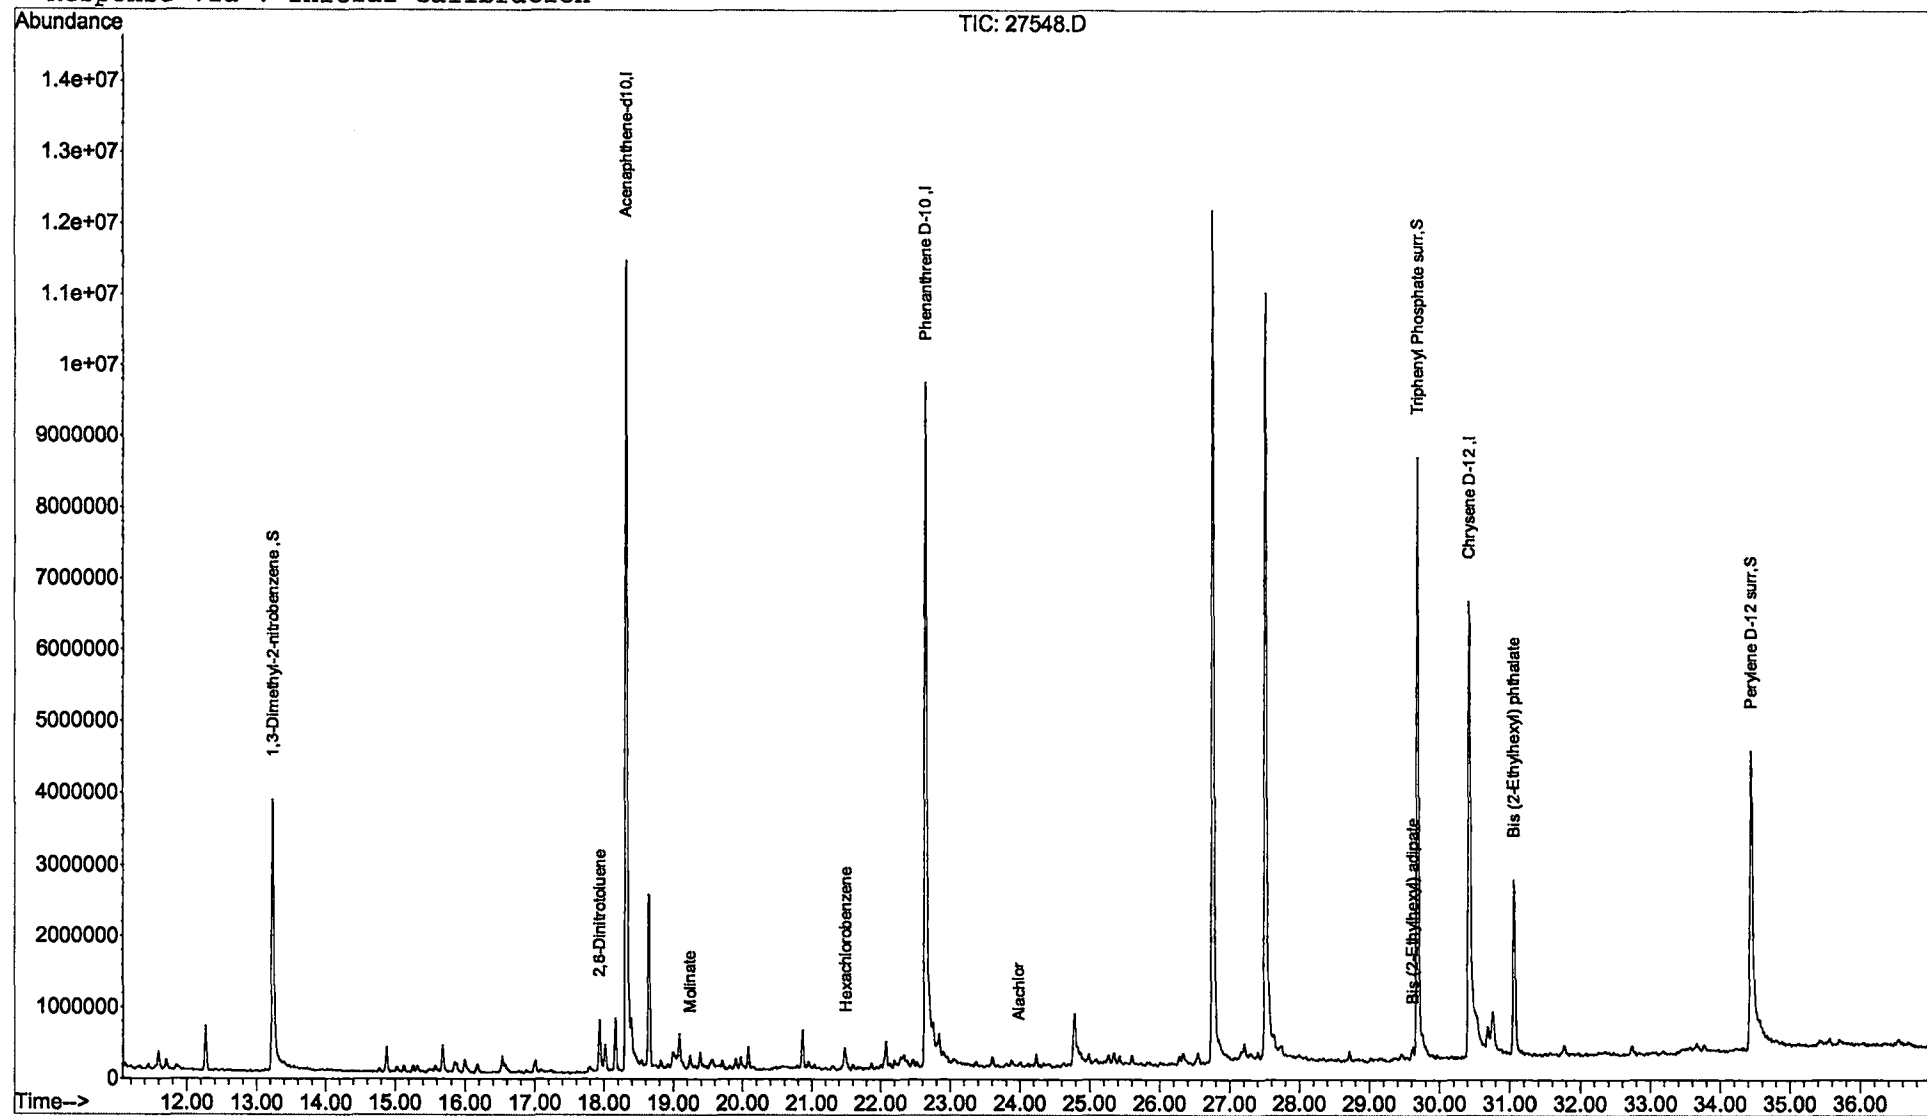

**Comments for Sample AD27548 - Analysis \$525**

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 01-10-2002 Time: 12:33:36

The recoveries for 6 of the 18 compounds in the LCS Standard were outside of their acceptance ranges.