

User: Bohlk, Ted
 Westchester Dept. of Labs & Research
 Date: 01/08/2002 Time: 13:22:12

Sample: AD27626
 Analysis: \$525 Organic Chemicals - 525.2
 Units: ug
 Started: 11/23/01 13:19 Ended: 12/8/01 13:19 Analyst: TB
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.20
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		< MDL		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenzen		5.4		1.0
20	Surr_Triphenyl phosphate		5.0		1.0
21	Surr_Perylene-d12		4.6		1.0

Chromatogram Plot

File: E:\27626EE

Date: Dec-08-1991 22:34:58

Comment: BOHLK; METHOD 525; INST 204; 12/08/01; SAMPLE 27626

Scan No: 1

Retention Time: 0:01


RIC: 0

Mass Range: 0 - 0

Plotted: 1 to 1859

Range: 1 to 1859

100% = 10038341

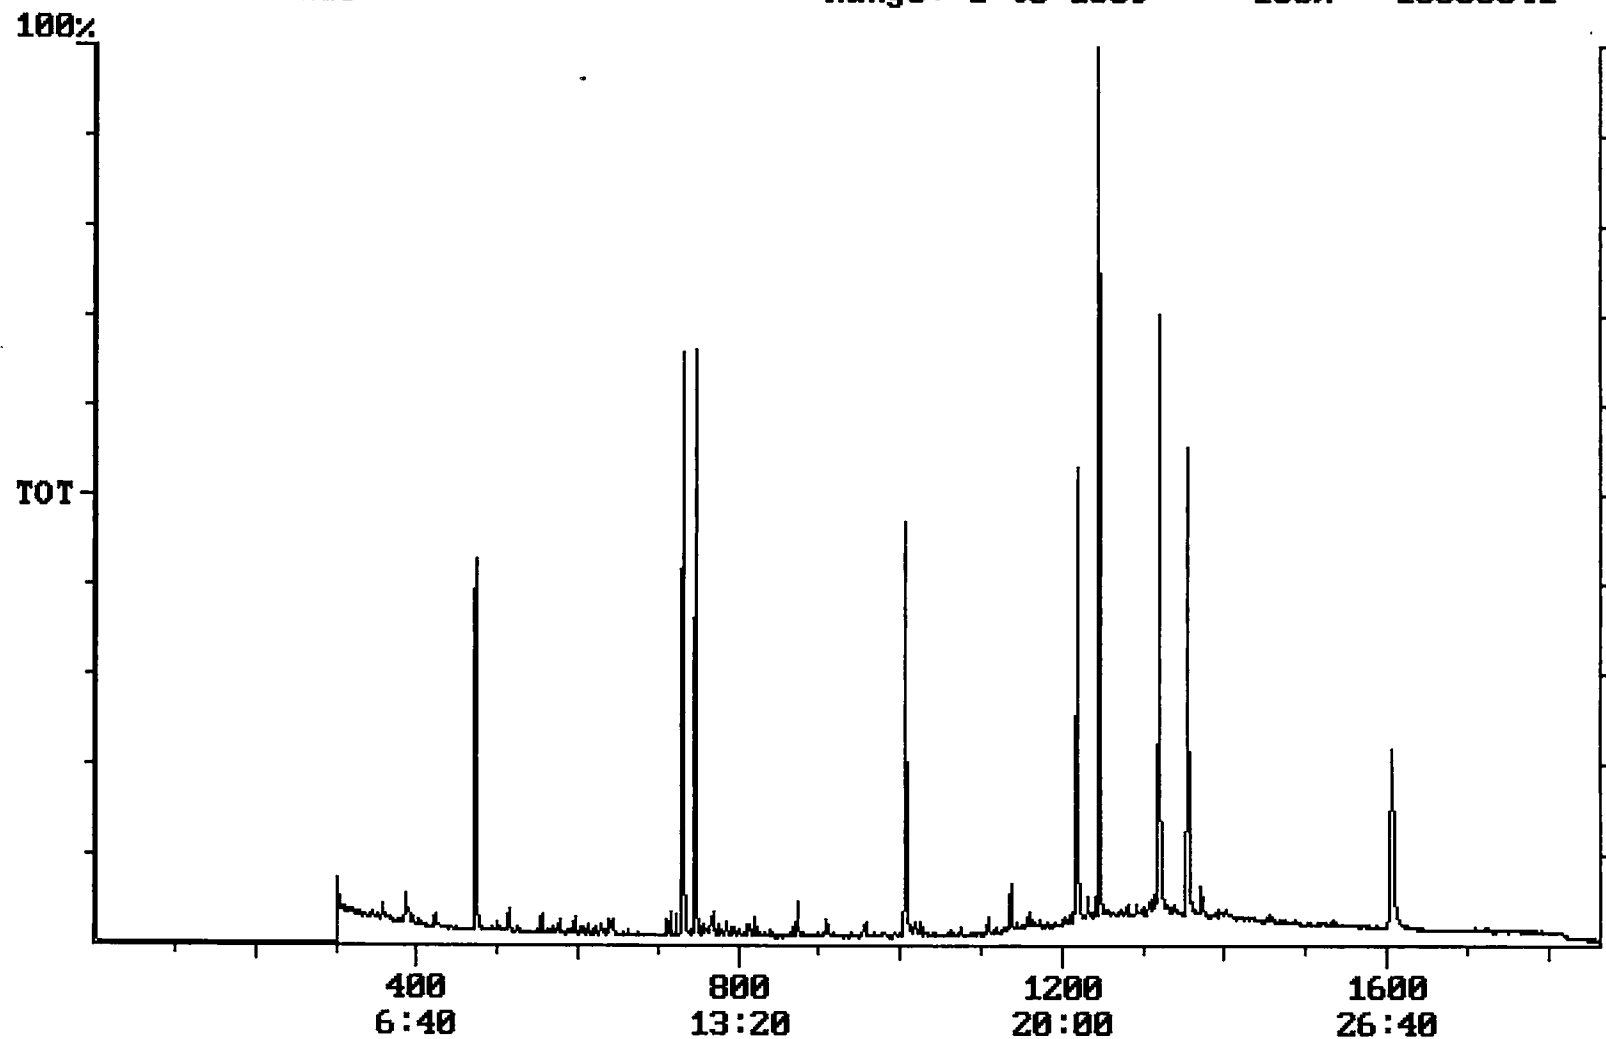

Integration Report

Quanfile: 27626EE

Quan Entries: 15

Comment: BOHLK; METHOD 525; INST 204; 12/08/01; SAMPLE 27626

Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10 (IS)	12:11	731	Auto	2,881,328	1,813,916
2	phenanthrene d-10 (IS)	16:46	1006	Auto	4,110,406	1,633,818
3	chrysene d-12 (IS)	22:34	1354	Auto	3,556,694	1,776,020
4	p-terphenyl d-14 (IS)	20:45	1245	Auto	5,270,210	3,385,605
5	acenaphthene d-10 (SURR)	12:11	731	Auto	2,881,328	1,813,916
6	phenanthrene d-10 (SURR)	16:46	1006	Auto	4,110,406	1,633,818
7	chrysene d-12 (SURR)	22:34	1354	Auto	3,556,694	1,776,020
8	1,3-dimethyl-2-nitrobenzene	7:53	473	Auto	1,455,064	664,344
9	triphenyl phosphate (S)	22:00	1320	Auto	1,717,776	885,927
10	perylene d-12 (SURR)	26:46	1606	Auto	2,374,631	475,615
11	bis(2-ethylhexyl)adipate	21:52	1312	Auto	15,517	5,539
12	bis(2-ethylhexyl)phthalate	22:51	1371	Auto	211,459	104,805
13	2,6-dinitrotoluene	11:51	711	Auto	39,683	22,076
14	butachlor	20:19	1219	Auto	29,264	11,607
15	4,4'-dichlorodiphenyl ether	20:41	1241	Auto	4,329	3,003

reviewed IS/Surr's

Quantitation Report

Quanfile: 27626EE

Quan Entries: 15

Comment: BOHLK; METHOD 525; INST 204; 12/08/01; SAMPLE 27626

Sorted via: Entry Number ↑

(S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10(IS)	I	731	12:11	BV	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1006	16:46	BV	5.000	UG/L
3	chrysene d-12(IS)	I	1354	22:34	BV	5.000	UG/L
4	p-terphenyl d-14(IS)	I	1245	20:45	BB	5.000	UG/L
5	acenaphthene d-10(SURR	A	731	12:11	BV	3.011	UG/L
6	phenanthrene d-10(SURR	A	1006	16:46	BV	3.355	UG/L
7	chrysene d-12 (SURR)	A	1354	22:34	BV	3.547	UG/L
8	1,3-dimethyl-2-nitrobe	A	473	7:53	BV	5.412	UG/L
9	triphenyl phosphate (S	A	1320	22:00	VV	4.985	UG/L
10	perylene d-12 (SURR)	A	1606	26:46	BB	4.583	UG/L
16	bis(2-ethylhexyl)adipa	A	1312	21:52	MM	0.030	UG/L
17	bis(2-ethylhexyl)phtha	A	1371	22:51	VV	0.203	UG/L
20	2,6-dinitrotoluene	A	711	11:51	BB	0.233	UG/L
27	butachlor	A	1219	20:19	BB	0.079	UG/L
28	4,4'-dde	A	1241	20:41	BB	0.012	UG/L

• **Comments for Sample AD27626 - Analysis \$525**

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 01-22-2002 Time: 14:18:33

The recoveries for 2 of the 18 compounds in the LCS Standard were below their acceptance ranges. The recoveries for 3 of the 18 compounds in the Spiked Sample were outside of their acceptance ranges. The breakdown for Endrin in the Breakdown Standard was 61%. The injection port is kept at 280 degrees Celcius which may be contributing to high Endrin Breakdown. An investigation into modifying injection port parameters will be made.