


User: Bohlk, Ted
Westchester Dept. of Labs & Research
Date: 01/08/2002 Time: 14:23:04

Sample: AD27771
Analysis: \$525 Organic Chemicals - 525.2
Units: ug
Started: 11/24/01 14:20 Ended: 12/9/01 14:20 Analyst: TB
Result source: manual entry
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.20
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		< MDL		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenzen		5.3		1.0
20					
21	Surr_Perylene-d12		5.0		1.0

Chromatogram Plot File: E:\2777111 Date: Dec-09-1991 22:40:18
 Comment: BOHLK; METHOD 525; INST 204; 12/09/01; SAMPLE 27771
 Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
 Plotted: 1 to 1860 Range: 1 to 1860 100% = 10849911

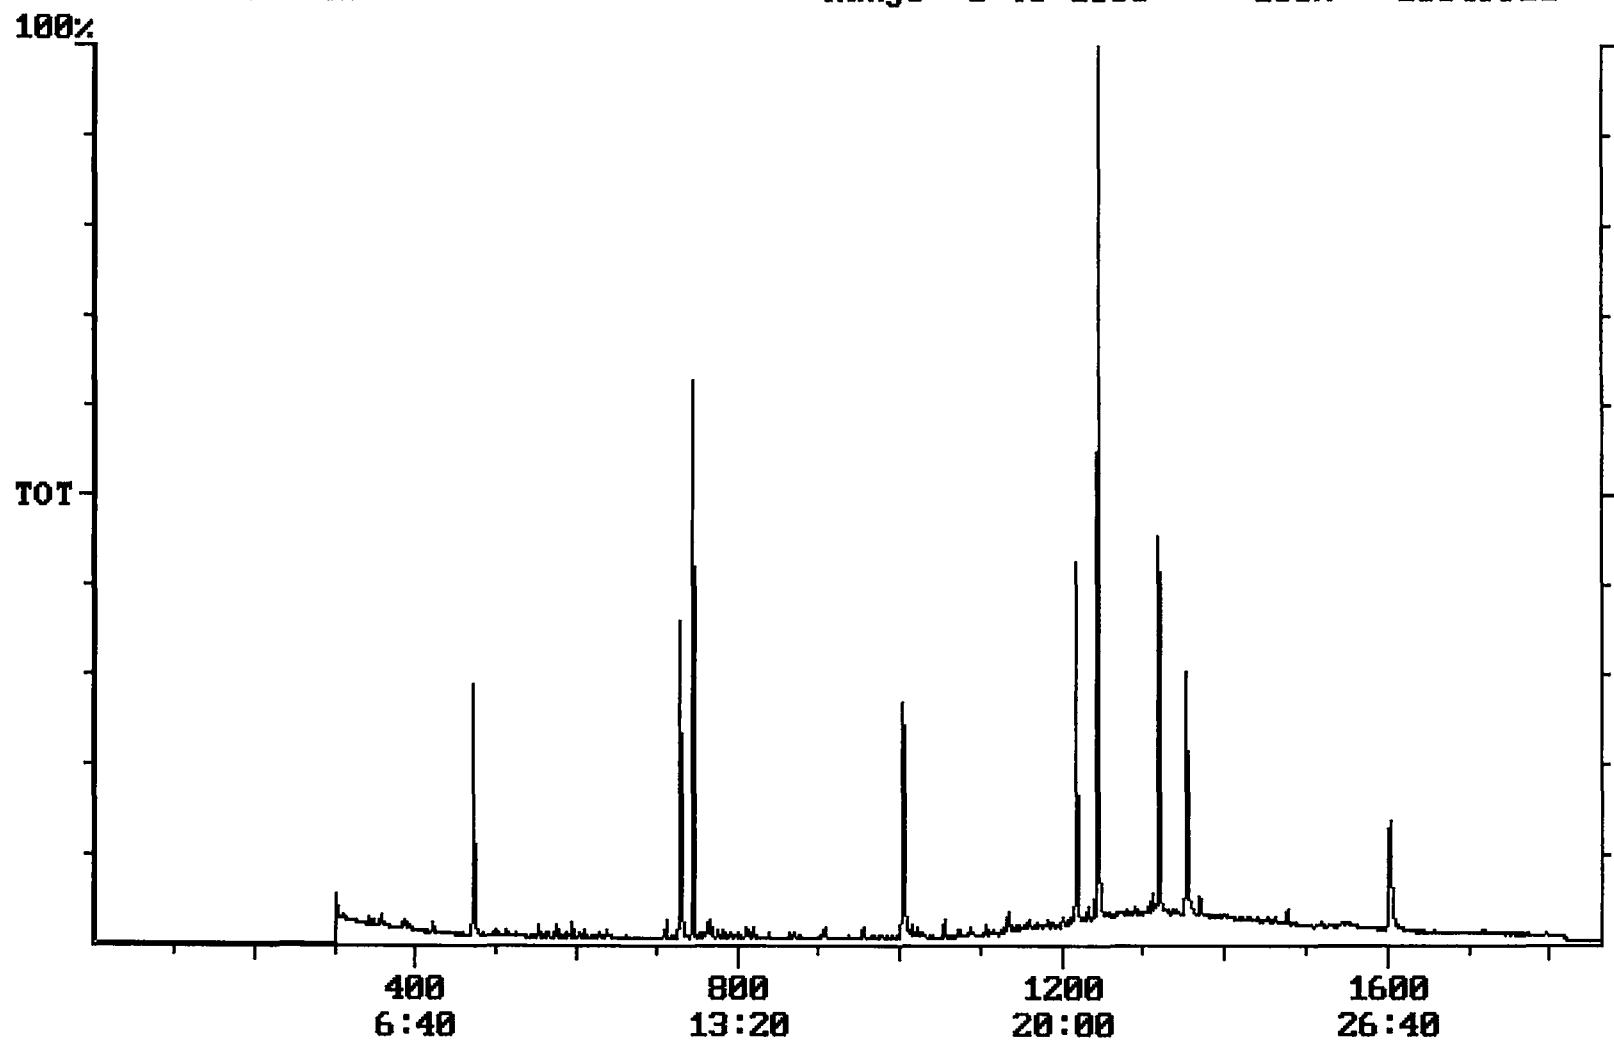

Integration Report Quanfile: 2777111 Quan Entries: 15
 Comment: BOHLK; METHOD 525; INST 204; 12/09/01; SAMPLE 27771
 Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10 (IS)	12:10	730	Auto	2,043,551	946,887
2	phenanthrene d-10 (IS)	16:44	1004	Auto	2,822,132	981,169
3	chrysene d-12 (IS)	22:33	1353	Auto	2,171,943	859,762
4	p-terphenyl d-14 (IS)	20:44	1244	Auto	5,697,586	3,877,724
5	acenaphthene d-10 (SURR)	12:10	730	Auto	2,043,551	946,887
6	phenanthrene d-10 (SURR)	16:44	1004	Auto	2,822,132	981,169
7	chrysene d-12 (SURR)	22:33	1353	Auto	2,171,943	859,762
8	1,3-dimethyl-2-nitrobenzene	7:51	471	Auto	1,002,516	492,445
9	triphenyl phosphate (S)	21:58	1318	Auto	1,411,056	677,016
10	perylene d-12 (SURR)	26:43	1603	Auto	1,585,364	347,301
11	bis(2-ethylhexyl)adipate	21:51	1311	Auto	20,988	8,834
12	bis(2-ethylhexyl)phthalate	22:49	1369	Auto	156,339	62,402
13	2,4-dinitrotoluene	13:01	781	Auto	853	853
14	butachlor	20:17	1217	Auto	22,869	9,027
15	4,4'-dichlorodiphenyl ether	20:39	1239	Auto	4,935	2,757

reviewed IS/surr's

Quantitation Report Quanfile: 2777111 Quan Entries: 15
 Comment: BOHLK; METHOD 525; INST 204; 12/09/01; SAMPLE 27771
 Sorted via: Entry Number ↑ (S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10 (IS)	I	730	12:10	BV	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1004	16:44	BV	5.000	UG/L
3	chrysene d-12 (IS)	I	1353	22:33	BB	5.000	UG/L
4	p-terphenyl d-14 (IS)	I	1244	20:44	BV	5.000	UG/L
5	acenaphthene d-10 (SURR)	A	730	12:10	BV	1.975	UG/L
6	phenanthrene d-10 (SURR)	A	1004	16:44	BV	2.131	UG/L
7	chrysene d-12 (SURR)	A	1353	22:33	BB	2.004	UG/L
8	1,3-dimethyl-2-nitrobenzene	A	471	7:51	BV	5.257	UG/L
9	triphenyl phosphate (S)	A	1318	21:58	BB	6.705	UG/L
10	perylene d-12 (SURR)	A	1603	26:43	BB	5.010	UG/L
16	bis(2-ethylhexyl)adipate	A	1311	21:51	MM	0.065	UG/L
17	bis(2-ethylhexyl)phthalate	A	1369	22:49	BV	0.246	UG/L
21	2,4-dinitrotoluene	A	781	13:01	BB	0.007	UG/L
27	butachlor	A	1217	20:17	BB	0.090	UG/L
28	4,4'-dichlorodiphenyl ether	A	1239	20:39	BB	0.020	UG/L

• **Comments for Sample AD27771 - Analysis \$525**

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 01-22-2002 Time: 15:13:45

The recoveries for 2 of the 18 compounds in the LCS Standard were below their acceptance ranges. The recoveries for 3 of the 18 compounds in the Spiked Sample were outside of their acceptance ranges. The recovery for 1 of the 3 Surrogate Standards in this sample was above its acceptance range. The breakdown for Endrin in the Breakdown Standard was 68%. The injection port is kept at 280 degrees Celcius which may be contributing to high Endrin Breakdown. An investigation into modifying injection port parameters will be made.