


User: Bohk, Ted
 Westchester Dept. of Labs & Research
 Date: 01/08/2002 Time: 14:40:21

Sample: AD27775
 Analysis: \$525 Organic Chemicals - 525.2
 Units: ug
 Started: 11/24/01 14:38 Ended: 12/9/01 14:38 Analyst: TB
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.20
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		< MDL		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenzen		5.0		1.0
20	Surr_Triphenyl phosphate		6.5		1.0
21	Surr_Perylene-d12		4.2		1.0

Chromatogram Plot
 File: E:\27775NN Date: Dec-10-1991 01:32:10
 Comment: BOHLK; METHOD 525; INST 204; 12/09/01; SAMPLE 27775
 Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
 Plotted: 1 to 1860 Range: 1 to 1860 100% = 13119500

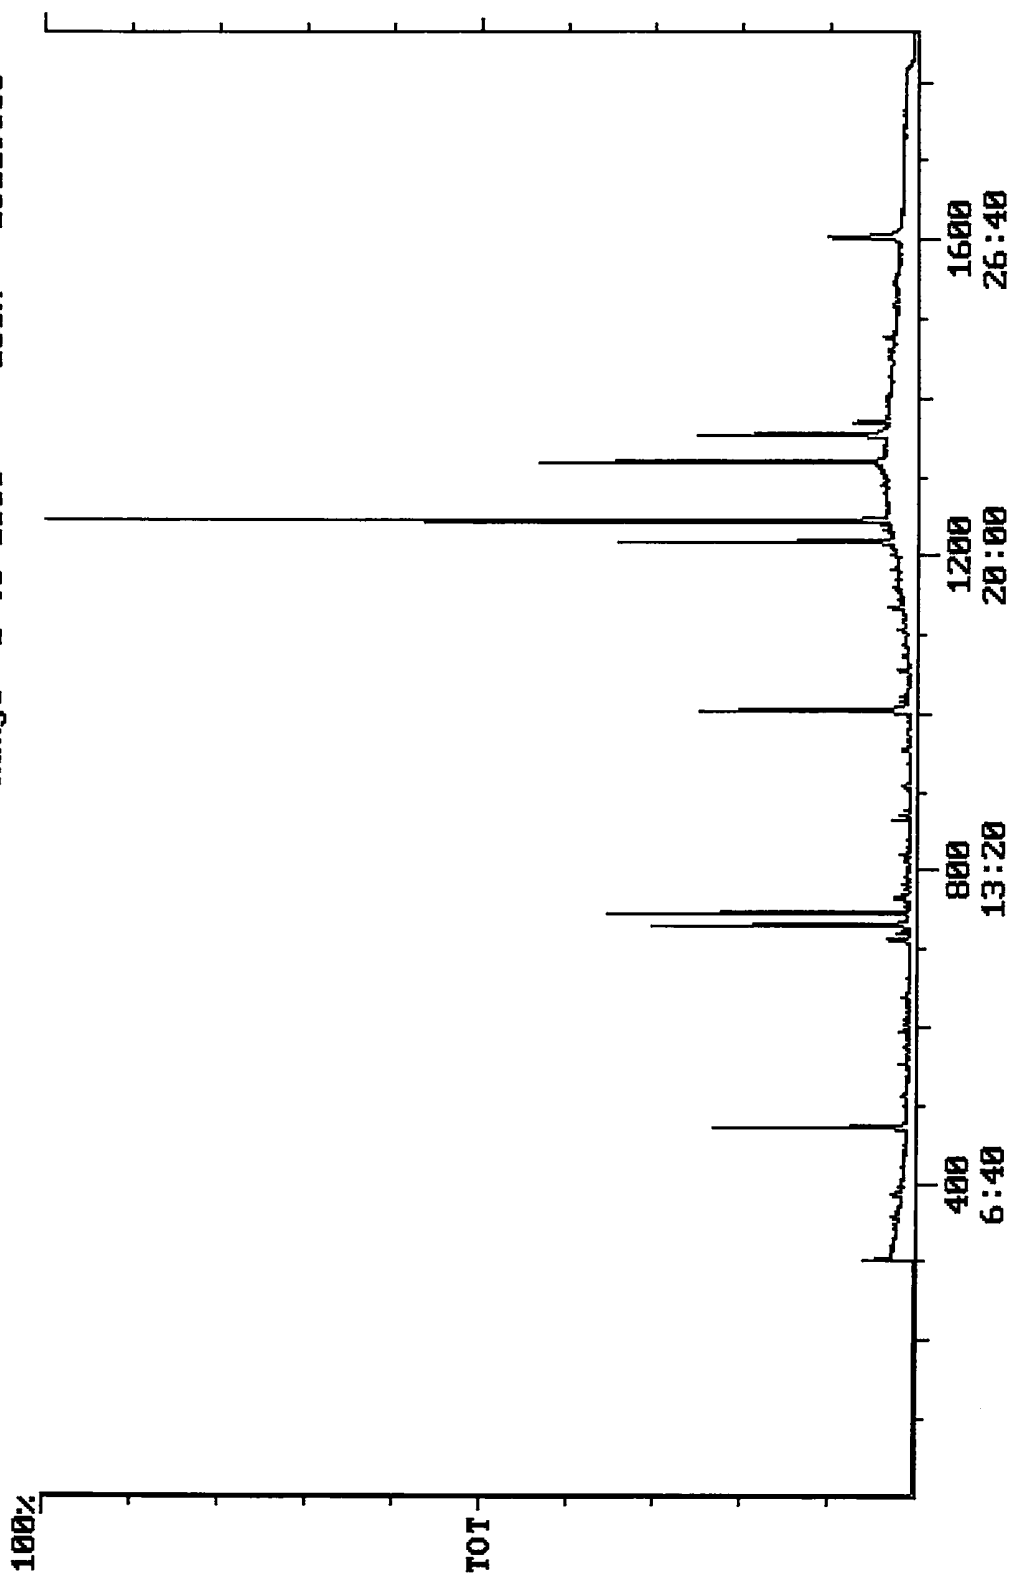

Integration Report Quantfile: 27775NN Quan Entries: 15
 Comment: BOHLK; METHOD 525; INST 204; 12/09/01; SAMPLE 27775
 Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10(IS)	12:10	730	Auto	1,932,287	988,340
2	phenanthrene d-10 (IS)	16:44	1004	Auto	3,026,332	1,123,588
3	chrysene d-12(IS)	22:33	1353	Auto	2,268,708	844,445
4	p-terphenyl d-14(IS)	20:44	1244	Auto	6,647,703	4,619,548
5	acenaphthene d-10(SURR)	12:10	730	Auto	1,932,287	988,340
6	phenanthrene d-10(SURR)	16:44	1004	Auto	3,026,332	1,123,588
7	chrysene d-12 (SURR)	22:33	1353	Auto	2,268,708	844,445
8	1,3-dimethyl-2-nitrobenzene	7:51	471	Auto	893,177	446,742
9	triphenyl phosphate (S)	21:58	1318	Auto	1,418,133	762,925
10	perylene d-12 (SURR)	26:43	1603	Auto	1,393,939	263,872
11	bis(2-ethylhexyl)adipate	21:51	1311	Auto	14,070	5,849
12	bis(2-ethylhexyl)phthalate	22:49	1369	Auto	350,389	156,935
13	2,6-dinitrotoluene	11:50	710	Auto	64,082	35,455
14	2,4-dinitrotoluene	13:01	781	Auto	11,920	1,871
15	butachlor	20:17	1217	Auto	25,543	14,314

reversed IS/surrs

Quantitation Report Quantfile: 27775NN Quan Entries: 15
 Comment: BOHLK; METHOD 525; INST 204; 12/09/01; SAMPLE 27775
 Sorted via: Entry Number ↑ (S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10(IS)	I	730	12:10	BV	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1004	16:44	BV	5.000	UG/L
3	chrysene d-12(IS)	I	1353	22:33	BB	5.000	UG/L
4	p-terphenyl d-14(IS)	I	1244	20:44	BB	5.000	UG/L
5	acenaphthene d-10(SURR)	A	730	12:10	BV	1.601	UG/L
6	phenanthrene d-10(SURR)	A	1004	16:44	BV	1.959	UG/L
7	chrysene d-12 (SURR)	A	1353	22:33	BB	1.794	UG/L
8	1,3-dimethyl-2-nitrobenzene	A	471	7:51	BV	4.954	UG/L
9	triphenyl phosphate (S)	A	1318	21:58	BV	6.451	UG/L
10	perylene d-12 (SURR)	A	1603	26:43	VB	4.217	UG/L
16	bis(2-ethylhexyl)adipate	A	1311	21:51	MM	0.042	UG/L
17	bis(2-ethylhexyl)phthalate	A	1369	22:49	BV	0.532	UG/L
20	2,6-dinitrotoluene	A	710	11:50	BB	0.564	UG/L
21	2,4-dinitrotoluene	A	781	13:01	MM	0.097	UG/L
27	butachlor	A	1217	20:17	VB	0.093	UG/L

Comments for Sample AD27775 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 01-22-2002 Time: 15:35:11

The recoveries for 2 of the 18 compounds in the LCS Standard were below their acceptance ranges. The recoveries for 3 of the 18 compounds in the Spiked Sample were outside of their acceptance ranges. The breakdown for Endrin in the Breakdown Standard was 68%. The injection port is kept at 280 degrees Celcius which may be contributing to high Endrin Breakdown. An investigation into modifying injection port parameters will be made.