

User: Fakhouri, Morgan  
 Westchester Dept. of Labs & Research  
 Date: 12/19/2001 Time: 11:10:30

Sample: AD28322  
 Analysis: \$LP525 Organic Extractables  
 Units: ug  
 Started: 12/19/01 11:06 Ended: 12/19/01 11:06 Analyst: MF  
 Page: 1

|   | Component Name | Viol | Result |
|---|----------------|------|--------|
| 1 | DFTPP          |      | passed |
| 2 | ENDRIN         |      | 7.5    |
| 3 | DDT            |      | 12.7 ✓ |

## DFTPP

Data File : C:\MSDCHEM\1\DATA\121801\DFTPP3.D

Acq On : 18 Dec 2001 9:38 am

Sample :

Misc :

MS Integration Params: BENZO.P

Vial: 2

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\121401.M (RTE Integrator)

Title : Quantitation For Method 525.2

## Spectrum Information: Scan 857

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 25.7         | 207424     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 4438       | PASS                |
| 69             | 198             | 0.00            | 100             | 32.1         | 258880     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 1139       | PASS                |
| 127            | 198             | 10              | 80              | 50.6         | 408320     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 50              | 100             | 100.0        | 806272     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 53416      | PASS                |
| 275            | 198             | 10              | 60              | 17.7         | 143104     | PASS                |
| 365            | 198             | 1               | 100             | 1.9          | 15488      | PASS                |
| 441            | 443             | 0.01            | 100             | 74.7         | 78352      | PASS                |
| 442            | 198             | 50              | 100             | 69.1         | 557184     | PASS                |
| 443            | 442             | 15              | 24              | 18.8         | 104912     | PASS                |

DFTPP3.D 121401.M

Tue Dec 18 11:58:48 2001

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\121801\DFTPP3.D

Acq On : 18 Dec 2001 9:38 am

Sample :

Misc :

MS Integration Params: BENZO.P

Vial: 2

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\121401.M (RTE Integrator)

Title : Quantitation For Method 525.2

Smoothing : ON

Sampling : 1

Start Thrs: 0.15

Stop Thrs : 0

Filtering: 5

Min Area: 2500 Area counts

Max Peaks: 10

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5



Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 27.876      | 1297          | 1301        | 1307         | rM       | 3343953        | 6222012       | 100.00%         | 92.487%       |
| 2         | 28.475      | 1364          | 1367        | 1370         | rM 4     | 101535         | 177056        | 2.85%           | 2.632%        |
| 3         | 29.527      | 1479          | 1483        | 1487         | rM 5     | 163839         | 328359        | 5.28%           | 4.881%        |

*7* *Curdian*

Sum of corrected areas: 6727427

File : C:\MSDCHEM\1\DATA\121801\DFTPP3.D  
 Operator : McLean  
 Acquired : 18 Dec 2001 9:38 am using AcqMethod BIG3  
 Instrument : Instrumen  
 Sample Name:  
 Misc Info :  
 Vial Number: 2

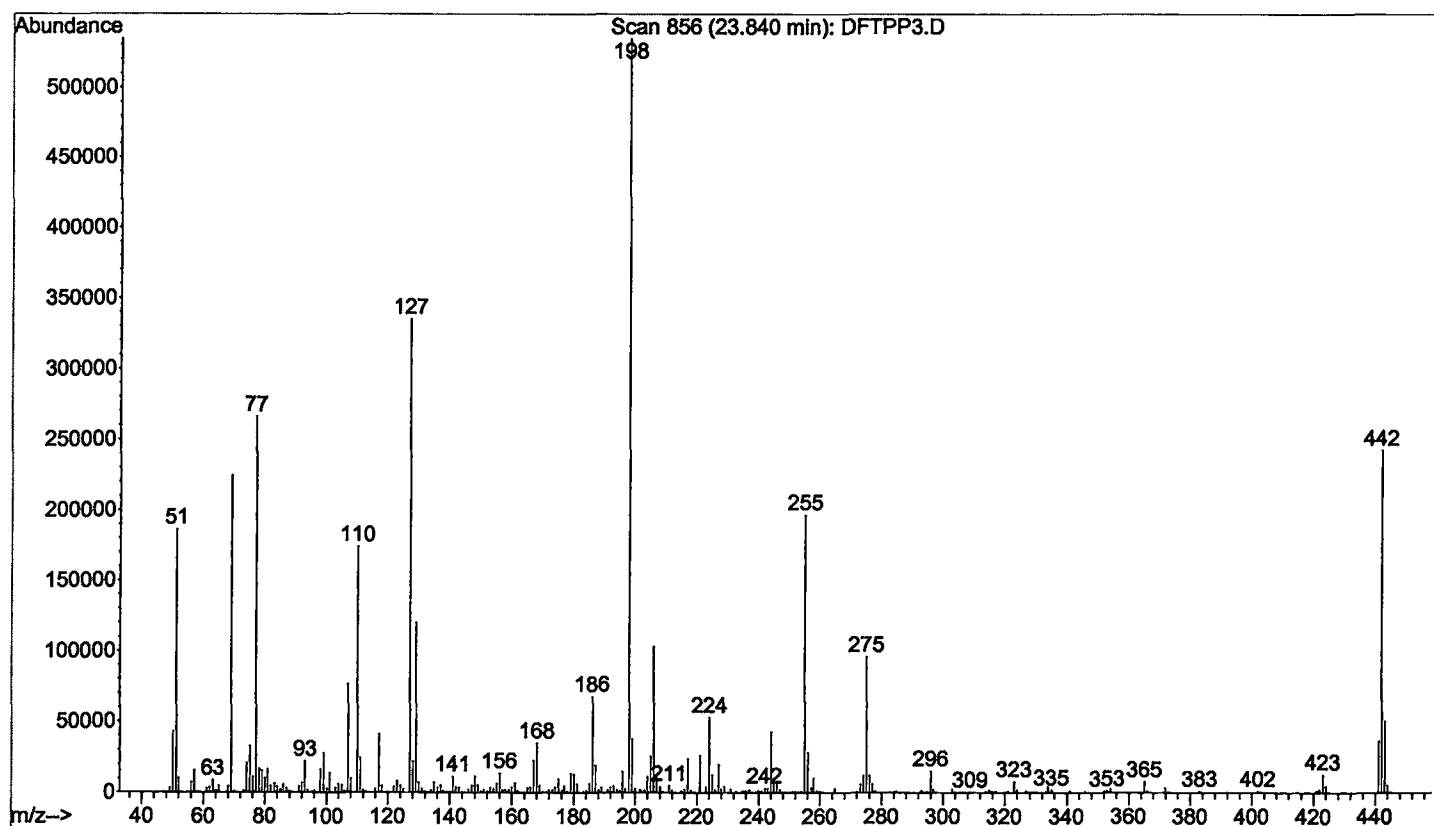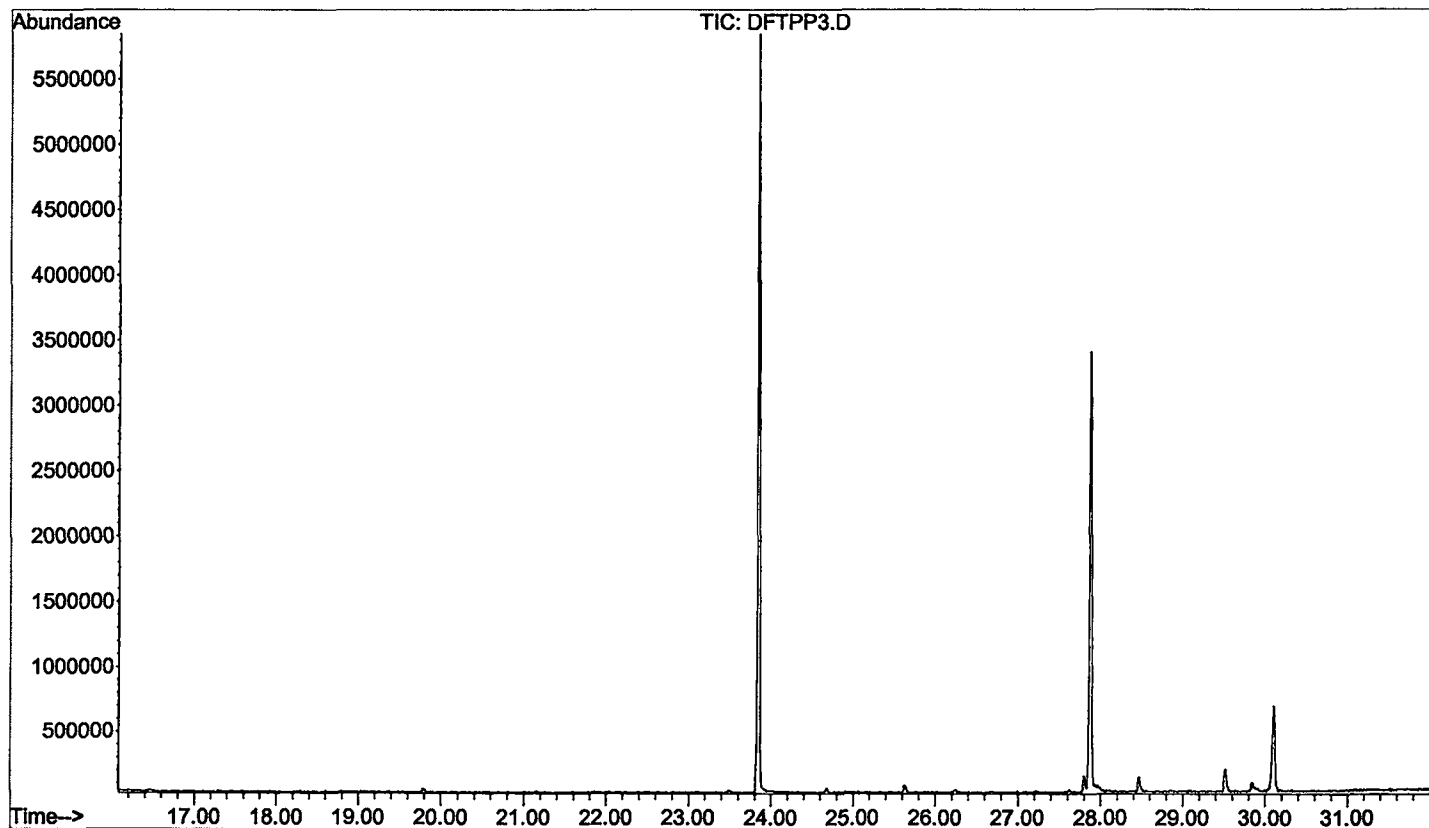

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\121801\DDT3.D

Acq On : 18 Dec 2001 10:18 am

Sample :

Misc :

MS Integration Params: BENZO.P

Vial: 3

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\121401.M (RTE Integrator)

Title : Quantitation For Method 525.2

Smoothing : ON

Sampling : 1

Start Thrs: 0.15

Stop Thrs : 0

Filtering: 5

Min Area: 2500 Area counts

Max Peaks: 10

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 28.266      | 1341          | 1344        | 1349         | rM 2     | 604898         | 1203757       | 14.57%          | 12.719%       |
| 2         | 29.146      | 1433          | 1441        | 1445         | rM       | 4607793        | 8260633       | 100.00%         | 87.281%       |

Sum of corrected areas: 9464390