


User: Bohlk, Ted
 Westchester Dept. of Labs & Research
 Date: 12/19/2001 Time: 10:15:02

Sample: AD26204
 Analysis: \$525 Organic Chemicals - 525.2
 Units: ug
 Started: 11/5/01 10:13 Ended: 11/21/01 10:13 Analyst: TB
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.20
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		1.1		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenze		4.8		1.0
20	Surr_Triphenyl phosphate		5.4		1.0
21	Surr_Perylene-d12 *		2.9		1.0

flag

Chromatogram Plot File: E:\26204A Date: Nov-21-1991 22:05:23
Comment: BOHLK; METHOD 525; INST 204; 11/21/01; SAMPLE 26204
Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
Plotted: 1 to 1860 Range: 1 to 1860 100% = 4302321

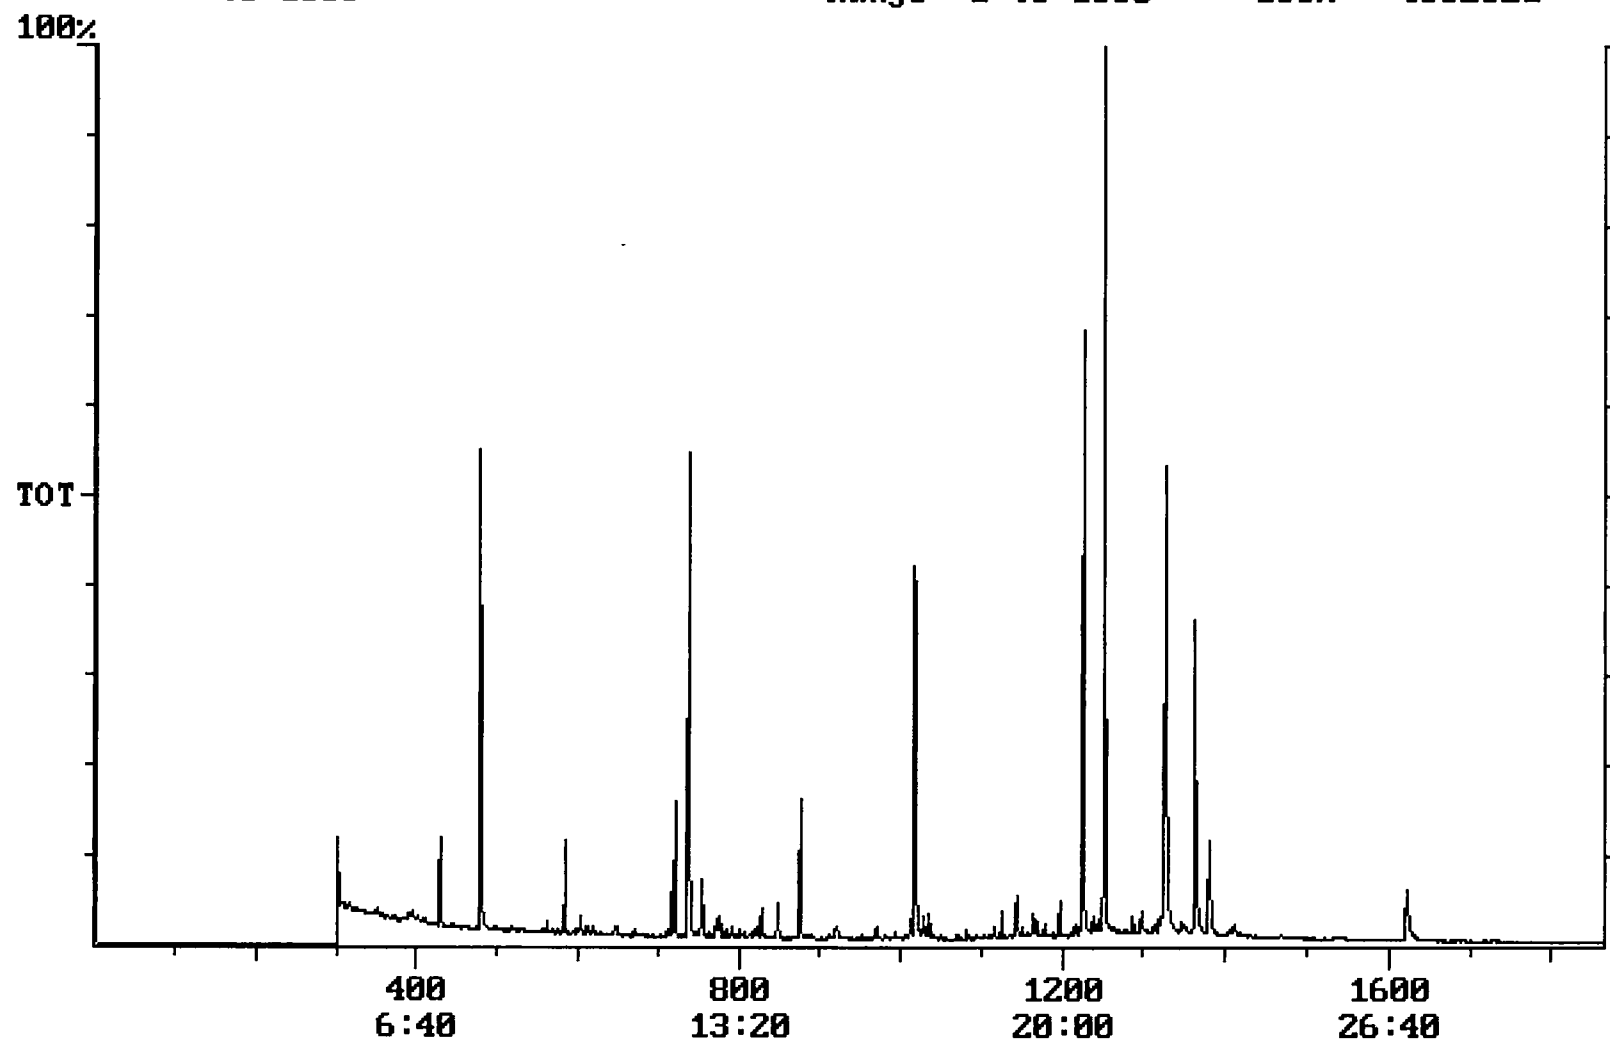

Integration Report Quanfile: 26204A Quan Entries: 13
 Comment: BOHLK; METHOD 525; INST 204; 11/21/01; SAMPLE 26204
 Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10(IS)	12:19	739	Auto	1,138,677	528,339
2	phenanthrene d-10 (IS)	16:57	1017	Auto	1,692,516	591,087
3	chrysene d-12(IS)	22:42	1362	Auto	1,142,426	448,753
4	p-terphenyl d-14(IS)	20:51	1251	Auto	1,981,924	1,261,144
5	acenaphthene d-10(SURR)	12:19	739	Auto	1,138,677	528,339
6	phenanthrene d-10(SURR)	16:57	1017	Auto	1,692,516	591,087
7	chrysene d-12 (SURR)	22:42	1362	Auto	1,142,426	448,753
8	1,3-dimethyl-2-nitrobenzene	7:59	479	Auto	676,050	357,461
9	triphenyl phosphate (S)	22:07	1327	Auto	879,018	301,500
10	perylene d-12 (SURR)	27:02	1622	Auto	398,488	63,810
11	bis(2-ethylhexyl)adipate	22:03	1323	Auto	27,225	2,756
12	bis(2-ethylhexyl)phthalate	22:59	1379	Auto	461,600	130,722
13	2,6-dinitrotoluene	11:58	718	Auto	57,092	29,094

reviewed IS/SURR's

Quantitation Report

Quanfile: 26204A

Quan Entries: 13

Comment: BOHLK; METHOD 525; INST 204; 11/21/01; SAMPLE 26204

Sorted via: Entry Number ↑

(S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10(IS)	I	739	12:19	BB	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1017	16:57	BV	5.000	UG/L
3	chrysene d-12(IS)	I	1362	22:42	BV	5.000	UG/L
4	p-terphenyl d-14(IS)	I	1251	20:51	BB	5.000	UG/L
5	acenaphthene d-10(SURR)	A	739	12:19	BB	3.780	UG/L
6	phenanthrene d-10(SURR)	A	1017	16:57	BV	3.665	UG/L
7	chrysene d-12 (SURR)	A	1362	22:42	BV	3.709	UG/L
8	1,3-dimethyl-2-nitrobenzene	A	479	7:59	BB	4.767	UG/L
9	triphenyl phosphate (S)	A	1327	22:07	BB	5.367	UG/L
10	perylene d-12 (SURR)	A	1622	27:02	BB	2.890	UG/L
16	bis(2-ethylhexyl)adipate	A	1323	22:03	MM	0.198	UG/L
17	bis(2-ethylhexyl)phthalate	A	1379	22:59	BB	1.060	UG/L
20	2,6-dinitrotoluene	A	718	11:58	BB	0.781	UG/L

Comments for Sample AD26204 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 12-21-2001 Time: 13:54:06

The breakdown for Endrin in the Breakdown Standard is 53%. Recoveries for 6 of the 18 compounds in the MDL Standard were outside of their acceptance ranges. Recoveries for 4 of the 18 compounds in the LCS Standard were outside of their acceptance ranges. The level for bis(2-Ethylhexyl)phthalate was 0.73 ug/L in the Laboratory Blank. The recovery for 1 of the 3 Surrogate Standards in this sample was below its acceptance range.