


User: Bohlk, Ted
 Westchester Dept. of Labs & Research
 Date: 12/19/2001 Time: 10:16:27

Sample: AD26205
 Analysis: §525 Organic Chemicals - 525.2
 Units: ug
 Started: 11/5/01 10:15 Ended: 11/21/01 10:15 Analyst: TB
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.20
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		0.80		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenze		4.8		1.0
20	Surr_Triphenyl phosphate		5.2		1.0
21	Surr_Perylene-d12		3.8		1.0

Chromatogram Plot File: E:\26205B Date: Nov-21-1991 22:39:47
Comment: BOHLK; METHOD 525; INST 204; 11/21/01; SAMPLE 26205
Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
Plotted: 1 to 1860 Range: 1 to 1860 100% = 3571409

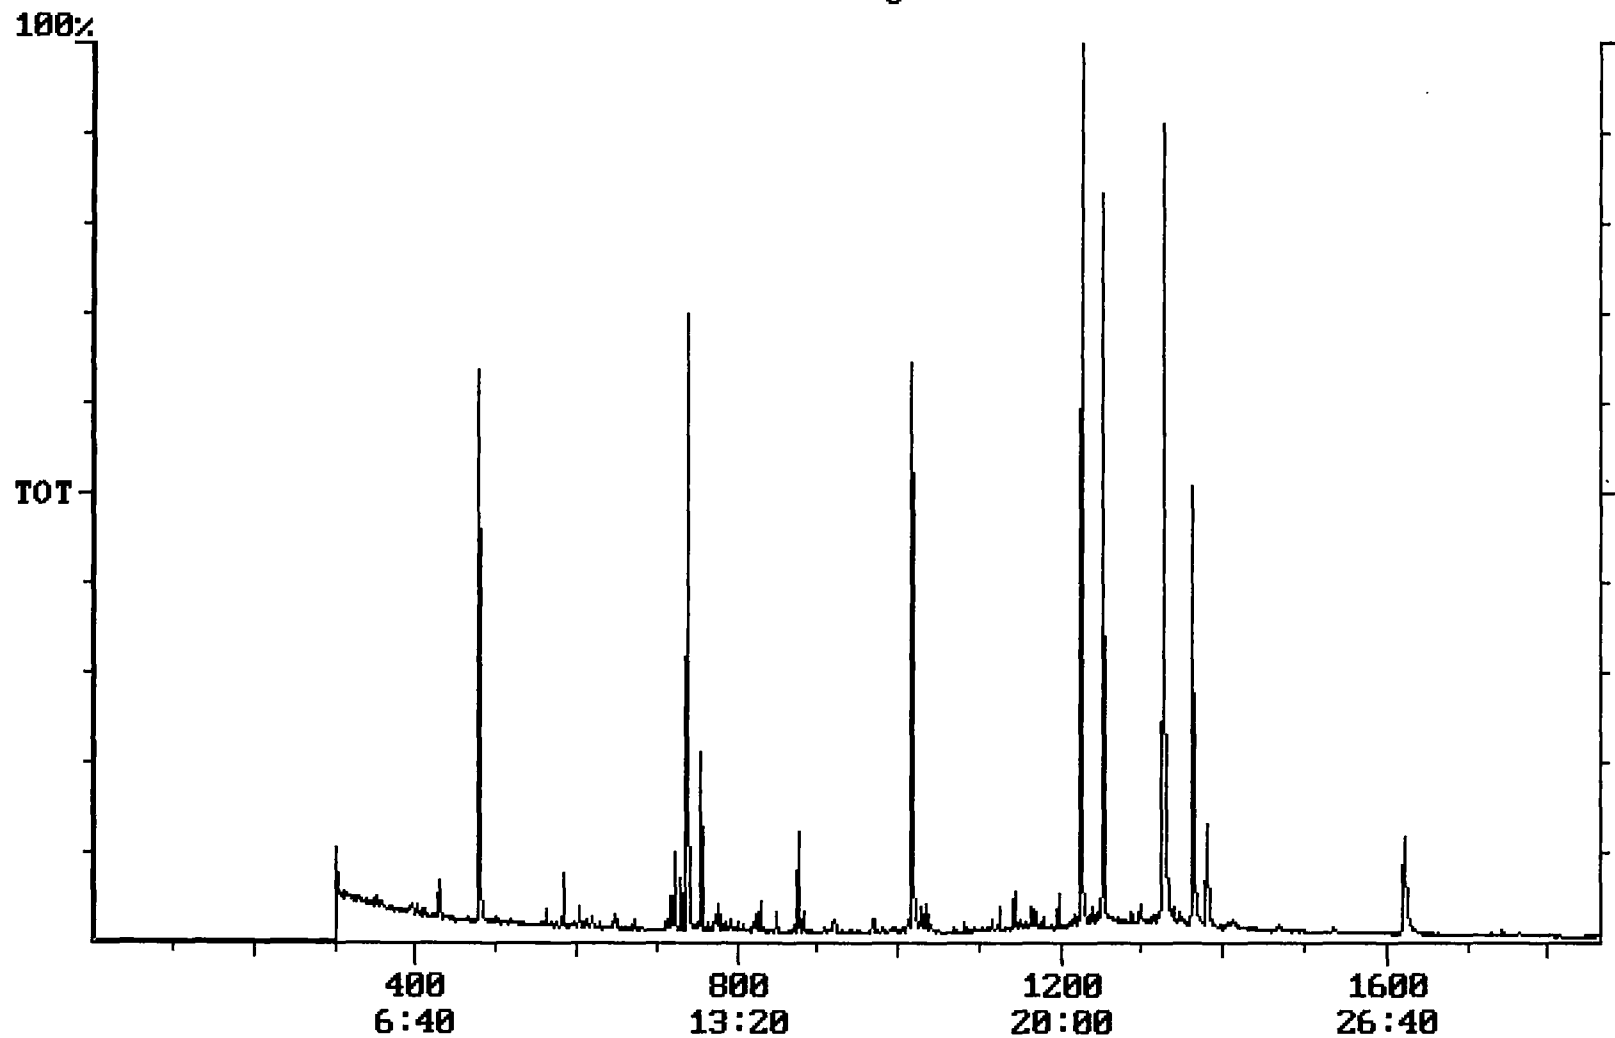

Integration Report

Quanfile: 26205B

Quan Entries: 14

Comment: BOHLK; METHOD 525; INST 204; 11/21/01; SAMPLE 26205

Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10(IS)	12:19	739	Auto	1,220,614	559,883
2	phenanthrene d-10 (IS)	16:57	1017	Auto	1,890,590	799,634
3	chrysene d-12(IS)	22:42	1362	Auto	1,304,846	501,363
4	p-terphenyl d-14(IS)	20:51	1251	Auto	1,623,594	878,655
5	acenaphthene d-10(SURR)	12:19	739	Auto	1,220,614	559,883
6	phenanthrene d-10(SURR)	16:57	1017	Auto	1,890,590	799,634
7	chrysene d-12 (SURR)	22:42	1362	Auto	1,304,846	501,363
8	1,3-dimethyl-2-nitrobenzene	7:59	479	Auto	730,289	362,500
9	triphenyl phosphate (S)	22:07	1327	Auto	974,691	425,218
10	perylene d-12 (SURR)	27:02	1622	Auto	599,479	102,952
11	bis(2-ethylhexyl)adipate	22:03	1323	Auto	26,530	2,675
12	bis(2-ethylhexyl)phthalate	23:00	1380	Auto	404,895	124,074
13	2,6-dinitrotoluene	11:58	718	Auto	43,733	19,007
14	2,4-dinitrotoluene	12:56	776	Auto	1,047	1,047

reversed IS/SURR's

Quantitation Report

Quanfile: 26205B

Quan Entries: 14

Comment: BOHLK; METHOD 525; INST 204; 11/21/01; SAMPLE 26205

Sorted via: Entry Number ↑

(S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10(IS)	I	739	12:19	BB	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1017	16:57	BV	5.000	UG/L
3	chrysene d-12(IS)	I	1362	22:42	BV	5.000	UG/L
4	p-terphenyl d-14(IS)	I	1251	20:51	BB	5.000	UG/L
5	acenaphthene d-10(SURR)	A	739	12:19	BB	4.947	UG/L
6	phenanthrene d-10(SURR)	A	1017	16:57	BV	4.997	UG/L
7	chrysene d-12 (SURR)	A	1362	22:42	BV	5.170	UG/L
8	1,3-dimethyl-2-nitrobenzene	A	479	7:59	BV	4.803	UG/L
9	triphenyl phosphate (S)	A	1327	22:07	BB	5.211	UG/L
10	perylene d-12 (SURR)	A	1622	27:02	BB	3.807	UG/L
16	bis(2-ethylhexyl)adipate	A	1323	22:03	MM	0.169	UG/L
17	bis(2-ethylhexyl)phthalate	A	1300	23:00	BB	0.805	UG/L
20	2,6-dinitrotoluene	A	718	11:58	BB	0.554	UG/L
21	2,4-dinitrotoluene	A	776	12:56	BB	0.012	UG/L

• Comments for Sample AD26205 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 12-21-2001 Time: 13:55:10

The breakdown for Endrin in the Breakdown Standard is 53%. Recoveries for 6 of the 18 compounds in the MDL Standard were outside of their acceptance ranges. Recoveries for 4 of the 18 compounds in the LCS Standard were outside of their acceptance ranges. The level for bis(2-Ethylhexyl)phthalate was 0.73 ug/L in the Laboratory Blank.