


User: Bohlk, Ted
 Westchester Dept. of Labs & Research
 Date: 12/19/2001 Time: 14:47:49

Sample: AD26207
 Analysis: \$525 Organic Chemicals - 525.2
 Units: ug
 Started: 11/5/01 14:46 Ended: 11/21/01 14:46 Analyst: TB
 Result source: manual entry
 Page: 1

	Component Name	Vial	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.40
4	Atrazine		< MDL		0.20
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		0.95		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Mollinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenze		4.4		1.0
20	Surr_Triphenyl phosphate		4.8		1.0
21	Surr_Perylene-d12		3.5		1.0

Chromatogram Plot File: E:\26207D Date: Nov-21-1991 23:48:39
 Comment: BOHLK; METHOD 525; INST 204; 11/21/01; SAMPLE 26207
 Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
 Plotted: 1 to 1860 Range: 1 to 1860 100% = 3533816

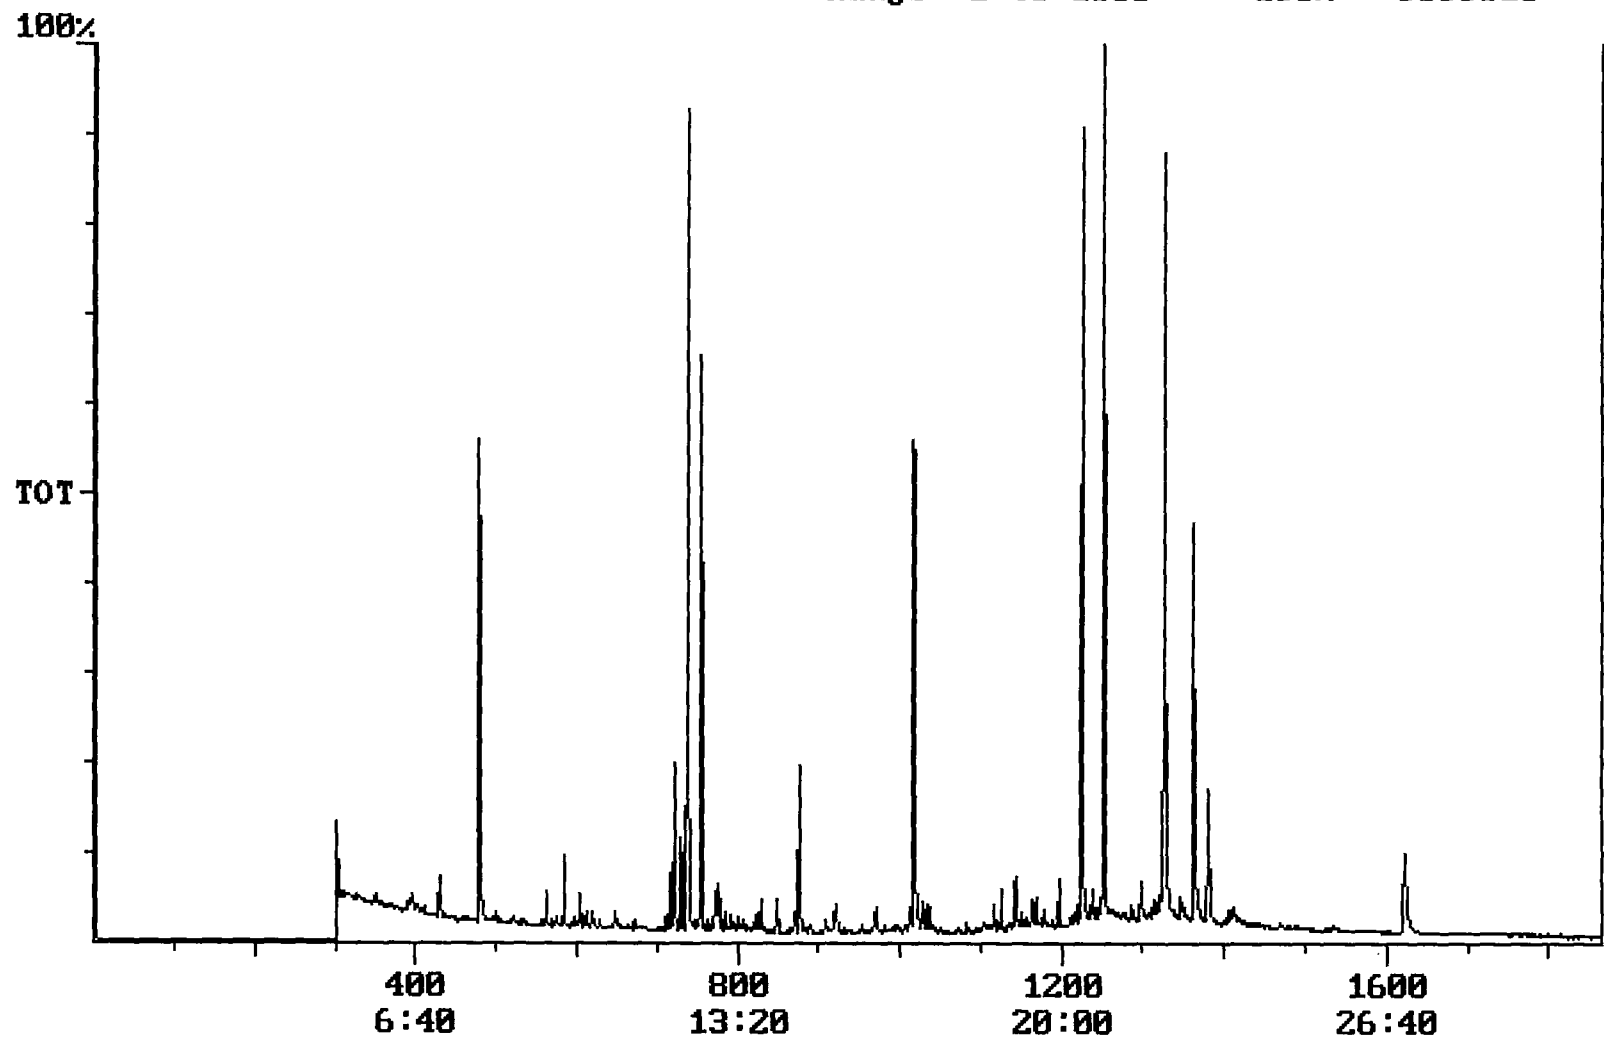

Integration Report Quanfile: 26207D Quan Entries: 15
 Comment: BOHLK; METHOD 525; INST 204; 11/21/01; SAMPLE 26207
 Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10 (IS)	12:19	739	Auto	1,166,894	772,051
2	phenanthrene d-10 (IS)	16:57	1017	Auto	1,824,007	683,385
3	chrysene d-12 (IS)	22:42	1362	Auto	1,223,187	467,030
4	p-terphenyl d-14 (IS)	20:52	1252	Auto	1,917,534	938,362
5	acenaphthene d-10 (SURR)	12:19	739	Auto	1,166,894	772,051
6	phenanthrene d-10 (SURR)	16:57	1017	Auto	1,824,007	683,385
7	chrysene d-12 (SURR)	22:42	1362	Auto	1,223,187	467,030
8	1,3-dimethyl-2-nitrobenzophenone	7:59	479	Auto	645,657	284,505
9	triphenyl phosphate (S)	22:07	1327	Auto	833,617	392,811
10	perylene d-12 (SURR)	27:02	1622	Auto	522,807	85,169
11	hexachlorocyclopentadiene	10:10	610	Auto	897	897
12	bis(2-ethylhexyl)adipate	22:04	1324	Auto	64,071	3,828
13	bis(2-ethylhexyl)phthalate	23:00	1380	Auto	446,205	153,031
14	2,6-dinitrotoluene	11:59	719	Auto	69,861	34,080
15	butachlor	20:25	1225	Auto	1,366	1,366

reviewed IS/SURR

Quantitation Report Quanfile: 26207D Quan Entries: 15
 Comment: BOHLK; METHOD 525; INST 204; 11/21/01; SAMPLE 26207
 Sorted via: Entry Number ↑ (S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10(IS)	I	739	12:19	BV	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1017	16:57	BV	5.000	UG/L
3	chrysene d-12(IS)	I	1362	22:42	BB	5.000	UG/L
4	p-terphenyl d-14(IS)	I	1252	20:52	BB	5.000	UG/L
5	acenaphthene d-10(SURR)	A	739	12:19	BV	4.004	UG/L
6	phenanthrene d-10(SURR)	A	1017	16:57	BV	4.082	UG/L
7	chrysene d-12 (SURR)	A	1362	22:42	BB	4.104	UG/L
8	1,3-dimethyl-2-nitrobenzene	A	479	7:59	BV	4.442	UG/L
9	triphenyl phosphate (S)	A	1327	22:07	BB	4.754	UG/L
10	perylene d-12 (SURR)	A	1622	27:02	BV	3.541	UG/L
11	hexachlorocyclopentadiene	A	610	10:10	BB	0.017	UG/L
16	bis(2-ethylhexyl)adipate	A	1324	22:04	MM	0.436	UG/L
17	bis(2-ethylhexyl)phthalate	A	1300	23:00	VB	0.952	UG/L
20	2,6-dinitrotoluene	A	719	11:59	BB	0.937	UG/L
27	butachlor	A	1225	20:25	BB	0.013	UG/L

Comments for Sample AD26207 - Analysis \$525

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 12-21-2001 Time: 13:58:00

The breakdown for Endrin in the Breakdown Standard is 53%. Recoveries for 6 of the 18 compounds in the MDL Standard were outside of their acceptance ranges. Recoveries for 4 of the 18 compounds in the LCS Standard were outside of their acceptance ranges. The level for bis(2-Ethylhexyl)phthalate was 0.73 ug/L in the Laboratory Blank.