

User: Fakhouri, Morgan
 Westchester Dept. of Labs & Research
 Date: 01/16/2002 Time: 14:33:36

Sample: AD28172
 Analysis: \$LP525 Organic Extractables
 Units: ug
 Started: 1/16/02 14:32 Ended: 1/16/02 14:32 Analyst: MF
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result
1	DFTPP		passed
2			
3	DDT		13

DFTPP

Data File : C:\MSDCHEM\1\DATA\121701\DFTPP1.D

Vial: 1

Acq On : 17 Dec 2001 12:43 pm

Operator: McLean

Sample : dftpp +end

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Method : C:\MSDCHEM\1\5973N\011402.M (RTE Integrator)

Title : Quantitation For Method 525.2



Spectrum Information: Scan 857

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	227456	PASS
68	69	0.00	2	1.4	4029	PASS
69	198	0.00	100	32.0	287488	PASS
70	69	0.00	2	0.8	2360	PASS
127	198	10	80	48.6	436224	PASS
197	198	0.00	1	0.4	4017	PASS
198	198	50	100	100.0	898176	PASS
199	198	5	9	6.4	57376	PASS
275	198	10	60	18.8	168896	PASS
365	198	1	100	1.5	13330	PASS
441	443	0.01	100	87.2	102480	PASS
442	198	50	100	67.0	601344	PASS
443	442	15	24	19.5	117528	PASS

DFTPP1.D 011402.M

Tue Jan 15 11:24:29 2002

File : C:\MSDCHEM\1\DATA\121701\DFTPP1.D
 Operator : McLean
 Acquired : 17 Dec 2001 12:43 pm using AcqMethod BIG3
 Instrument : Instrumen
 Sample Name: dftpp +end
 Misc Info :
 Vial Number: 1

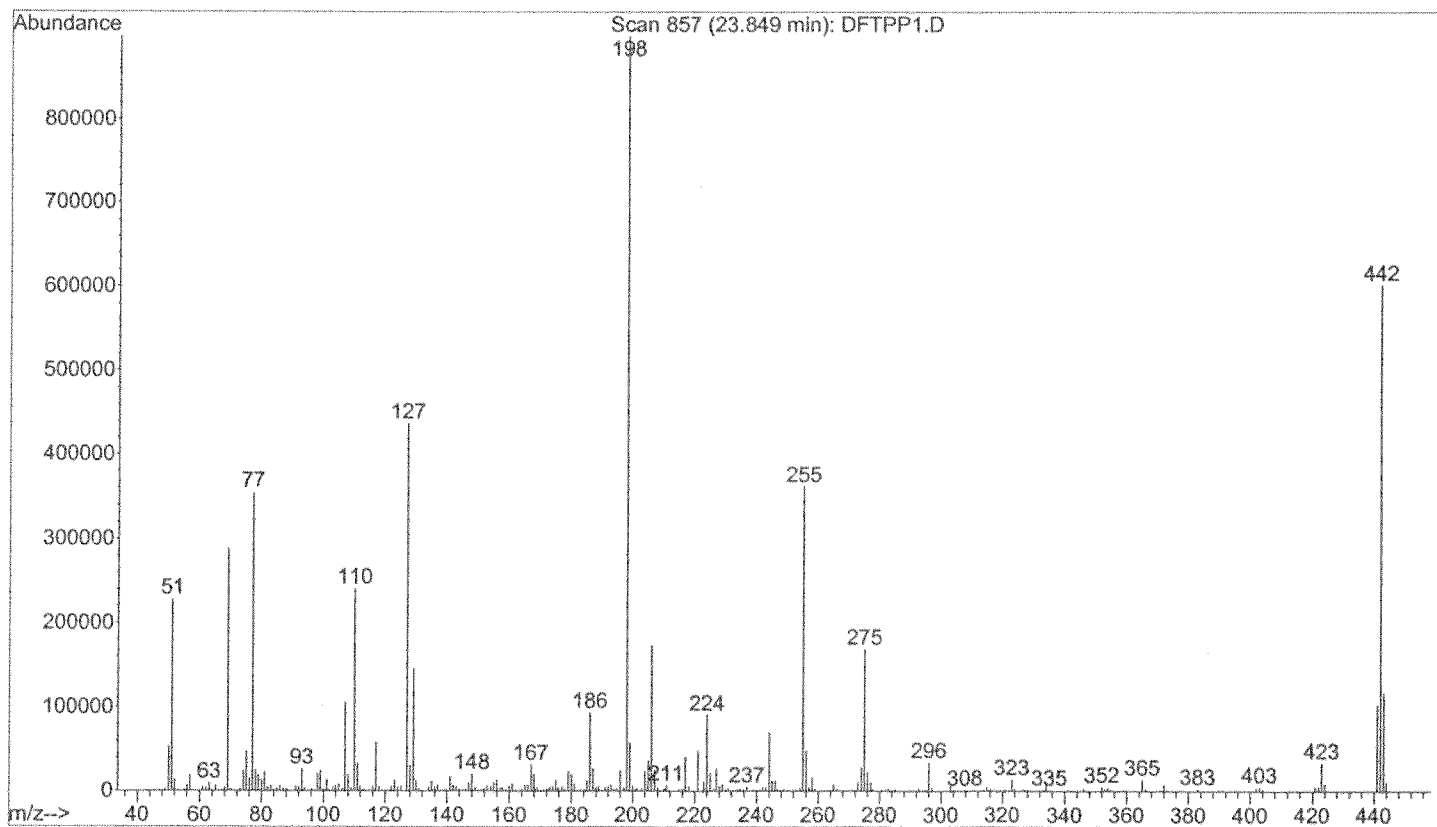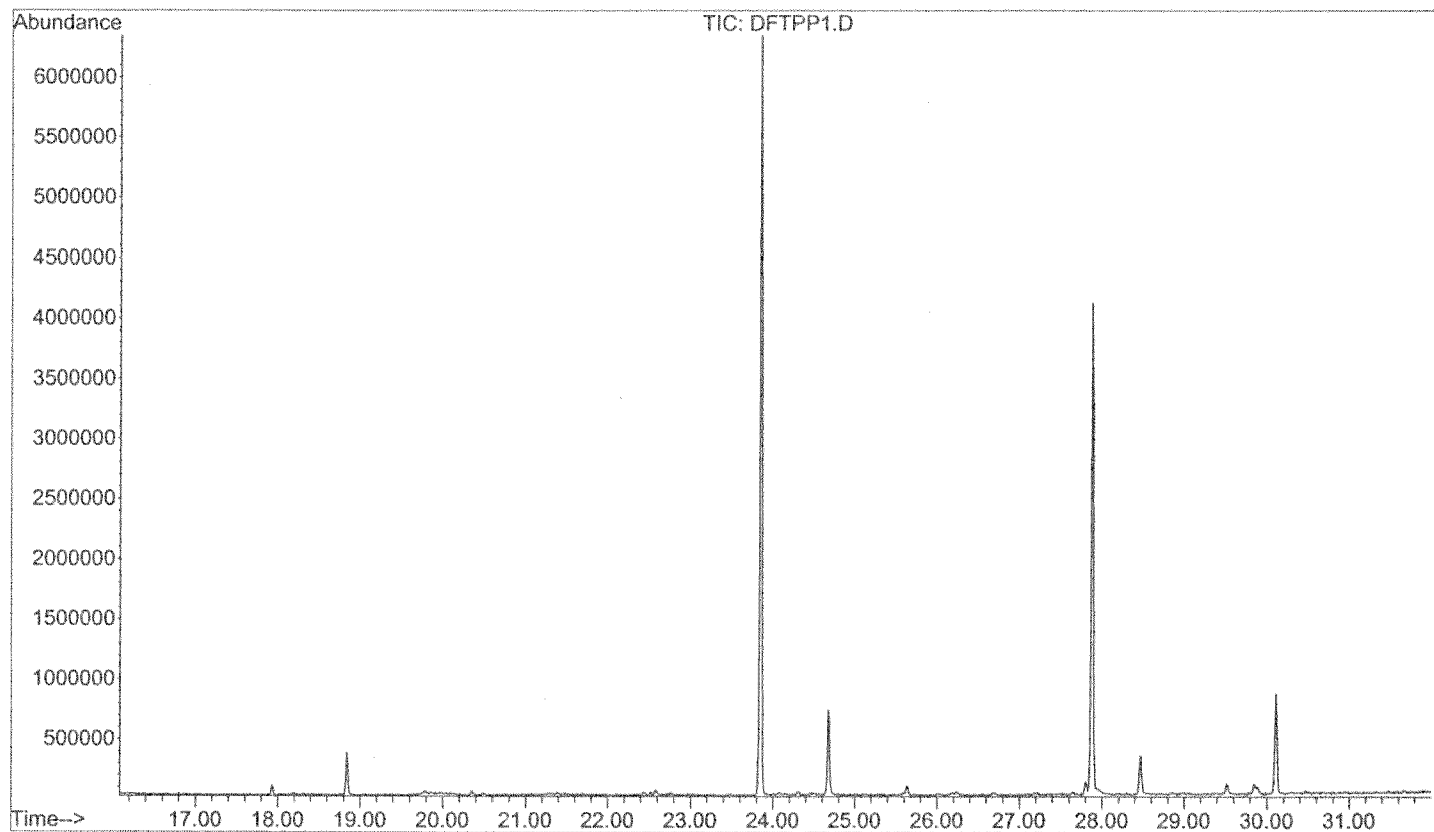

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\121701\DFTPP1.D

Vial: 1

Acq On : 17 Dec 2001 12:43 pm

Operator: McLean

Sample : dftpp +end

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Method : C:\MSDCHEM\1\5973N\011402.M (RTE Integrator)

Title : Quantitation For Method 525.2

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 2500 Area counts

Start Thrs: 0.15

Max Peaks: 10

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5


Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	27.876	1297	1301	1306	rM	4085186	7460487	100.00%	78.777%
2	28.475	1363	1367	1369	rM 3	295196	548092	7.35%	5.787%
3	30.107	1544	1547	1551	rM 2	804368	1461849	19.59%	15.436%

Sum of corrected areas: 9470428

> *Andrus*
21.2%

File : C:\MSDCHEM\1\DATA\121701\DFTPP1.D
 Operator : McLean
 Acquired : 17 Dec 2001 12:43 pm using AcqMethod BIG3
 Instrument : Instrumen
 Sample Name: dftpp +end
 Misc Info :
 Vial Number: 1

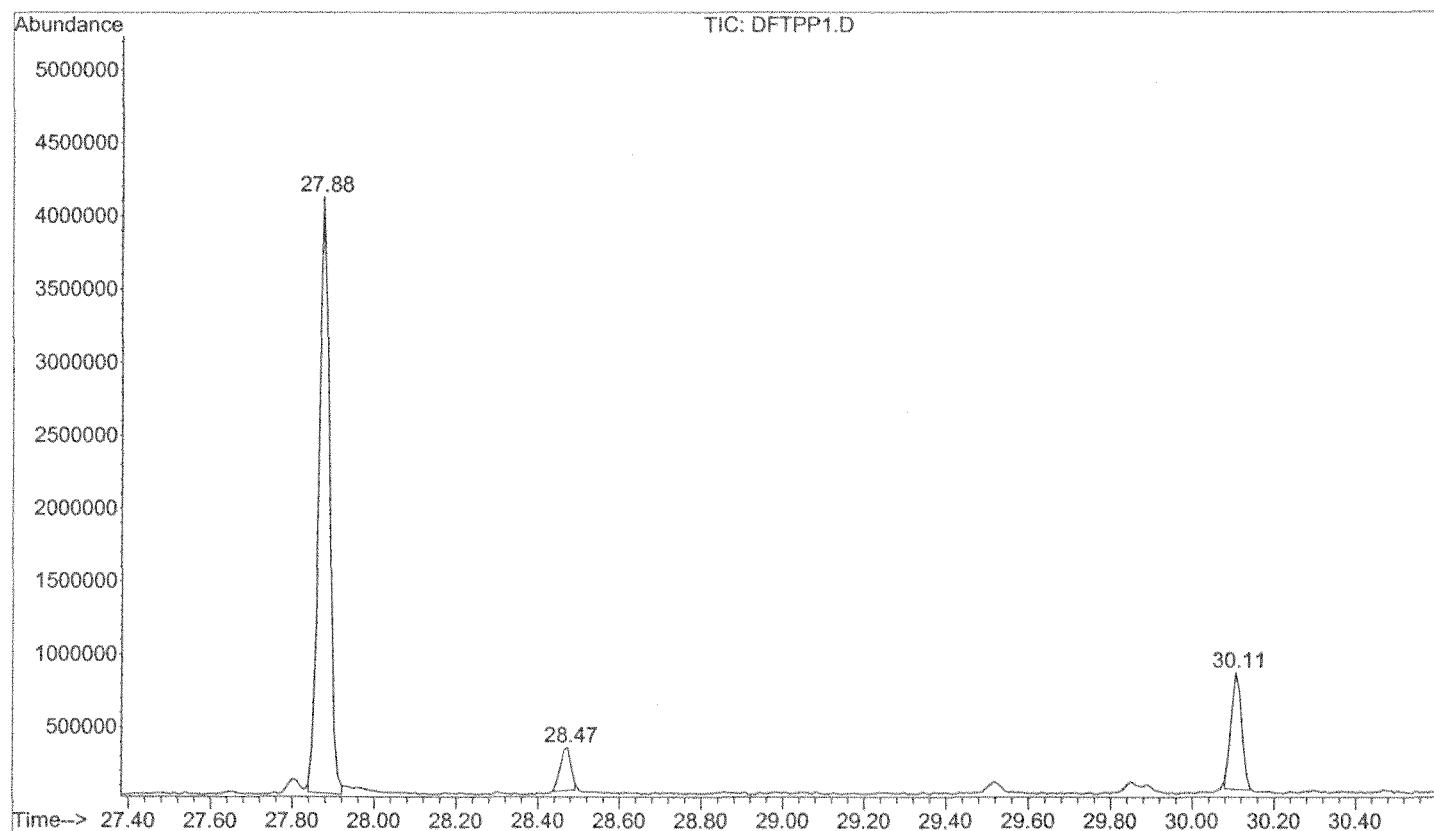

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\121701\DDT1.D

Acq On : 17 Dec 2001 1:22 pm

Sample : ddt

Misc :

MS Integration Params: BENZO.P

Vial: 2

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\011402.M (RTE Integrator)

Title : Quantitation For Method 525.2

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 2500 Area counts

Start Thrs: 0.15

Max Peaks: 10

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	28.266	1340	1344	1349	rM	832994	1400924	15.50%	13.416%
2	29.146	1432	1441	1451	rM	4748263	9041027	100.00%	86.584%

— DDT
13.4%

Sum of corrected areas: 10441951