

User: Fakhouri, Morgan
 Westchester Dept. of Labs & Research
 Date: 12/18/2001 Time: 11:01:38

Sample: AD28048
 Analysis: \$LP525 Organic Extractables
 Units: ug
 Started: 11/26/01 10:59 Ended: 12/14/01 10:59 Analyst: MF
 Page: 1

	Component Name	Viol	Result
1	DFTPP		passes
2	ENDRIN		18.7
3	DDT		11.2

DFTPP

Data File : C:\MSDCHEM\1\DATA\121401\DFTPP1.D Vial: 1
Acq On : 14 Dec 2001 5:01 pm Operator: McLean
Sample : dftpp +ddt+end Inst : Instrumen
Misc : Multiplr: 1.00
MS Integration Params: BENZO.P

Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)
Title : Quantitation For Method 525.2

Spectrum Information: Scan 857

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.9	188544	PASS
68	69	0.00	2	1.6	4058	PASS
69	198	0.00	100	31.4	258048	PASS
70	69	0.00	2	0.4	1111	PASS
127	198	10	80	50.2	412672	PASS
197	198	0.00	2	0.4	3480	PASS
198	198	50	100	100.0	822272	PASS
199	198	5	9	6.2	51264	PASS
275	198	10	60	19.3	158784	PASS
365	198	1	100	2.0	16119	PASS
441	443	0.01	100	69.4	82424	PASS
442	198	50	100	74.9	616256	PASS
443	442	15	24	19.3	118840	PASS

DFTPP1.D 120501.M Mon Dec 17 09:26:59 2001

Data File : C:\MSDCHEM\1\DATA\121401\DFTPP1.D

Vial: 1

Acq On : 14 Dec 2001 5:01 pm

Operator: McLean

Sample : dftpp +ddt+end

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Dec 17 9:30 2001


Quant Results File: 120501.RES

Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)

Title : Quantitation For Method 525.2

Last Update : Mon Dec 17 09:20:49 2001

Response via : Initial Calibration

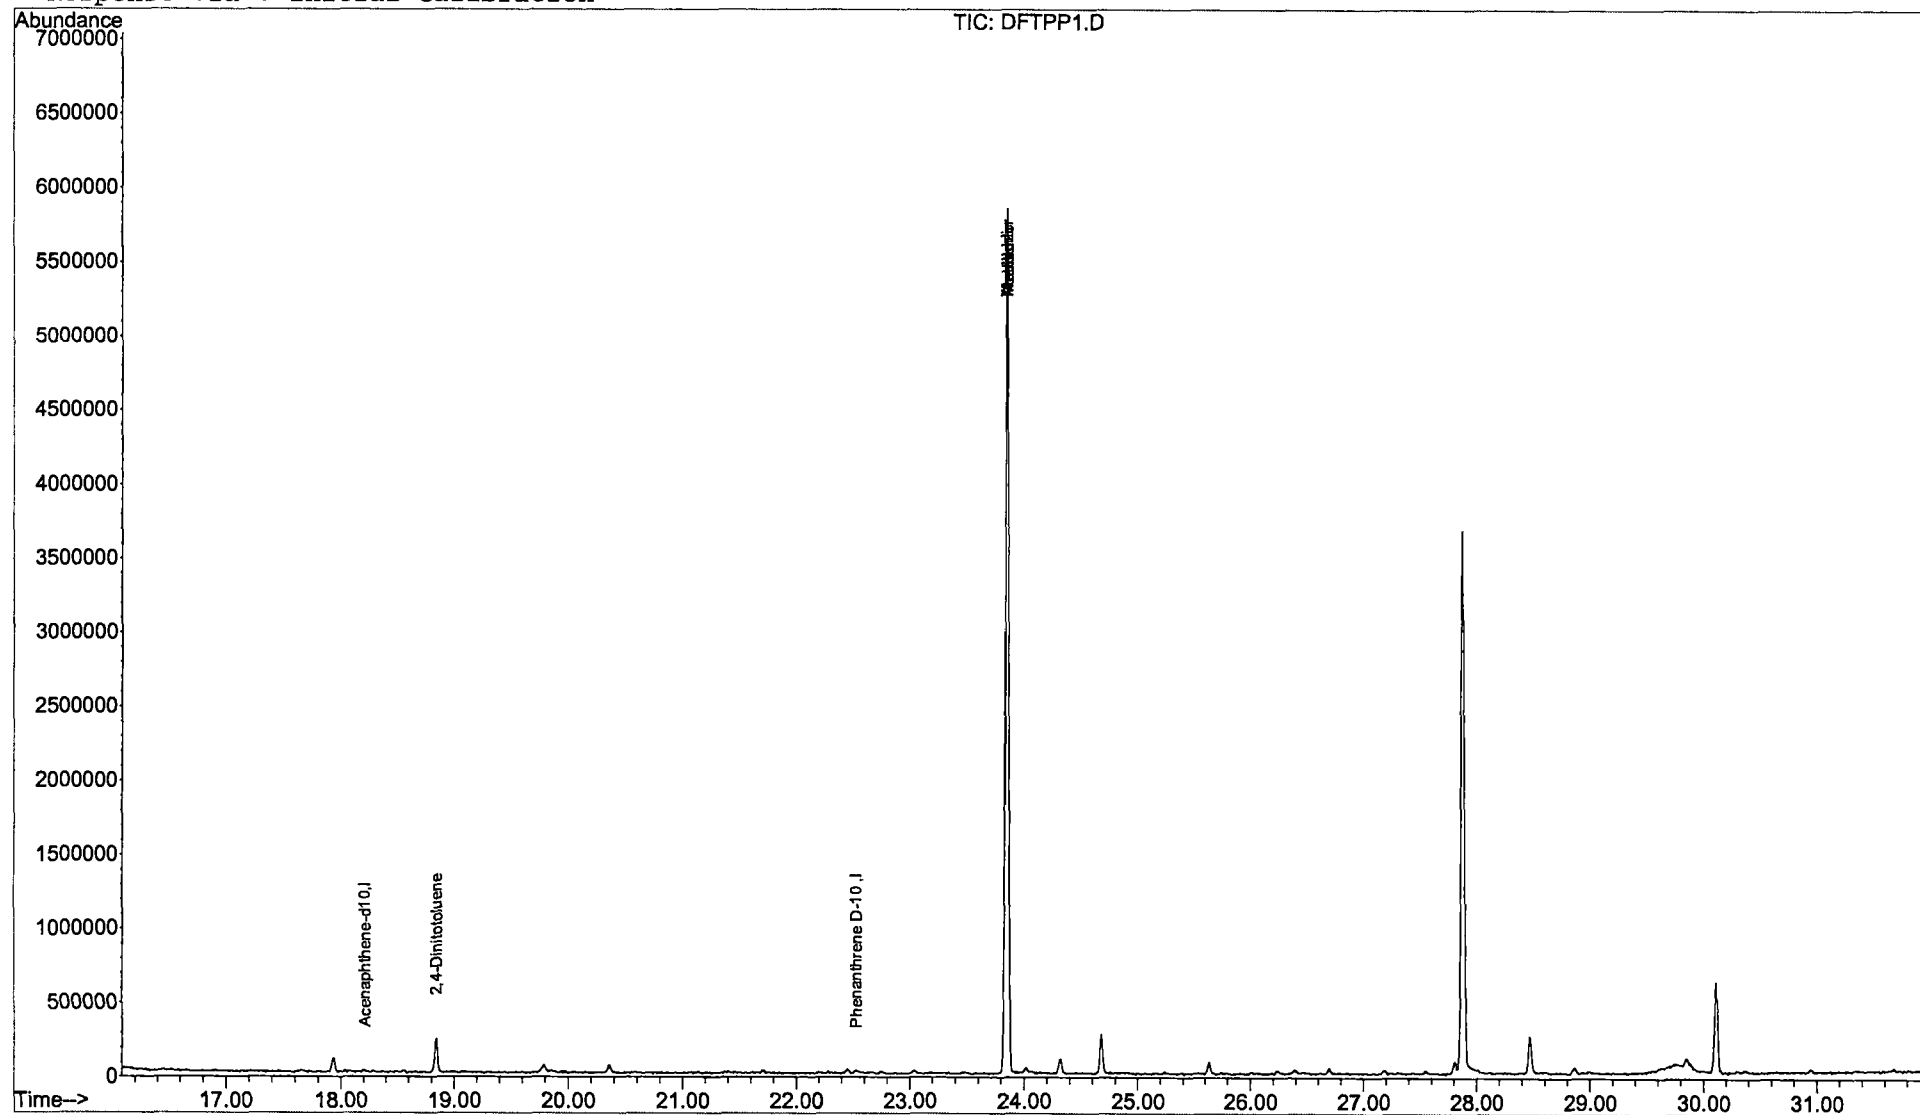

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\121401\DFTPP1.D

Acq On : 14 Dec 2001 5:01 pm

Sample : dftpp +ddt+end

Misc :

MS Integration Params: BENZO.P

Vial: 1

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)

Title : Quantitation For Method 525.2

Smoothing : ON

Sampling : 1

Start Thrs: 0.15

Stop Thrs : 0

Filtering: 5

Min Area: 2500 Area counts

Max Peaks: 10

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	27.876	1295	1301	1311	rM 2	3643564	7030510	100.00%	81.205%
2	28.466	1362	1366	1372	rM 2	252239	496517	7.06%	5.735%
3	30.107	1543	1547	1551	rM 2	602595	1130689	16.08%	13.060%

Sum of corrected areas: 8657716

y Andrus

Data File : C:\MSDCHEM\1\DATA\121401\DDT1.D

Vial: 2

Acq On : 14 Dec 2001 5:40 pm

Operator: McLean

Sample : ddt

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Dec 17 9:38 2001


Quant Results File: 120501.RES

Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)

Title : Quantitation For Method 525.2

Last Update : Mon Dec 17 09:20:49 2001

Response via : Initial Calibration

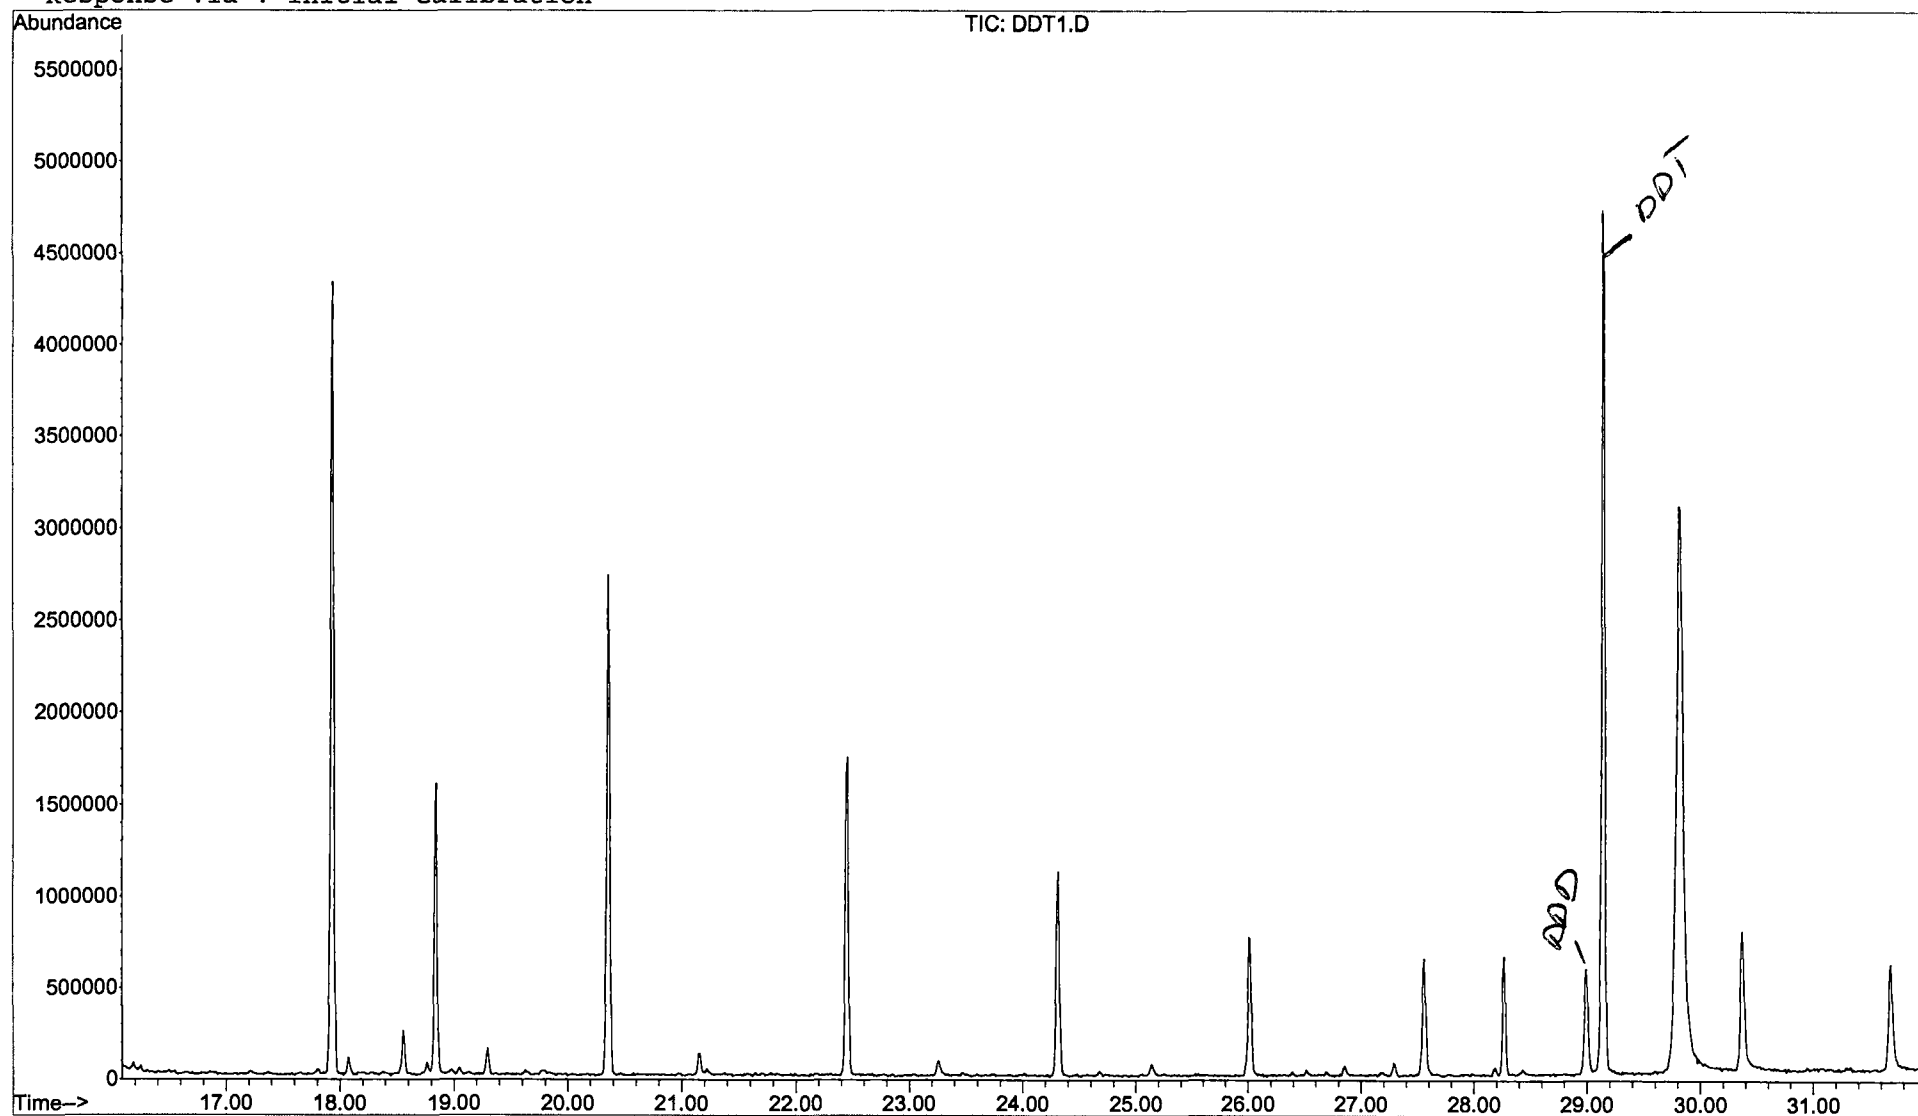

Area Percent Report

Data File : C:\MSDCHEM\1\DATA\121401\DDT1.D
 Acq On : 14 Dec 2001 5:40 pm
 Sample : ddt
 Misc :
 MS Integration Params: BENZO.P

Vial: 2
 Operator: McLean
 Inst : Instrumen
 Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\120501.M (RTE Integrator)
 Title : Quantitation For Method 525.2
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 2500 Area counts
 Start Thrs: 0.15 Max Peaks: 10
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	28.992	1420	1424	1428	rM 2	536999	1111096	12.64%	11.223%
2	29.137	1435	1440	1445	rM	4666403	8789422	100.00%	88.777%

DDT B D

Sum of corrected areas: 9900518