

Sequence Name: C:\HPCHEM\1\SEQUENCE\MAR2702.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\mar2702\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch


☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0308	
2	Sample	2	CAL40	GCMS0308	
3	Sample	3	LB	GCMS0308	gc/ms scan 3/2
4	Sample	4	REF1	GCMS0308	gc/ms scan 3/2
5	Sample	5	REF2	GCMS0308	gc/ms scan 3/2
6	Sample	6	4416	GCMS0308	gc/ms scan 3/2
7	Sample	7	4516	GCMS0308	gc/ms scan 3/2
8	Sample	8	4517	GCMS0308	gc/ms scan 3/2
9	Sample	9	4518	GCMS0308	gc/ms scan 3/2
10	Sample	10	4519	GCMS0308	gc/ms scan 3/2 fb
11	Sample	11	4588	GCMS0308	gc/ms scan 3/2
12	Sample	12	4589	GCMS0308	gc/ms scan 3/2

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR2702\DFTPP.D
 Acq On : 27 Mar 2002 1:38 pm
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

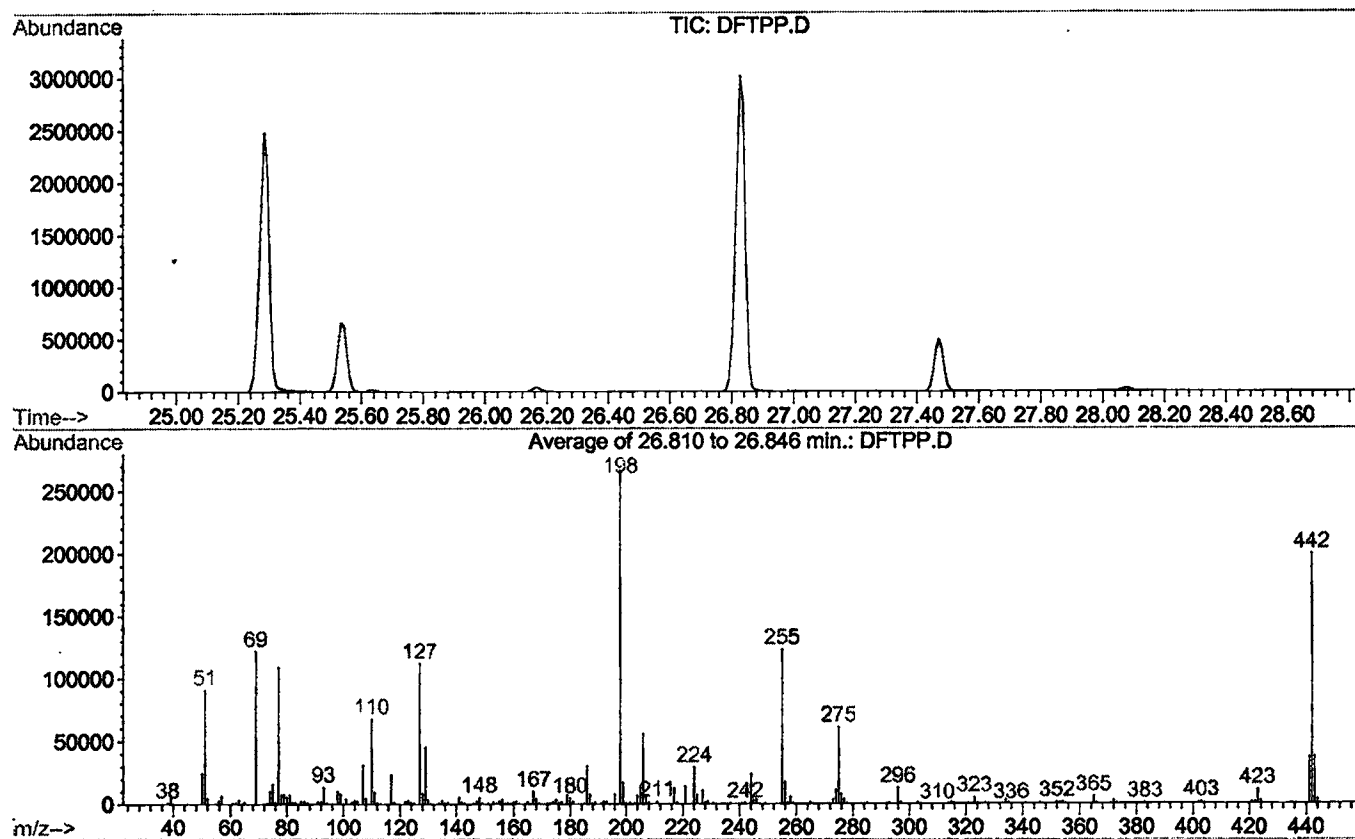

Spectrum Information: Average of 26.810 to 26.846 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.2	91099	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.8	122038	PASS
70	69	0.00	2	0.0	34	PASS
127	198	40	60	42.1	112226	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	266560	PASS
199	198	5	9	6.7	17882	PASS
275	198	10	30	23.1	61634	PASS
365	198	1	100	2.4	6398	PASS
441	443	0.01	100	98.3	37816	PASS
442	198	40	110	75.1	200296	PASS
443	442	17	23	19.2	38458	PASS