

Method GCMS Scan

Date Extracted 3-4-02

Page 123

#GCMS-17723

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
	LB	500mL		1mL			1mL	2A	7	
	Ref 1				1mL			1B		
	Ref 2				1mL			8B		
	4733							7A		
	4734							1A		
	4735							4A		
	4736							9A		
	4737							10B		
	4799							11A		
	4800							4B		
	4801							9B		
	4802							7B		
Remarks										
Reviewed by, <u>C/B 8/12/02</u>										
drip rate must be between 5-15 ml/min for liq-liq extractors										
drip rate -										
Extraction type <u>Sep funnel</u>		Solv. lot# <u>V42E17</u>		NaCl lot# <u>V39618</u>		Na2SO4 lot# <u>V46628</u>				
STANDARD	INT STD LOG#									
CALIBRATION	<u>HP03015</u>									
REF/SPIKE	<u>2193</u>									
MDL/MDRF										
Q. CHECK										
INT. STD.	<u>031802</u>									
SURROGATE	<u>8160R</u>									
LPC										
ENDRIN/DDT										

Analyst MJ
revision 4/12/01

Verified by Anz

Reviewed by DW
Date 4/12

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR2802\DFTPP.D

Acq On : 28 Mar 2002 8:31 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

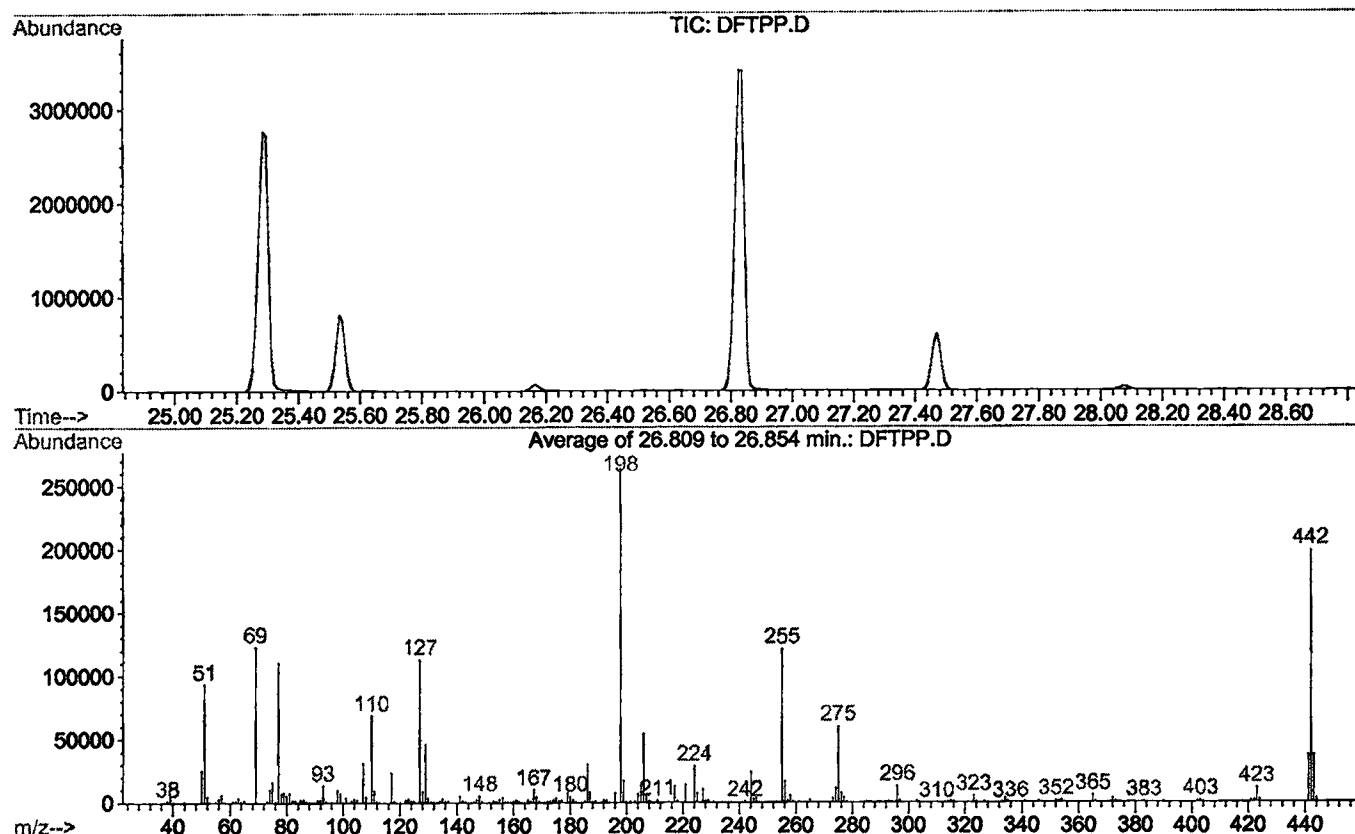

Spectrum Information: Average of 26.809 to 26.854 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	35.5	93536	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.7	123096	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	42.9	113099	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	263588	PASS
199	198	5	9	6.7	17680	PASS
275	198	10	30	23.0	60514	PASS
365	198	1	100	2.4	6315	PASS
441	443	0.01	100	99.2	38131	PASS
442	198	40	110	75.6	199345	PASS
443	442	17	23	19.3	38437	PASS

DFTPP.D GCMS0308.M

Mon Apr 01 09:38:10 2002