

Method 508 mod.

Date Extracted 3/4/02

Page 129

REF

\$GCMS-17689

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
UB		500ml		1ml			1ml	10A	7			
REF ₁					1ml			9A				
REF ₂					↓			10B				
4590								1B				
4591								1A				
4592								4A				
4593								4B				
4594								3A				
4595	FB							3A				
4730								2B				
4731								2A				
4732								1B				
2580								2A				
2582	FB	↓		↓			↓	1A	↓			
Remarks												
Reviewed by <u>C/B 8/13/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors												
Extraction type		Sep Fun	Solv. lot#	V39466	drip rate -		NaCl lot#	V39618	Na2SO4 lot#		V46623	
STANDARD	INT STD LOG#											
CALIBRATION	HP030102											
(REF) SPIKE	2193											
MDL/MDRF												
Q. CHECK												
INT. STD.	032102											
SURROGATE	GCMS 21600											
LPC												
ENDRIN/DDT												

Analyst EH
Revision 4/12/01

Verified by my

Reviewed by DW
Date 4/2/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\MAR2602.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\mar2602\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

(X) Full Method

(X) Inject Anyway

() Reprocessing Only

() Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0308	
2	Sample	2	CAL10	GCMS0308	
3	Sample	3	LB	GCMS0308	gc/ms scan 3/4
4	Sample	4	REF	GCMS0308	gc/ms scan 3/4
5	Sample	27	SURR	GCMS0308	
6	Sample	5	REF1	GCMS0308	gc/ms scan 3/4
7	Sample	6	4590	GCMS0308	gc/ms scan 3/4
8	Sample	7	4591	GCMS0308	gc/ms scan 3/4
9	Sample	8	4592	GCMS0308	gc/ms scan 3/4
10	Sample	9	4593	GCMS0308	gc/ms scan 3/4
11	Sample	10	4594	GCMS0308	gc/ms scan 3/4
12	Sample	11	4595	GCMS0308	gc/ms scan 3/4 fb
13	Sample	12	4730	GCMS0308	gc/ms scan 3/4
14	Sample	13	4731	GCMS0308	gc/ms scan 3/4
15	Sample	14	4732	GCMS0308	gc/ms scan 3/4
16	Sample	15	2580	GCMS0308	re-extract
17	Sample	16	2582	GCMS0308	re-extract fb
18	Sample	17	LBA	GCMS0308	gc/ms scan 3/7
19	Sample	18	REFA	GCMS0308	gc/ms scan 3/7
20	Sample	19	REFA1	GCMS0308	gc/ms scan 3/7
21	Sample	20	4948	GCMS0308	gc/ms scan 3/7 fb
22	Sample	21	4848	GCMS0308	gc/ms scan 3/7
23	Sample	22	1503	GCMS0308	re-extract
24	Sample	23	5031	GCMS0308	gc/ms scan 3/7
25	Sample	24	5032	GCMS0308	gc/ms scan 3/7
26	Sample	25	5033	GCMS0308	gc/ms scan 3/7
27	Sample	26	5034	GCMS0308	gc/ms scan 3/7 fb

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR2602\DFTPP.D

Acq On : 26 Mar 2002 8:44 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

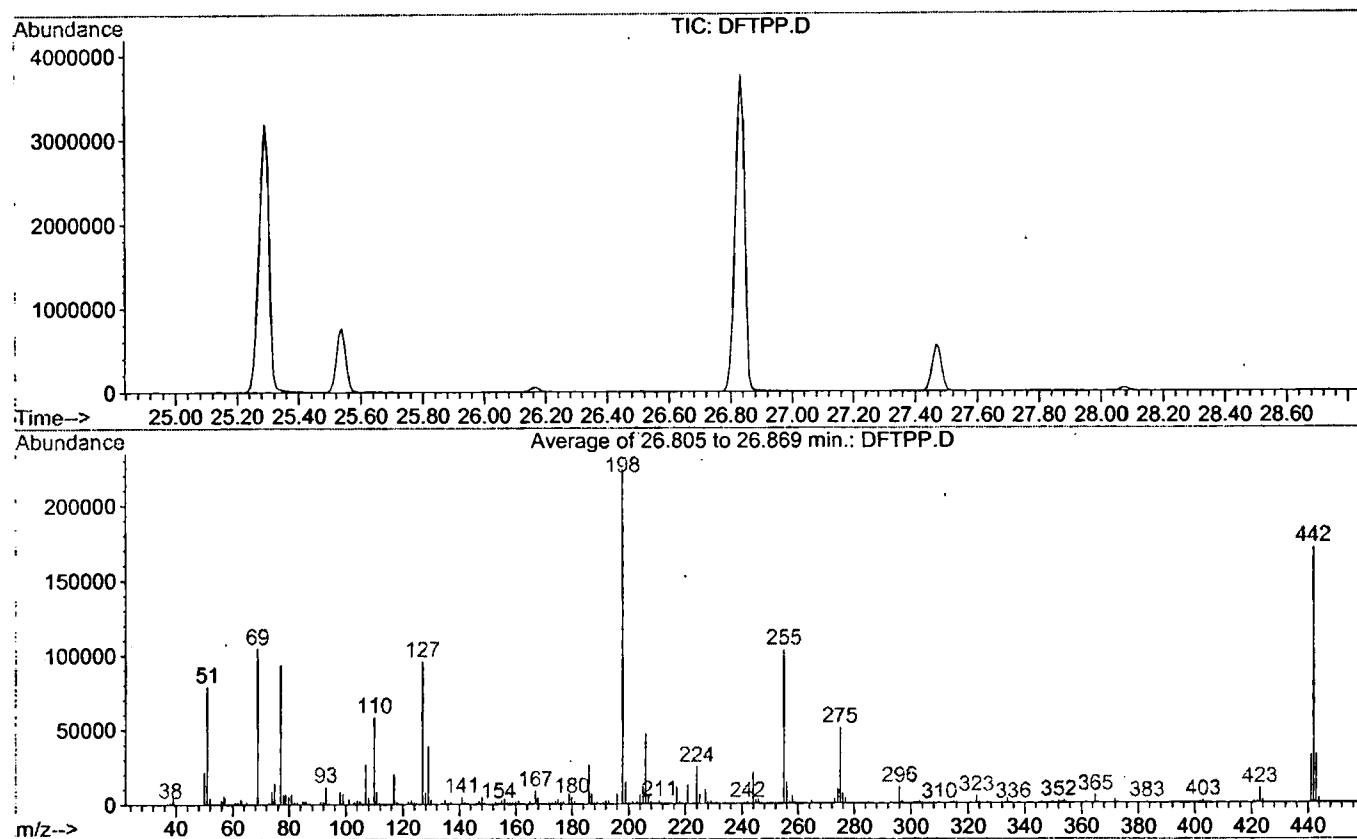

Spectrum Information: Average of 26.805 to 26.869 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	35.3	78897	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.7	104438	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	42.9	95766	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	223469	PASS
199	198	5	9	6.8	15088	PASS
275	198	10	30	22.8	50955	PASS
365	198	1	100	2.4	5350	PASS
441	443	0.01	100	98.1	32294	PASS
442	198	40	110	76.6	171182	PASS
443	442	17	23	19.2	32936	PASS

DFTPP.D GCMS0308.M

Thu Mar 28 15:01:51 2002