

Method 508 mod.

Date Extracted 3/5/02

Page 130

REF

#GCMS-17733

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB		500ml		1ml			1ml	4A	7			
REF					1ml			1A				
REF					↓			4B				
48032								2A				
4804	FB							1B				
4805								4B				
4806	FB							1B				
4843								2B				
4844								1A				
4845								4A				
4846								2B				
4847								2A				
*4848								3B				
Remarks * Sample #4848 dried out on Turbo Vap. Reviewed by, <u>1/5 8/13/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors Extraction type - <u>sep</u> Solv. lot# <u>V16469</u> NaCl lot# <u>V39618</u> Na2SO4 lot# <u>V46623</u>												
STANDARD	INT STD LOG#											
CALIBRATION	<u>HPD 30102</u>											
REF/SPIKE	<u>2193</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.	<u>032802</u>											
SURROGATE	<u>GCMS 2160D</u>											
LPC												
ENDRIN/DDT												

Analyst EH
revision 4/12/01

Verified by mg

Reviewed by ON
Date 4/5/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\MAR2802.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\mar2802\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

On A Barcode Mismatch

☒ Full Method☒ Inject Anyway☐ Reprocessing Only☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
------	------	------	----------	--------	-------------

1	Sample	1	DFTPP	GCMS0308	
2	Sample	2	CAL25	GCMS0308	
3	Sample	3	LB	GCMS0308	gc/ms scan 3/4
4	Sample	4	REF1	GCMS0308	gc/ms scan 3/4
5	Sample	5	REF2	GCMS0308	gc/ms scan 3/4
6	Sample	6	4733	GCMS0308	gc/ms scan 3/4
7	Sample	7	4734	GCMS0308	gc/ms scan 3/4
8	Sample	8	4735	GCMS0308	gc/ms scan 3/4
9	Sample	9	4736	GCMS0308	gc/ms scan 3/4
10	Sample	10	4737	GCMS0308	gc/ms scan 3/4
11	Sample	11	4799	GCMS0308	gc/ms scan 3/4
12	Sample	12	4800	GCMS0308	gc/ms scan 3/4
13	Sample	13	4801	GCMS0308	gc/ms scan 3/4
14	Sample	14	4802	GCMS0308	gc/ms scan 3/4
15	Sample	15	LBA	GCMS0308	gc/ms scan 3/5
16	Sample	16	REFA1	GCMS0308	gc/ms scan 3/5
17	Sample	17	REFA2	GCMS0308	gc/ms scan 3/5
18	Sample	18	4803	GCMS0308	gc/ms scan 3/5
19	Sample	19	4804	GCMS0308	gc/ms scan 3/5 fb
20	Sample	20	4805	GCMS0308	gc/ms scan 3/5
21	Sample	21	4806	GCMS0308	gc/ms scan 3/5 fb
22	Sample	22	4843	GCMS0308	gc/ms scan 3/5
23	Sample	23	4844	GCMS0308	gc/ms scan 3/5
24	Sample	24	4845	GCMS0308	gc/ms scan 3/5
25	Sample	25	4846	GCMS0308	gc/ms scan 3/5
26	Sample	26	4847	GCMS0308	gc/ms scan 3/5
27	Sample	27	CAL10	SW030702	
28	Sample	27	CAL10	SW030702	
29	Sample	27	CAL10	SW030702	
30	Sample	27	CAL10	SW030702	
31	Sample	27	CAL10	SW030702	

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR2802\DFTPP.D

Acq On : 28 Mar 2002 8:31 am

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

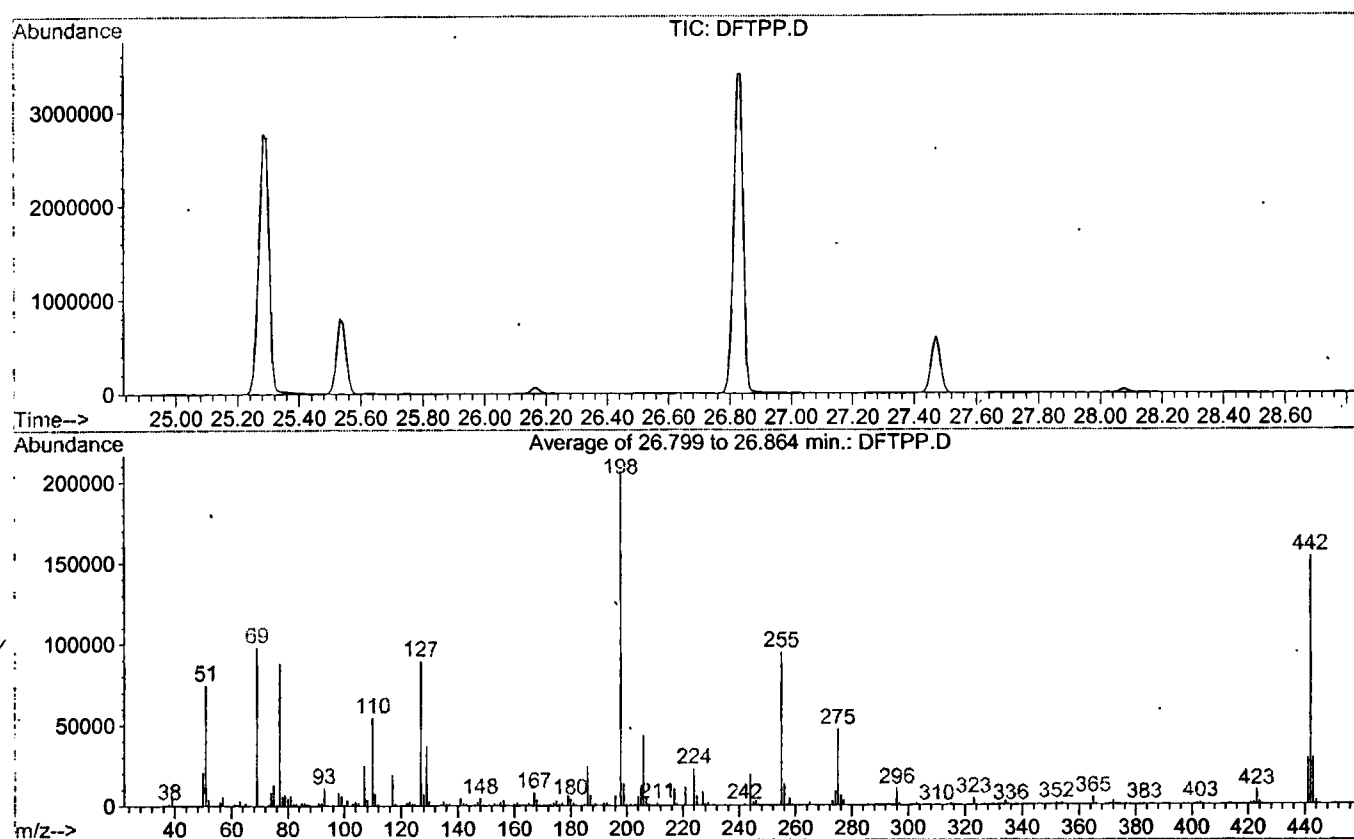

Spectrum Information: Average of 26.799 to 26.864 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	36.1	74505	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.4	97887	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	43.2	89194	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	206407	PASS
199	198	5	9	6.7	13865	PASS
275	198	10	30	22.8	47091	PASS
365	198	1	100	2.4	4871	PASS
441	443	0.01	100	98.8	29370	PASS
442	198	40	110	74.6	153924	PASS
443	442	17	23	19.3	29740	PASS

DFTPP.D GCMS0308.M

Fri Mar 29 08:50:25 2002