

Method 508 MOD.

Date Extracted 3-6-02

Page 133

Ref

#GCMs-17740

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
L.B.		500ml		1ml			1ml	9A	7			
Ref 1					1ml			9B				
Ref 2					1ml			3B				
4849								3B				
4850	F.B.							10A				
4941								7A				
4942								6A				
4943								4A				
4944								10B				
4945	See 4/3							8B				
4946								7B				
4947								4B				
3016								8A				
Remarks 3016 RE-EXTRACT Ref 2 DRY up Reviewed by, <u>CP 8/13/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors Extraction type - <u>SEP. FUR</u> Solv. lot# <u>V4470</u> NaCl lot# <u>V39618</u> Na2SO4 lot# <u>V46623</u>												
STANDARD	INT STD LOG#											
CALIBRATION	<u>HP0301A</u>											
REF/SPIKE	<u>2193</u>											
MDL/MDRF												
Q. CHECK												
INT. STD.	<u>1503150V</u>											
SURROGATE	<u>2160D</u>											
LPC												
ENDRIN/DOT												

Analyst A.D.
revision 4/12/01

Verified by my

Reviewed by CP 8/13/02
Date

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR3002\DFTPP.D

Acq On : 29 Mar 2002 3:56 pm

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

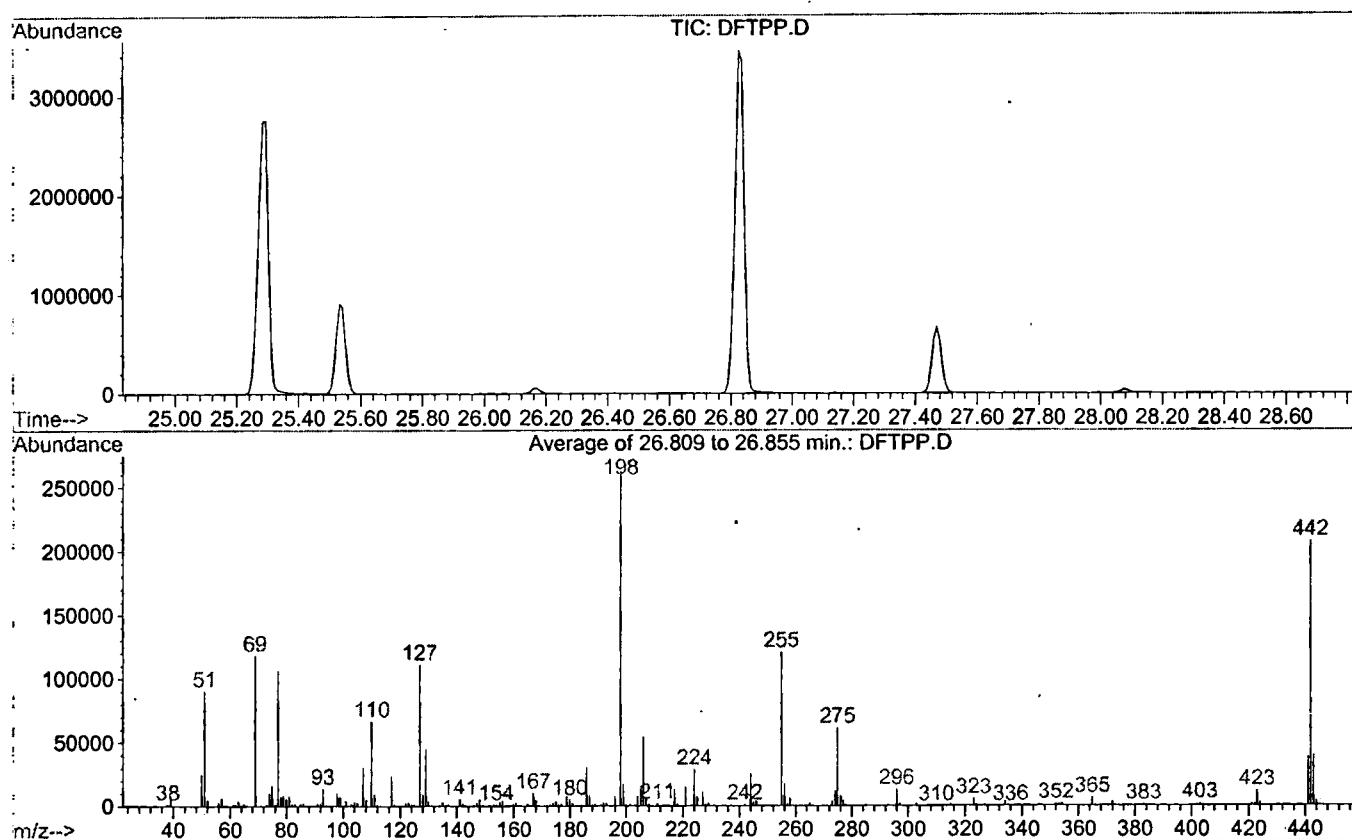

Spectrum Information: Average of 26.809 to 26.855 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.5	90287	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.1	118085	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	42.4	111198	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	262011	PASS
199	198	5	9	6.6	17251	PASS
275	198	10	30	23.5	61444	PASS
365	198	1	100	2.4	6337	PASS
441	443	0.01	100	96.8	38649	PASS
442	198	40	110	79.3	207644	PASS
443	442	17	23	19.2	39926	PASS

DFTPP.D GCMS0308.M

Tue Apr 02 10:04:59 2002