

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR3002\DFTPP.D

Acq On : 29 Mar 2002 3:56 pm

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

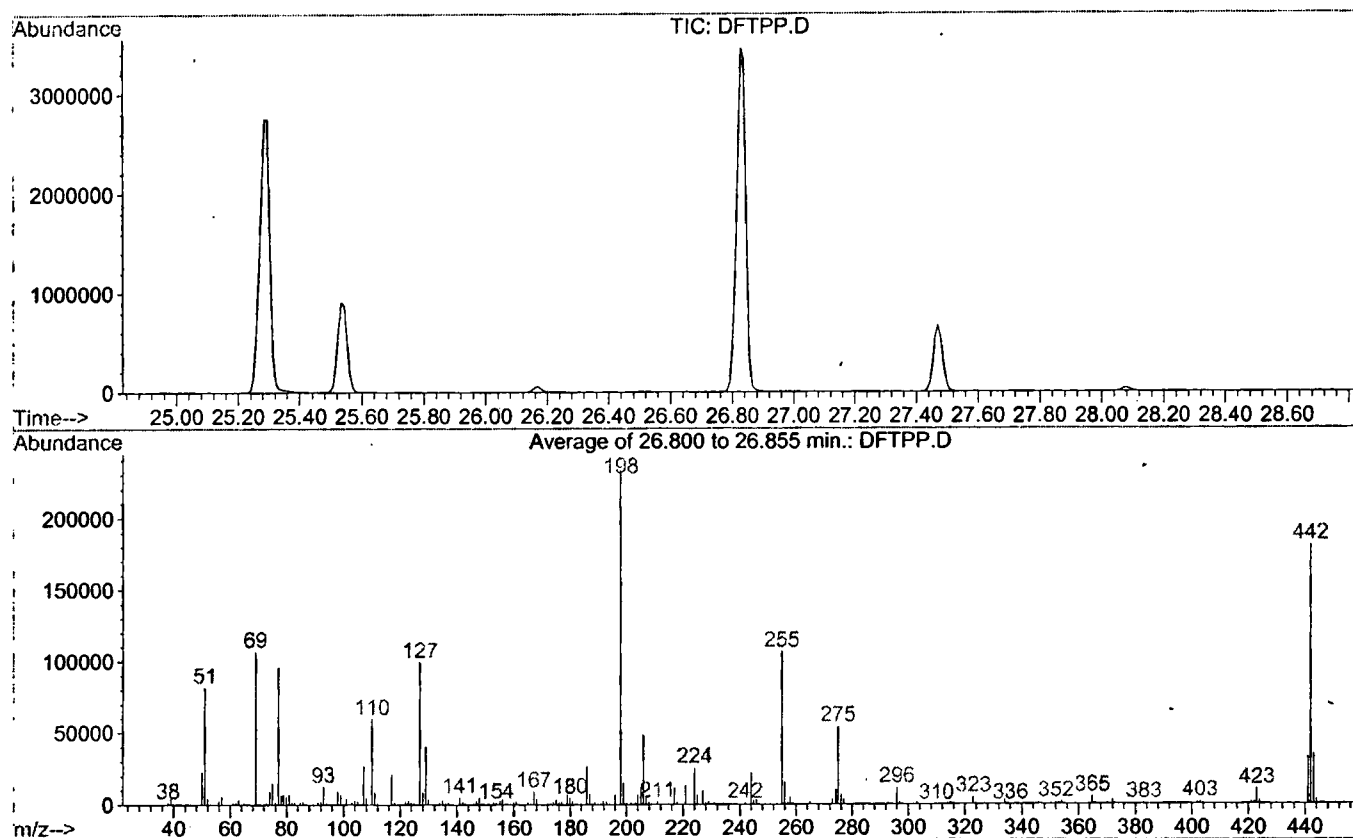

Spectrum Information: Average of 26.800 to 26.855 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	35.1	81740	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.8	106796	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	42.7	99443	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	233078	PASS
199	198	5	9	6.6	15387	PASS
275	198	10	30	23.3	54213	PASS
365	198	1	100	2.4	5572	PASS
441	443	0.01	100	95.0	33127	PASS
442	198	40	110	77.6	180976	PASS
443	442	17	23	19.3	34857	PASS

DFTPP.D GCMS0308.M

Tue Apr 02 12:26:25 2002