NYC 9/11 Public Portal Document

Comments for Sample AE05037 - Analysis $GCMS

Westchester Dept. of Labs & Research
User: Vinci, David L
Date: 04-05-2002 Time: 14:49:38

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/05/2002 Time: 14:49:40

Sample: AE05037
Analysis: $GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/5/02 14:49 Ended: 4/5/02 14:49 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds				
2	Surr_2,4-DDD		93		5.0

NYC 9/11 Public Portal Document

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAR3002\5037.D Vial: 21
Acq On : 30 Mar 2002 10:49 am Operator:
Sample : gc/ms scan 3/7 Inst : GC/MS 209
Misc : Multiplr: 1.00
MS Integration Params: GOOFY.P
Quant Time: Mar 30 11:37 2002 Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Mar 29 10:31:28 2002
Response via : Initial Calibration
DataAcq Meth : GCMS0308

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.25	152	524189	20.00	ug/l	-0.10
10) Naphthalene-d8	15.89	136	1917837	20.00	ug/l	-0.11
17) Acenaphthene-d10	21.19	164	1071534	20.00	ug/l	-0.12
29) Phenanthrene-d10	25.63	188	1510055	20.00	ug/l	-0.13
38) Chrysene-d12	33.69	240	750046	20.00	ug/l	-0.15
44) Perylene-d12	37.94	264	417968	20.00	ug/l	-0.19
System Monitoring Compounds						
37) 2,4-DDD	30.71	235	70777	4.67	ug/mL	0.21
Spiked Amount 5.000			Recovery = 93.40%			
Target Compounds						Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.		
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.		
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.		
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	15.93	128	310	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-Chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.		
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
25) Diethylphthalate	22.67	149	232	N.D.		
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		

(#) = qualifier out of range (m) = manual integration

NYC-WTC_000058856

NYC 9/11 Public Portal Document

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAR3002\5037.D Vial: 21
Acq On : 30 Mar 2002 10:49 am Operator:
Sample : gc/ms scan 3/7 Inst : GC/MS 209
Misc : Multiplr: 1.00
MS Integration Params: GOOFY.P
Quant Time: Mar 30 11:37 2002 Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Mar 29 10:31:28 2002
Response via : Initial Calibration
DataAcq Meth : GCMS0308

	Compound	R.T.	QIon	Response	Conc Unit	Qvalue
30)	N-Nitrosodiphenylamine	0.00	168	0	N.D.	
31)	4-Bromophenyl-phenylether	0.00	248	0	N.D.	
32)	Hexachlorobenzene	0.00	284	0	N.D.	
33)	Phenanthrene	25.63	178	457	N.D.	
34)	Anthracene	25.63	178	457	N.D.	
35)	Di-n-butylphthalate	27.60	149	1912	N.D.	
36)	Fluoranthene	0.00	202	0	N.D.	
39)	Pyrene	0.00	202	0	N.D.	
40)	Butylbenzylphthalate	0.00	149	0	N.D.	
41)	Benzo(a)anthracene	33.69	228	1983	N.D.	
42)	Bis(2-ethylhexyl)phthalate	33.91	149	1119	N.D.	
43)	Chrysene	33.69	228	1984	N.D.	
45)	Di-n-Octylphthalate	0.00	149	0	N.D.	
46)	Benzo(b)fluoranthene	36.76	252	114	N.D.	
47)	Benzo(k)fluoranthene	36.83	252	406	N.D.	
48)	Benzo(a)pyrene	37.95	252	1512	N.D.	
49)	Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
50)	Dibenz(a,h)anthracene	0.00	278	0	N.D.	
51)	Benzo(g,h,i)perylene	0.00	276	0	N.D.	

(#) = qualifier out of range (m) = manual integration

NYC-WTC_000058857

NYC 9/11 Public Portal Document

Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAR3002\5037.D Vial: 21
Acq On : 30 Mar 2002 10:49 am Operator:
Sample : gc/ms scan 3/7 Inst : GC/MS 209
Misc : Multiplr: 1.00
MS Integration Params: GOOFY.P
Quant Time: Mar 30 11:37 2002 Quant Results File: GCMS0308.RES

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Mar 29 10:31:28 2002
Response via : Initial Calibration

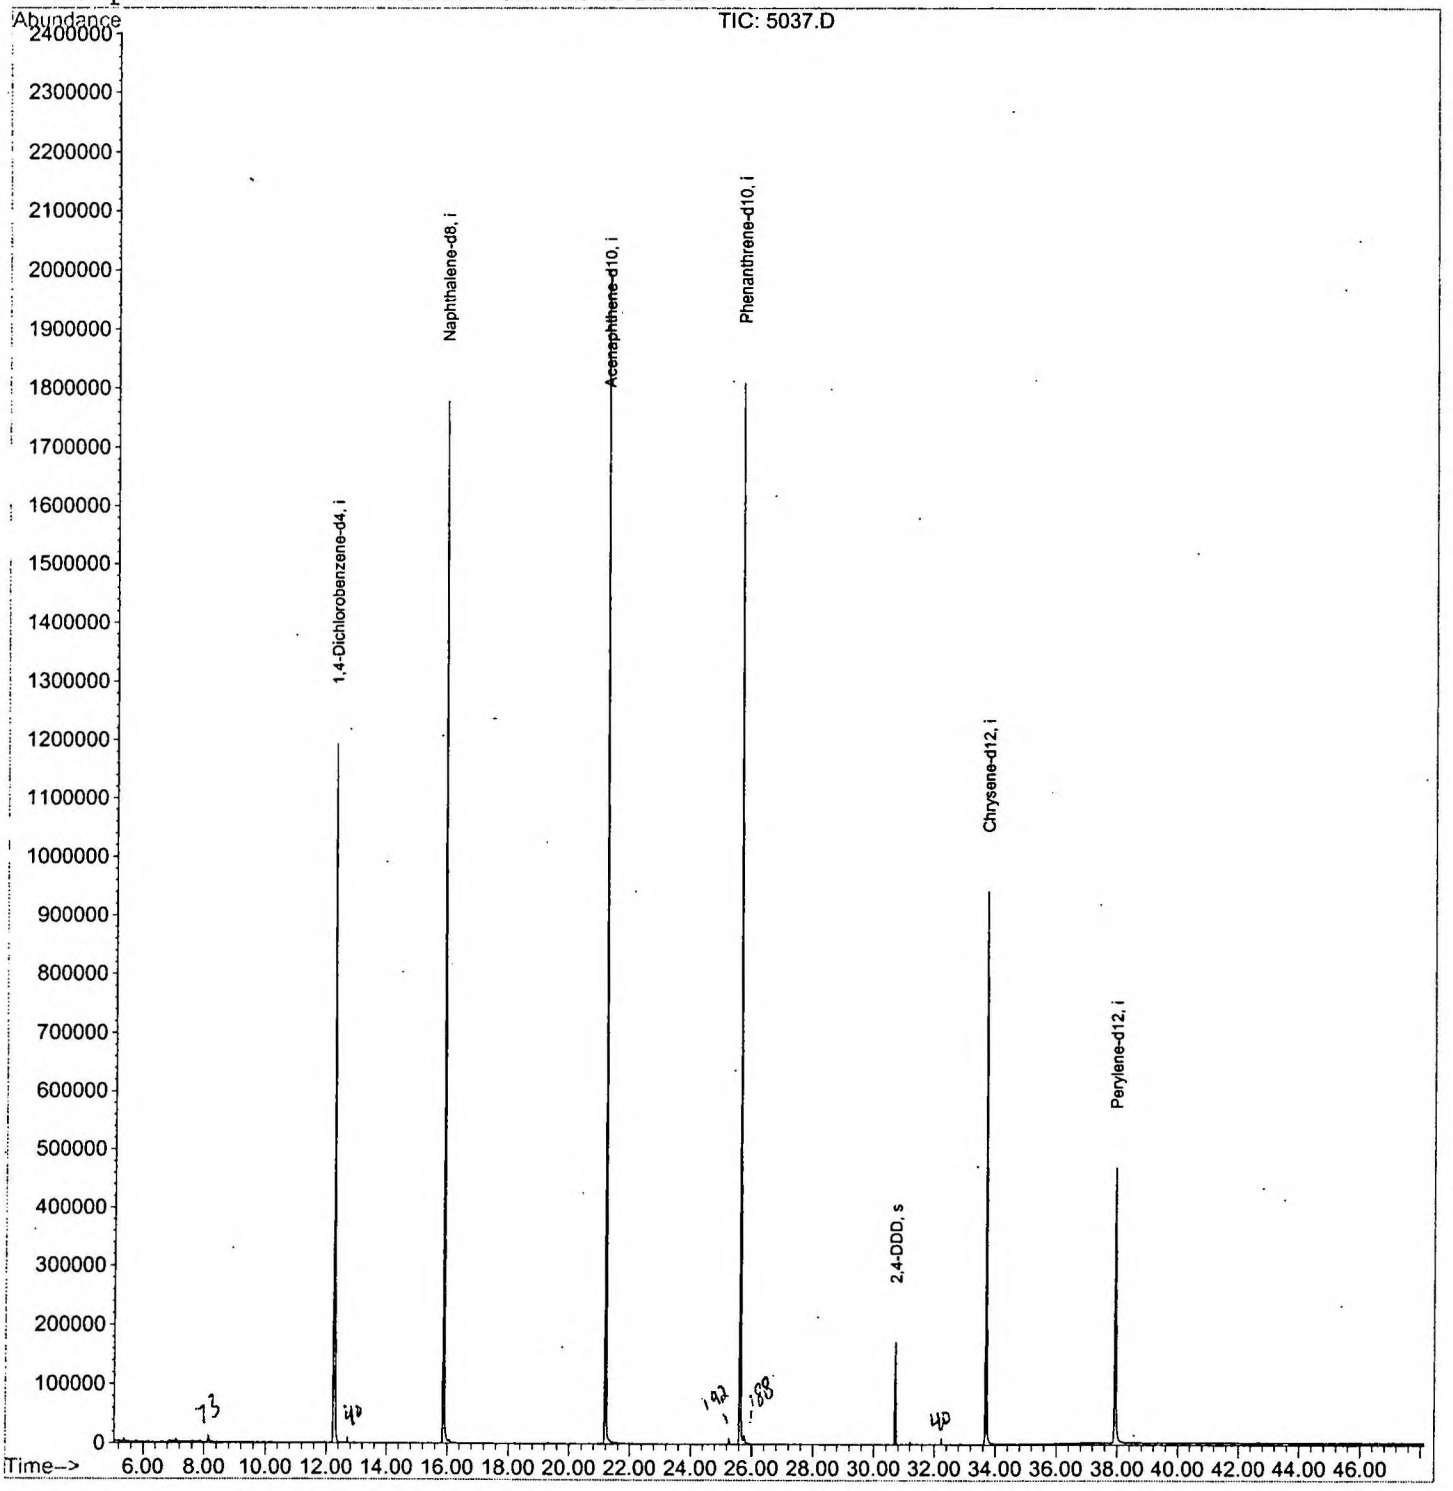

NYC-WTC_000058858

NYC 9/11 Public Portal Document

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAR3002\5037.D Vial: 21
Acq On : 30 Mar 2002 10:49 am Operator:
Sample : gc/ms scan 3/7 Inst : GC/MS 209
Misc : Multiplr: 1.00
MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	12.250	779	785	802	rBV	1192589	2809198	69.46%	15.464%
2	15.885	1175	1181	1198	rBV	1777809	3612913	89.34%	19.888%
3	21.191	1752	1759	1772	rBV	2001779	4044147	100.00%	22.262%
4	25.635	2236	2243	2255	rBV2	1810676	3766984	93.15%	20.736%
5	30.711	2791	2796	2805	rVB	173878	341313	8.44%	1.879%
6	33.695	3114	3121	3138	rBV	944621	2177683	53.85%	11.987%
7	37.936	3575	3583	3599	rBV2	470470	1414184	34.97%	7.785%

Sum of corrected areas: 18166422

5037.D GCMS0308.M Tue Apr 02 14:10:08 2002

NYC-WTC_000058859

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAR3002\5037.D
Operator :
Acquired : 30 Mar 2002 10:49 am using AcqMethod GCMS0308
Instrument : GC/MS 209
Sample Name: gc/ms scan 3/7
Misc Info :
Vial Number: 21
Quant File :GCMS0308.RES (RTE Integrator)

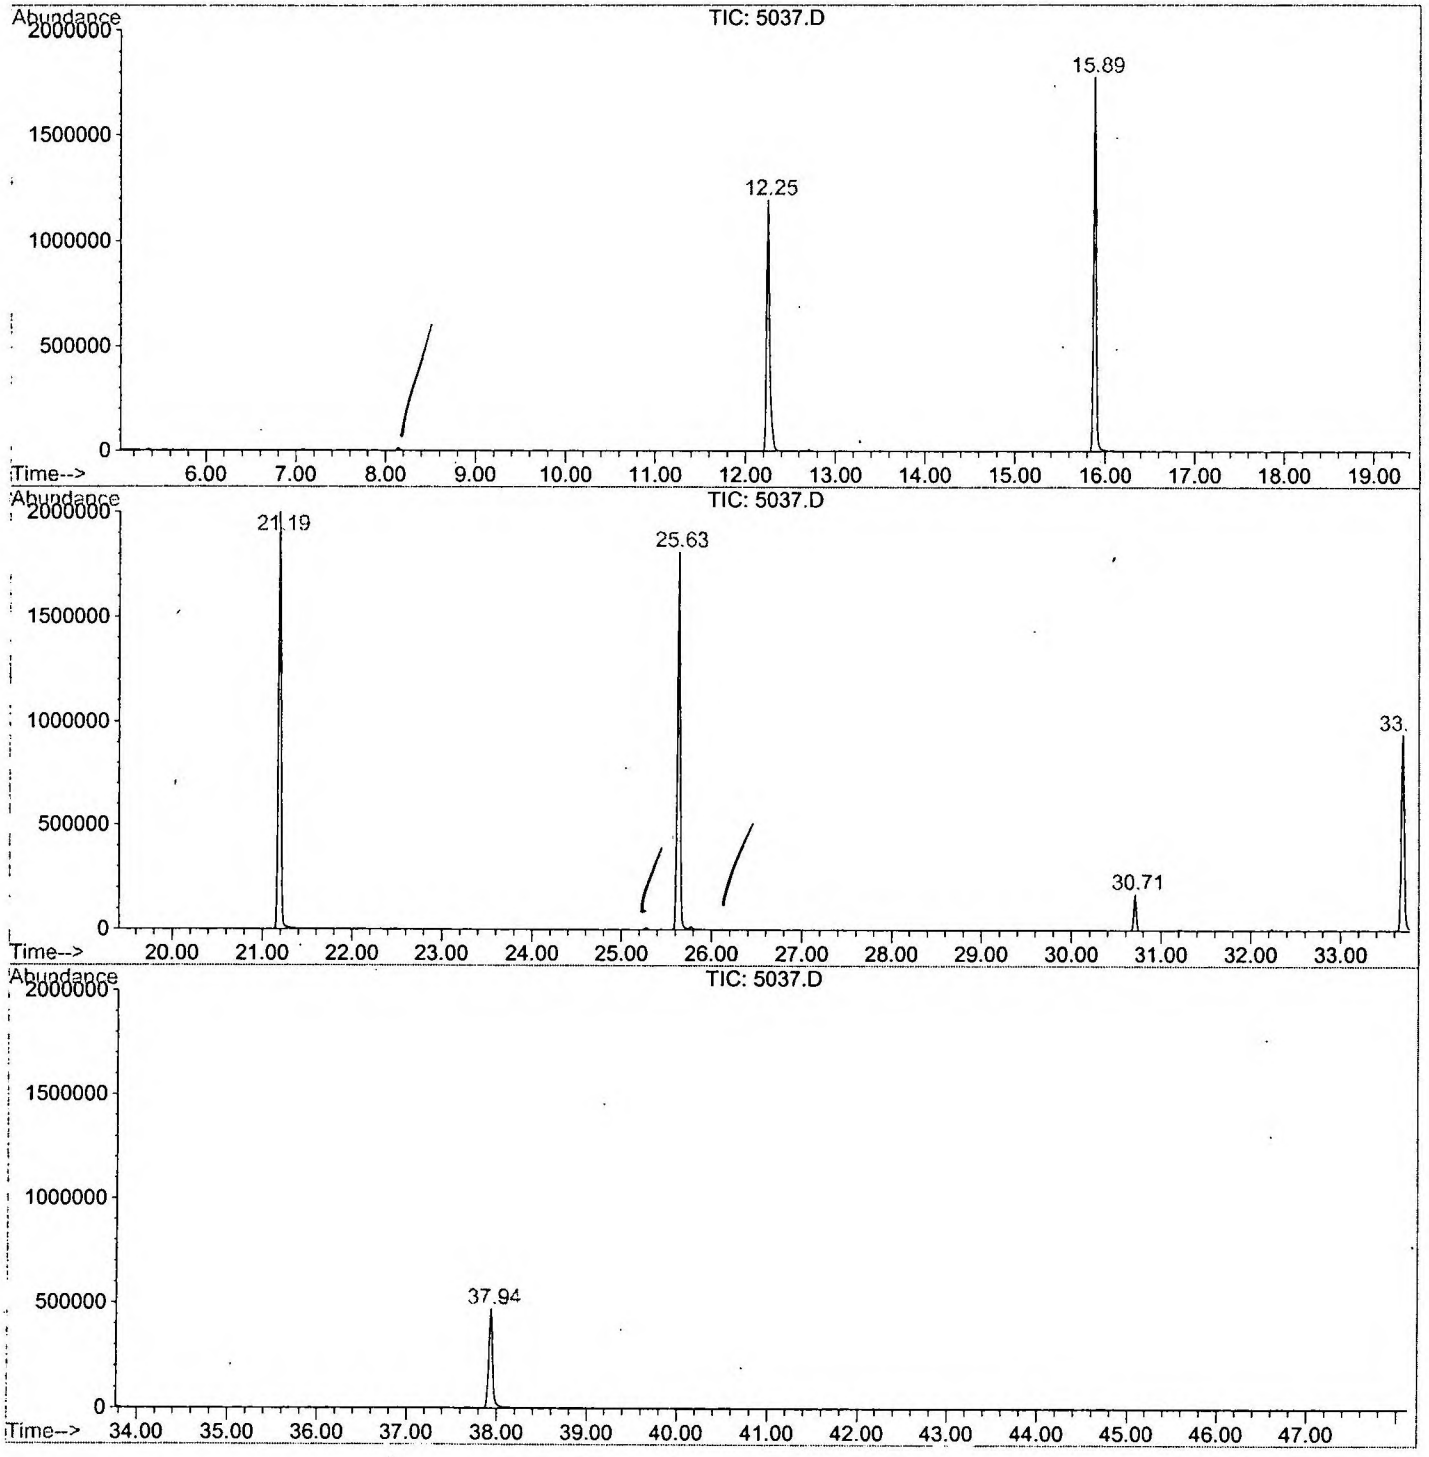

5037.D GCMS0308.M Tue Apr 02 14:10:14 2002

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 30 Mar 2002 10:49 am
Data File: C:\HPCHEM\1\DATA\MAR3002\5037.D
Name: gc/ms scan 3/7
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc

5037.D GCMS0308.M Tue Apr 02 14:10:18 2002