

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR3002\DFTPP1.D

Acq On : 30 Mar 2002 3:46 pm

Sample :

Misc :

MS Integration Params: GOOFY.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)


Title : 209 625/TCLP calibration table

Vial: 1

Operator:

Inst : GC/MS 209

Multiplr: 1.00

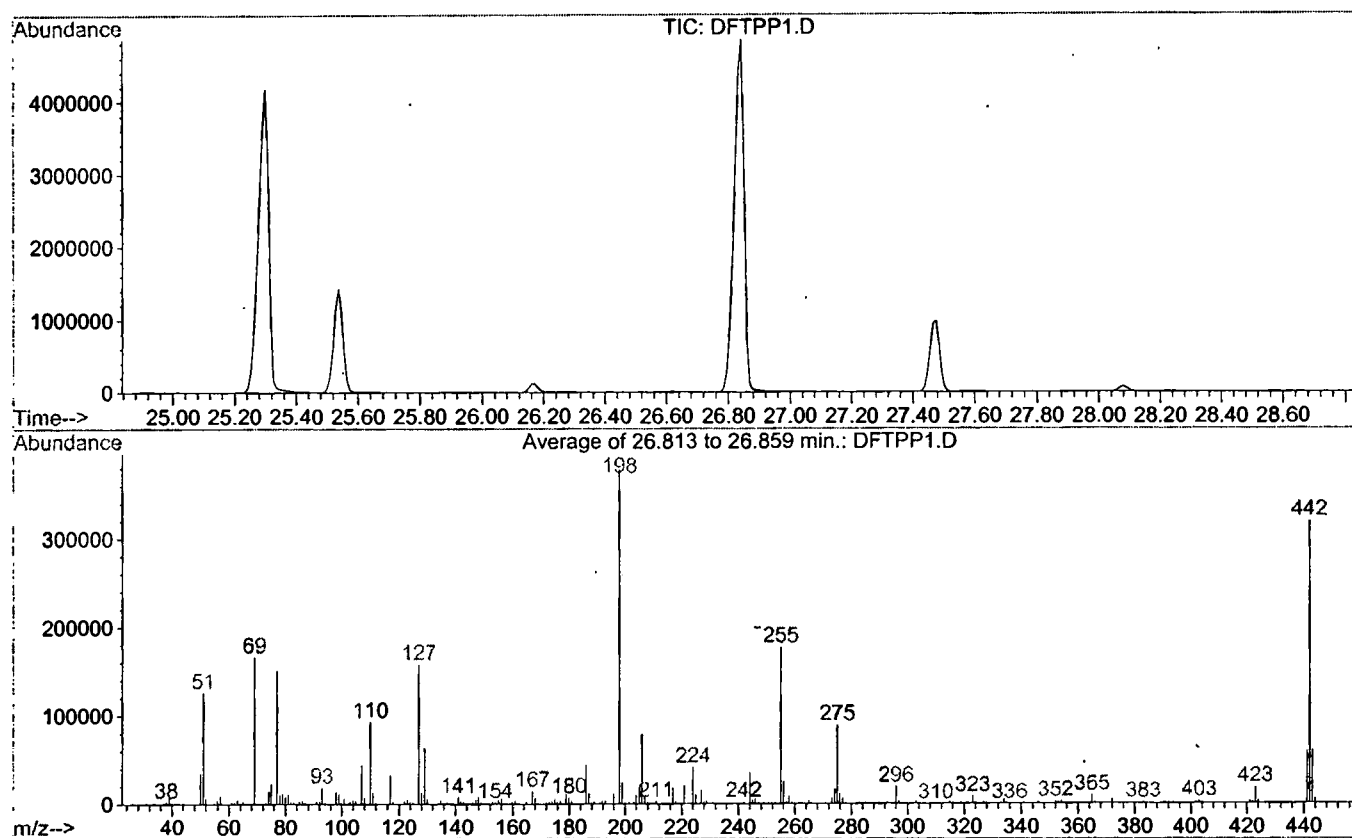

Spectrum Information: Average of 26.813 to 26.859 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	33.3	125688	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.0	166391	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	41.9	158164	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	377887	PASS
199	198	5	9	6.6	24788	PASS
275	198	10	30	23.8	89817	PASS
365	198	1	100	2.6	9637	PASS
441	443	0.01	100	98.1	60475	PASS
442	198	40	110	84.5	319211	PASS
443	442	17	23	19.3	61615	PASS

DFTPP1.D GCMS0308.M

Tue Apr 02 15:05:49 2002