

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/09/2002 Time: 10:37:23

Sample: AE05055
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/9/02 10:36 Ended: 4/9/02 10:36 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		86		5.0

Comments for Sample AE05055 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-09-2002 Time: 10:37:27

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAR3002\5055.D

Vial: 31

Acq On : 30 Mar 2002 10:42 pm

Operator:

Sample : gc/ms scan 3/8

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 30 23:31 2002

Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Mar 29 10:31:28 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0308

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.25	152	432903	20.00	ug/l	-0.10
10) Naphthalene-d8	15.89	136	1574960	20.00	ug/l	-0.11
17) Acenaphthene-d10	21.19	164	882408	20.00	ug/l	-0.12
29) Phenanthrene-d10	25.63	188	1229573	20.00	ug/l	-0.13
38) Chrysene-d12	33.69	240	596760	20.00	ug/l	-0.15
44) Perylene-d12	37.94	264	344637	20.00	ug/l	-0.19

System Monitoring Compounds

37) 2,4-DDD	30.71	235	79119	6.41	ug/mL	0.21
Spiked Amount	5.000		Recovery	=	128.20%	85.692

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.94	128	336	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	22.68	149	501	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#)= qualifier out of range (m) = manual integration

5055.D GCMS0308.M

Tue Apr 02 15:21:01 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAR3002\5055.D

Vial: 31

Acq On : 30 Mar 2002 10:42 pm

Operator:

Sample : gc/ms scan 3/8

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 30 23:31 2002

Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Mar 29 10:31:28 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0308

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.70	178	297	N.D.		
34) Anthracene	25.70	178	297	N.D.		
35) Di-n-butylphthalate	27.61	149	1442	N.D.		
36) Fluoranthene	29.33	202	340	N.D.		
39) Pyrene	30.00	202	210	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.69	228	1413	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.91	149	998	N.D.		
43) Chrysene	33.76	228	373	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	36.75	252	432	N.D.		
47) Benzo(k)fluoranthene	36.83	252	585	N.D.		
48) Benzo(a)pyrene	37.95	252	1414	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

5055.D GCMS0308.M

Tue Apr 02 15:21:05 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAR3002\5055.D
Acq On : 30 Mar 2002 10:42 pm
Sample : gc/ms scan 3/8
Misc :
MS Integration Params: GOOFY.P
Quant Time: Mar 30 23:31 2002

Vial: 31
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0308.RES

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Mar 29 10:31:28 2002
Response via : Initial Calibration

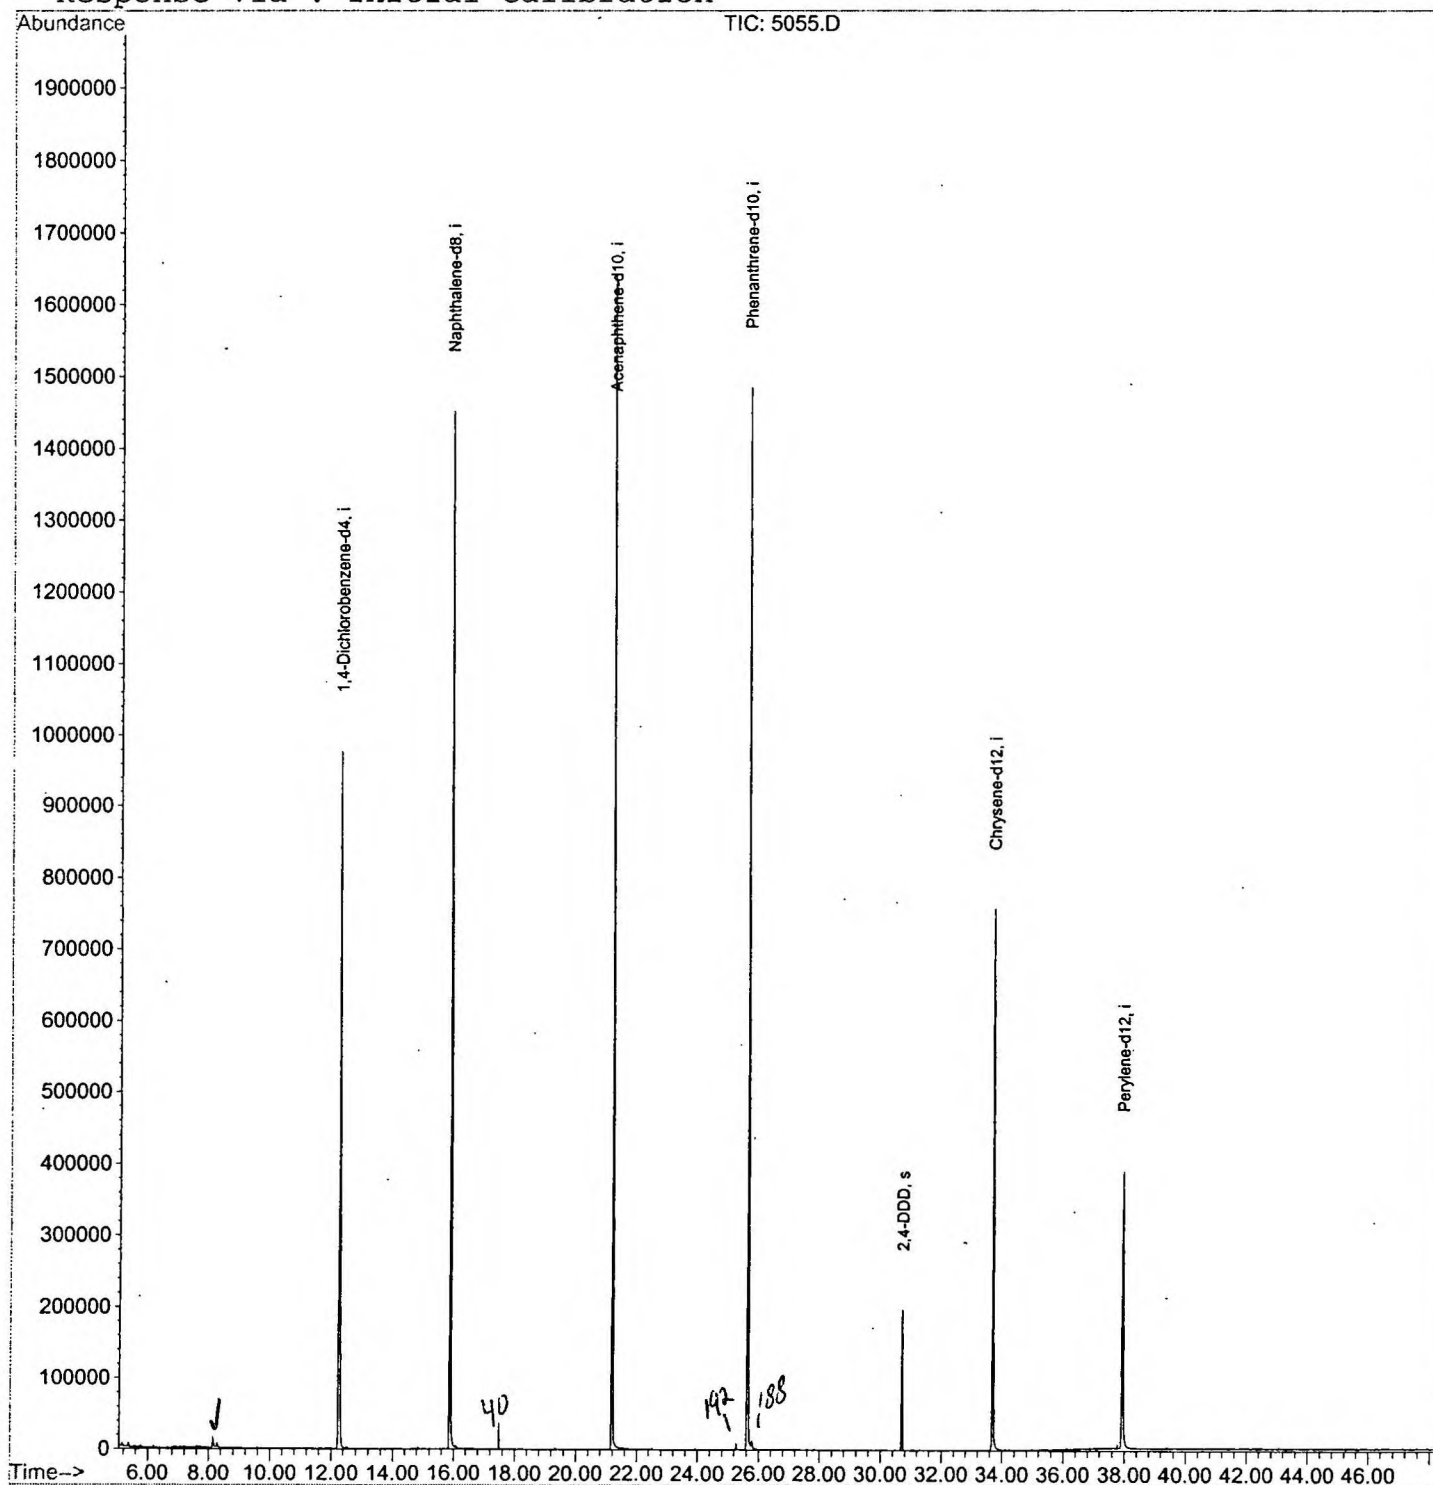

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAR3002\5055.D

Vial: 31

Acq On : 30 Mar 2002 10:42 pm

Operator:

Sample : gc/ms scan 3/8

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.137	333	337	346	rBV	15192	36371	1.07%	0.241%
2	12.250	779	785	801	rBV	976036	2326057	68.30%	15.401%
3	15.885	1175	1181	1198	rBV	1451053	2980783	87.52%	19.736%
4	21.191	1752	1759	1778	rBV	1642791	3405703	100.00%	22.549%
5	25.635	2236	2243	2254	rBV	1484237	3069540	90.13%	20.323%
6	30.711	2790	2796	2804	rVB	197193	389269	11.43%	2.577%
7	33.695	3114	3121	3141	rBV2	757038	1728052	50.74%	11.441%
8	37.936	3575	3583	3601	rBV2	387403	1167668	34.29%	7.731%


Sum of corrected areas: 15103443

5055.D GCMS0308.M

Tue Apr 02 15:33:03 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAR3002\5055.D
 Operator :
 Acquired : 30 Mar 2002 10:42 pm using AcqMethod GCMS0308
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 3/8
 Misc Info :
 Vial Number: 31
 Quant File :GCMS0308.RES (RTE Integrator)

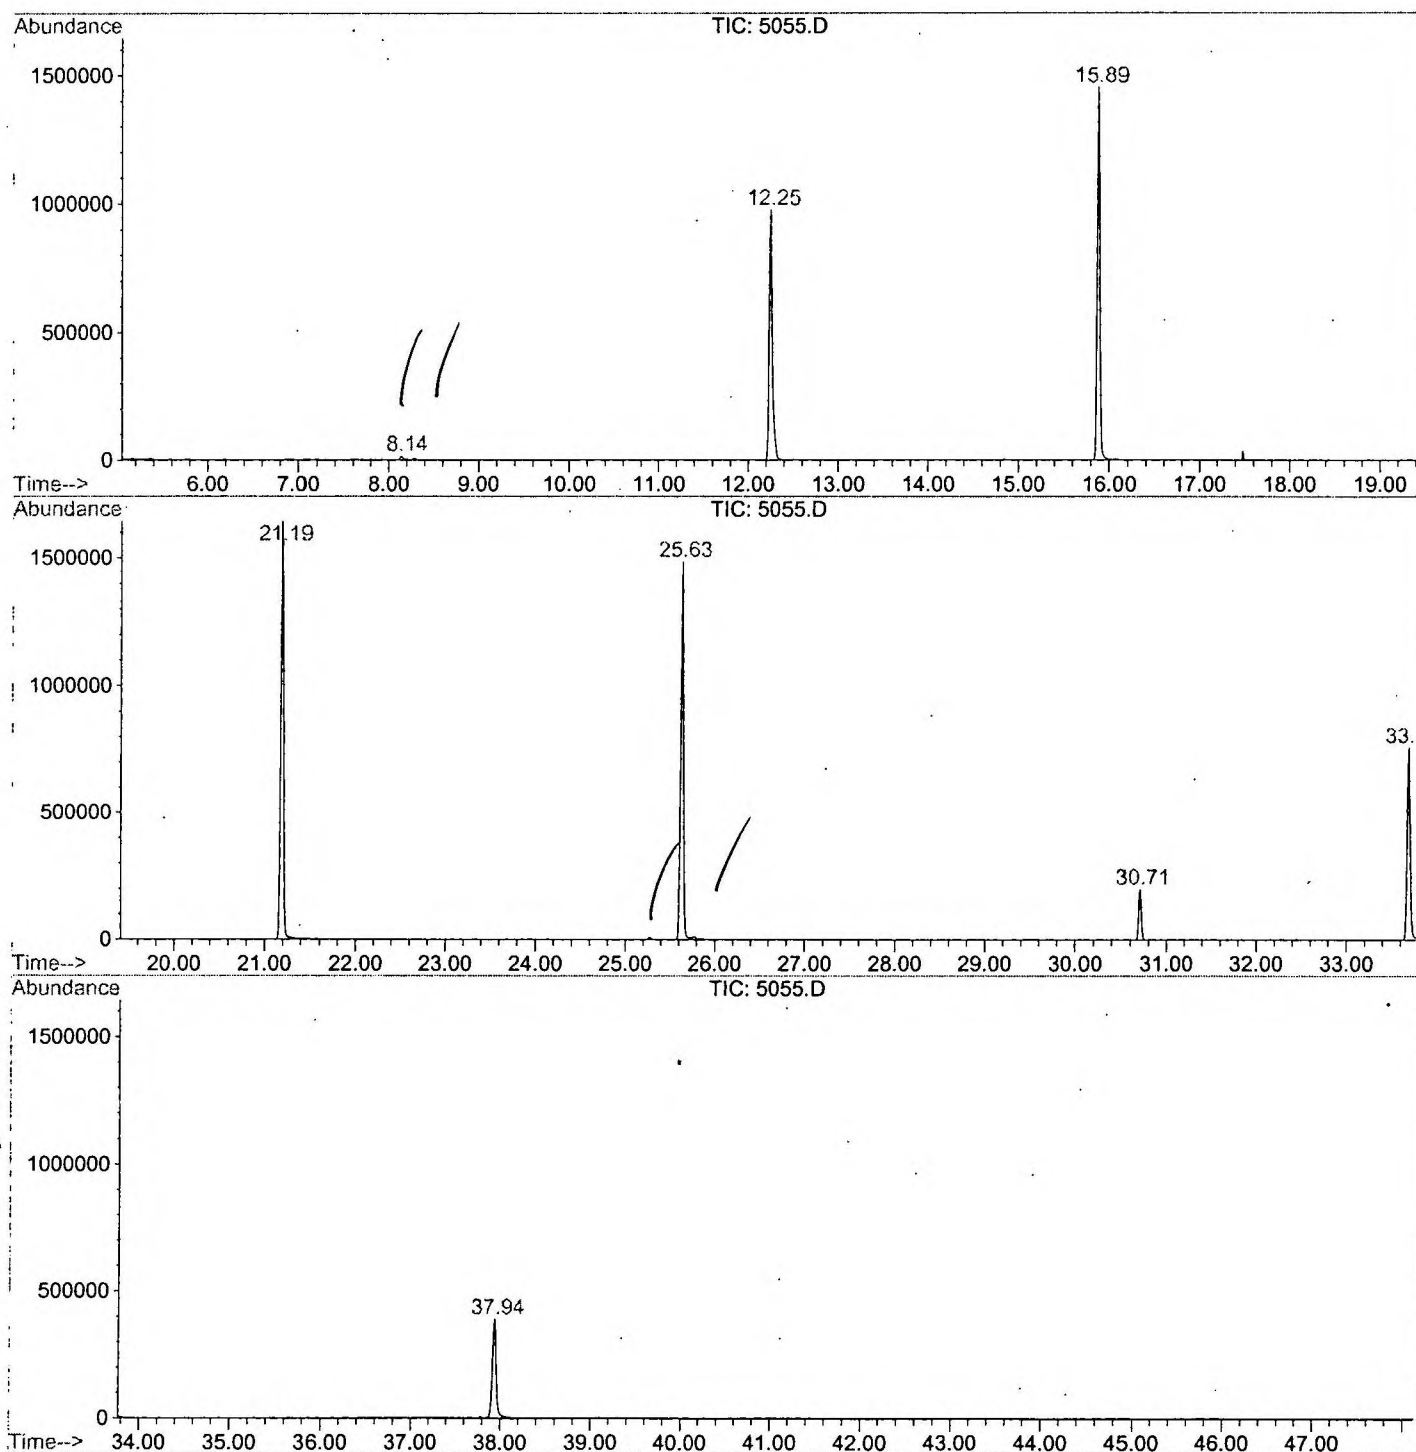

5055.D GCMS0308.M

Tue Apr 02 15:33:09 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAR3002\5055.D

Acq On : 30 Mar 2002 10:42 pm

Sample : gc/ms scan 3/8

Misc :

MS Integration Params: LSCINT.P

Vial: 31

Operator:

Inst : GC/MS 209

Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)










Title : 209 625/TCLP calibration table

Library : C:\DATABASE\NBS75K.L

Peak Number 1 N-Ethylformamide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.14	0.31 ug/l	36371	1,4-Dichlorobenzene-d4	12.25

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			N-Ethylformamide	73	C3H7NO	000627-45-2	9
2			1-Hexanol, 6-amino-	117	C6H15NO	004048-33-3	9
3			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	9
4			Methane, isothiocyanato-	73	C2H3NS	000556-61-6	4

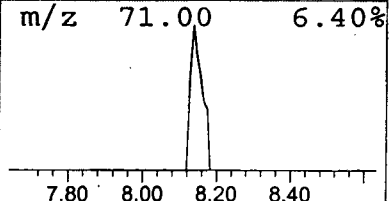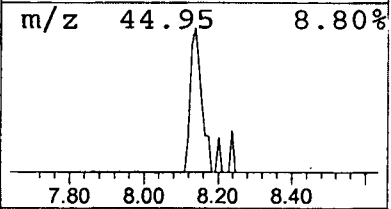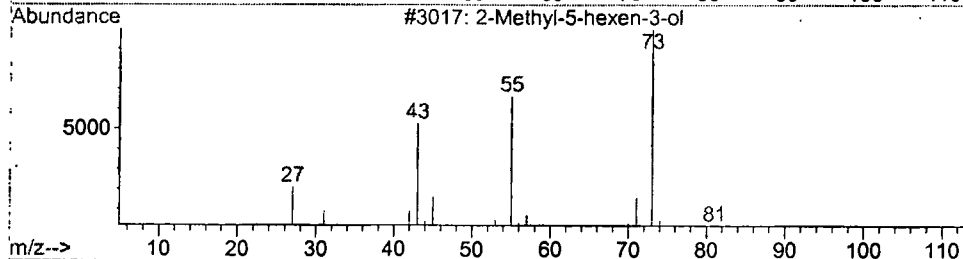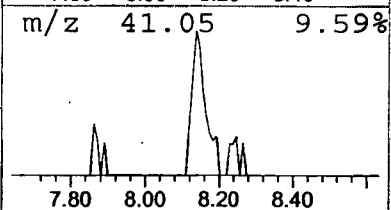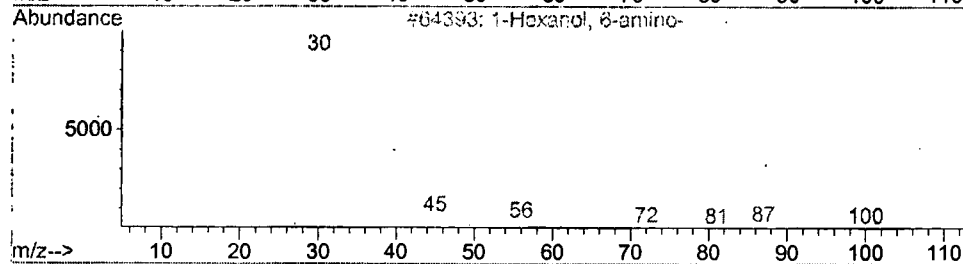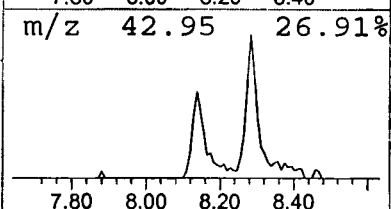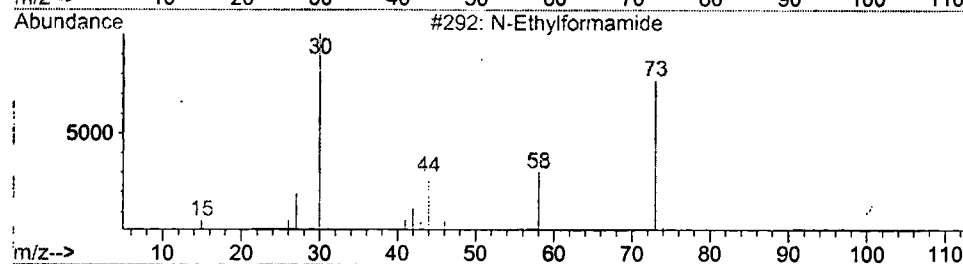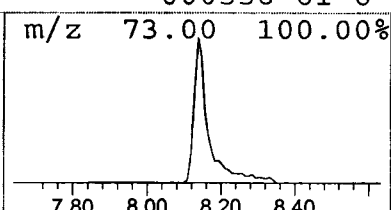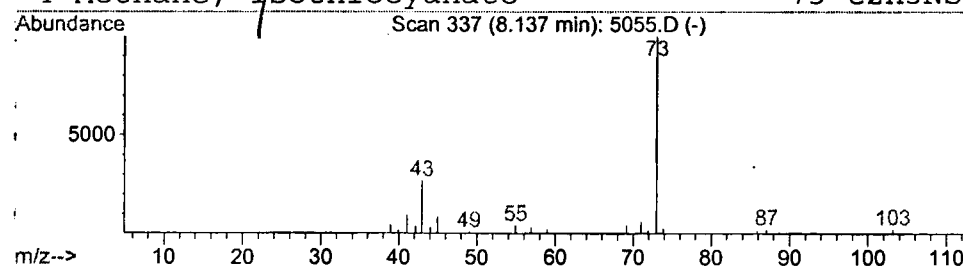

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 30 Mar 2002 10:42 pm
Data File: C:\HPCHEM\1\DATA\MAR3002\5055.D
Name: gc/ms scan 3/8
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
N-Ethylformamide	8.14	0.3	ug/l	36371	ISTD01	12.25	2326060	20.0

5055.D GCMS0308.M Tue Apr 02 15:33:17 2002