


DFTPP

Data File : C:\MSDCHEM\1\DATA\031602\DFT0316.D
 Acq On : 16 Mar 2002 9:15 am
 Sample : DFTPP
 Misc :
 MS Integration Params: BENZO.P
 Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)
 Title : Quantitation For Method 508gcscan

Vial: 1
 Operator: McLean
 Inst : Instrumen
 Multiplr: 1.00

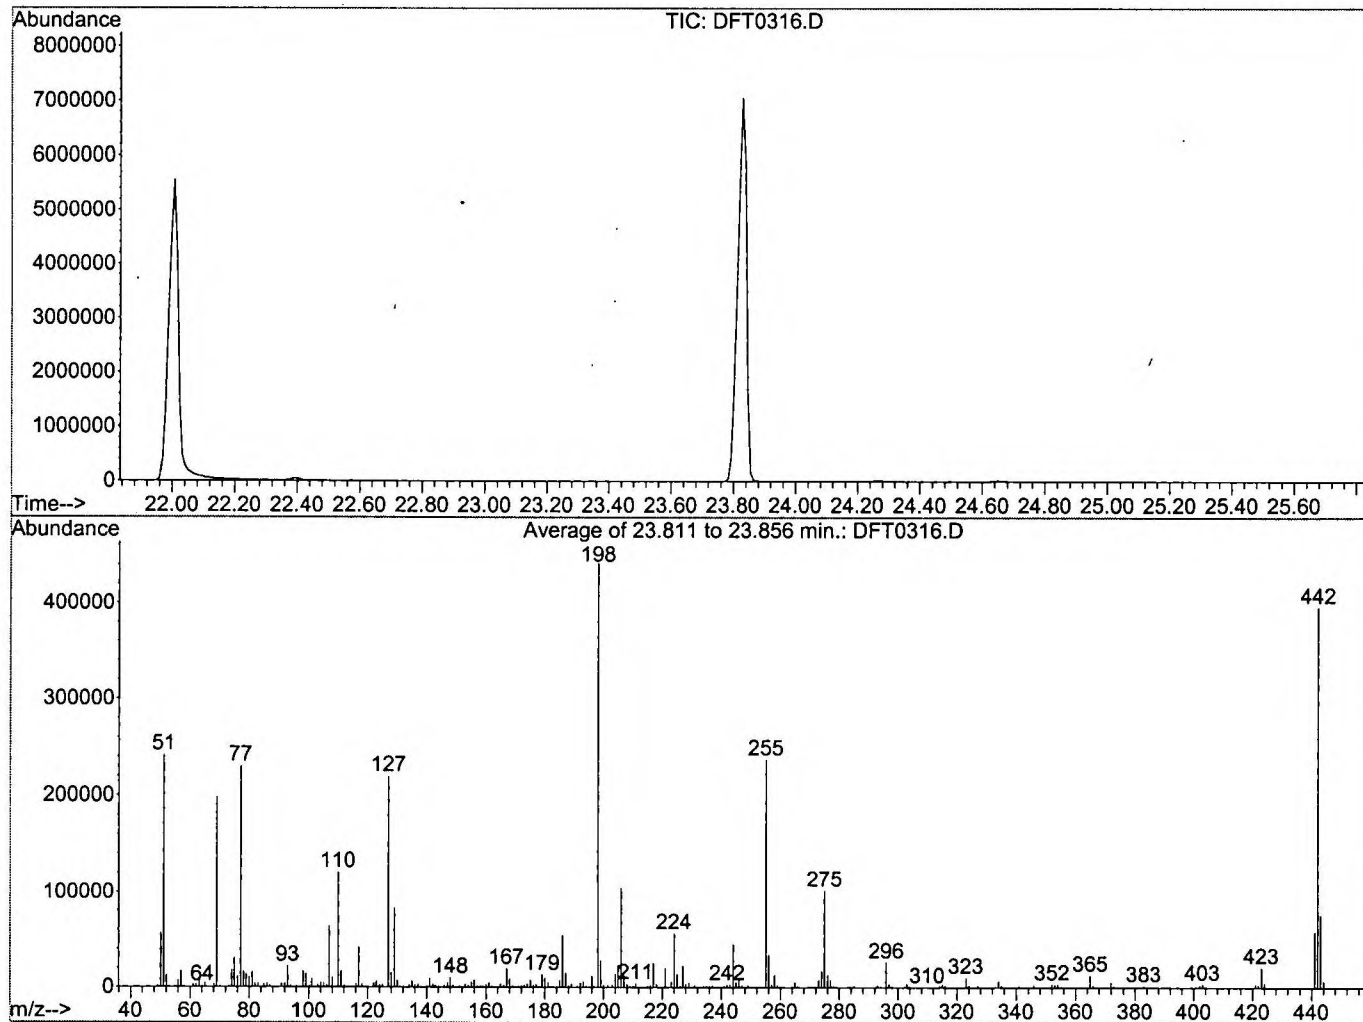

Spectrum Information: Average of 23.811 to 23.856 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.6	241107	PASS
68	69	0.00	2	1.5	3040	PASS
69	198	0.00	100	44.9	198042	PASS
70	69	0.00	2	0.4	836	PASS
127	198	10	80	49.7	219467	PASS
197	198	0.00	2	0.3	1425	PASS
198	198	50	100	100.0	441303	PASS
199	198	5	9	6.4	28255	PASS
275	198	10	60	22.8	100732	PASS
365	198	1	100	2.8	12305	PASS
441	443	0.01	100	77.1	58565	PASS
442	198	50	100	89.7	395801	PASS
443	442	15	24	19.2	75923	PASS