NYC 9/11 Public Portal Document

Method 508 mod. Date Extracted 3/9/02 Page 142

Ref #GCMS - 17766

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	~~Spk~~ add	IS add	Final vol.	T.V. pos.	pH	Count		
LB		500ml		1ml			1ml	4B	7			
Ref 1					1ml			2B				
Ref 2								1B				
5231								4A				
5232								1A				
5233								1B				
5234	FB							10A				
5235								2A				
5236								10A				
5237								1A				

Remarks

Reviewed by, 8/13/02

drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -

Extraction type - sep fun Solv.lot# V41470 NaCl lot# V39618 Na2SO4 lot# V46626

STANDARD	INT STD LOG#
CALIBRATION	HP030102
REF/SPIKE	2193
MDL/MDRF	
Q. CHECK	
INT. STD.	ISD32500
SURROGATE	GCMS 2160D
LPC	
ENDRIN/DDT	

Analyst EH
Revision 4/12/01

Verified by MJ

Reviewed by
Date 8/13/02

NYC-WTC_000059103

NYC 9/11 Public Portal Document

DFTPP

Data File : C:\HPCHEM\1\DATA\MAR3002\DFTPP1.D
Acq On : 30 Mar 2002 3:46 pm
Sample :
Misc :
MS Integration Params: GOOFY.P
Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title : 209 625/TCLP calibration table

Vial: 1
Operator:
Inst : GC/MS 209
Multiplr: 1.00

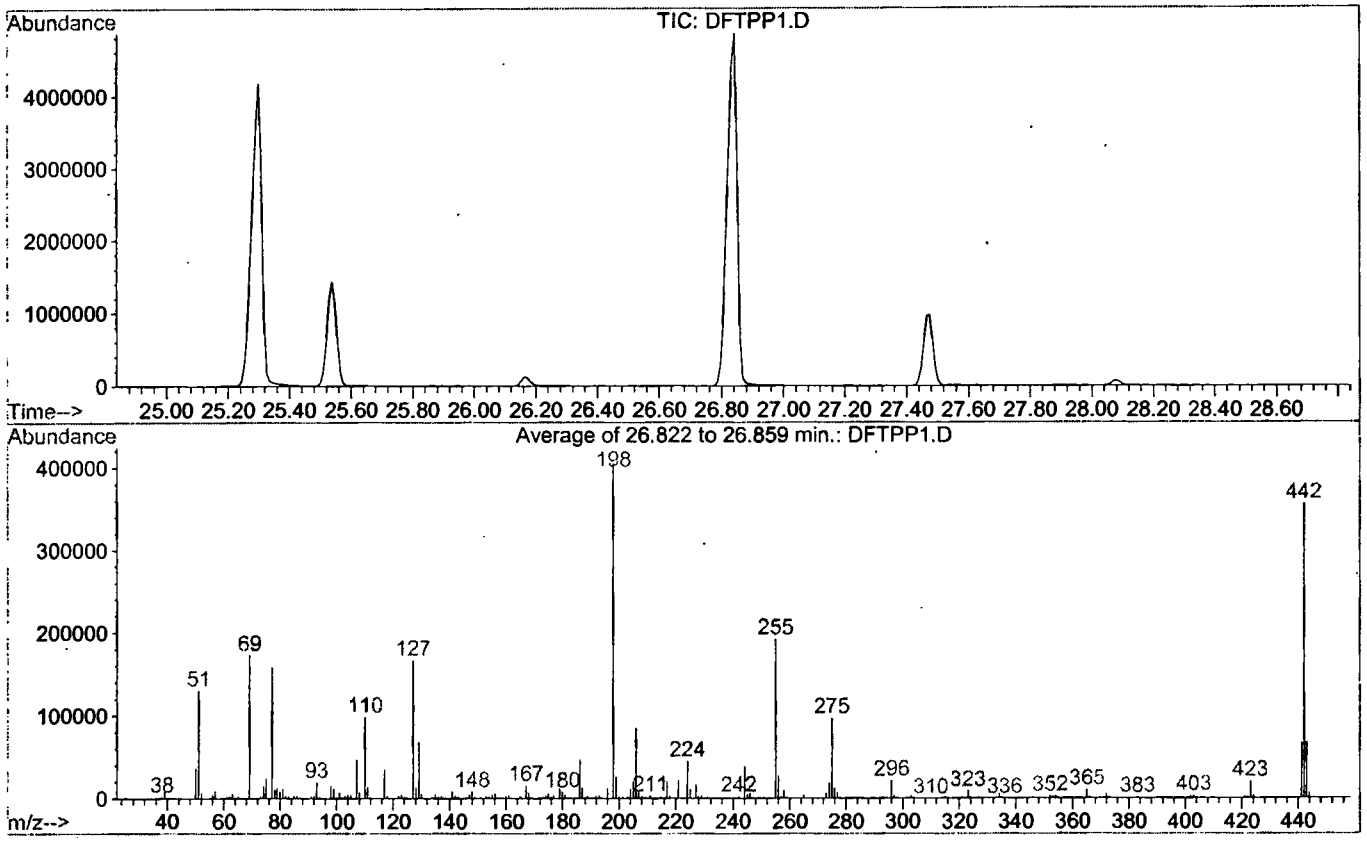

Spectrum Information: Average of 26.822 to 26.859 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	32.2	130212	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.8	172994	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	41.3	166826	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	404158	PASS
199	198	5	9	6.5	26336	PASS
275	198	10	30	24.1	97214	PASS
365	198	1	100	2.6	10574	PASS
441	443	0.01	100	98.6	67442	PASS
442	198	40	110	87.9	355200	PASS
443	442	17	23	19.3	68411	PASS

DFTPP1.D GCMS0308.M Wed Apr 03 13:31:40 2002