

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 04/03/2002 Time: 15:01:42

Sample: AE05231
 Analysis: \$B1GCMS Blank for GCMS Scan
 Units: ug
 Started: 4/3/02 14:57 Ended: 4/3/02 14:57 Analyst: MG
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	n-Nitrosodimethylamine		< MDL		2.0
2	bis(2-Chloroethyl)ether		< MDL		2.0
3	1,3-Dichlorobenzene		< MDL		2.0
4	1,4-Dichlorobenzene		< MDL		2.0
5	1,2-Dichlorobenzene		< MDL		2.0
6	2,2'-oxybis(1-Chloropropane)		< MDL		2.0
7	n-Nitrosodi-n-propylamine		< MDL		2.0
8	Hexachloroethane		< MDL		2.0
9	Nitrobenzene		< MDL		2.0
10	Isophorone		< MDL		2.0
11	bis(2-Chloroethoxy)methane		< MDL		2.0
12	1,2,4-Trichlorobenzene		< MDL		2.0
13	Naphthalene		< MDL		2.0
14	Hexachlorobutadiene		< MDL		2.0
15	2-Chloronaphthalene		< MDL		2.0
16	Dimethylphthalate		< MDL		2.0
17	2,6-Dinitrotoluene		< MDL		2.0
18	Acenaphthylene		< MDL		2.0
19	Acenaphthene		< MDL		2.0
20	2,4-Dinitrotoluene		< MDL		2.0
21	Diethylphthalate		< MDL		2.0
22	4-Chlorophenylphenylether		< MDL		2.0
23	Fluorene		< MDL		2.0
24	Azobenzene/1,2-Diphenylhydraz		< MDL		2.0
25	n-Nitrosodiphenylamine		< MDL		2.0
26	4-Bromophenylphenylether		< MDL		2.0
27	Hexachlorobenzene		< MDL		2.0
28	Phenanthrene		< MDL		2.0
29	Anthracene		< MDL		2.0
30	Di-n-butylphthalate		< MDL		2.0
31	Fluoranthene		< MDL		2.0
32	Pyrene		< MDL		2.0
33	Butylbenzylphthalate		< MDL		2.0
34	Benzo(a)anthracene		< MDL		2.0
35	bis(2-Ethylhexyl)phthalate		< MDL		2.0
36	Chrysene		< MDL		2.0
37	Di-n-octylphthalate		< MDL		2.0
38	Benzo(b)fluoranthene		< MDL		2.0
39	Benzo(k)fluoranthene		< MDL		2.0
40	Benzo(a)pyrene		< MDL		2.0
41	Indeno(1,2,3-cd)pyrene		< MDL		2.0
42	Dibenz(a,h)anthracene		< MDL		2.0
43	Benzo(g,h,i)perylene		< MDL		2.0

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAR3002\LBC.D
 Acq On : 31 Mar 2002 6:39 am
 Sample : gc/ms scan 3/9
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Mar 31 7:28 2002

Vial: 39
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00
 Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Mar 29 10:31:28 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0308

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.25	152	417714	20.00	ug/l	-0.10
10) Naphthalene-d8	15.89	136	1515128	20.00	ug/l	-0.11
17) Acenaphthene-d10	21.19	164	860319	20.00	ug/l	-0.12
29) Phenanthrene-d10	25.63	188	1186088	20.00	ug/l	-0.14
38) Chrysene-d12	33.69	240	562603	20.00	ug/l	-0.16
44) Perylene-d12	37.93	264	314928	20.00	ug/l	-0.19

System Monitoring Compounds

37) 2,4-DDD	30.70	235	72898	6.13	ug/mL	0.21
Spiked Amount	5.000		Recovery	=	122.60%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	12.15	146	290	N.D.	
5) 1,4-Dichlorobenzene	12.30	146	317	N.D.	
6) 1,2-Dichlorobenzene	12.82	146	258	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	15.77	180	259	N.D.	
15) Naphthalene	15.94	128	597	N.D.	
16) Hexachlorobutadiene	16.48	225	377	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	

(#) = qualifier out of range (m) = manual integration

LBC.D GCMS0308.M Wed Apr 03 13:33:40 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\MAR3002\LBC.D

Vial: 39

Acq On : 31 Mar 2002 6:39 am

Operator:

Sample : gc/ms scan 3/9

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Mar 31 7:28 2002

Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Mar 29 10:31:28 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0308

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.63	178	242	N.D.		
34) Anthracene	25.63	178	242	N.D.		
35) Di-n-butylphthalate	27.60	149	1496	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.70	228	1232	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.91	149	790	N.D.		
43) Chrysene	33.70	228	1232	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.94	252	1019	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

LBC.D GCMS0308.M

Wed Apr 03 13:33:44 2002


Page 2

Quantitation Report

Data File : C:\HPCHEM\1\DATA\MAR3002\LBC.D
Acq On : 31 Mar 2002 6:39 am
Sample : gc/ms scan 3/9
Misc :
MS Integration Params: GOOFY.P
Quant Time: Mar 31 7:28 2002

Vial: 39
Operator:
Inst : GC/MS 209
Multiplr: 1.00
Quant Results File: GCMS0308.RES

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title : 209.625/TCLP calibration table
Last Update : Fri Mar 29 10:31:28 2002
Response via : Initial Calibration

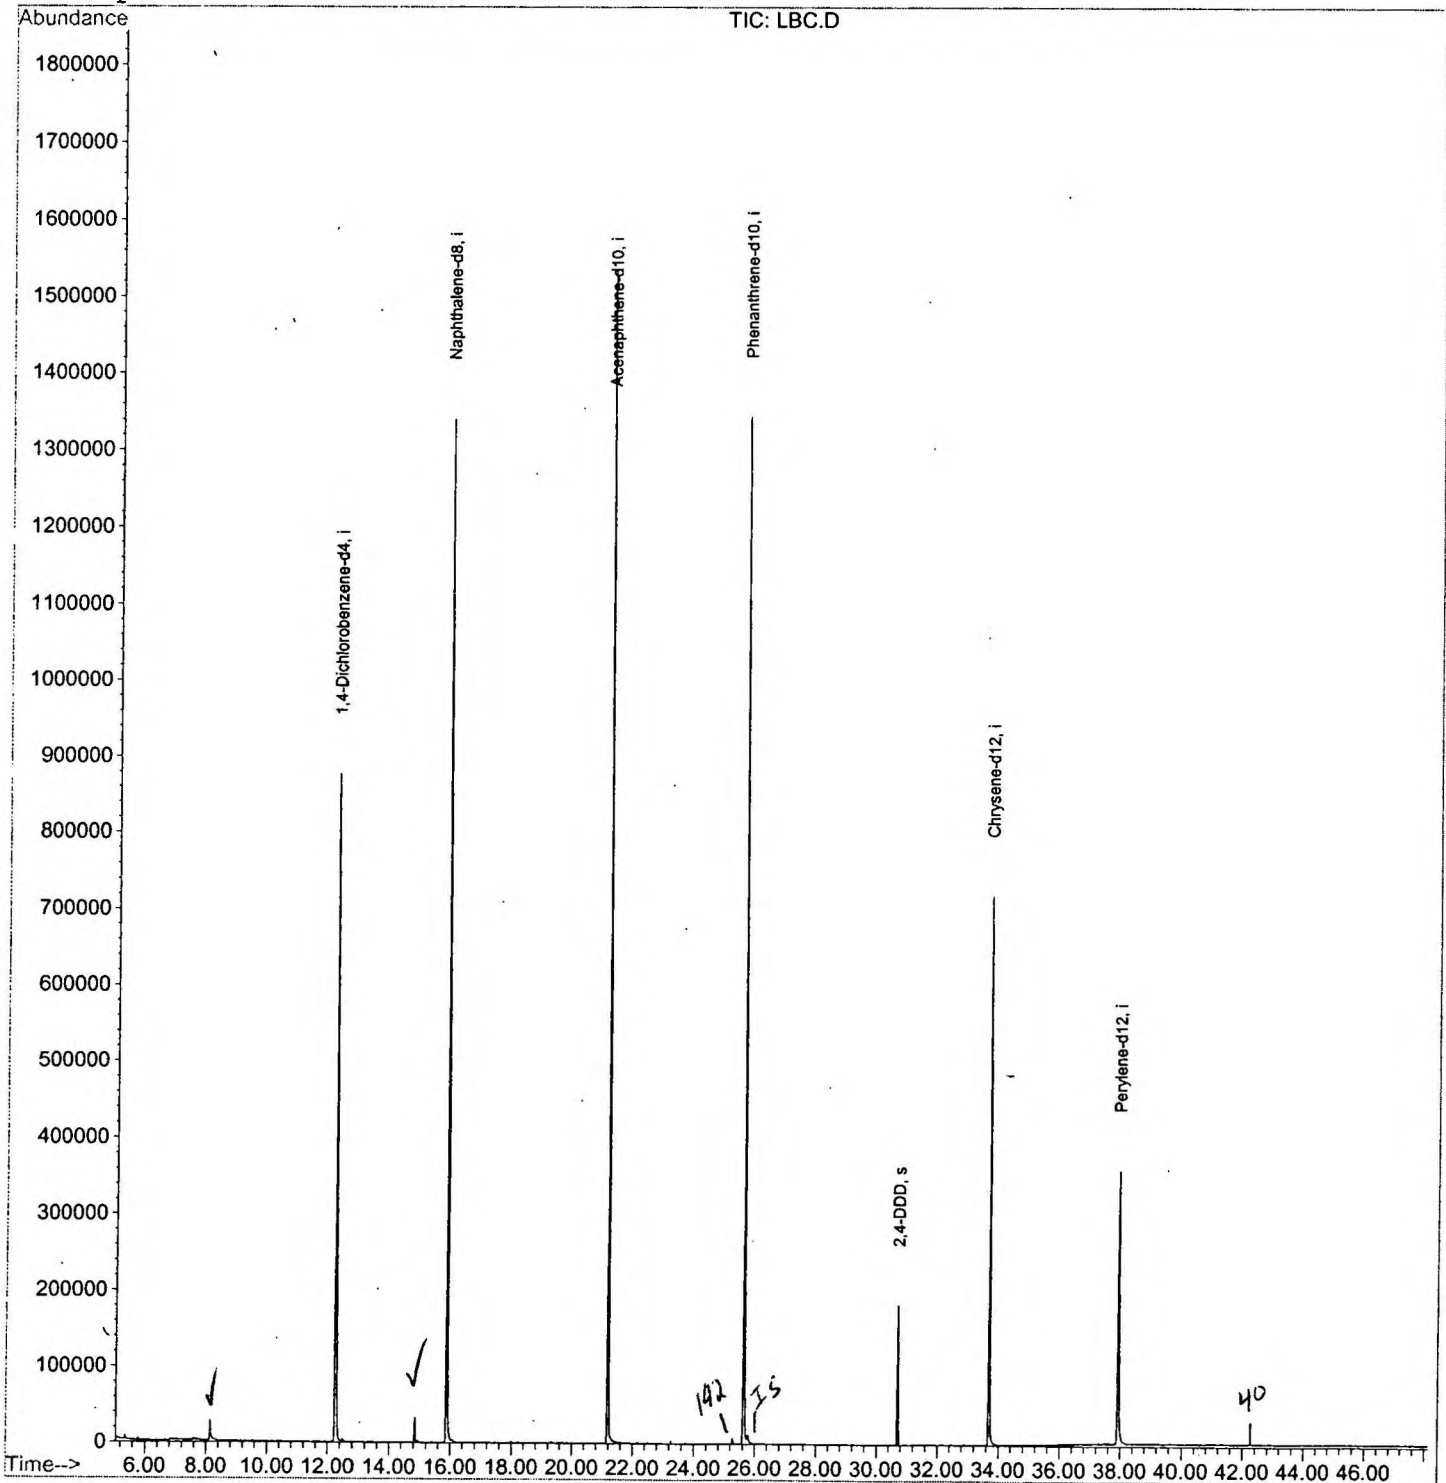

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\MAR3002\LBC.D

Vial: 39

Acq On : 31 Mar 2002 6:39 am

Operator:

Sample : gc/ms scan 3/9

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.139	332	337	348	rBV	26483	69293	2.12%	0.477%
2	12.251	779	785	806	rBV	875410	2237470	68.45%	15.415%
3	14.849	1063	1068	1073	rVB	32661	65399	2.00%	0.451%
4	15.887	1175	1181	1198	rBV	1339254	2852637	87.27%	19.653%
5	21.193	1752	1759	1778	rBV	1536253	3268727	100.00%	22.520%
6	25.636	2236	2243	2252	rBV2	1343711	2969762	90.85%	20.460%
7	30.704	2790	2795	2802	rBV	184265	360551	11.03%	2.484%
8	33.687	3113	3120	3141	rBV2	719768	1626115	49.75%	11.203%
9	37.929	3575	3582	3603	rBV	357810	1065037	32.58%	7.337%


Sum of corrected areas: 14514991

LBC.D GCMS0308.M

Wed Apr 03 14:04:00 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\MAR3002\LBC.D
 Operator :
 Acquired : 31 Mar 2002 6:39 am using AcqMethod GCMS0308
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 3/9
 Misc Info :
 Vial Number: 39
 Quant File :GCMS0308.RES (RTE Integrator)

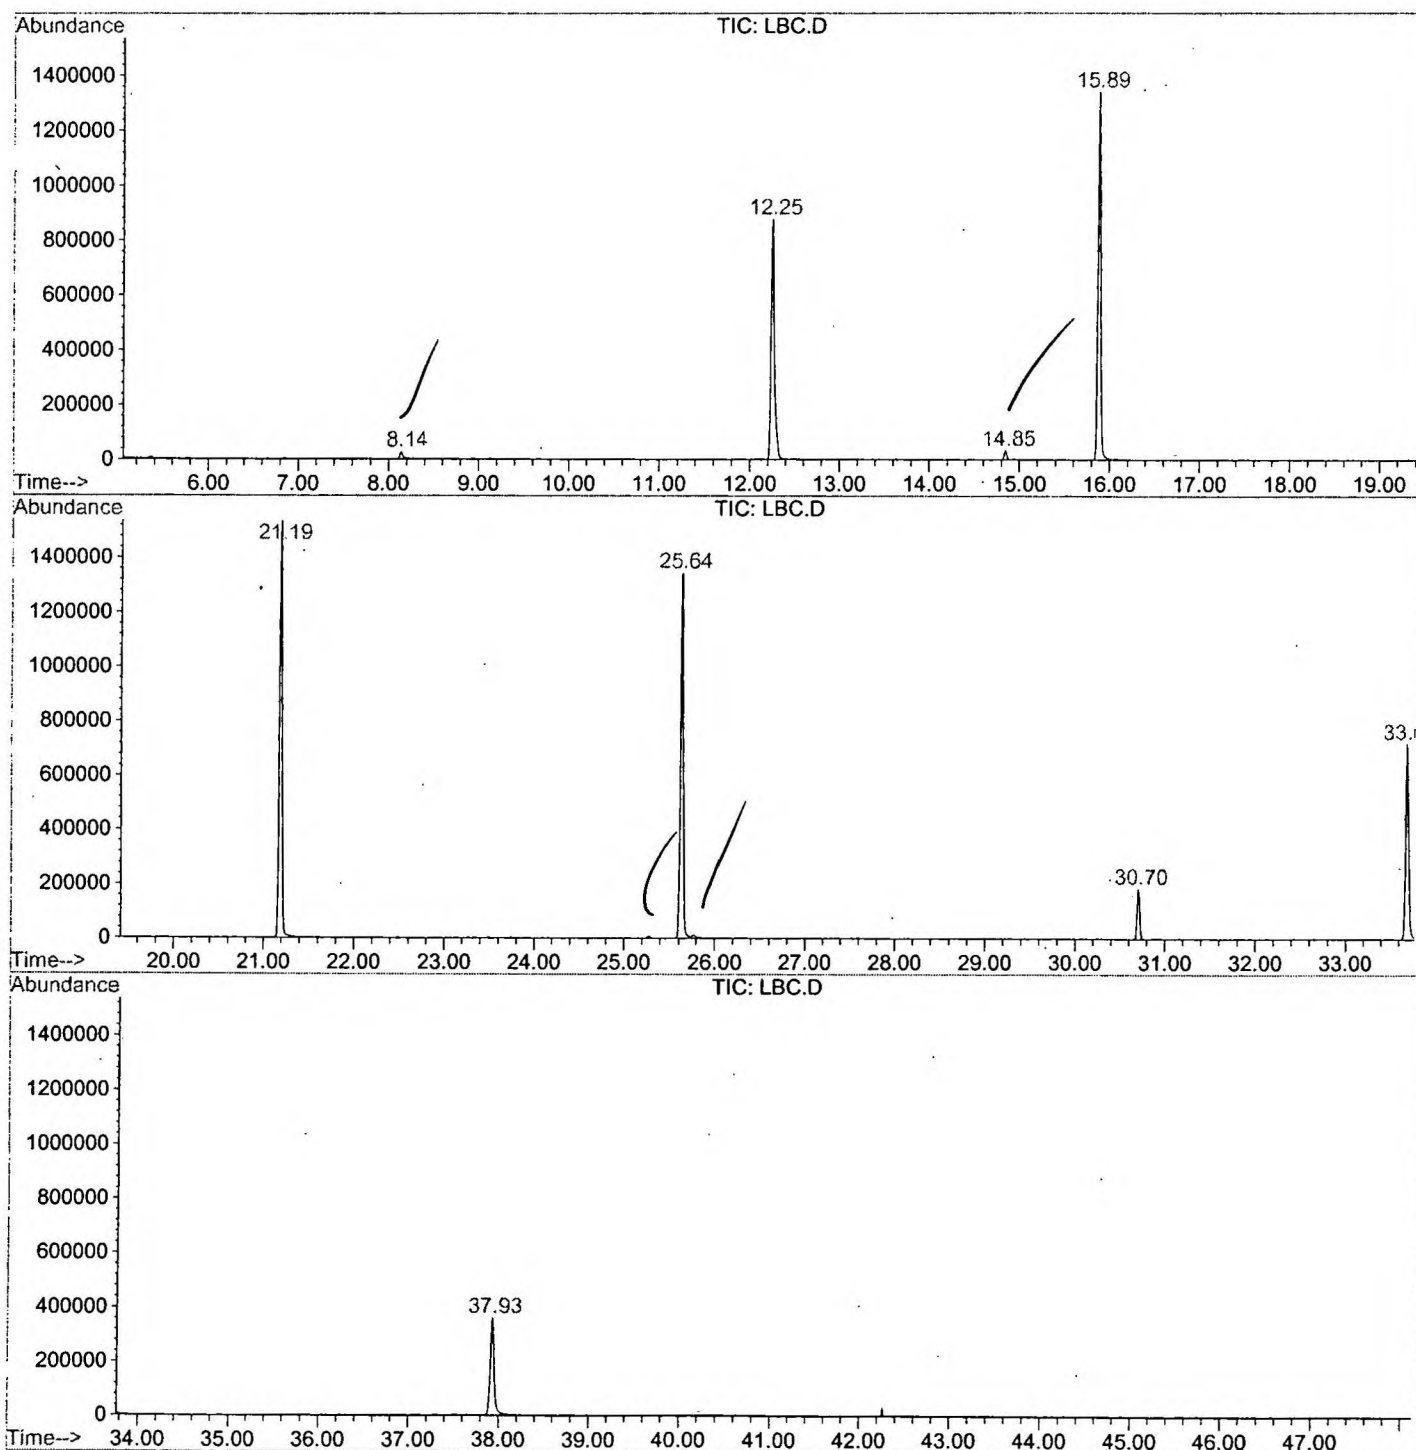

LBC.D GCMS0308.M

Wed Apr 03 14:04:05 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAR3002\LBC.D
 Acq On : 31 Mar 2002 6:39 am
 Sample : gc/ms scan 3/9
 Misc :
 MS Integration Params: LSCINT.P


Vial: 39
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 N-Ethylformamide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.14	0.62 ug/l	69293	1,4-Dichlorobenzene-d4	12.25

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			N-Ethylformamide	73	C3H7NO	000627-45-2	9
2			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9
4			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	9

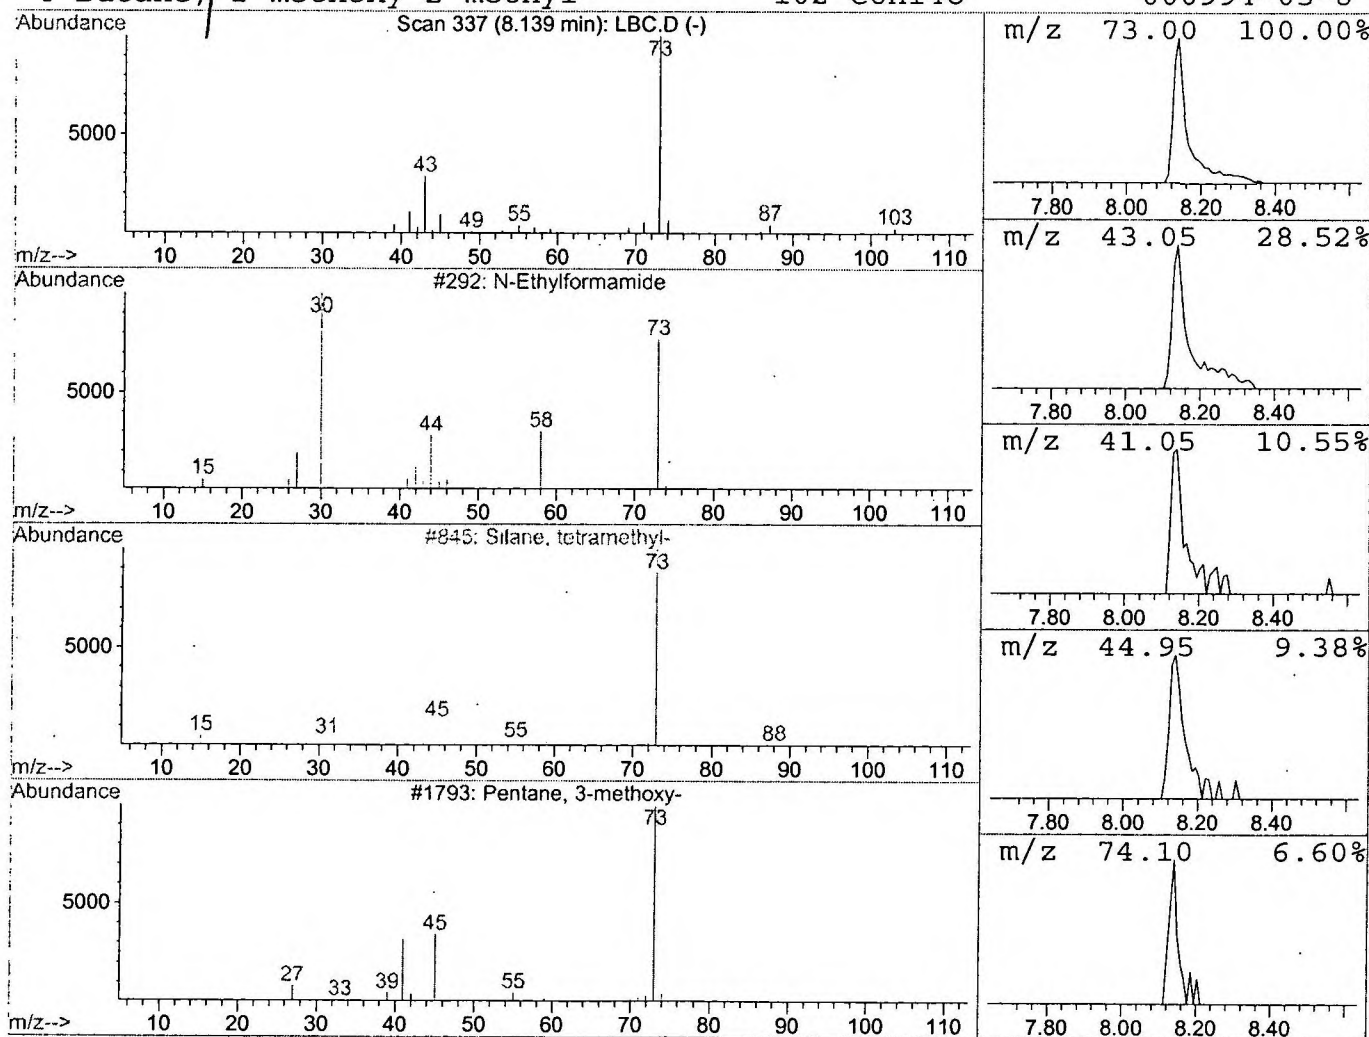

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\MAR3002\LBC.D
Acq On : 31 Mar 2002 6:39 am
Sample : gc/ms scan 3/9
Misc :
MS Integration Params: LSCINT.P



Vial: 39
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L



Peak Number 2 Cyclopentasiloxane, decamethyl Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.85	0.46 ug/l	65399	Naphthalene-d8	15.89





Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	91
2			Silane, [[4-[1,2-bis(trimethylsilyl)oxy]ethyl]-1,2	458	C20H42O4Si4	056114-62-6	43
3			Noradrenaline, tetra-TMS	457	C20H43NO3Si4	000000-00-0	37
4			N-(Trifluoroacetyl)-N,O,O',O''-tetr	553	C22H42F3NO4Si4	000000-00-0	37

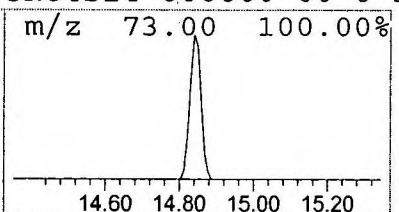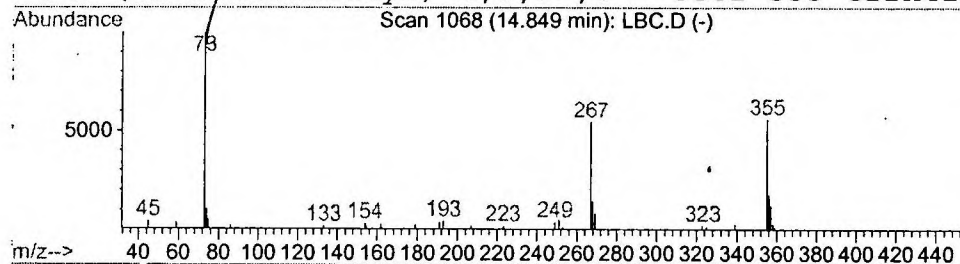

m/z 355.05 56.16%

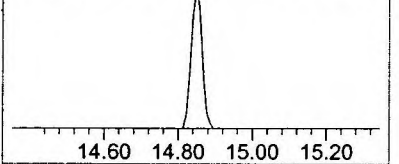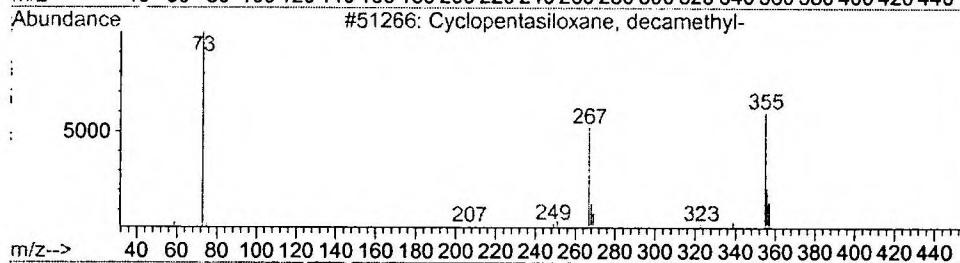

m/z 356.05 17.49%

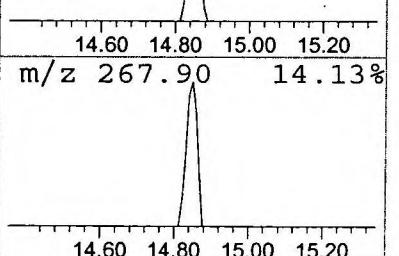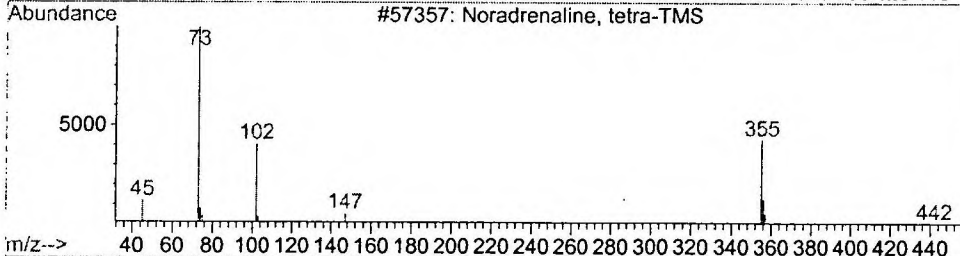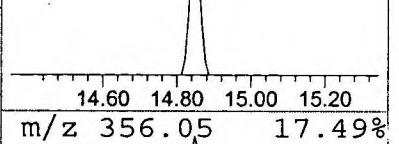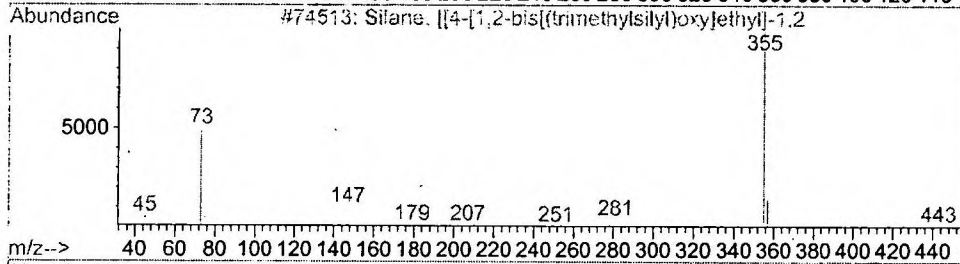

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 31 Mar 2002 6:39 am
Data File: C:\HPCHEM\1\DATA\MAR3002\LBC.D
Name: gc/ms scan 3/9
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
N-Ethylformamide	8.14	0.6	ug/l	69293	ISTD01	12.25	2237470	20.0
Cyclopentasiloxane,	14.85	0.5	ug/l	65399	ISTD02	15.89	2852640	20.0

LBC.D GCMS0308.M Wed Apr 03 14:04:18 2002