

Method 508 mod.

Date Extracted 3/11/02

Page 144

Ref

#GCMs-17783

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Sol add	IS add	Final vol.	T.V. pos.	pH	Count		
1B		500ml		1ml			1ml	2B	7			
Ref					1ml			2A				
Ref					↓			6A				
5515								8B				
5516								7A				
5517								1A				
5518								9A				
5519	FB							9B				
5696								7B				
5697								1B				
5698								4A				
5699	FB							8A				
3700		↓		↓			↓	4B	↓			
Remarks												
Reviewed by <u>CB 8/13/02</u>												
drip rate must be between 5-15 ml/min for liq-liq extractors												
drip rate -												
Extraction type - <u>sep fun</u> Solv. lot# <u>V39466</u> NaCl lot# <u>V39618</u> Na2SO4 lot# <u>V46623</u>												
STANDARD	INT STD LOG#											
CALIBRATION	<u>11035012</u>											
REF SPIKE	<u>2193</u>											
MDL/MDRF												
Q. CHECK	<u>2</u>											
INT. STD.	<u>032802</u>											
SURROGATE	<u>GCMs</u>	<u>2160 D</u>										
LPC												
ENDRIN/DDT												

Analyst EA
revision 4/12/01


Verified by mg

Reviewed by DM
Date 4/10/02

DFTPP

Data File : C:\HPCHEM\1\DATA\APR0102\DFTPP.D
 Acq On : 1 Apr 2002 11:12 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0403.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

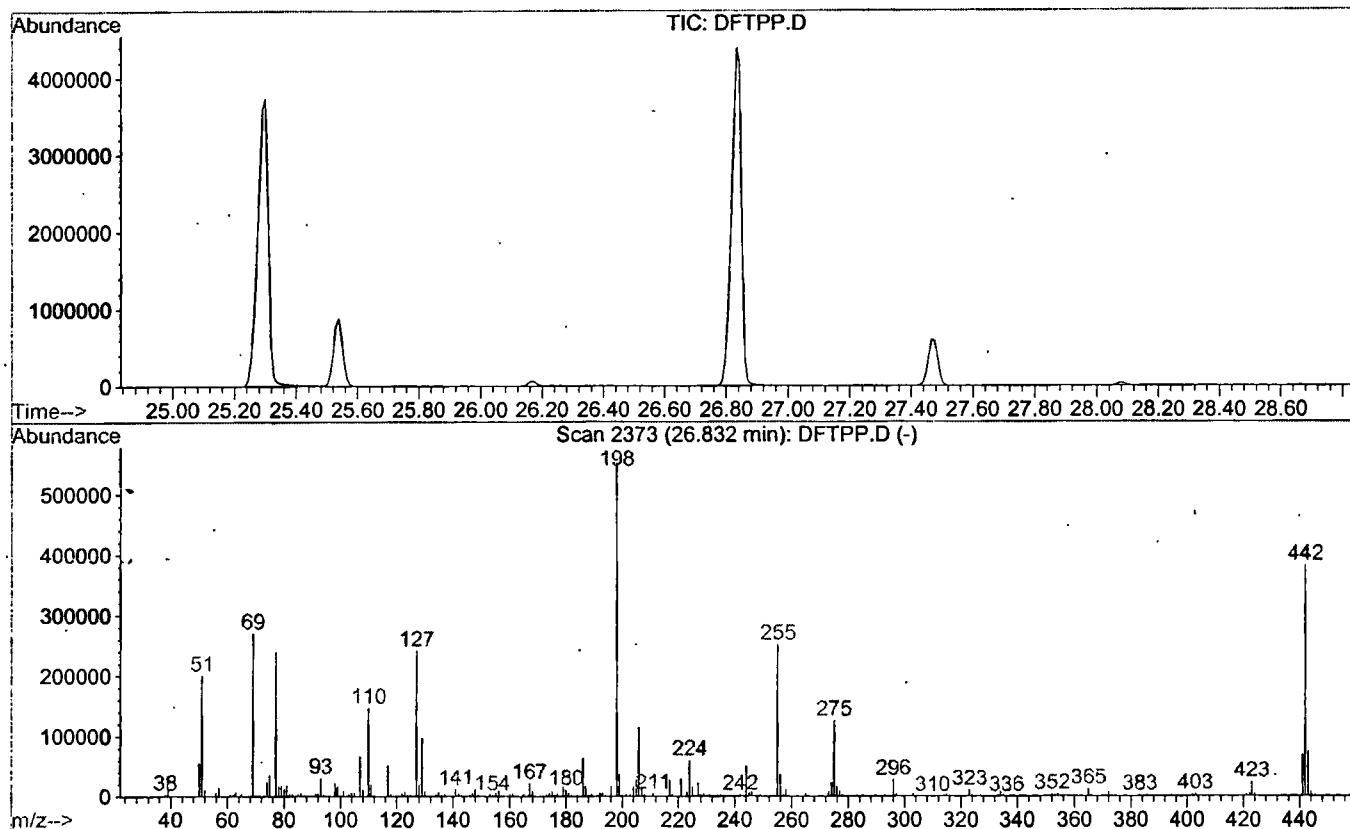

Spectrum Information: Scan 2373

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	36.4	200654	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.0	270336	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	43.8	241856	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	552000	PASS
199	198	5	9	6.8	37808	PASS
275	198	10	30	22.9	126560	PASS
365	198	1	100	2.2	12367	PASS
441	443	0.01	100	93.0	70288	PASS
442	198	40	110	69.3	382464	PASS
443	442	17	23	19.8	75608	PASS