

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/09/2002 Time: 15:27:29

Sample: AE05699
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/9/02 15:27 Ended: 4/9/02 15:27 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		92		5.0

Comments for Sample AE05699 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-09-2002 Time: 15:27:49

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR0102\5699.D
 Acq On : 2 Apr 2002 1:08 am
 Sample : gc/ms scan 3/11 fb
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 2 1:57 2002

Vial: 14
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Mar 29 10:31:28 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0308

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.25	152	558115	20.00	ug/l	-0.10
10) Naphthalene-d8	15.89	136	2053742	20.00	ug/l	-0.11
17) Acenaphthene-d10	21.19	164	1145395	20.00	ug/l	-0.12
29) Phenanthrene-d10	25.64	188	1593616	20.00	ug/l	-0.13
38) Chrysene-d12	33.70	240	774355	20.00	ug/l	-0.15
44) Perylene-d12	37.94	264	415350	20.00	ug/l	-0.18

System Monitoring Compounds

37) 2,4-DDD	30.71	235	73680	4.61	ug/mL	0.22
Spiked Amount	5.000		Recovery	=	92.20%	

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.		
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.		
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.		
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	0.00	128	0	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-Chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.		
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	21.52	165	193	N.D.		
25) Diethylphthalate	0.00	149	0	N.D.		
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		

(#) = qualifier out of range (m) = manual integration

5699.D GCMS0403.M Thu Apr 04 13:46:45 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR0102\5699.D Vial: 14
 Acq On : 2 Apr 2002 1:08 am Operator:
 Sample : gc/ms scan 3/11 fb Inst : GC/MS 209
 Misc : Multiplr: 1.00
 MS Integration Params: GOOFY.P
 Quant Time: Apr 2 1:57 2002 Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Mar 29 10:31:28 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0308

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.64	178	518	N.D.		
34) Anthracene	25.64	178	518	N.D.		
35) Di-n-butylphthalate	27.60	149	20964	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.70	228	1524	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.91	149	3254	N.D.		
43) Chrysene	33.70	228	1524	N.D.		
45) Di-n-Octylphthalate	0.00	149	0	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.94	252	1482	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

5699.D GCMS0403.M Thu Apr 04 13:46:48 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR0102\5699.D
Acq On : 2 Apr 2002 1:08 am
Sample : gc/ms scan 3/11 fb
Misc :
MS Integration Params: GOOFY.P
Quant Time: Apr 2 1:57 2002

Vial: 14
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0308.RES

Method : C:\HPCHEM\1\METHODS\GCMS0403.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Thu Apr 04 09:06:35 2002
Response via : Initial Calibration

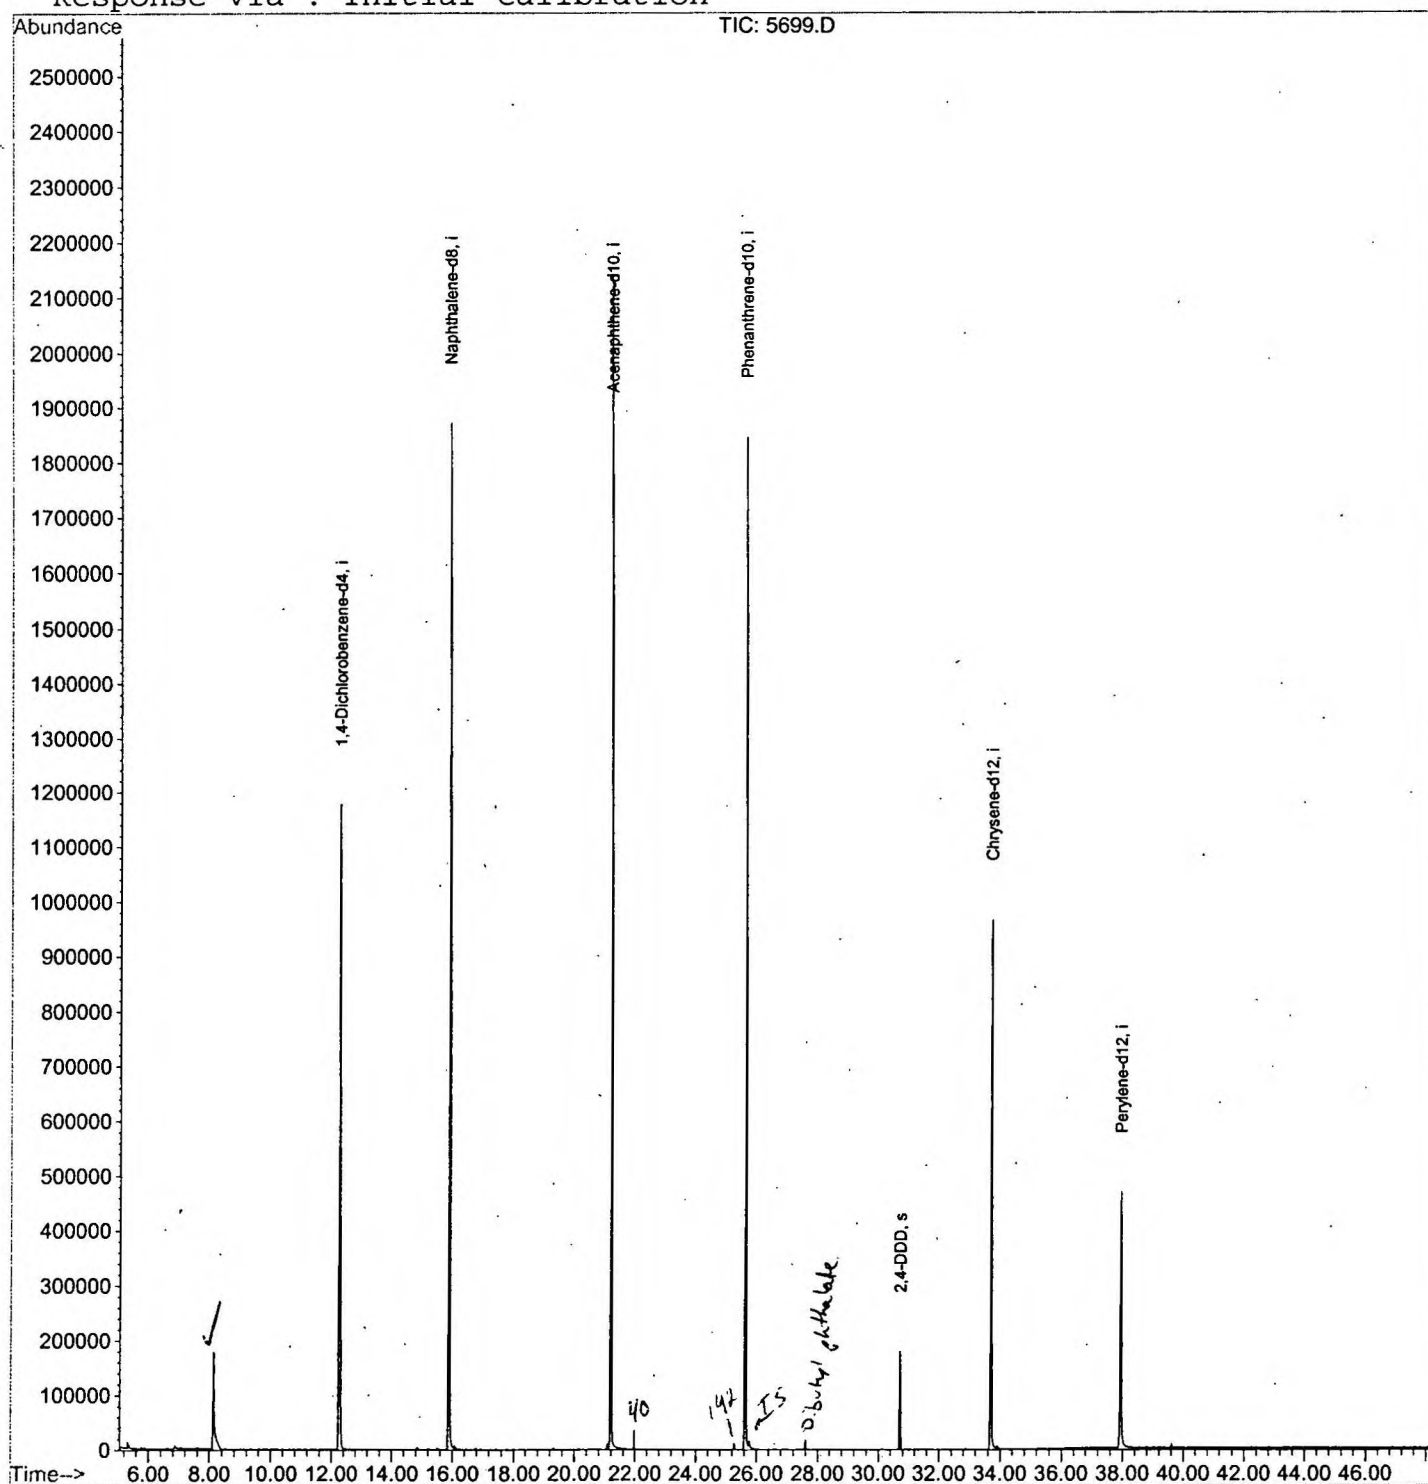

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR0102\5699.D
 Acq On : 2 Apr 2002 1:08 am
 Sample : gc/ms scan 3/11 fb
 Misc :
 MS Integration Params: LSCINT.P

Vial: 14
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0403.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.130	332	336	362	rVB	176831	503724	11.45%	2.547%
2	12.252	779	785	806	rVB	1176456	3028837	68.83%	15.315%
3	15.887	1175	1181	1194	rBV	1871919	3865934	87.85%	19.548%
4	21.193	1752	1759	1778	rBV	2141278	4400698	100.00%	22.252%
5	25.637	2236	2243	2254	rBV	1845938	3981440	90.47%	20.132%
6	30.704	2790	2795	2801	rBV	178674	363747	8.27%	1.839%
7	33.697	3114	3121	3135	rBV	967259	2230665	50.69%	11.279%
8	37.938	3575	3583	3597	rBV2	467858	1401505	31.85%	7.087%

Sum of corrected areas: 19776550

5699.D GCMS0403.M Thu Apr 04 13:59:03 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR0102\5699.D
Operator :
Acquired : 2 Apr 2002 1:08 am using AcqMethod GCMS0308
Instrument : GC/MS 209
Sample Name: gc/ms scan 3/11 fb
Misc Info :
Vial Number: 14
Quant File :GCMS0308.RES (RTE Integrator)

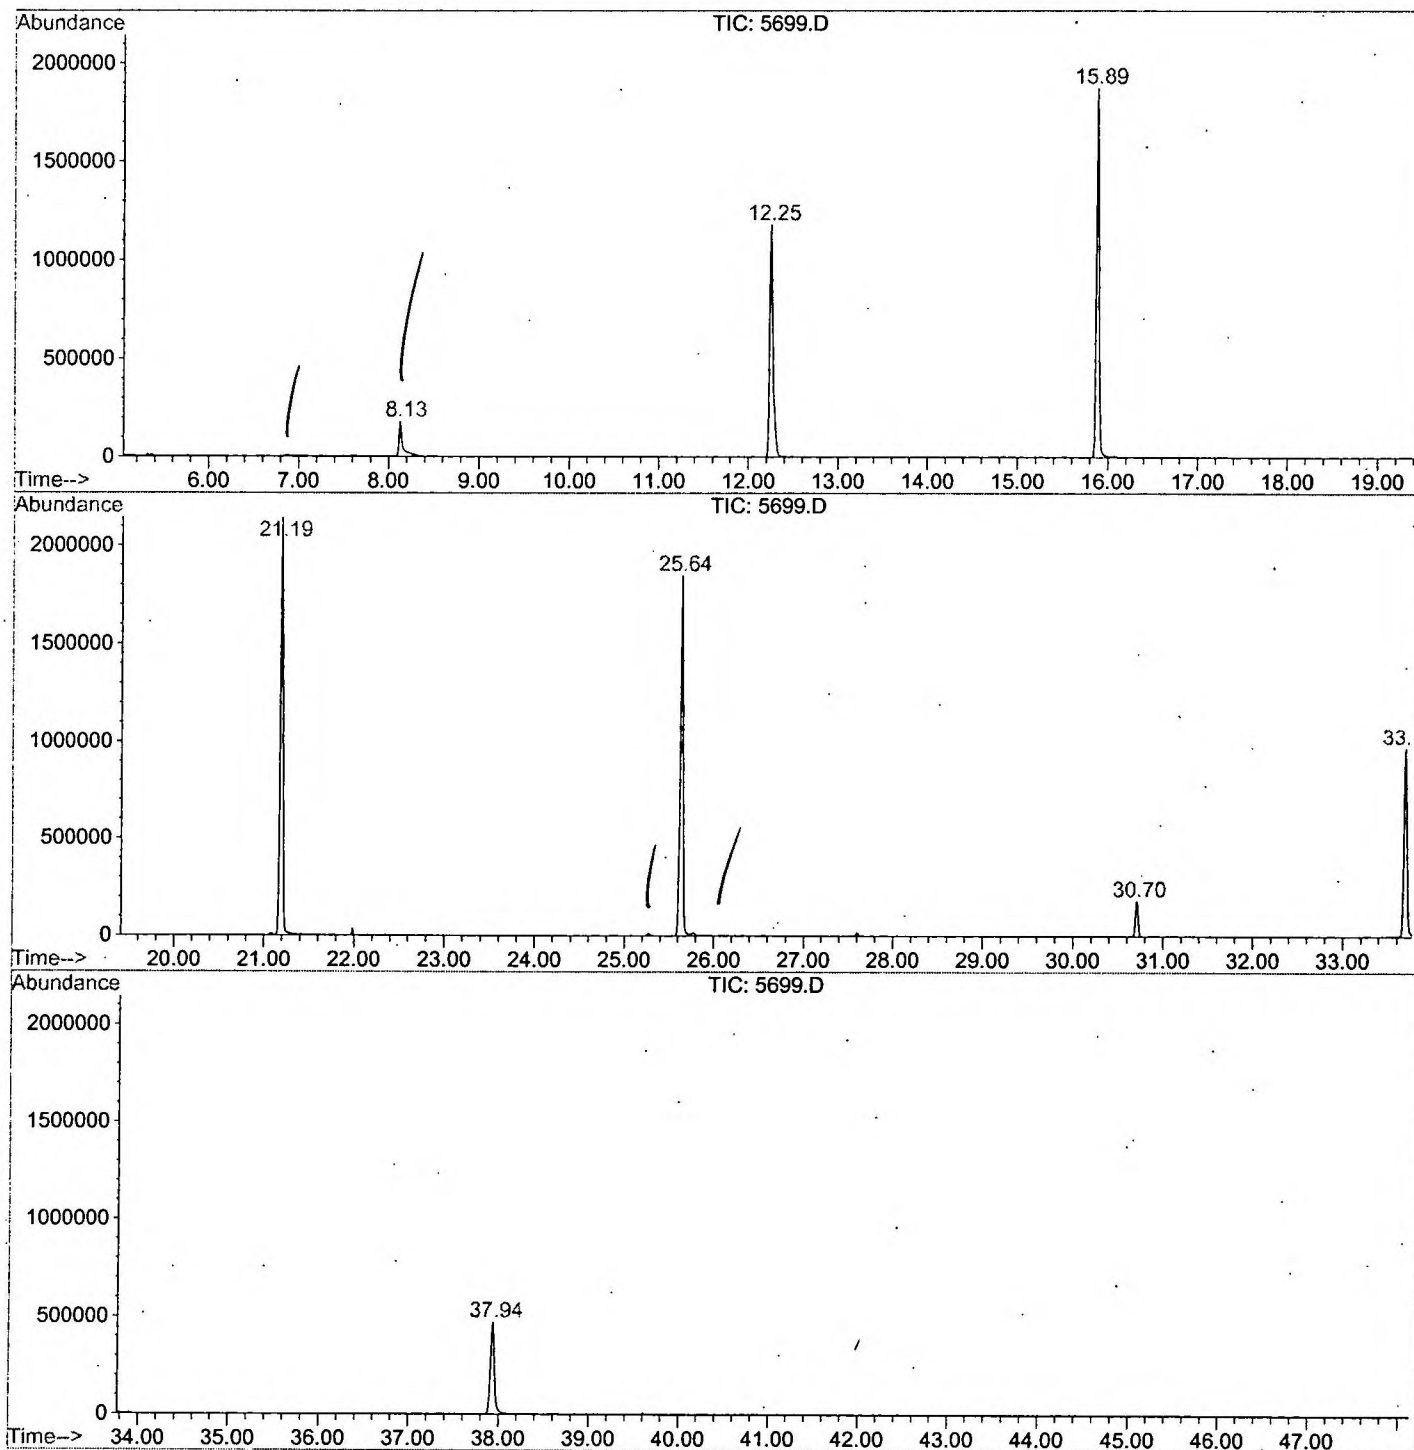

5699.D GCMS0403.M

Thu Apr 04 13:59:08 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR0102\5699.D
Acq On : 2 Apr 2002 1:08 am
Sample : gc/ms scan 3/11 fb
Misc :
MS Integration Params: LSCINT.P


Vial: 14
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 N-Ethylformamide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.13	3.33 ug/l	503724	1,4-Dichlorobenzene-d4	12.25

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		N-Ethylformamide	73	C3H7NO	000627-45-2	9
2		Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
3		Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	9
4		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	9

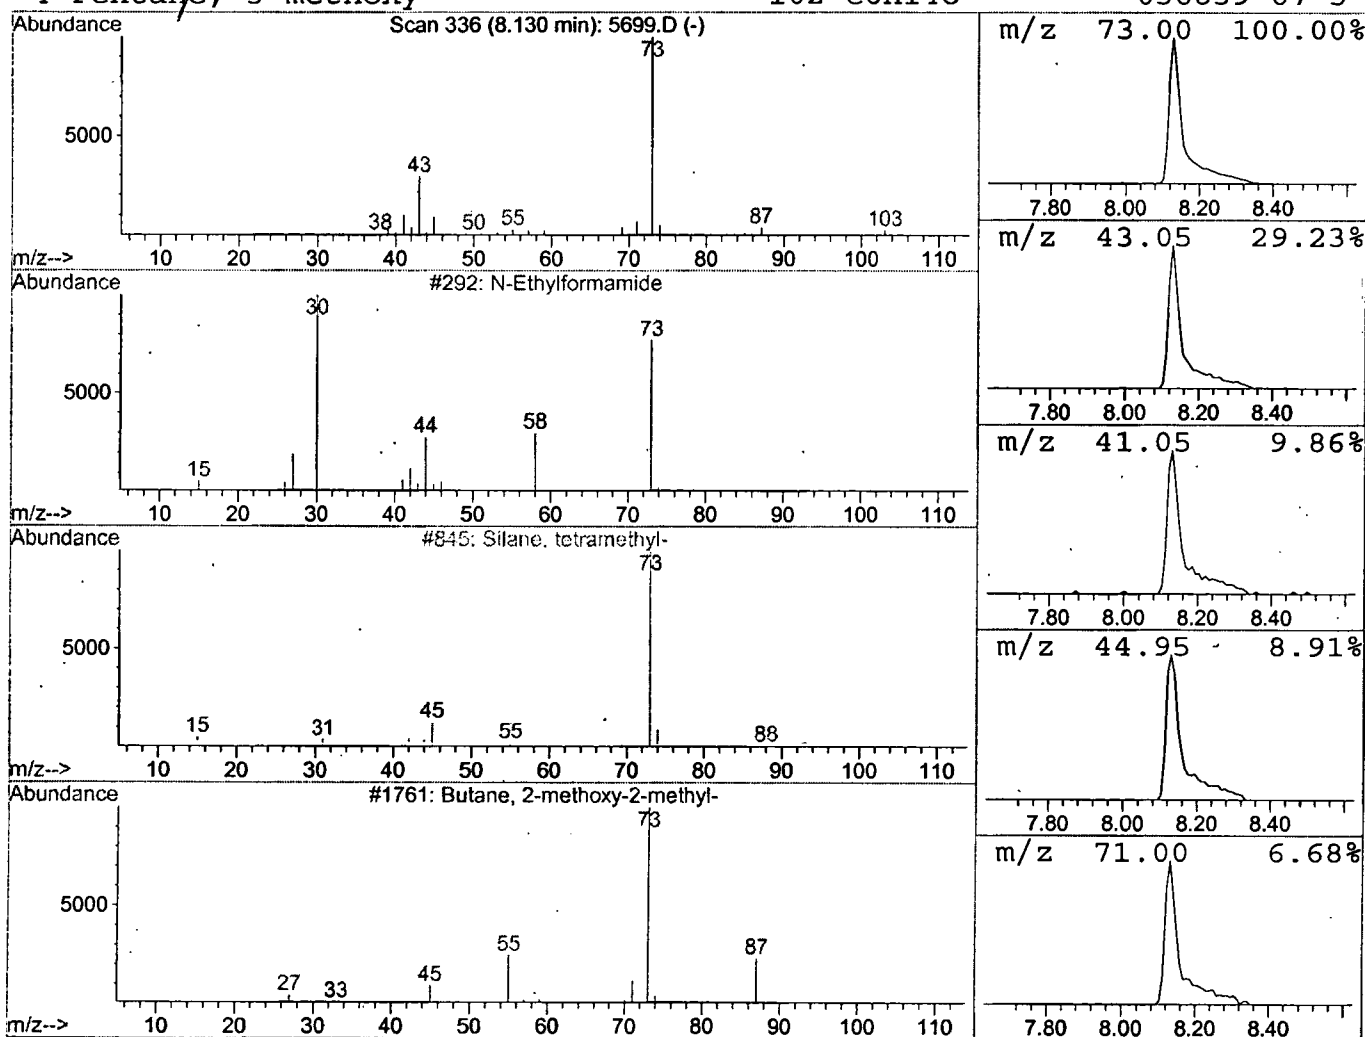

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 2 Apr 2002 1:08 am
 Data File: C:\HPCHEM\1\DATA\APR0102\5699.D
 Name: gc/ms scan 3/11 fb
 Misc:
 Method: C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
 Title: 209 625/TCLP calibration table
 Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
N-Ethylformamide	8.13	3.3	ug/l	503724	ISTD01	12.25	3028840	20.0

5699.D GCMS0403.M Thu Apr 04 13:59:17 2002