

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/09/2002 Time: 15:55:22

Sample: AE05698
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/9/02 15:54 Ended: 4/9/02 15:54 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds				
2	Surr_2,4-DDD		102		5.0

Comments for Sample AE05698 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-09-2002 Time: 15:55:27

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR0102\5698.D
 Acq On : 2 Apr 2002 12:09 am
 Sample : gc/ms scan 3/11
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 2 0:58 2002

Vial: 13
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Fri Mar 29 10:31:28 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0308

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.25	152	521182	20.00	ug/l	-0.10
10) Naphthalene-d8	15.88	136	1916799	20.00	ug/l	-0.11
17) Acenaphthene-d10	21.19	164	1083565	20.00	ug/l	-0.12
29) Phenanthrene-d10	25.63	188	1506884	20.00	ug/l	-0.13
38) Chrysene-d12	33.69	240	779520	20.00	ug/l	-0.15
44) Perylene-d12	37.94	264	444238	20.00	ug/l	-0.19

System Monitoring Compounds

37) 2,4-DDD	30.71	235	77289	5.11	ug/mL	0.21
Spiked Amount	5.000		Recovery	=	102.20%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	15.94	128	319	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.
25) Diethylphthalate	22.68	149	256	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#) = qualifier out of range (m) = manual integration

5698.D GCMS0403.M Thu Apr 04 13:00:37 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR0102\5698.D

Vial: 13

Acq On : 2 Apr 2002 12:09 am

Operator:

Sample : gc/ms scan 3/11

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Apr 2 0:58 2002

Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Mar 29 10:31:28 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0308

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.63	178	366	N.D.		
34) Anthracene	25.63	178	366	N.D.		
35) Di-n-butylphthalate	27.60	149	15450	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	32.40	149	325	N.D.		
41) Benzo(a)anthracene	33.70	228	1837	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.91	149	51916	1.67 ug/l		97
43) Chrysene	33.70	228	1837	N.D.		
45) Di-n-Octylphthalate	35.67	149	9516	N.D.		
46) Benzo(b)fluoranthene	0.00	252	0	N.D.		
47) Benzo(k)fluoranthene	0.00	252	0	N.D.		
48) Benzo(a)pyrene	37.94	252	1847	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenzo(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

5698.D GCMS0403.M Thu Apr 04 13:00:40 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR0102\5698.D
 Acq On : 2 Apr 2002 12:09 am
 Sample : gc/ms scan 3/11
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 2 0:58 2002

Vial: 13
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Results File: GCMS0308.RES

Method : C:\HPCHEM\1\METHODS\GCMS0403.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Thu Apr 04 09:06:35 2002
 Response via : Initial Calibration

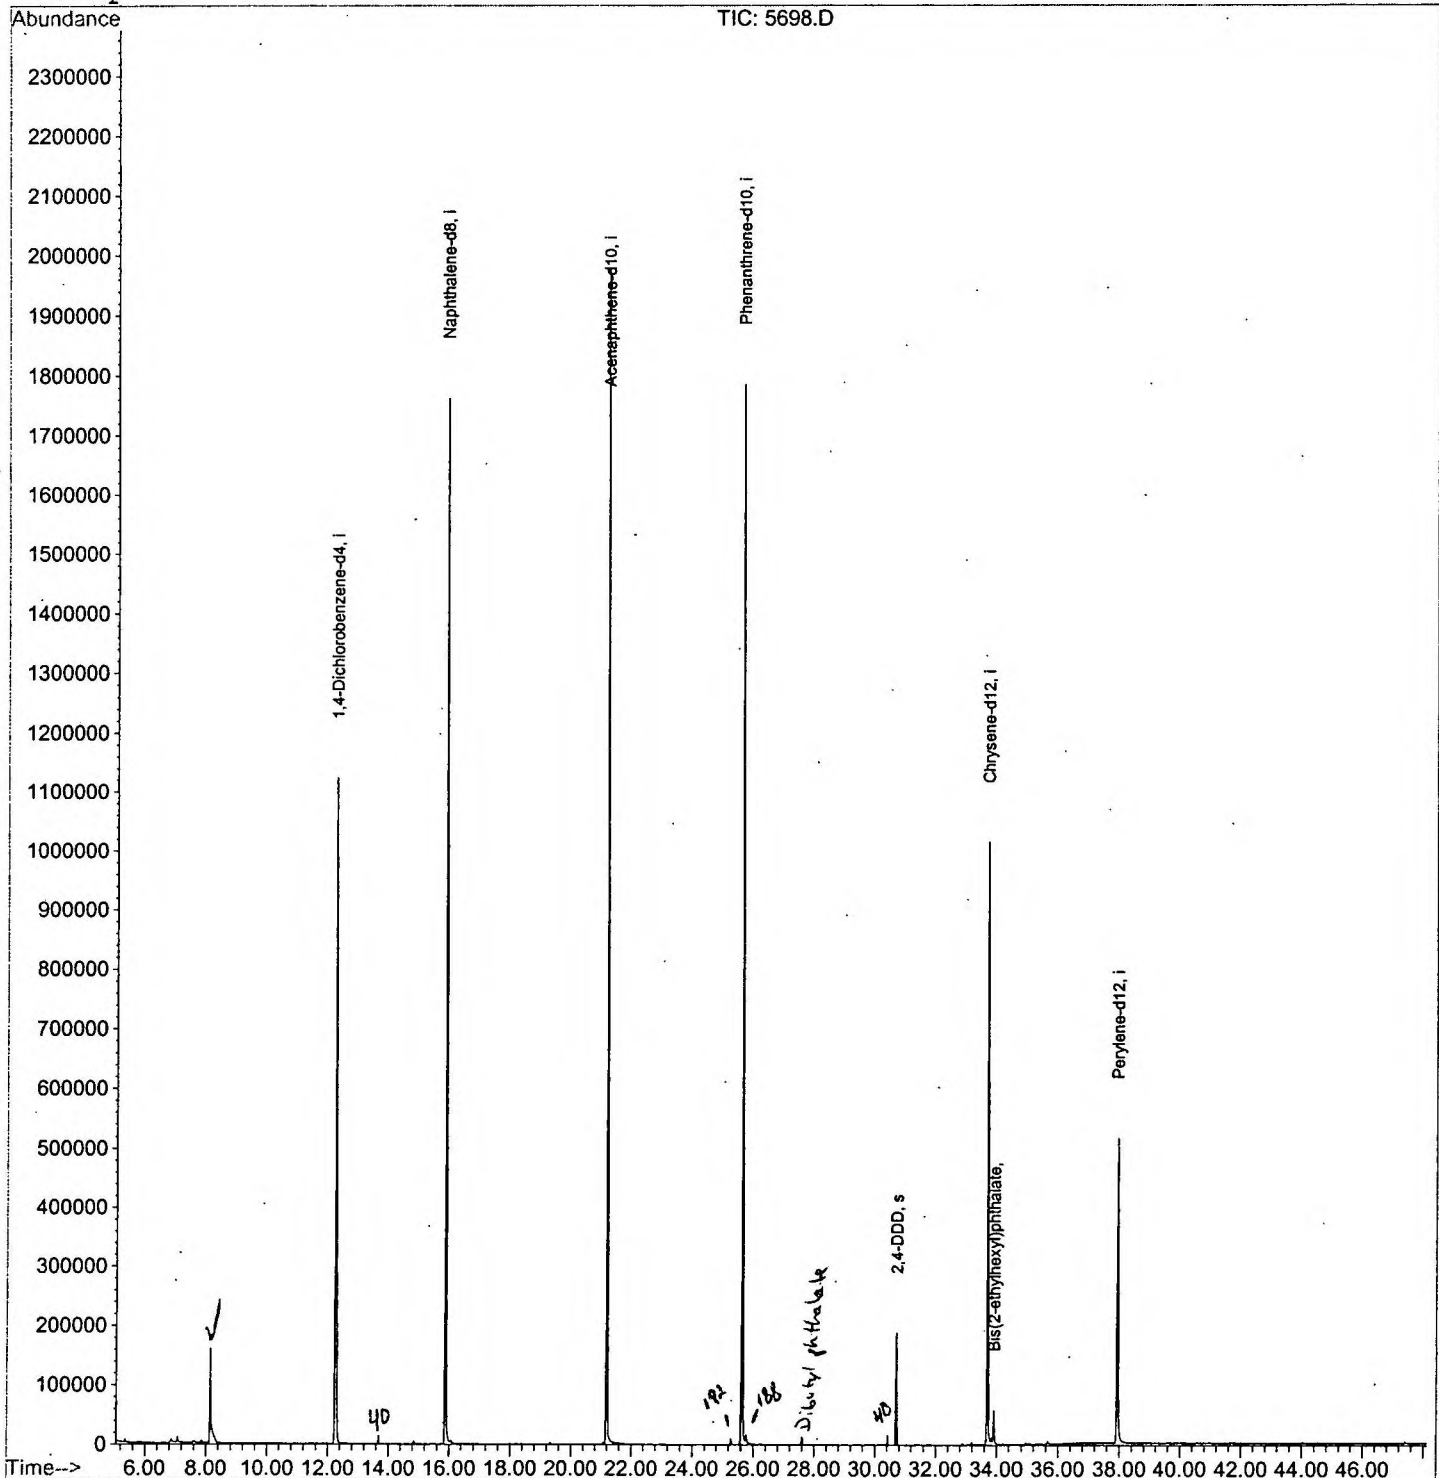

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR0102\5698.D
Acq On : 2 Apr 2002 12:09 am
Sample : gc/ms scan 3/11
Misc :
MS Integration Params: LSCINT.P

Vial: 13
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0403.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Signal : TIC


peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.127	332	336	365	rVB	159156	463486	11.23%	2.429%
2	12.249	779	785	802	rBV	1122362	2830406	68.57%	14.833%
3	15.885	1175	1181	1198	rBV	1761183	3620513	87.71%	18.973%
4	21.191	1752	1759	1772	rBV	1979399	4127917	100.00%	21.632%
5	25.634	2236	2243	2254	rBV2	1783930	3759281	91.07%	19.700%
6	30.711	2791	2796	2801	rBV	188547	380386	9.21%	1.993%
7	33.695	3114	3121	3132	rBV2	1015551	2253269	54.59%	11.808%
8	33.906	3140	3144	3156	rVB	56051	130582	3.16%	0.684%
9	37.936	3574	3583	3601	rBV2	513596	1516612	36.74%	7.948%

Sum of corrected areas: 19082452

5698.D GCMS0403.M Thu Apr 04 13:58:27 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR0102\5698.D
Operator :
Acquired : 2 Apr 2002 12:09 am using AcqMethod GCMS0308
Instrument : GC/MS 209
Sample Name: gc/ms scan 3/11
Misc Info :
Vial Number: 13
Quant File :GCMS0308.RES (RTE Integrator)

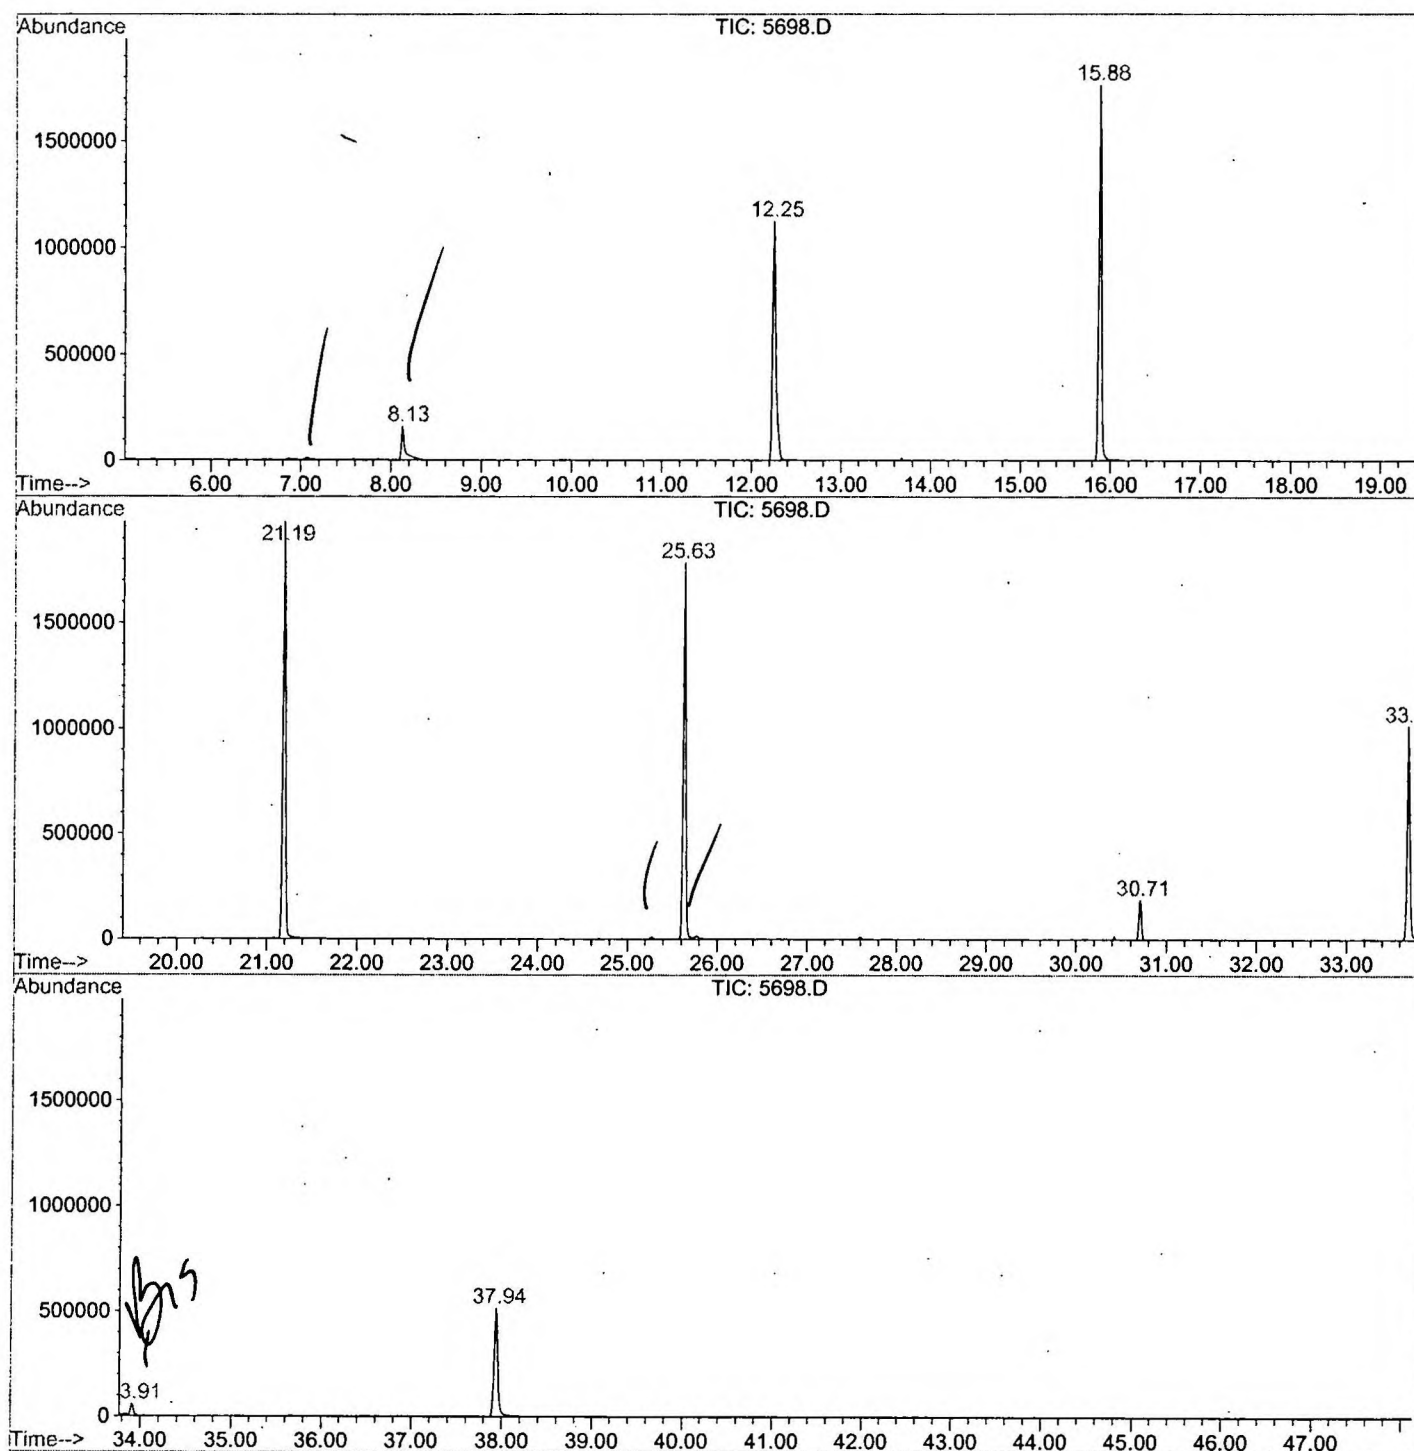

5698.D GCMS0403.M

Thu Apr 04 13:58:32 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR0102\5698.D
 Acq On : 2 Apr 2002 12:09 am
 Sample : gc/ms scan 3/11
 Misc :
 MS Integration Params: LSCINT.P


Vial: 13
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Library : C:\DATABASE\NBS75K.L

 Peak Number 1 Silane, tetramethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.13	3.28 ug/l	463486	1,4-Dichlorobenzene-d4	12.25

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
2			1,3-Dioxolane, 2-pentadecyl-	284	C18H36O2	004360-57-0	9
3			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	9
4			1-Butanamine, 3-methyl-	87	C5H13N	000107-85-7	7

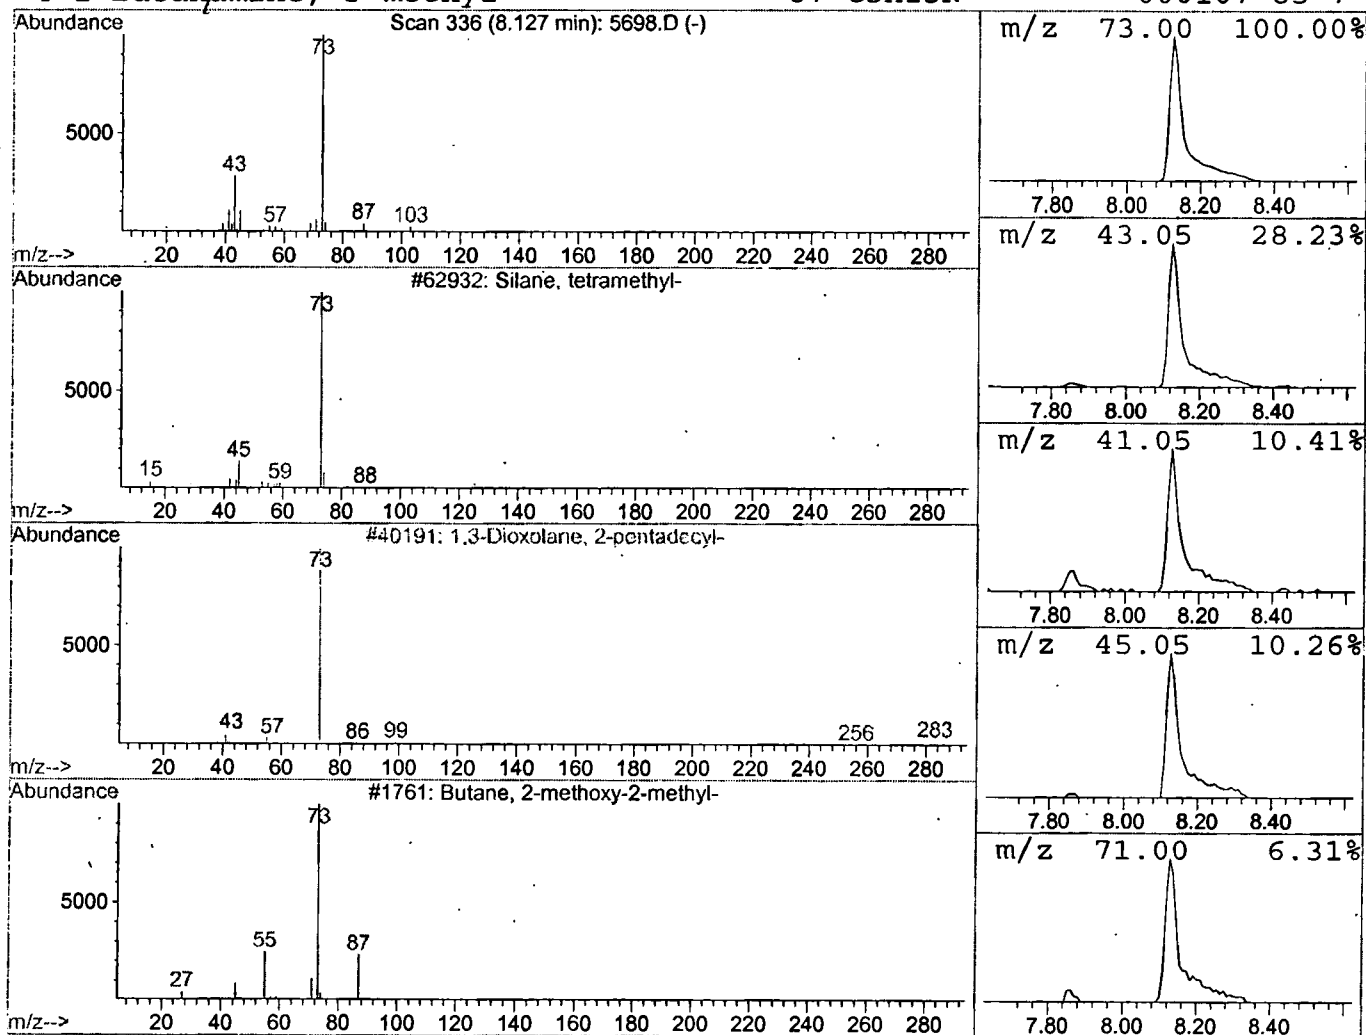

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 2 Apr 2002 12:09 am
Data File: C:\HPCHEM\1\DATA\APR0102\5698.D
Name: gc/ms scan 3/11
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
Silane, tetramethyl-	8.13	3.3	ug/l	463486	ISTD01	12.25	2830410	20.0

5698.D GCMS0403.M Thu Apr 04 13:58:41 2002