

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/11/2002 Time: 08:34:40

Sample: AE05744
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/11/02 08:34 Ended: 4/11/02 08:34 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		105		5.0

Comments for Sample AE05744 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-11-2002 Time: 08:35:12

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recovery for 1 of the 43 compounds in the LCS Standard was low.

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR0102\5744.D

Vial: 23

Acq On : 2 Apr 2002 11:00 pm

Operator:

Sample : gc/ms scan 3/12

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Apr 2 23:48 2002

Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Mar 29 10:31:28 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0308

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	12.25	152	555819	20.00	ug/l	-0.11
10) Naphthalene-d8	15.88	136	2073261	20.00	ug/l	-0.12
17) Acenaphthene-d10	21.19	164	1158879	20.00	ug/l	-0.13
29) Phenanthrene-d10	25.63	188	1651285	20.00	ug/l	-0.14
38) Chrysene-d12	33.69	240	826652	20.00	ug/l	-0.15
44) Perylene-d12	37.93	264	459684	20.00	ug/l	-0.19

System Monitoring Compounds

37) 2,4-DDD	30.71	235	86808	5.24	ug/mL	0.21
Spiked Amount	5.000		Recovery	=	104.80%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	15.94	128	254	N.D.
16) Hexachlorobutadiene	0.00	225	0	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	21.48	165	101	N.D.
25) Diethylphthalate	22.67	149	695	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.

(#)= qualifier out of range (m) = manual integration

5744.D GCMS0403.M

Fri Apr 05 10:23:08 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR0102\5744.D

Vial: 23

Acq On : 2 Apr 2002 11:00 pm

Operator:

Sample : gc/ms scan 3/12

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Apr 2 23:48 2002

Quant Results File: GCMS0308.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Fri Mar 29 10:31:28 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0308

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) N-Nitrosodiphenylamine	0.00	168	0	N.D.		
31) 4-Bromophenyl-phenylether	0.00	248	0	N.D.		
32) Hexachlorobenzene	0.00	284	0	N.D.		
33) Phenanthrene	25.63	178	670	N.D.		
34) Anthracene	25.63	178	670	N.D.		
35) Di-n-butylphthalate	27.60	149	17158	N.D.		
36) Fluoranthene	0.00	202	0	N.D.		
39) Pyrene	0.00	202	0	N.D.		
40) Butylbenzylphthalate	0.00	149	0	N.D.		
41) Benzo(a)anthracene	33.70	228	1679	N.D.		
42) Bis(2-ethylhexyl)phthalate	33.90	149	4474	N.D.		
43) Chrysene	33.70	228	1679	N.D.		
45) Di-n-Octylphthalate	35.65	149	549	N.D.		
46) Benzo(b)fluoranthene	36.76	252	1063	N.D.		
47) Benzo(k)fluoranthene	36.82	252	1154	N.D.		
48) Benzo(a)pyrene	37.73	252	557	N.D.		
49) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.		
50) Dibenz(a,h)anthracene	0.00	278	0	N.D.		
51) Benzo(g,h,i)perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

5744.D GCMS0403.M

Fri Apr 05 10:23:11 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR0102\5744.D
Acq On : 2 Apr 2002 11:00 pm
Sample : gc/ms scan 3/12
Misc :
MS Integration Params: GOOFY.P
Quant Time: Apr 2 23:48 2002

Vial: 23
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Results File: GCMS0308.RES

Method : C:\HPCHEM\1\METHODS\GCMS0403.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Fri Apr 05 08:33:02 2002
Response via : Initial Calibration

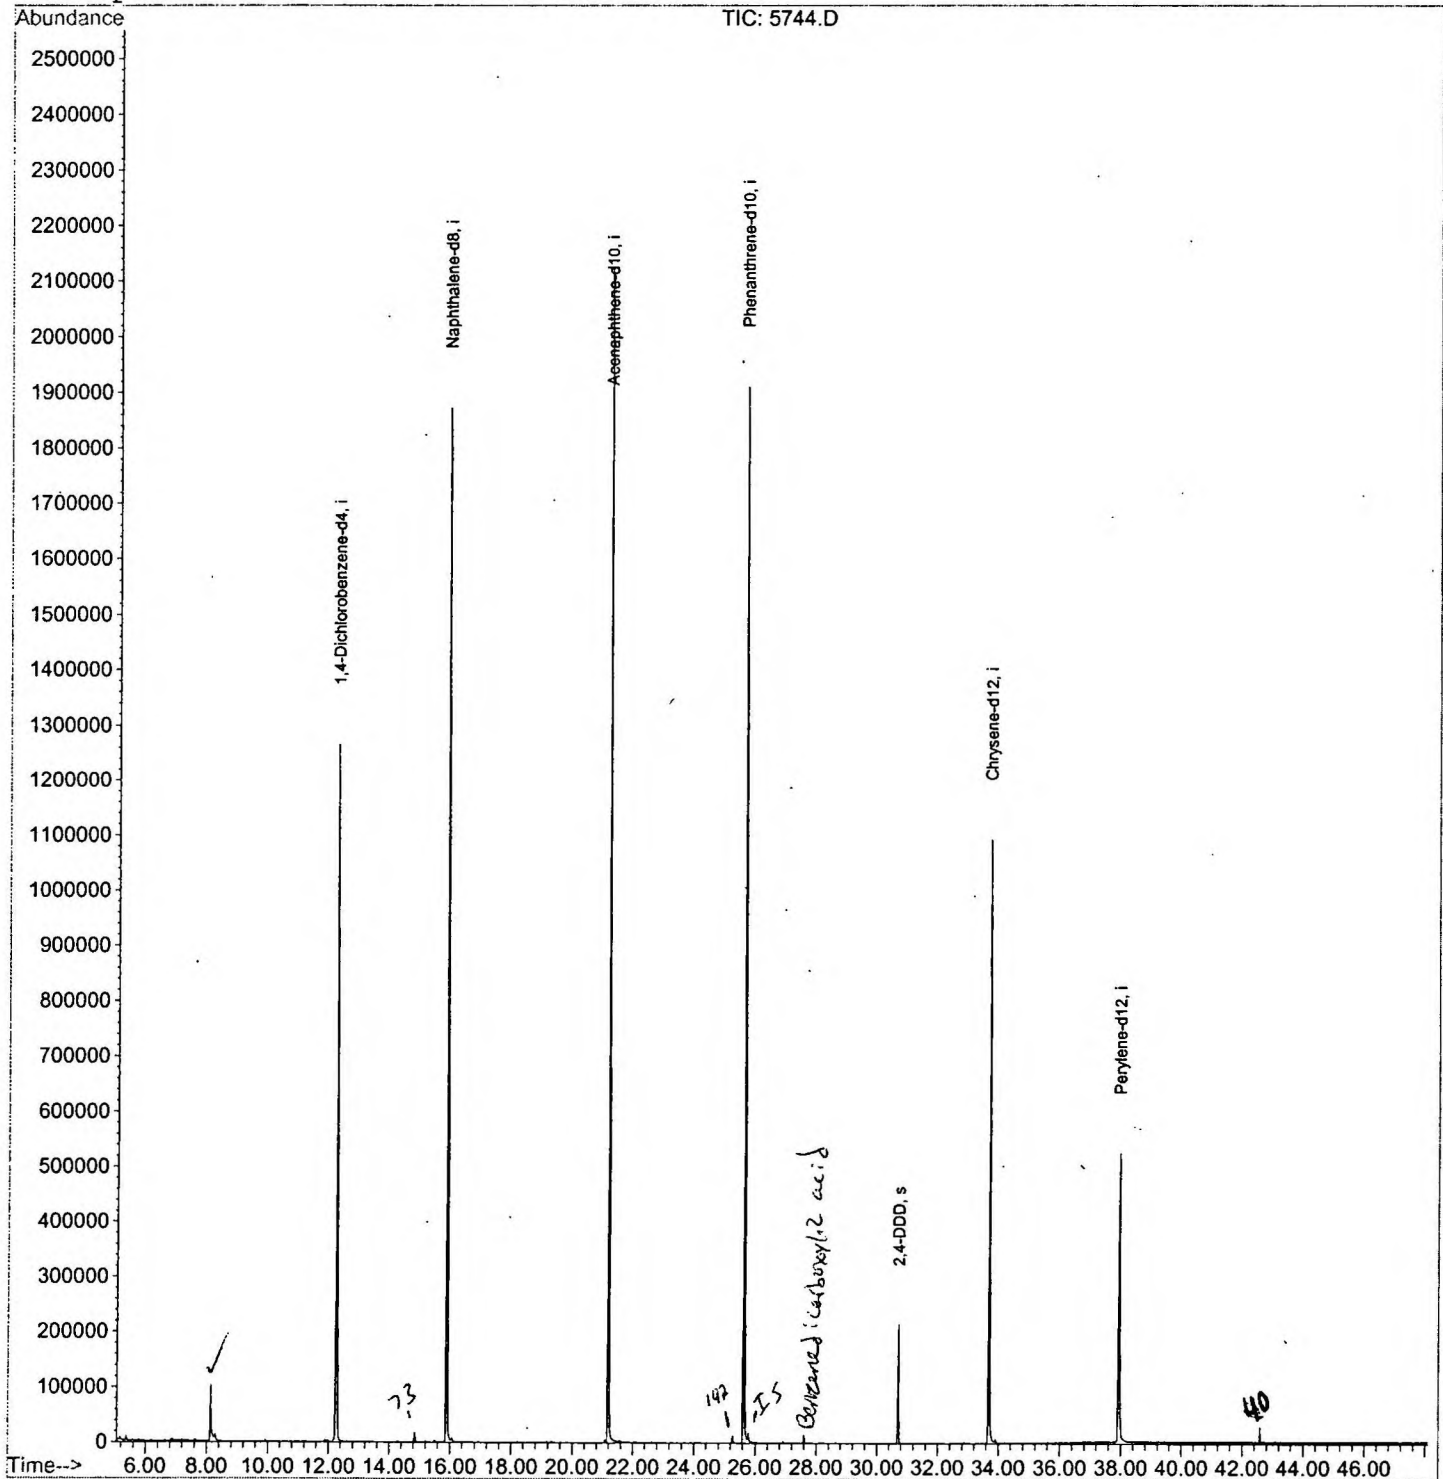

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR0102\5744.D

Vial: 23

Acq On : 2 Apr 2002 11:00 pm

Operator:

Sample : gc/ms scan 3/12

Inst : GC/MS 209

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\HPCHEM\1\METHODS\GCMS0403.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	8.133	331	336	349	rBV	101322	260866	5.86%	1.291%
2	12.246	779	784	802	rVB	1263314	3008470	67.62%	14.883%
3	15.881	1174	1180	1195	rBV	1872435	3925341	88.22%	19.419%
4	21.187	1752	1758	1773	rBV	2125420	4449339	100.00%	22.011%
5	25.631	2235	2242	2253	rBV2	1910455	4170873	93.74%	20.634%
6	30.707	2790	2795	2802	rVB	213775	421829	9.48%	2.087%
7	33.691	3113	3120	3135	rBV2	1093534	2401017	53.96%	11.878%
8	37.932	3574	3582	3604	rBV2	522499	1576081	35.42%	7.797%


Sum of corrected areas: 20213816

5744.D GCMS0403.M

Fri Apr 05 10:36:47 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR0102\5744.D
 Operator :
 Acquired : 2 Apr 2002 11:00 pm using AcqMethod GCMS0308
 Instrument : GC/MS 209
 Sample Name: gc/ms scan 3/12
 Misc Info :
 Vial Number: 23
 Quant File :GCMS0308.RES (RTE Integrator)

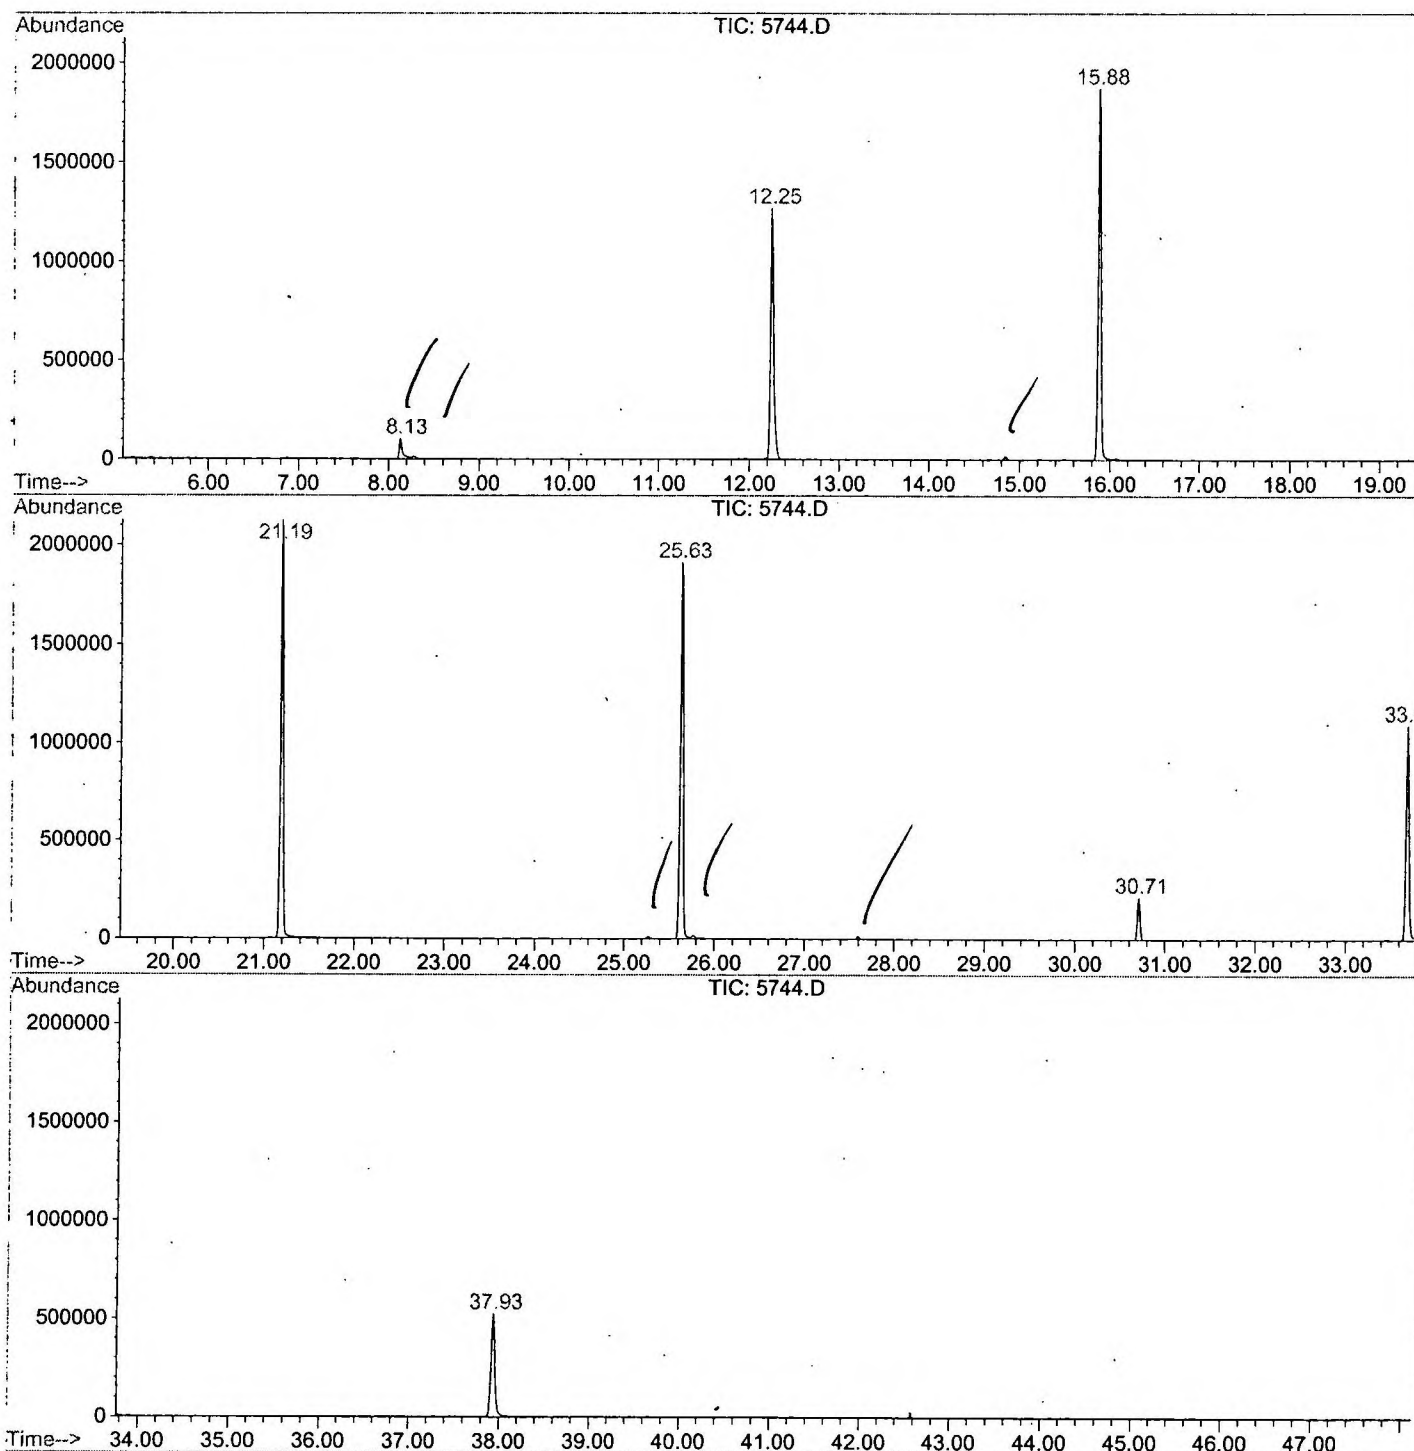

5744.D GCMS0403.M

Fri Apr 05 10:36:53 2002

Library Search Compound Report

Data File : C:\HPCHEM\1\DATA\APR0102\5744.D
Acq On : 2 Apr 2002 11:00 pm
Sample : gc/ms scan 3/12
Misc :
MS Integration Params: LSCINT.P










Vial: 23
Operator:
Inst : GC/MS 209
Multiplr: 1.00

Quant Method : C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Library : C:\DATABASE\NBS75K.L

Peak Number 1 N-Ethylformamide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.13	1.73 ug/l	260866	1,4-Dichlorobenzene-d4	12.25

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			N-Ethylformamide	73	C3H7NO	000627-45-2	9
2			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
3			1,3-Dioxolane, 2-(3-bromo-5,5,5-tri	352	C10H16BrCl3O2	000000-00-0	9
4			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	9

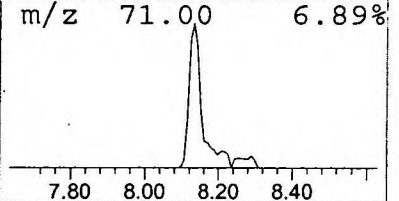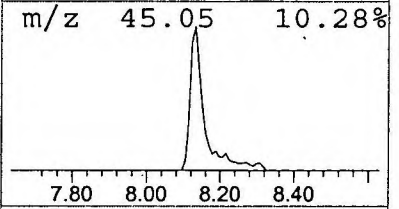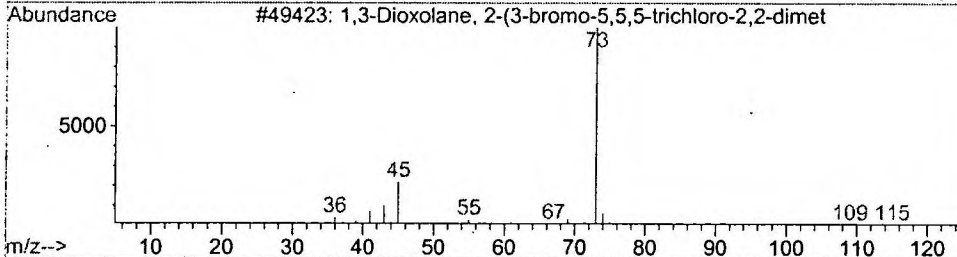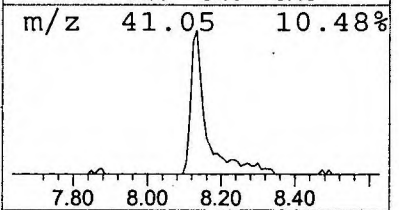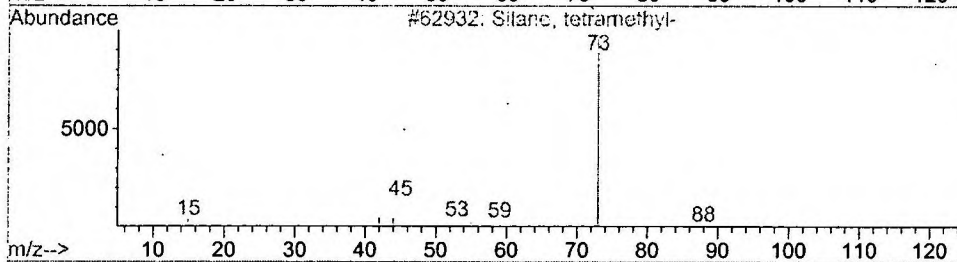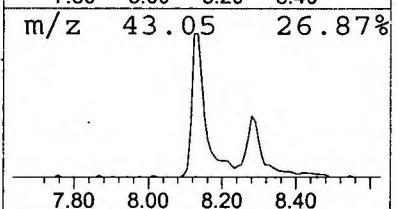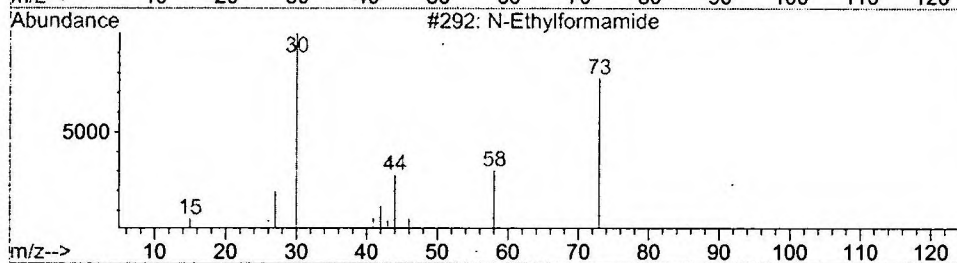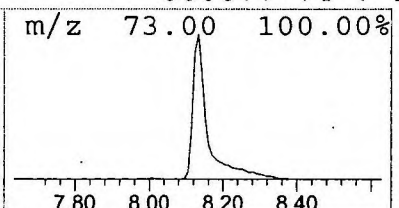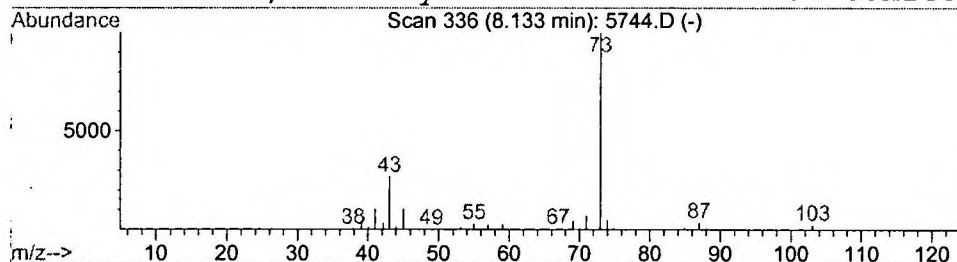

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 2 Apr 2002 11:00 pm
Data File: C:\HPCHEM\1\DATA\APR0102\5744.D
Name: gc/ms scan 3/12
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0308.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
N-Ethylformamide	8.13	1.7	ug/l	260866	ISTD01	12.25	3008470	20.0

5744.D GCMS0403.M Fri Apr 05 10:37:01 2002