

Method 508 mod.

Date Extracted 3/12/02

Page 147

GCMS - 17879

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count	Notes
1B		500ml		1ml			1ml	3A	7		
Ref,					1ml			1B			
Ref,					↓			1A			
5750	See 4/10							9A			
5844	See 4/10							7A			
5845	See 4/17							2B			
5846	See 4/10							10A			
5847								4A			
5848								8A			
5849								8B			
5850								9B			
5851								4B			
5852	See 4/11							7B			
5286	See 4/3	↓		↓			↓	10B	↓		✓
Remarks											
Reviewed by <u>CB 8/13/02</u>											
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate -											
Extraction type <u>Sep Fun</u> Solv. lot# <u>39466</u> NaCl lot# <u>V39618</u> Na2SO4 lot# <u>V46623</u>											
STANDARD	INT STD LOG#										
CALIBRATION	<u>HP040102</u>										
REF/SPIKE	<u>2193</u>										
MDL/MDRF											
Q. CHECK											
INT. STD.	<u>040302</u>										
SURROGATE	<u>GCMS 2160D</u>										
LPC											
ENDRIN/ODT											

Analyst EH/B.N.
revision 4/12/01

Verified by my

Reviewed by DN
Date 4/17/02

Sequence Name: C:\HPCHEM\1\SEQUENCE\APR0302.S

Comment:

Operator:

Data Path: C:\HPCHEM\1\DATA\apr03022\

Pre-Seq Cmd:

Post-Seq Cmd:

Method Sections To Run

☒ Full Method☐ Reprocessing Only

On A Barcode Mismatch


☒ Inject Anyway☐ Don't Inject

Line	Type	Vial	DataFile	Method	Sample Name
1	Sample	1	DFTPP	GCMS0308	
2	Sample	2	CAL40	GCMS0403	
3	Sample	3	LB	GCMS0403	gc/ms scan 3/28
4	Sample	27	SURR	GCMS0403	
5	Sample	4	REF1	GCMS0403	gc/ms scan 3/28
6	Sample	5	REF2	GCMS0403	gc/ms scan 3/28
7	Sample	6	1965	GCMS0403	re-extract
8	Sample	7	7311	GCMS0403	gc/ms scan 3/28
9	Sample	8	7312	GCMS0403	gc/ms scan 3/28
10	Sample	9	7313	GCMS0403	gc/ms scan 3/28
11	Sample	10	7314	GCMS0403	gc/ms scan 3/28
12	Sample	11	7315	GCMS0403	gc/ms scan 3/28
13	Sample	12	7316	GCMS0403	gc/ms scan 3/28
14	Sample	13	7317	GCMS0403	gc/ms scan 3/28
15	Sample	14	7318	GCMS0403	gc/ms scan 3/28 fb
16	Sample	1	DFTPP2	GCMS0403	
17	Sample	2	CAL40A	GCMS0403	
18	Sample	28	LBB	GCMS0403	gc/ms scan 2/14
19	Sample	29	REFA1	GCMS0403	gc/ms scan 2/14
20	Sample	30	REFA2	GCMS0403	gc/ms scan 2/14
21	Sample	31	3391	GCMS0403	gc/ms scan 2/14
22	Sample	15	LBA	GCMS0403	gc/ms scan 3/12
23	Sample	32	SURR2	GCMS0403	
24	Sample	16	REFA	GCMS0403	gc/ms scan 3/12
25	Sample	17	5750	GCMS0403	gc/ms scan 3/12
26	Sample	18	5844	GCMS0403	gc/ms scan 3/12
27	Sample	19	5845	GCMS0403	gc/ms scan 3/12
28	Sample	33	NEWSURR	GCMS0403	
29	Sample	20	5846	GCMS0403	gc/ms scan 3/12
30	Sample	21	5847	GCMS0403	gc/ms scan 3/12
31	Sample	22	5848	GCMS0403	gc/ms scan 3/12
32	Sample	23	5849	GCMS0403	gc/ms scan 3/12
33	Sample	24	5850	GCMS0403	gc/ms scan 3/12
34	Sample	25	5851	GCMS0403	gc/ms scan 3/12
35	Sample	26	5852	GCMS0403	gc/ms scan 3/12

DFTPP

Data File : C:\HPCHEM\1\DATA\APR0302\DFTPP2.D
 Acq On : 4 Apr 2002 2:32 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0408.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : GC/MS 209
 Multiplr: 1.00

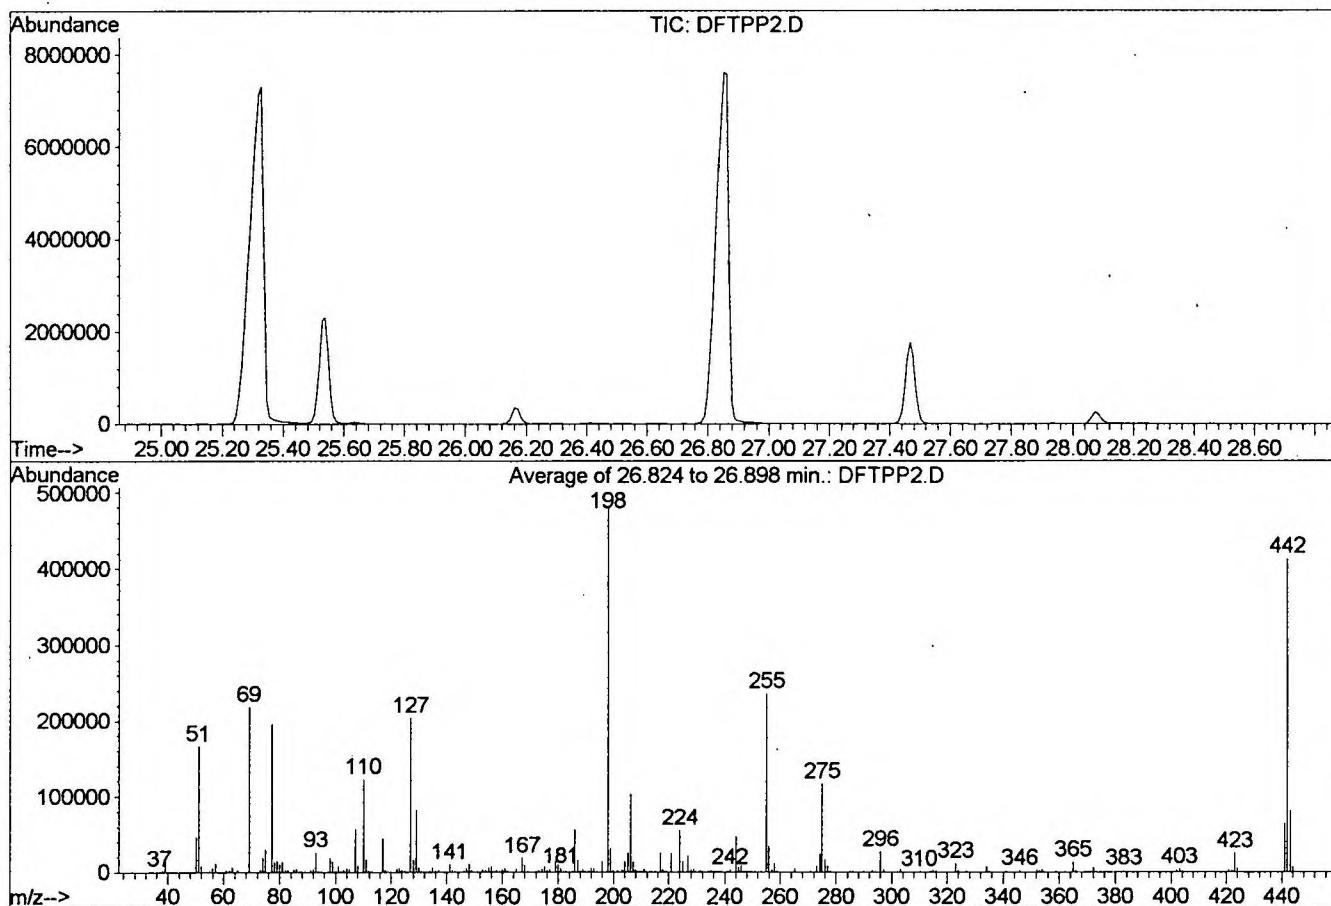

Spectrum Information: Average of 26.824 to 26.898 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	34.6	166638	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.4	218854	PASS
70	69	0.00	2	0.0	19	PASS
127	198	40	60	42.4	204368	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	482291	PASS
199	198	5	9	6.6	31887	PASS
275	198	10	30	24.5	118099	PASS
365	198	1	100	2.7	13202	PASS
441	443	0.01	100	79.4	63817	PASS
442	198	40	110	85.8	413568	PASS
443	442	17	23	19.4	80373	PASS