

User: Fakhouri, Morgan
 Westchester Dept. of Labs & Research
 Date: 04/05/2002 Time: 12:00:59

Sample: AE05914
 Analysis: \$B1GCMS Blank for GCMS Scan
 Units: ug
 Started: 4/5/02 11:58 Ended: 4/5/02 11:58 Analyst: MF
 Result source: manual entry
 Page: 1

	Component Name	Viol.	Result	Qualifier	MDL
1	n-Nitrosodimethylamine		< MDL		2.0
2	bis(2-Chloroethyl)ether		< MDL		2.0
3	1,3-Dichlorobenzene		< MDL		2.0
4	1,4-Dichlorobenzene		< MDL		2.0
5	1,2-Dichlorobenzene		< MDL		2.0
6	2,2'-oxybis(1-Chloropropane)		< MDL		2.0
7	n-Nitrosodi-n-propylamine		< MDL		2.0
8	Hexachloroethane		< MDL		2.0
9	Nitrobenzene		< MDL		2.0
10	Isophorone		< MDL		2.0
11	bis(2-Chloroethoxy)methane		< MDL		2.0
12	1,2,4-Trichlorobenzene		< MDL		2.0
13	Naphthalene		< MDL		2.0
14	Hexachlorobutadiene		< MDL		2.0
15	2-Chloronaphthalene		< MDL		2.0
16	Dimethylphthalate		< MDL		2.0
17	2,6-Dinitrotoluene		< MDL		2.0
18	Acenaphthylene		< MDL		2.0
19	Acenaphthene		< MDL		2.0
20	2,4-Dinitrotoluene		< MDL		2.0
21	Diethylphthalate		< MDL		2.0
22	4-Chlorophenylphenylether		< MDL		2.0
23	Fluorene		< MDL		2.0
24	Azobenzene/1,2-Diphenylhydraz		< MDL		2.0
25	n-Nitrosodiphenylamine		< MDL		2.0
26	4-Bromophenylphenylether		< MDL		2.0
27	Hexachlorobenzene		< MDL		2.0
28	Phenanthrene		< MDL		2.0
29	Anthracene		< MDL		2.0
30	Di-n-butylphthalate		< MDL		2.0
31	Fluoranthene		< MDL		2.0
32	Pyrene		< MDL		2.0
33	Butylbenzylphthalate		< MDL		2.0
34	Benzo(a)anthracene		< MDL		2.0
35	bis(2-Ethylhexyl)phthalate		< MDL		2.0
36	Chrysene		< MDL		2.0
37	Di-n-octylphthalate		< MDL		2.0
38	Benzo(b)fluoranthene		< MDL		2.0
39	Benzo(k)fluoranthene		< MDL		2.0
40	Benzo(a)pyrene		< MDL		2.0
41	Indeno(1,2,3-cd)pyrene		< MDL		2.0
42	Dibenz(a,h)anthracene		< MDL		2.0
43	Benzo(g,h,i)perylene		< MDL		2.0

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\032202\LBJ0322.D

Acq On : 22 Mar 2002 10:39 pm

Sample : LB 3/14/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 05 07:41:05 2002

Vial: 5

Operator: McLean

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080302.RES

Quant Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Wed Mar 27 06:57:36 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	9.55	150	1303695	20.00	ug/L	0.00
10) Naphthalene-d8	13.03	136	3717282	20.00	ug/L	0.00
17) Acenaphthene-d10	18.14	164	2110975	20.00	ug/L	0.00
29) Phenanthrene-d10	22.50	188	3183980	20.00	ug/L	0.00
38) Chrysene-d12	30.31	240	2507072	20.00	ug/L	-0.02
44) Perylene-d12	34.18	264	1121428	20.00	ug/L	0.00

System Monitoring Compounds

37) 2,4-DDD (SURR)	27.43	235	180853	4.76	ug/L	0.00
Spiked Amount	5.000		Recovery	=	95.20%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
30) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
31) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
32) Hexachlorobenzene	0.00	284	0	N.D.	
33) Phenanthrene	0.00	178	0	N.D.	
34) Anthracene	0.00	178	0	N.D.	
35) Di-n-butylphthalate	24.64	149	3820	N.D.	
36) Fluoranthene	0.00	202	0	N.D.	
39) Pyrene	0.00	202	0	N.D.	
40) Butylbenzylphthalate	0.00	149	0	N.D.	
41) Benzo (a) anthracene	30.31	228	6182	N.D.	
42) Bis (2-ethylhexyl) phthala	0.00	149	0	N.D.	
43) Chrysene	30.31	228	6182	N.D.	
45) Di-n-Octylphthalate	0.00	149	0	N.D.	
46) Benzo (b) fluoranthene	0.00	252	0	N.D.	

(#) = qualifier out of range (m) = manual integration

LBJ0322.D 5080302.M

Fri Apr 05 07:41:25 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\032202\LBJ0322.D Vial: 5
Acq On : 22 Mar 2002 10:39 pm Operator: McLean
Sample : LB 3/14/02 Inst : Instrumen
Misc : Multiplr: 1.00
MS Integration Params: BENZO.P
Quant Time: Apr 05 07:41:05 2002 Quant Results File: 5080302.RES

Quant Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)
Title : Quantitation For Method 508gcscan
Last Update : Wed Mar 27 06:57:36 2002
Response via : Initial Calibration
DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
47) Benzo (k) fluoranthene	0.00	252	0	N.D.	
48) Benzo (a) pyrene	34.18	252	4239	N.D.	
49) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.	
50) Dibenz (a,h) anthracene	0.00	278	0	N.D.	
51) Benzo (g,h,i) perylene	0.00	276	0	N.D.	

(#) = qualifier out of range (m) = manual integration
LBJ0322.D 5080302.M Fri Apr 05 07:41:25 2002

Data File : C:\MSDCHEM\1\DATA\032202\LBJ0322.D

Vial: 5

Acq On : 22 Mar 2002 10:39 pm

Operator: McLean

Sample : LB 3/14/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 5 7:41 2002


Quant Results File: 5080302.RES

Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Wed Mar 27 06:57:36 2002

Response via : Initial Calibration

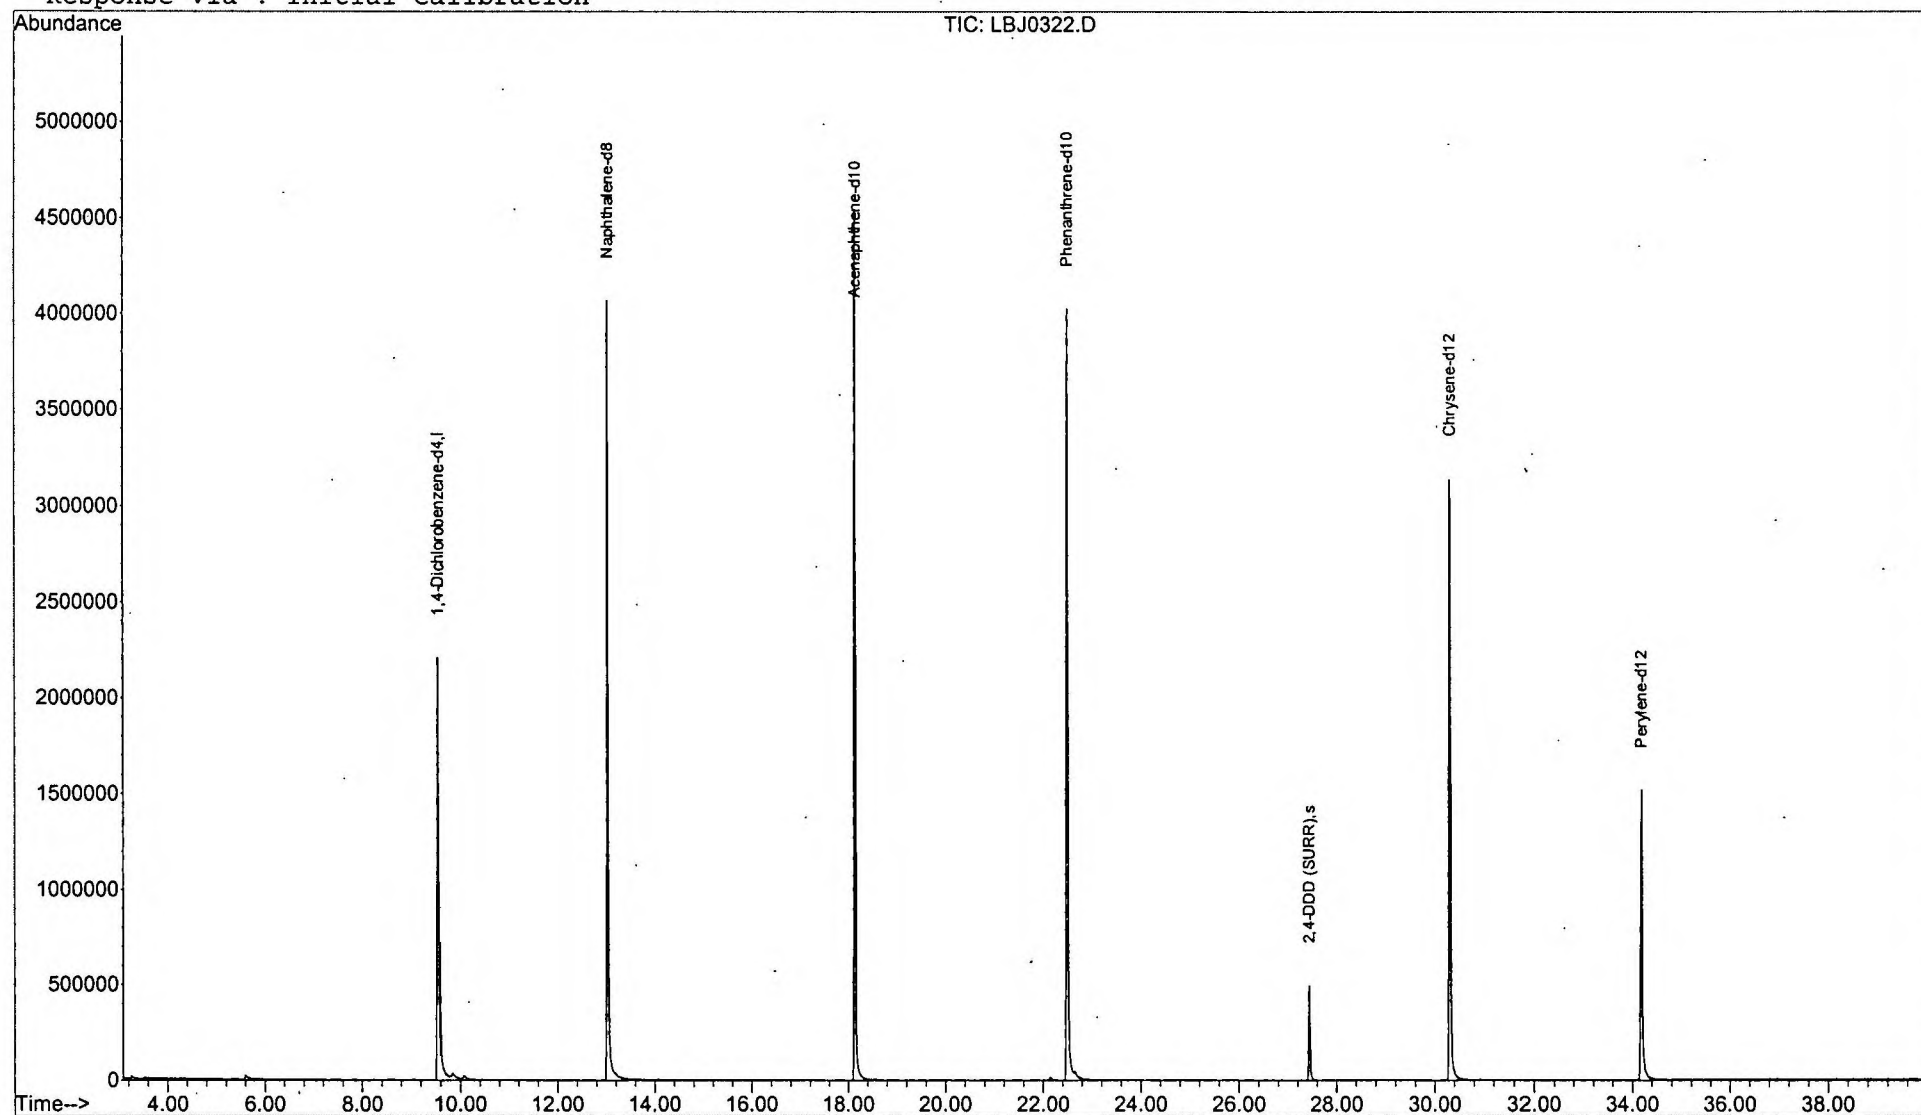

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\032202\LBJ0322.D
Acq On : 22 Mar 2002 10:39 pm
Sample : LB 3/14/02
Misc :
MS Integration Params: LSCINT.P

Vial: 5
Operator: McLean
Inst : Instrumen
Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)
Title : Quantitation For Method 508gcscan
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.548	1094	1101	1126	rBV	2205827	5824559	63.71%	13.035%
2	13.027	1684	1693	1715	rBV	4067714	8320546	91.02%	18.620%
3	18.138	2551	2563	2591	rBV	4538451	9141755	100.00%	20.458%
4	22.498	3295	3305	3328	rBV2	4025895	9060258	99.11%	20.276%
5	22.651	3328	3331	3343	rVB3	34032	97970	1.07%	0.219%
6	27.434	4138	4145	4158	rBV2	491294	968724	10.60%	2.168%
7	30.307	4624	4634	4653	rBV2	3135129	7441128	81.40%	16.652%
8	34.179	5281	5293	5318	rBV	1513968	3830561	41.90%	8.572%

Sum of corrected areas: 44685501

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\032202\LBJ0322.D
 Operator : McLean
 Acquired : 22 Mar 2002 10:39 pm using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: LB 3/14/02
 Misc Info :
 Vial Number: 5
 Quant File :5080302.RES (RTE Integrator)

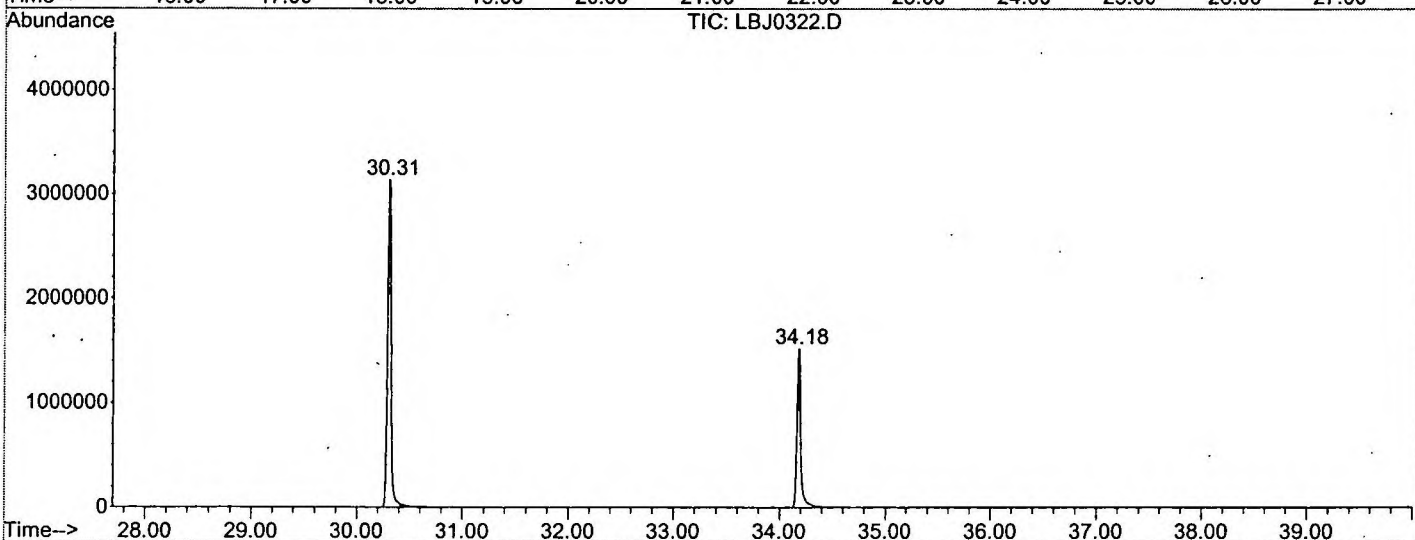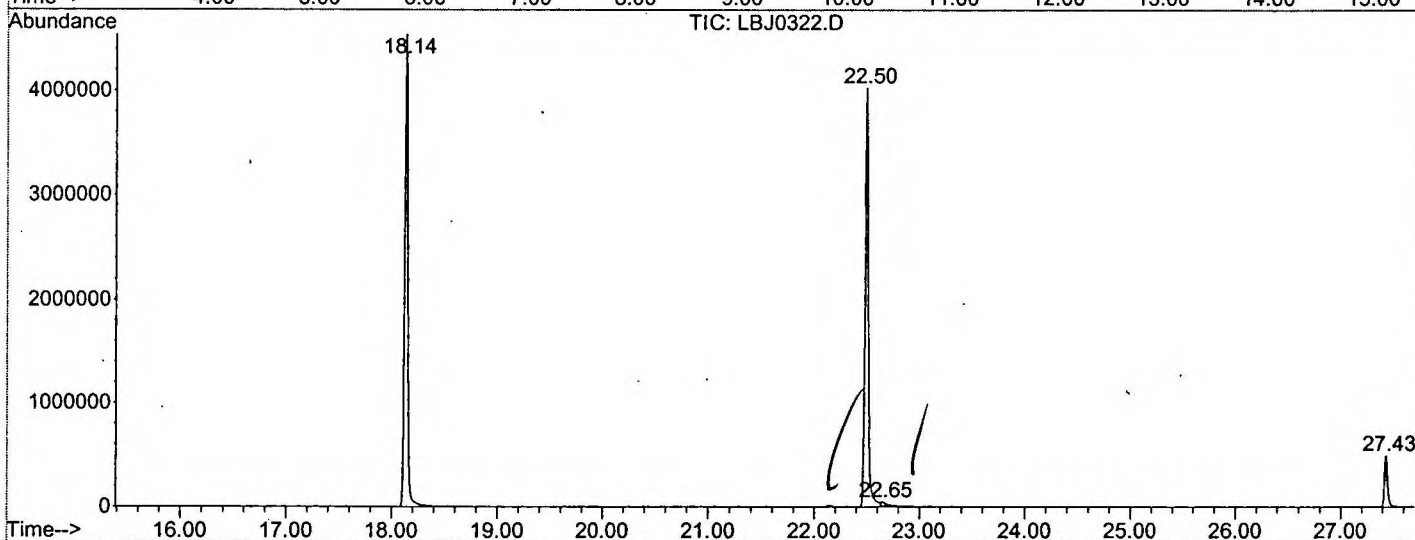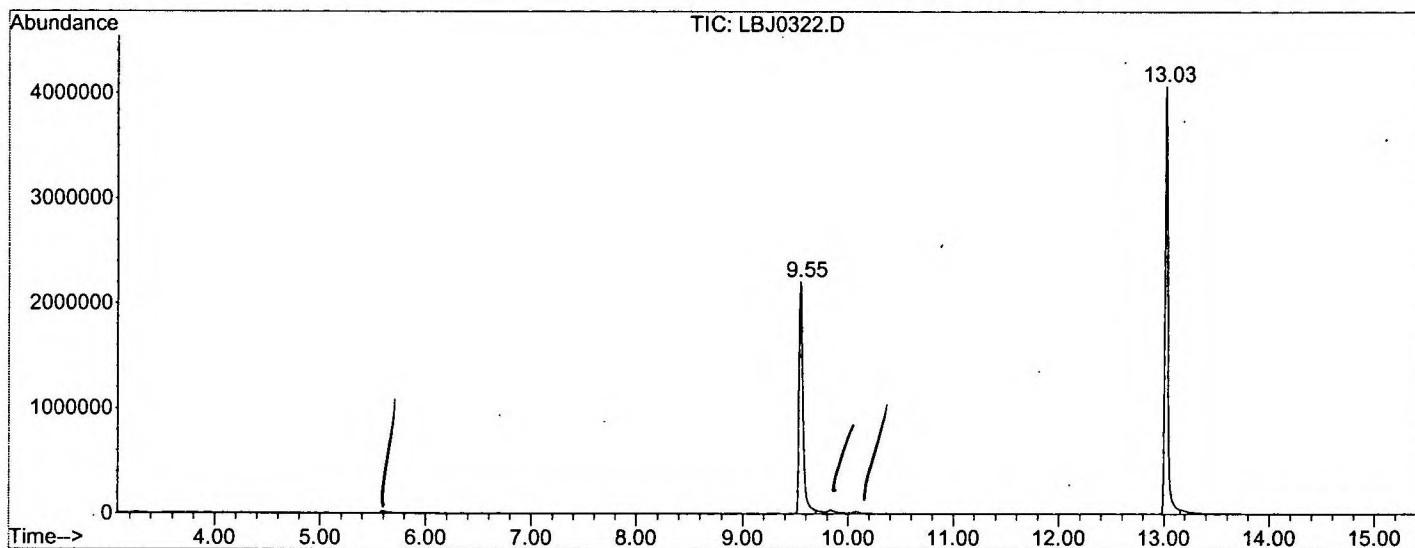

Tentatively Identified Compound (LSC) summary

Operator ID: McLean Date Acquired: 22 Mar 2002 10:39 pm
 Data File: C:\MSDCHEM\1\DATA\032202\LBJ0322.D
 Name: LB 3/14/02
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080302.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
