

User: Bohlk, Ted
 Westchester Dept. of Labs & Research
 Date: 04/08/2002 Time: 12:42:12

Sample: AE06090
 Analysis: \$B1GCMS Blank for GCMS Scan
 Units: ug
 Started: 3/15/02 12:34 Ended: 4/5/02 12:34 Analyst: TB
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	n-Nitrosodimethylamine		< MDL		2.0
2	bis(2-Chloroethyl)ether		< MDL		2.0
3	1,3-Dichlorobenzene		< MDL		2.0
4	1,4-Dichlorobenzene		< MDL		2.0
5	1,2-Dichlorobenzene		< MDL		2.0
6	2,2'-oxybis(1-Chloropropane)		< MDL		2.0
7	n-Nitrosodi-n-propylamine		< MDL		2.0
8	Hexachloroethane		< MDL		2.0
9	Nitrobenzene		< MDL		2.0
10	Isophorone		< MDL		2.0
11	bis(2-Chloroethoxy)methane		< MDL		2.0
12	1,2,4-Trichlorobenzene		< MDL		2.0
13	Naphthalene		< MDL		2.0
14	Hexachlorobutadiene		< MDL		2.0
15	2-Chloronaphthalene		< MDL		2.0
16	Dimethylphthalate		< MDL		2.0
17	2,6-Dinitrotoluene		< MDL		2.0
18	Acenaphthylene		< MDL		2.0
19	Acenaphthene		< MDL		2.0
20	2,4-Dinitrotoluene		< MDL		2.0
21	Diethylphthalate		< MDL		2.0
22	4-Chlorophenylphenylether		< MDL		2.0
23	Fluorene		< MDL		2.0
24	Azobenzene/1,2-Diphenylhydrazine		< MDL		2.0
25	n-Nitrosodiphenylamine		< MDL		2.0
26	4-Bromophenylphenylether		< MDL		2.0
27	Hexachlorobenzene		< MDL		2.0
28	Phenanthrene		< MDL		2.0
29	Anthracene		< MDL		2.0
30	Di-n-butylphthalate		< MDL		2.0
31	Fluoranthene		< MDL		2.0
32	Pyrene		< MDL		2.0
33	Butylbenzylphthalate		< MDL		2.0
34	Benzo(a)anthracene		< MDL		2.0
35	bis(2-Ethylhexyl)phthalate		< MDL		2.0
36	Chrysene		< MDL		2.0
37	Di-n-octylphthalate		< MDL		2.0
38	Benzo(b)fluoranthene		< MDL		2.0
39	Benzo(k)fluoranthene		< MDL		2.0
40	Benzo(a)pyrene		< MDL		2.0
41	Indeno(1,2,3-cd)pyrene		< MDL		2.0
42	Dibenz(a,h)anthracene		< MDL		2.0
43	Benzo(g,h,i)perylene		< MDL		2.0

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\040402B\LBJ0404.D

Vial: 10

Acq On : 5 Apr 2002 5:01 am

Operator: Bohlk

Sample : LB 3/15/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 05 06:23:05 2002

Quant Results File: 5080402.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Fri Apr 05 05:56:22 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	9.46	152	989737	20.00	ug/L	-0.01
10) Naphthalene-d8	12.93	136	4533729	20.00	ug/L	-0.01
17) Acenaphthene-d10	18.05	164	2629204	20.00	ug/L	0.00
29) Phenanthrene-d10	22.41	188	3799818	20.00	ug/L	-0.01
38) Chrysene-d12	30.23	240	2731079	20.00	ug/L	-0.02
44) Perylene-d12	34.11	264	1680468	20.00	ug/L	-0.01

System Monitoring Compounds

37) 2,4-DDD (SURR)	27.36	235	195216	5.18	ug/L	0.00
Spiked Amount	5.000		Recovery	=	103.60%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	d
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
30) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
31) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
32) Hexachlorobenzene	0.00	284	0	N.D.	
33) Phenanthrene	0.00	178	0	N.D.	
34) Anthracene	0.00	178	0	N.D.	
35) Di-n-butylphthalate	0.00	149	0	N.D.	
36) Fluoranthene	0.00	202	0	N.D.	
39) Pyrene	0.00	202	0	N.D.	
40) Butylbenzylphthalate	0.00	149	0	N.D.	
41) Benzo (a) anthracene	0.00	228	0	N.D.	d
42) Bis (2-ethylhexyl) phthala	30.85	149	15228	0.17	ug/L 92
43) Chrysene	0.00	228	0	N.D.	d
45) Di-n-Octylphthalate	0.00	149	0	N.D.	
46) Benzo (b) fluoranthene	0.00	252	0	N.D.	

(#)= qualifier out of range (m) = manual integration

LBJ0404.D 5080402.M Fri Apr 05 06:25:41 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\040402B\LBJ0404.D Vial: 10
Acq On : 5 Apr 2002 5:01 am Operator: Bohlk
Sample : LB 3/15/02 Inst : Instrumen
Misc : Multiplr: 1.00
MS Integration Params: BENZO.P
Quant Time: Apr 05 06:23:05 2002 Quant Results File: 5080402.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)
Title : Quantitation For Method 508gcscan
Last Update : Fri Apr 05 05:56:22 2002
Response via : Initial Calibration
DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
47) Benzo (k) fluoranthene	0.00	252	0	N.D.		
48) Benzo (a) pyrene	0.00	252	0	N.D.	d	
49) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
50) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
51) Benzo (g,h,i) perylene	0.00	276	0	N.D.	d	

(#) = qualifier out of range (m) = manual integration
LBJ0404.D 5080402.M Fri Apr 05 06:25:42 2002

Data File : C:\MSDCHEM\1\DATA\040402B\LBJ0404.D

Vial: 10

Acq On : 5 Apr 2002 5:01 am

Operator: Bohlk

Sample : LB 3/15/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 5 6:25 2002


Quant Results File: 5080402.RES

Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Fri Apr 05 05:56:22 2002

Response via : Initial Calibration

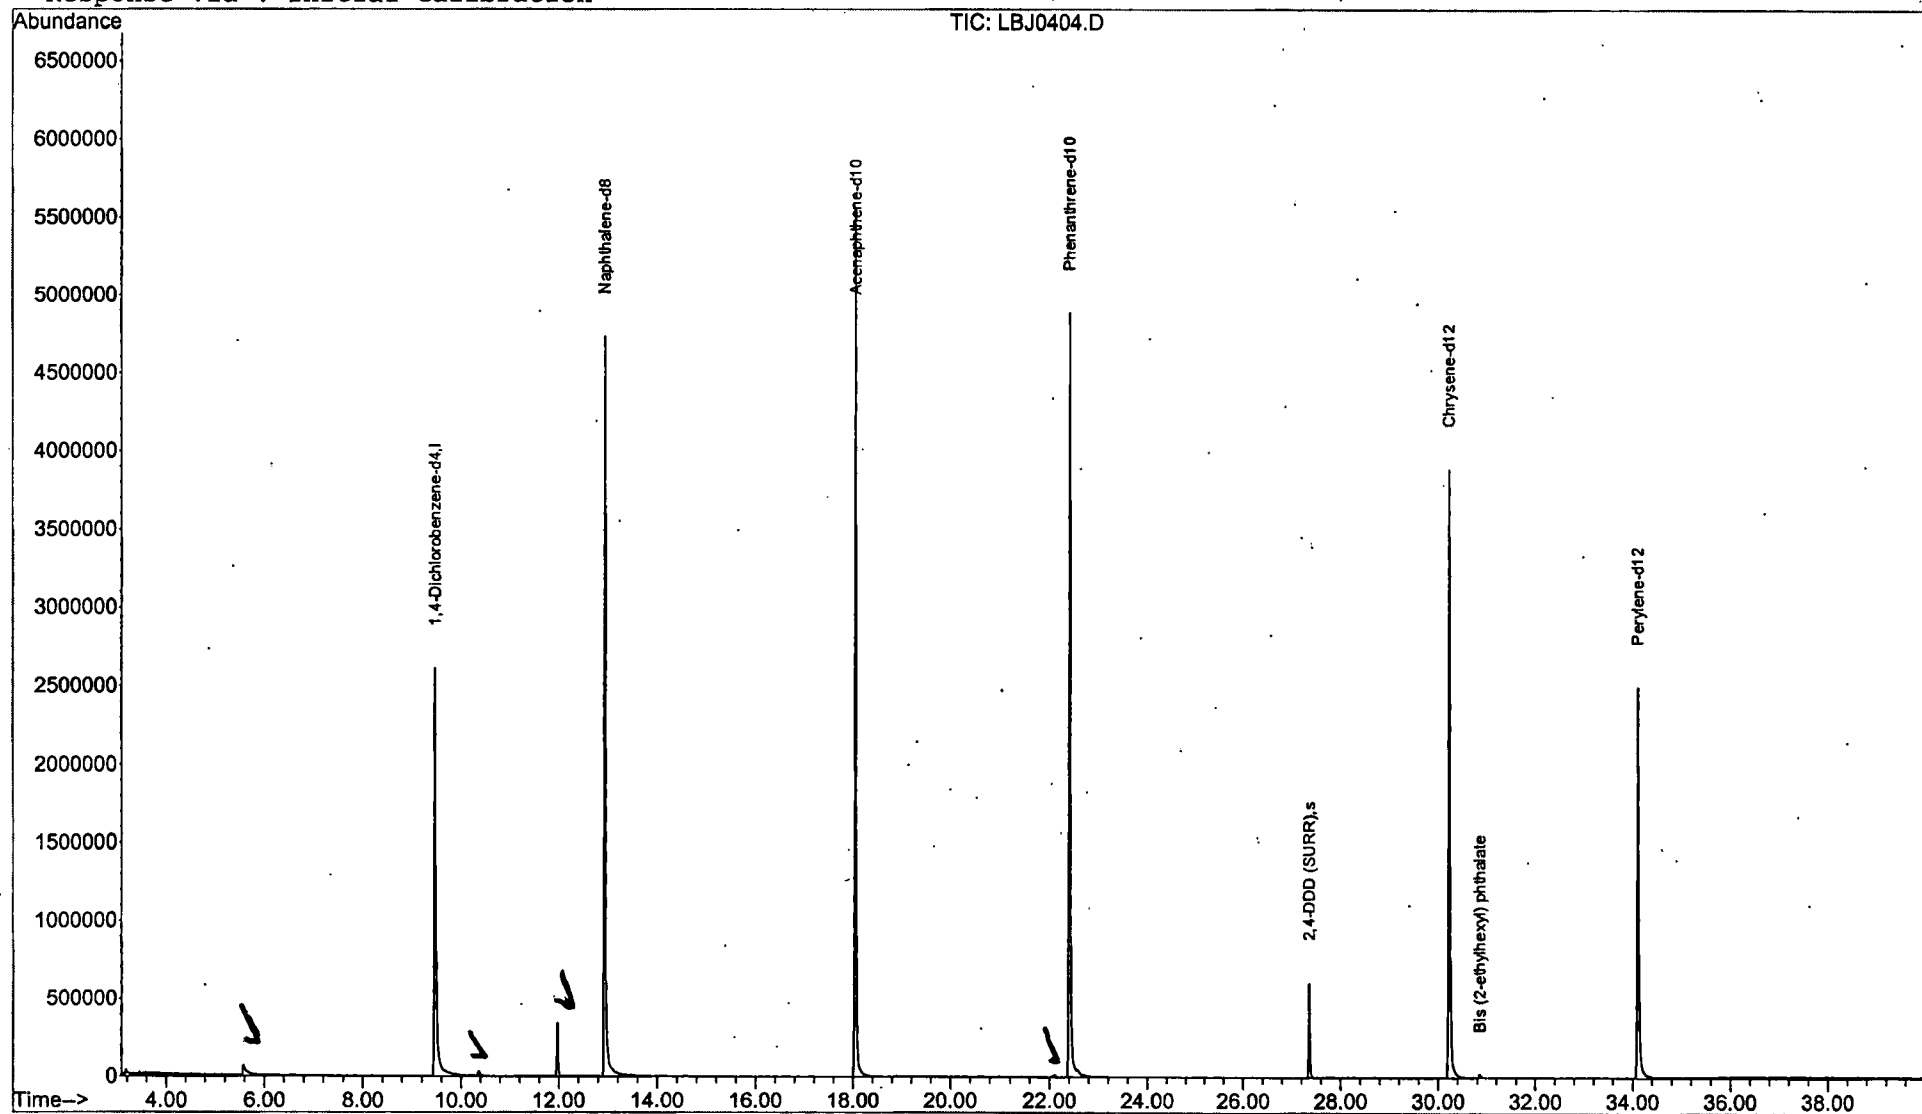

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\040402B\LBJ0404.D
 Acq On : 5 Apr 2002 5:01 am
 Sample : LB 3/15/02
 Misc :
 MS Integration Params: LSCINT.P

Vial: 10
 Operator: Bohlk
 Inst : Instrumen
 Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)
 Title : Quantitation For Method 508gcscan
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.570	422	424	433	rBV	61077	161597	1.41%	0.287%
2	9.460	1079	1086	1113	rBV	2610218	6685849	58.30%	11.868%
3	11.975	1505	1514	1526	rBV	347642	617338	5.38%	1.096%
4	12.932	1669	1677	1699	rBV	4735435	9899706	86.32%	17.573%
5	18.050	2538	2548	2575	rBV	5557418	11468366	100.00%	20.357%
6	22.410	3280	3290	3309	rBV2	4890865	11041569	96.28%	19.600%
7	27.357	4125	4132	4150	rBV	607254	1155662	10.08%	2.051%
8	30.230	4610	4621	4642	rBV2	3888850	8922382	77.80%	15.838%
9	34.114	5271	5282	5301	rBV2	2495440	6383092	55.66%	11.330%

Sum of corrected areas: 56335561

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\040402B\LBJ0404.D
 Operator : Bohlk
 Acquired : 5 Apr 2002 5:01 am using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: LB 3/15/02
 Misc Info :
 Vial Number: 10
 Quant File :5080402.RES (RTE Integrator)

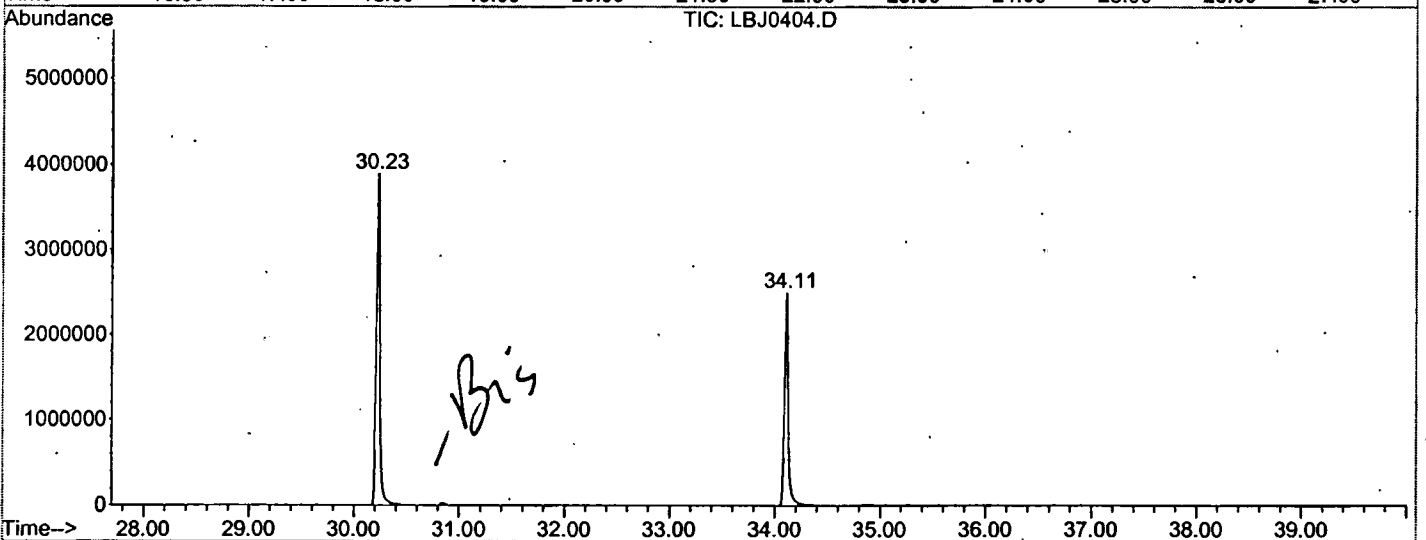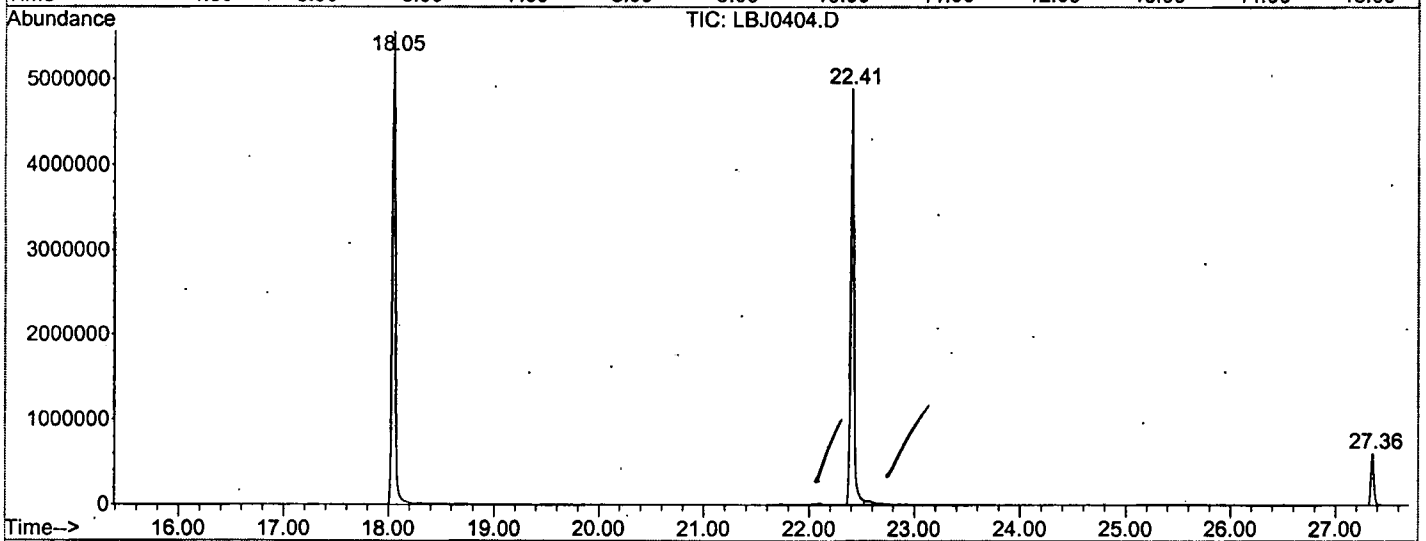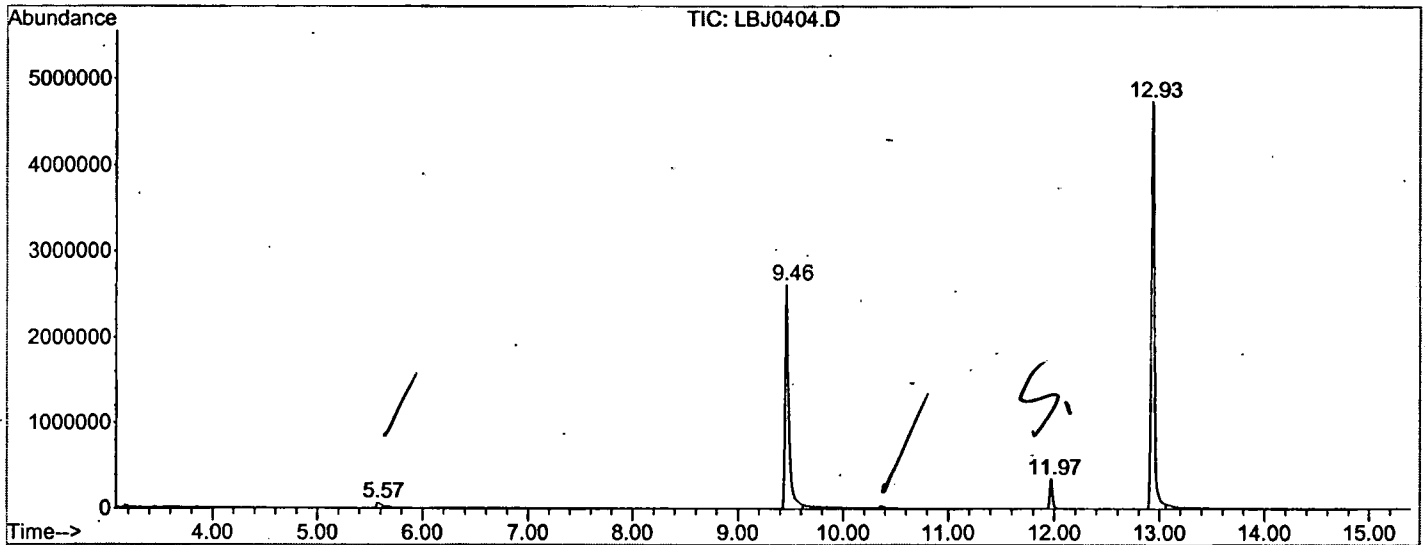

Library Search Compound Report

Data File : C:\MSDCHEM\1\DATA\040402B\LBJ0404.D
Acq On : 5 Apr 2002 5:01 am
Sample : LB 3/15/02
Misc :
MS Integration Params: LSCINT.P









Vial: 10
Operator: Bohlk
Inst : Instrumen
Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)
Title : Quantitation For Method 508gcscan
Library : C:\DATABASE\WILEY7N.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.57	0.48 ug/L	161597	1,4-Dichlorobenzene-d4	9.46

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	78
2			2-Pentanone, 4-hydroxy-4-methyl-...	116	C6H12O2	000123-42-2	78
3			2-Pentanone, 4-hydroxy-4-methyl-...	116	C6H12O2	000123-42-2	53
4			2-Pentanone, 4-hydroxy-4-methyl-...	116	C6H12O2	000123-42-2	53

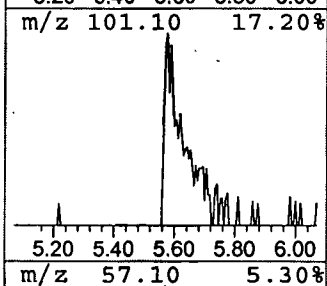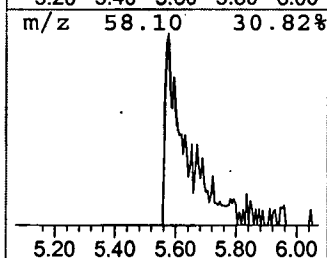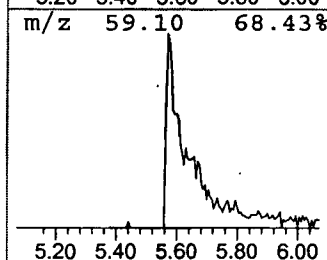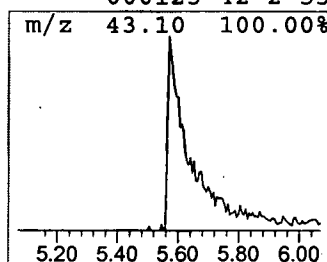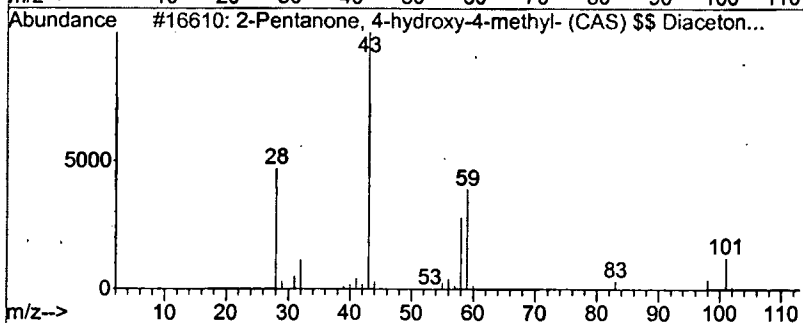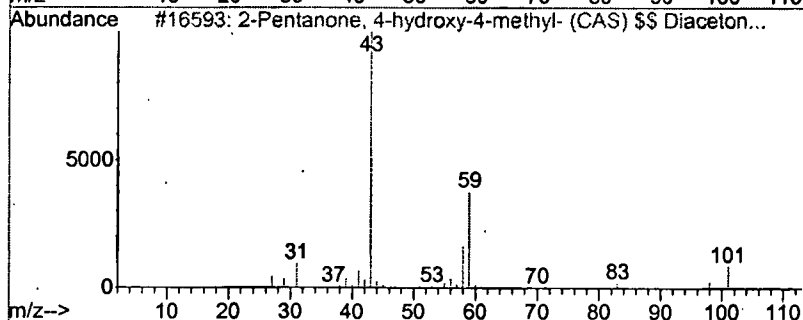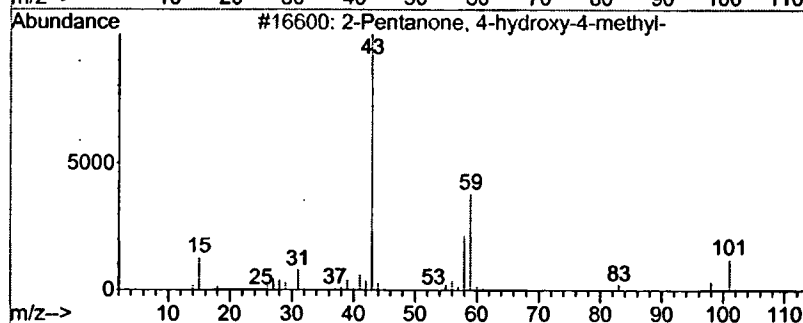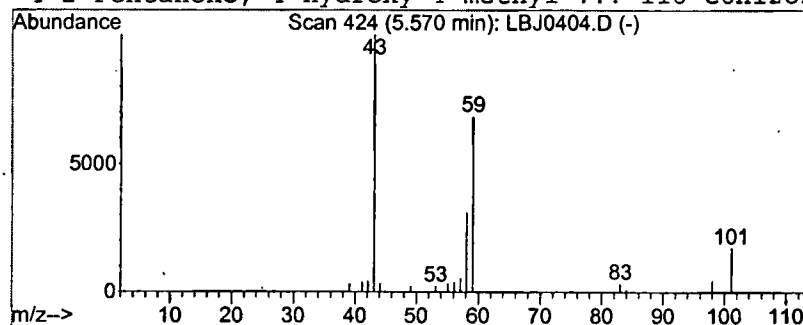

Library Search Compound Report

Data File : C:\MSDCHEM\1\DATA\040402B\LB0404.D
 Acq On : 5 Apr 2002 5:01 am
 Sample : LB 3/15/02
 Misc :
 MS Integration Params: LSCINT.P









Vial: 10
 Operator: Bohlk
 Inst : Instrumen
 Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)
 Title : Quantitation For Method 508gcscan
 Library : C:\DATABASE\WILEY7N.L

 Peak Number 2 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.97	1.25 ug/L	617338	Naphthalene-d8	12.93

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	52
2		Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	47
3		Benzeneethanamine, N-[(pentaflu...	563	C24H34F5NO3Si3	055429-13-5	38
4		2,6-DIHYDROXYBENZOIC ACID 3TMS \$...	370	C16H30O4Si3	003782-85-2	38

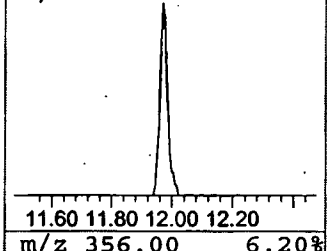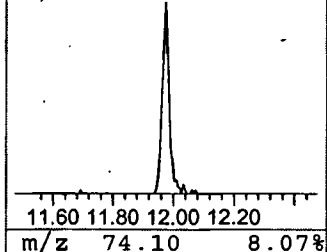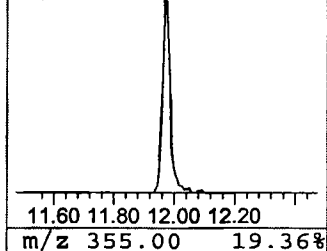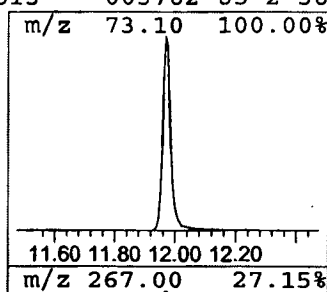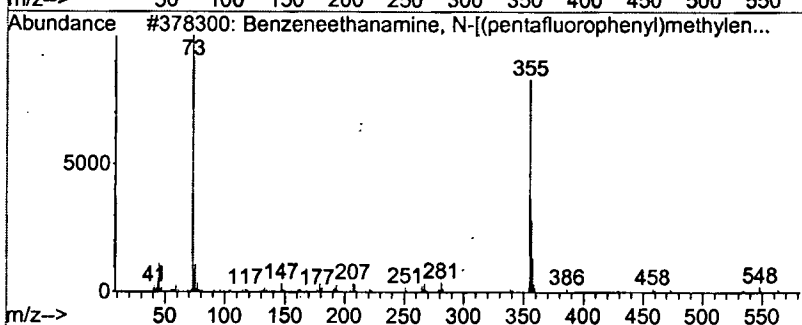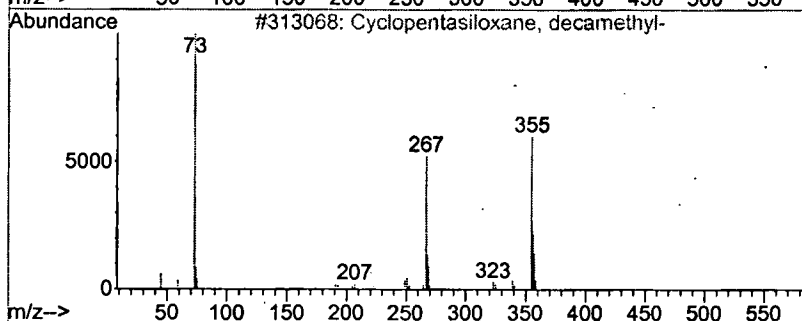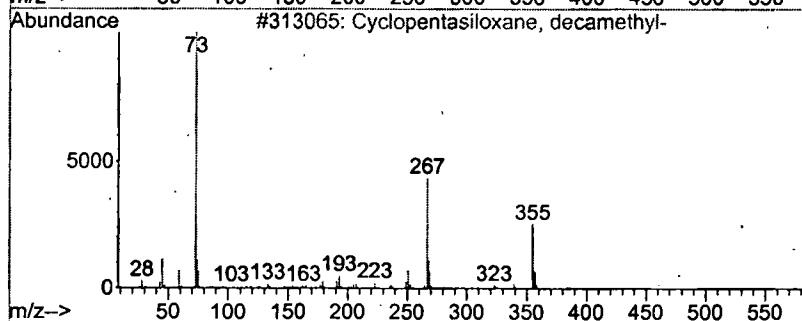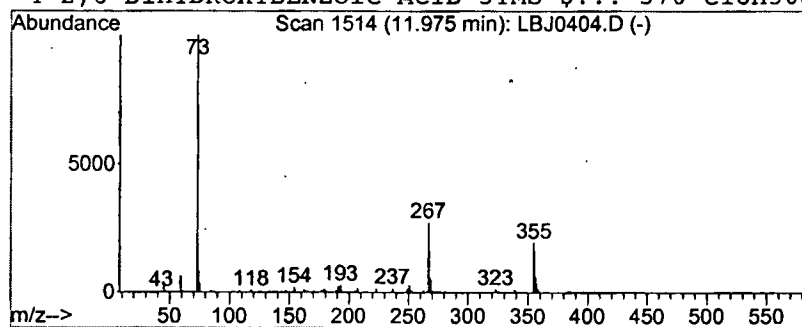

Tentatively Identified Compound (LSC) summary

Operator ID: Bohlk Date Acquired: 5 Apr 2002 5:01 am
Data File: C:\MSDCHEM\1\DATA\040402B\LBj0404.D
Name: LB 3/15/02
Misc:
Method: C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)
Title: Quantitation For Method 508gcscan
Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.57	0.5	ug/L	161597	1	9.46	6685850	20.0
Cyclopentasiloxan...	11.97	1.2	ug/L	617338	2	12.93	9899710	20.0