

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/18/2002 Time: 11:37:46

Sample: AE06094
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/18/2002 11:37 Ended: 4/18/2002 11:37 Analyst: DLV
Page: 1

	Component Name	Viol	Result	MDL
1	Other unknown compounds			
2	Surr_2,4-DDD		113	5.0

Comments for Sample AE06094 - Analysis \$GCMS

Vestchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-18-2002 Time: 11:37:55

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\040402B\6094.D

Vial: 17

Acq On : 5 Apr 2002 8:35 am

Operator: Bohlk

Sample : SAMPLE 6094 3/15/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 05 09:20:08 2002

Quant Results File: 5080402.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Fri Apr 05 05:56:22 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.46	152	995937	20.00	ug/L	-0.01
10) Naphthalene-d8	12.93	136	4673842	20.00	ug/L	-0.01
17) Acenaphthene-d10	18.05	164	2645536	20.00	ug/L	0.00
29) Phenanthrene-d10	22.41	188	3772526	20.00	ug/L	-0.01
38) Chrysene-d12	30.23	240	2859413	20.00	ug/L	-0.02
44) Perylene-d12	34.11	264	1721904	20.00	ug/L	0.00

System Monitoring Compounds

37) 2,4-DDD (SURR)	27.36	235	211694	5.65	ug/L	0.00
Spiked Amount	5.000		Recovery	= 113.00%		

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D. d	
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D. d	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
30) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
31) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
32) Hexachlorobenzene	0.00	284	0	N.D.	
33) Phenanthrene	0.00	178	0	N.D.	
34) Anthracene	0.00	178	0	N.D.	
35) Di-n-butylphthalate	24.57	149	4968	0.03 ug/L	79
36) Fluoranthene	0.00	202	0	N.D.	
39) Pyrene	0.00	202	0	N.D.	
40) Butylbenzylphthalate	0.00	149	0	N.D.	
41) Benzo (a) anthracene	0.00	228	0	N.D. d	
42) Bis (2-ethylhexyl) phthala	30.86	149	6743	0.07 ug/L	83
43) Chrysene	0.00	228	0	N.D. d	
45) Di-n-Octylphthalate	0.00	149	0	N.D.	
46) Benzo (b) fluoranthene	0.00	252	0	N.D.	

(#)= qualifier out of range (m) = manual integration

6094.D 5080402.M Fri Apr 05 09:22:53 2002

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\040402B\6094.D

Vial: 17

Acq On : 5 Apr 2002 8:35 am

Operator: Bohlk

Sample : SAMPLE 6094 3/15/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 05 09:20:08 2002

Quant Results File: 5080402.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Fri Apr 05 05:56:22 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
47) Benzo (k) fluoranthene	0.00	252	0	N.D.		
48) Benzo (a) pyrene	0.00	252	0	N.D.	d	
49) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
50) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
51) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

6094.D 5080402.M Fri Apr 05 09:22:53 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\040402B\6094.D

Vial: 17

Acq On : 5 Apr 2002 8:35 am

Operator: Bohlk

Sample : SAMPLE 6094 3/15/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 5 9:22 2002


Quant Results File: 5080402.RES

Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Fri Apr 05 05:56:22 2002

Response via : Initial Calibration

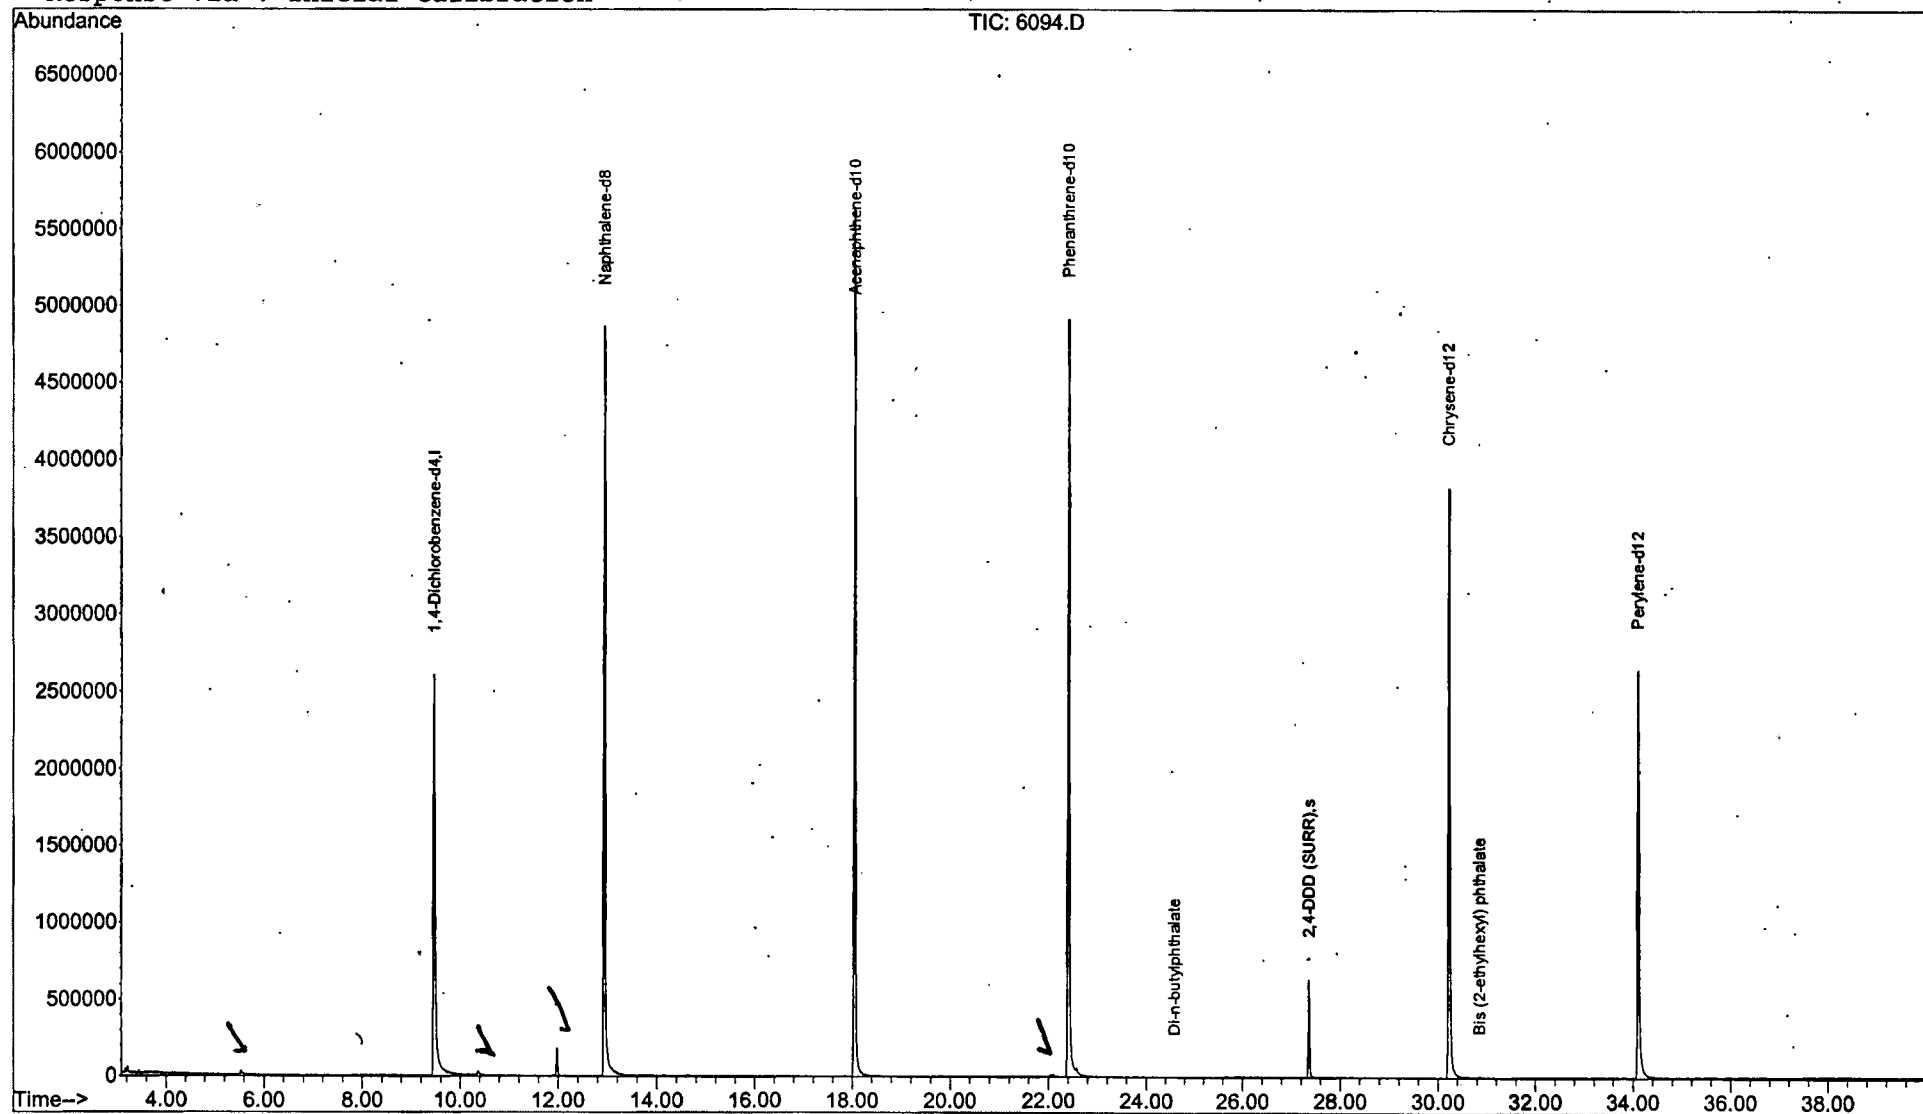

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\040402B\6094.D
Acq On : 5 Apr 2002 8:35 am
Sample : SAMPLE 6094 3/15/02
Misc :
MS Integration Params: LSCINT.P

Vial: 17
Operator: Bohlk
Inst : Instrumen
Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)
Title : Quantitation For Method 508gcscan
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.460	1079	1086	1118	rBV	2601684	6899294	60.35%	12.075%
2	11.975	1506	1514	1526	rVB2	179918	335187	2.93%	0.587%
3	12.933	1669	1677	1700	rBV	4861080	10240793	89.58%	17.923%
4	18.050	2537	2548	2564	rBV	5637037	11432065	100.00%	20.008%
5	22.410	3280	3290	3314	rBV2	4915730	11123017	97.30%	19.467%
6	27.357	4124	4132	4144	rBV	636422	1250747	10.94%	2.189%
7	30.230	4611	4621	4647	rBV2	3824068	9238245	80.81%	16.169%
8	34.114	5271	5282	5302	rBV2	2641905	6617731	57.89%	11.582%

Sum of corrected areas: 57137079

LSC Report -- Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\040402B\6094.D
 Operator : Bohlk
 Acquired : 5 Apr 2002 8:35 am using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: SAMPLE 6094 3/15/02
 Misc Info :
 Vial Number: 17
 Quant File :5080402.RES (RTE Integrator)

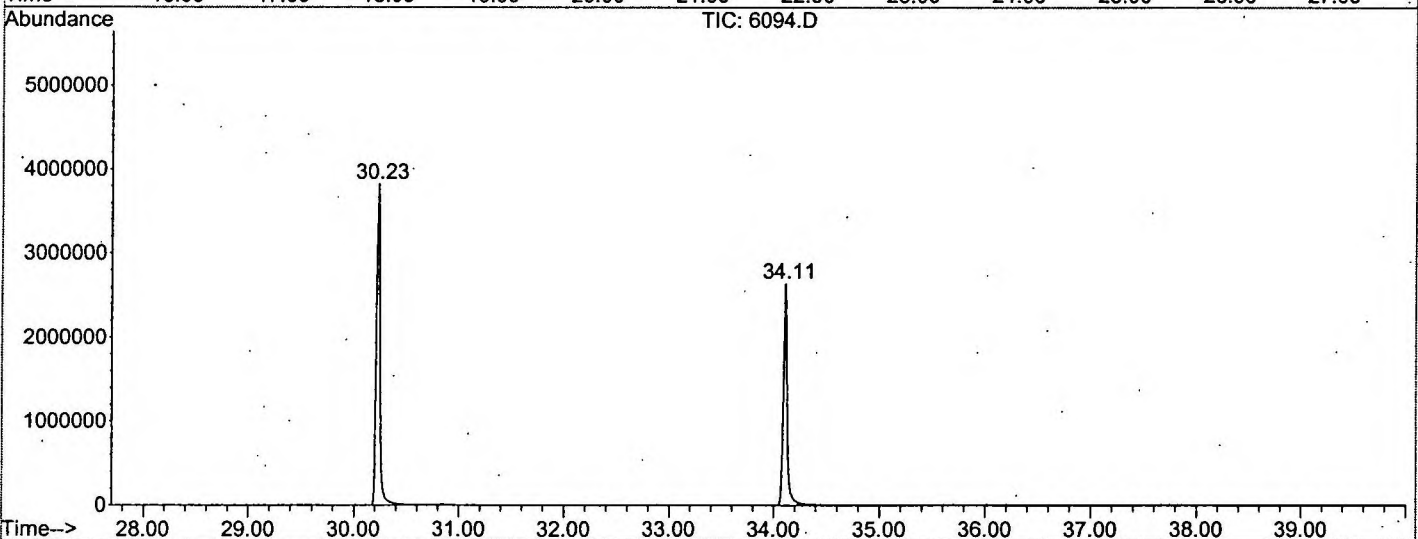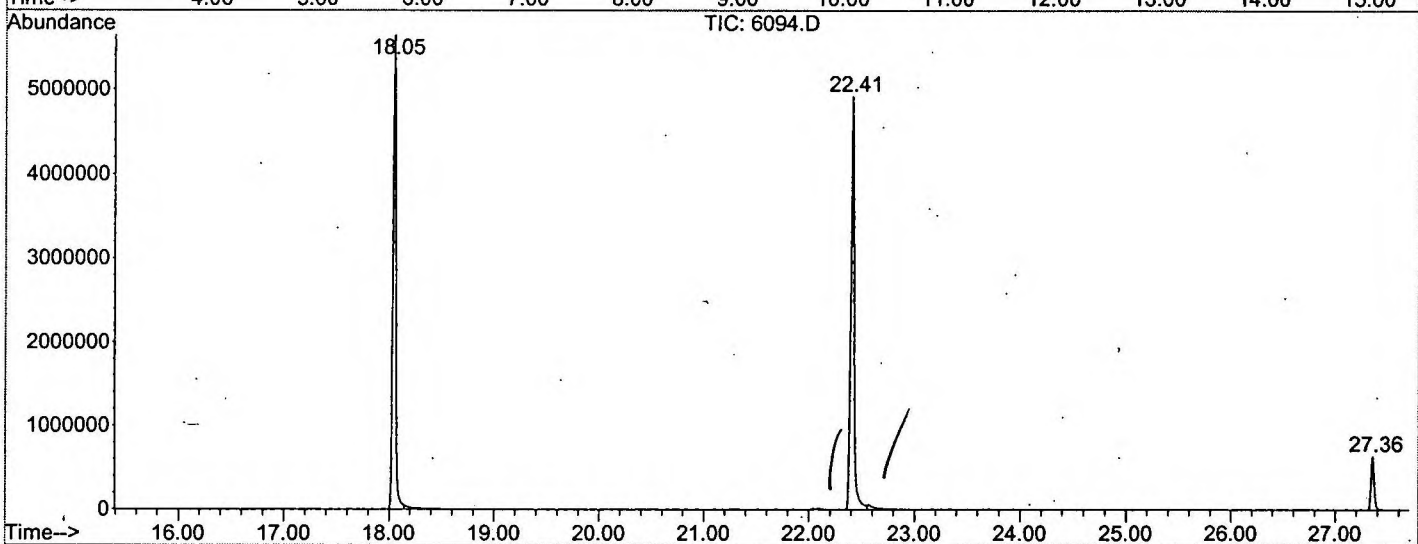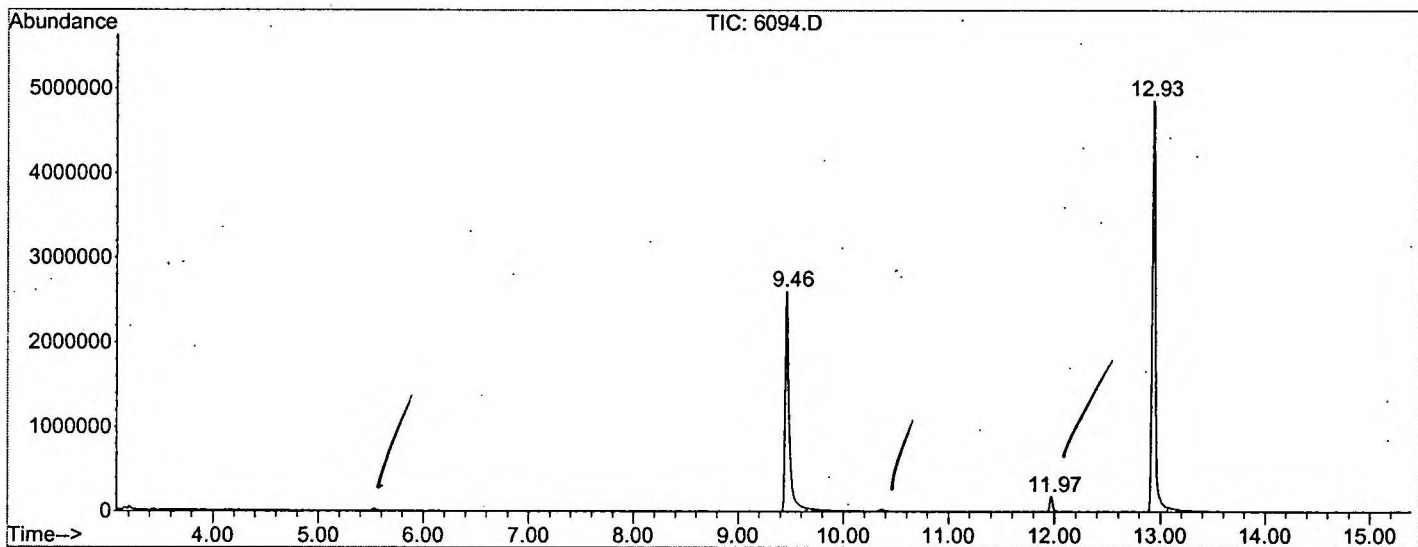

Library Search Compound Report

Data File : C:\MSDCHEM\1\DATA\040402B\6094.D

Acq On : 5 Apr 2002 8:35 am

Sample : SAMPLE 6094 3/15/02

Misc :

MS Integration Params: LSCINT.P

Vial: 17

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)









Title : Quantitation For Method 508gcscan

Library : C:\DATABASE\WILEY7N.L

Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.97	0.65 ug/L	335187	Naphthalene-d8	12.93

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	74
2			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	53
3			Benzeneethanamine, N-[(pentafluo...	475	C21H26F5NO2Si2	055429-85-1	37
4			Pentasiloxane, 1,1,3,3,5,5,7,7,9...	356	C10H32O4Si5	000995-83-5	33

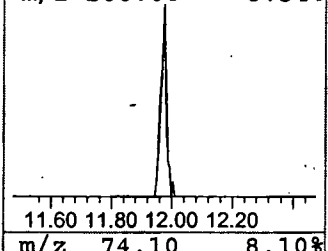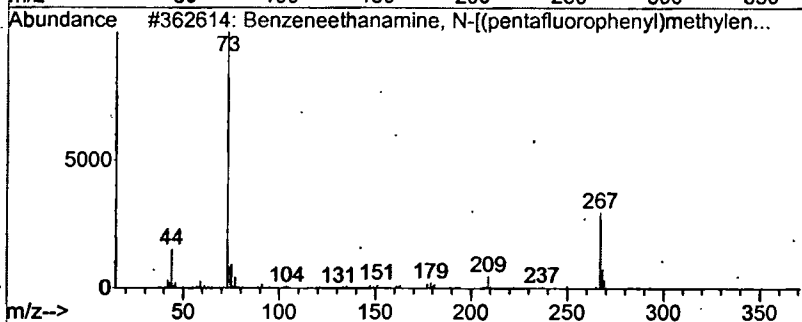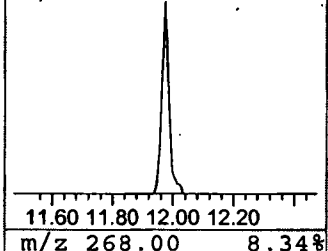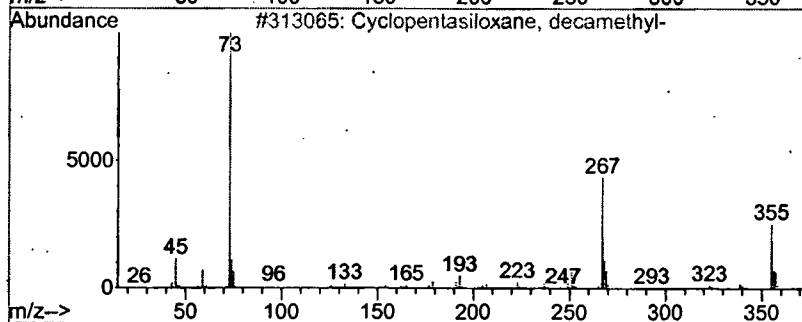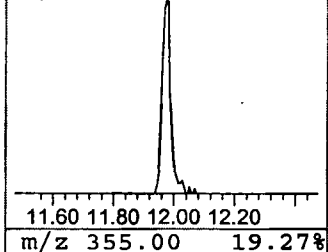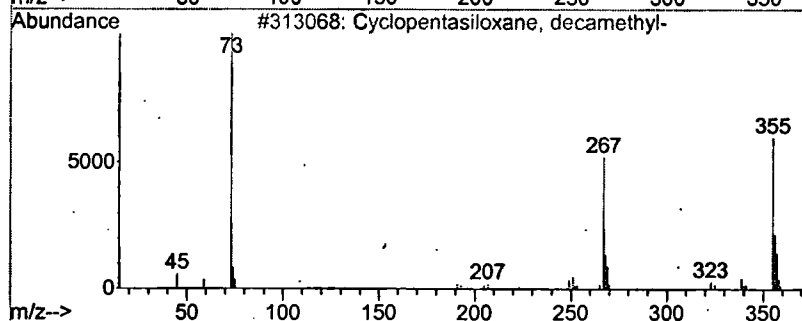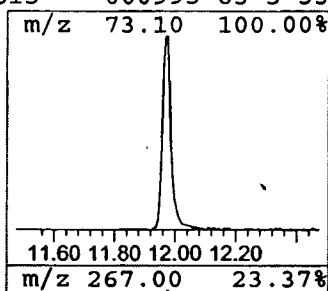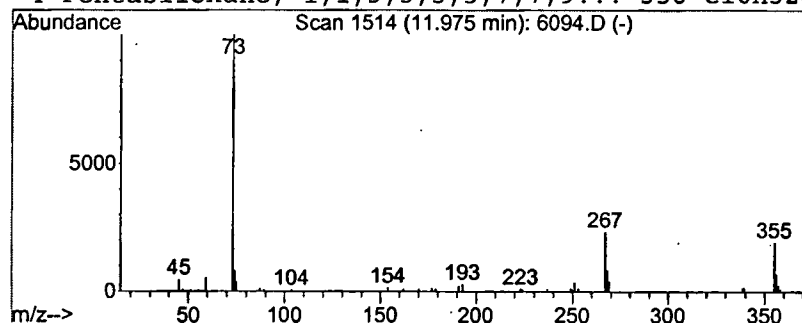

Tentatively Identified Compound (LSC) summary

Operator ID: Bohlk Date Acquired: 5 Apr 2002 8:35 am
Data File: C:\MSDCHEM\1\DATA\040402B\6094.D
Name: SAMPLE 6094 3/15/02
Misc:
Method: C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)
Title: Quantitation For Method 508gcscan
Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentasiloxan...	11.97	0.7	ug/L	335187	2	12.93	10240800	20.0