

Page 23


Reviewed by,
C/B 8/13/02
Na2SO4 lot# V4

Reviewed by _____
Date 4/18/22

DFTPP

Data File : C:\HPCHEM\1\DATA\APR1602\DFTPP.D
 Acq On : 16 Apr 2002 12:06 pm
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

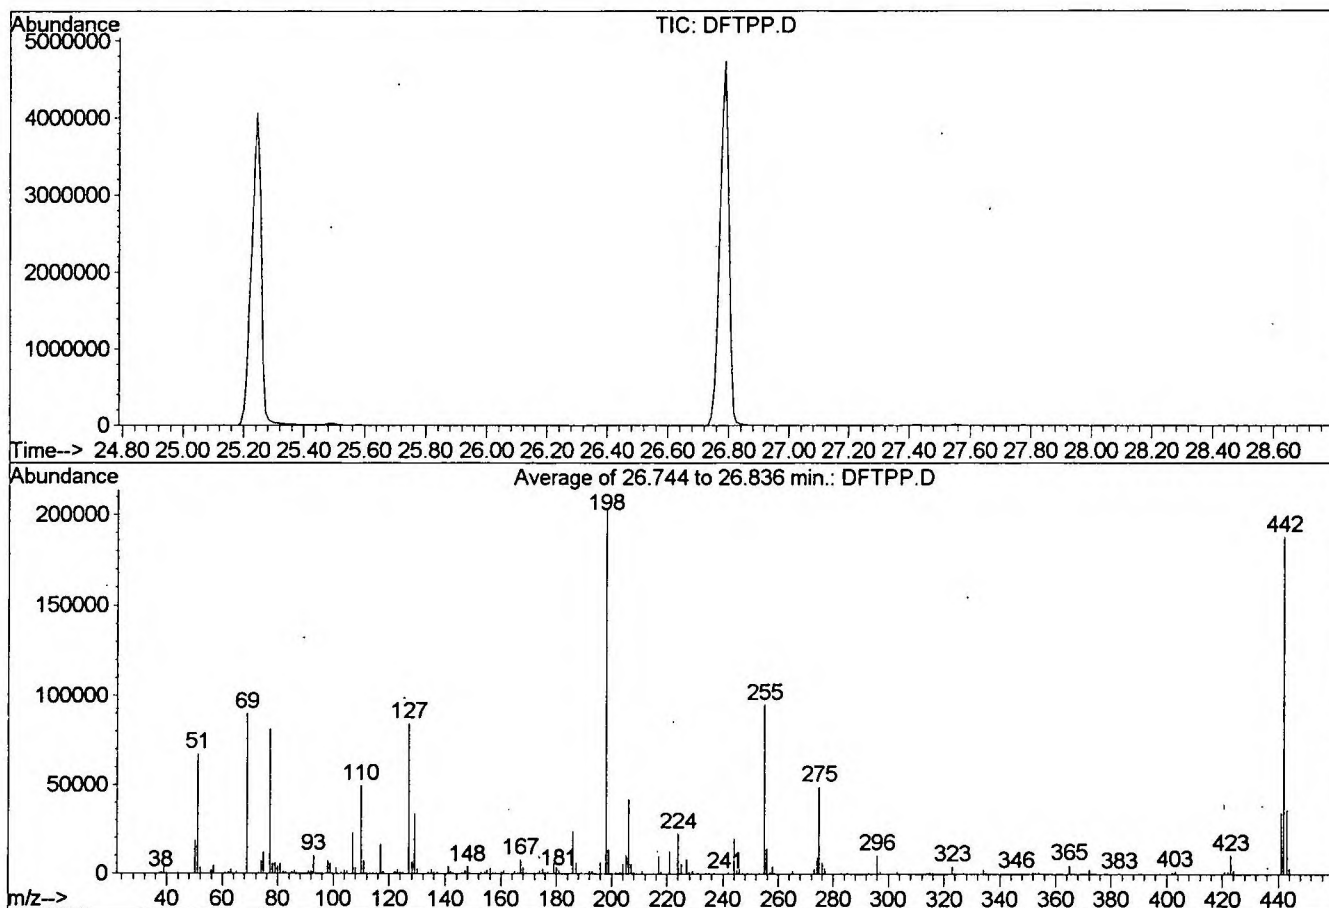

Spectrum Information: Average of 26.744 to 26.836 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	33.1	67553	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.2	90107	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	41.5	84642	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	203842	PASS
199	198	5	9	6.6	13534	PASS
275	198	10	30	24.2	49290	PASS
365	198	1	100	2.5	5061	PASS
441	443	0.01	100	94.9	34309	PASS
442	198	40	110	92.3	188222	PASS
443	442	17	23	19.2	36160	PASS