

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/12/2002 Time: 08:21:29

Sample: AE05908
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/12/02 08:20 Ended: 4/12/02 08:20 Analyst: DLV
Page: 1

	Component Name	Vol	Result	Qualifier	MDL
1	Other unknown compounds				
2					

not JS

Comments for Sample AE05908 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-12-2002 Time: 08:21:55

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recoveries for 8 of the 43 compounds in the LCS Standard were high.

Quantitation Report

(QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\040502\5908RE.D

Vial: 50

Acq On : 7 Apr 2002 12:00 pm

Operator: Bohlk

Sample : SAMPLE 5908 3/22/02 RE-EXT

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 10 08:56:14 2002

Quant Results File: 5080402.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Apr 08 06:47:22 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.46	152	952038	20.00	ug/L	-0.01
10) Naphthalene-d8	12.93	136	4276678	20.00	ug/L	-0.01
17) Acenaphthene-d10	18.04	164	2337025	20.00	ug/L	-0.01
29) Phenanthrene-d10	22.40	188	3279706	20.00	ug/L	-0.02
38) Chrysene-d12	30.22	240	2378649	20.00	ug/L	-0.02
44) Perylene-d12	34.11	264	1539453	20.00	ug/L	-0.01

System Monitoring Compounds

37) 2,4-DDD (SURR)	27.36	235	231328	7.11	ug/L	0.00
Spiked Amount	5.000		Recovery	=	142.20%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D. d	
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D. d	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
30) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
31) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
32) Hexachlorobenzene	0.00	284	0	N.D.	
33) Phenanthrene	0.00	178	0	N.D.	
34) Anthracene	0.00	178	0	N.D.	
35) Di-n-butylphthalate	0.00	149	0	N.D.	
36) Fluoranthene	0.00	202	0	N.D.	
39) Pyrene	0.00	202	0	N.D.	
40) Butylbenzylphthalate	0.00	149	0	N.D.	
41) Benzo (a) anthracene	0.00	228	0	N.D. d	
42) Bis (2-ethylhexyl) phthala	30.85	149	7841	0.10	ug/L 88
43) Chrysene	0.00	228	0	N.D. d	
45) Di-n-Octylphthalate	0.00	149	0	N.D.	
46) Benzo (b) fluoranthene	0.00	252	0	N.D.	

(#)=qualifier out of range (m) = manual integration

5908RE.D 5080402.M Wed Apr 10 08:57:39 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\040502\5908RE.D

Vial: 50

Acq On : 7 Apr 2002 12:00 pm

Operator: Bohlk

Sample : SAMPLE 5908 3/22/02 RE-EXT

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 10 08:56:14 2002

Quant Results File: 5080402.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Apr 08 06:47:22 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
47) Benzo (k) fluoranthene	0.00	252	0	N.D.		
48) Benzo (a) pyrene	0.00	252	0	N.D.	d	
49) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
50) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
51) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

5908RE.D 5080402.M Wed Apr 10 08:57:39 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\040502\5908RE.D

Vial: 50

Acq On : 7 Apr 2002 12:00 pm

Operator: Bohlk

Sample : SAMPLE 5908 3/22/02 RE-EXT

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 10 11:57 2002


Quant Results File: 5080402.RES

Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Apr 08 06:47:22 2002

Response via : Initial Calibration

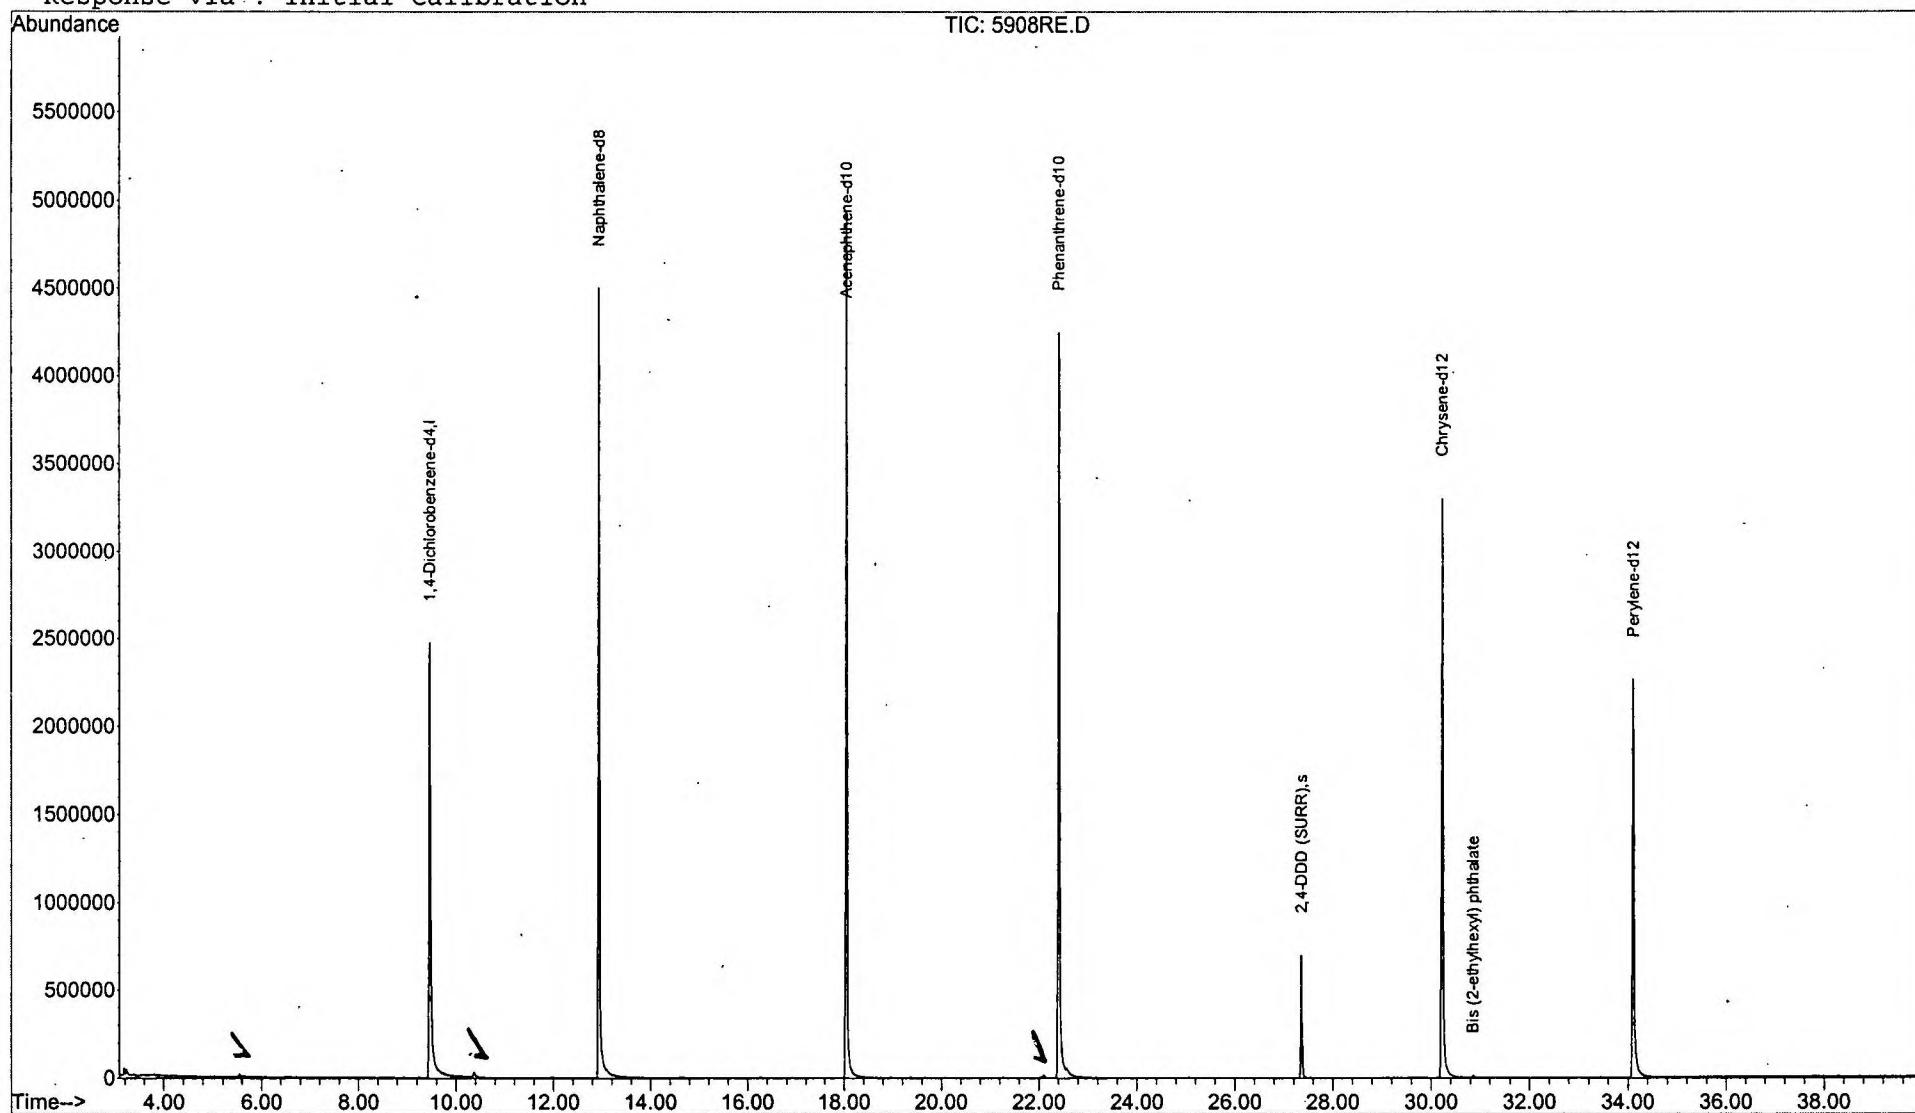

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\040502\5908RE.D

Vial: 50

Acq On : 7 Apr 2002 12:00 pm

Operator: Bohlk

Sample : SAMPLE 5908 3/22/02 RE-EXT

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: LSCINT.P

Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : OFF Filtering: 5

Sampling : 1 Min Area: 1 % of largest Peak

Start Thrs: 0.2 Max Peaks: 100

Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.460	1079	1086	1116	rBV	2472167	6420907	63.24%	12.713%
2	12.932	1669	1677	1698	rBV	4499932	9254464	91.14%	18.323%
3	18.044	2536	2547	2562	rBV	4937026	10153659	100.00%	20.103%
4	22.404	3280	3289	3311	rBV2	4245643	9592340	94.47%	18.992%
5	22.562	3313	3316	3329	rVB6	37308	115455	1.14%	0.229%
6	27.351	4124	4131	4144	rBV	697061	1369148	13.48%	2.711%
7	30.224	4610	4620	4646	rBV2	3298850	7777256	76.60%	15.398%
8	34.108	5270	5281	5303	rBV2	2264672	5823996	57.36%	11.531%

Sum of corrected areas: 50507225

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\040502\5908RE.D
Operator : Bohlk
Acquired : 7 Apr 2002 12:00 pm using AcqMethod 508SCAN
Instrument : Instrumen
Sample Name: SAMPLE 5908 3/22/02 RE-EXT
Misc Info :
Vial Number: 50
Quant File :5080402.RES (RTE Integrator)

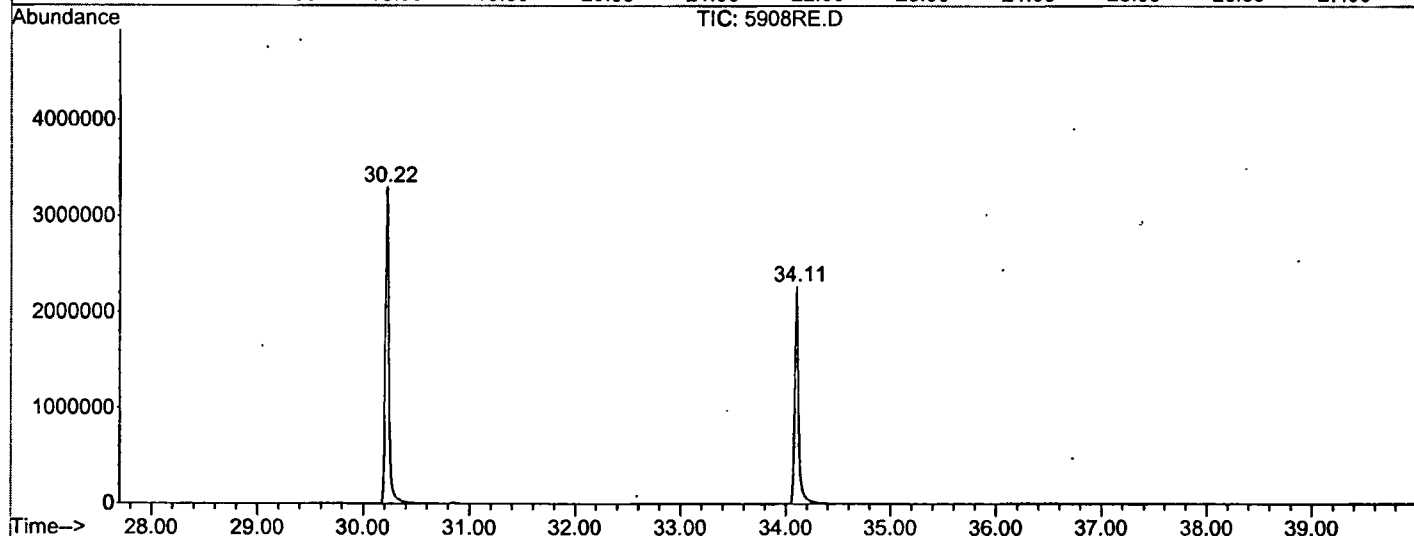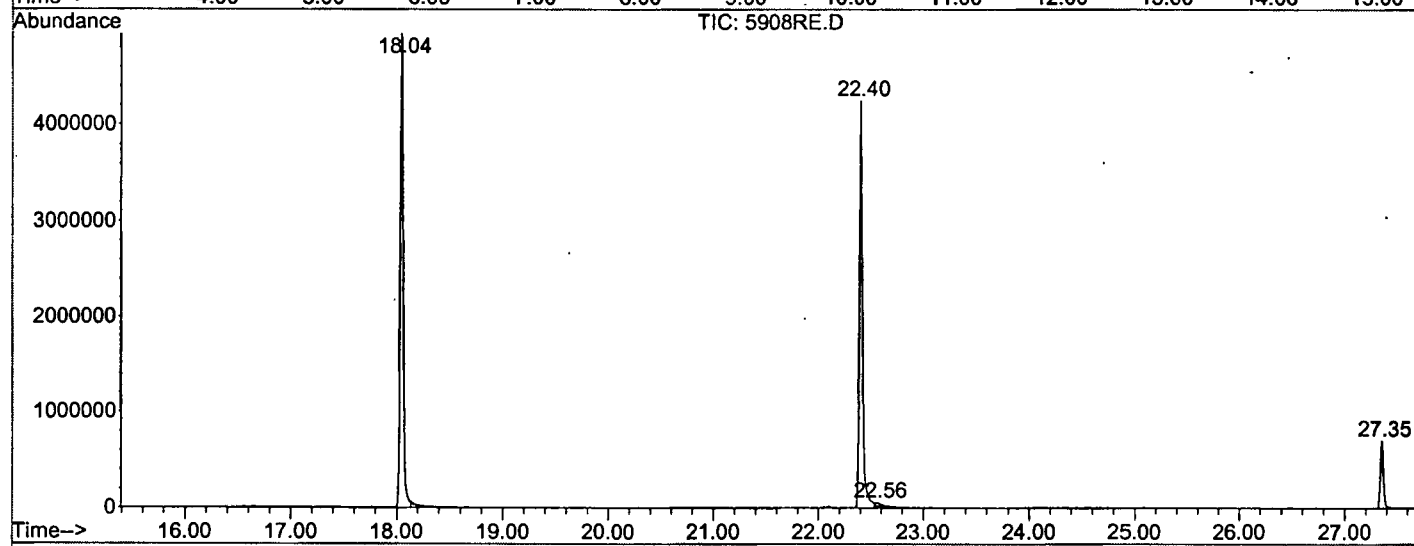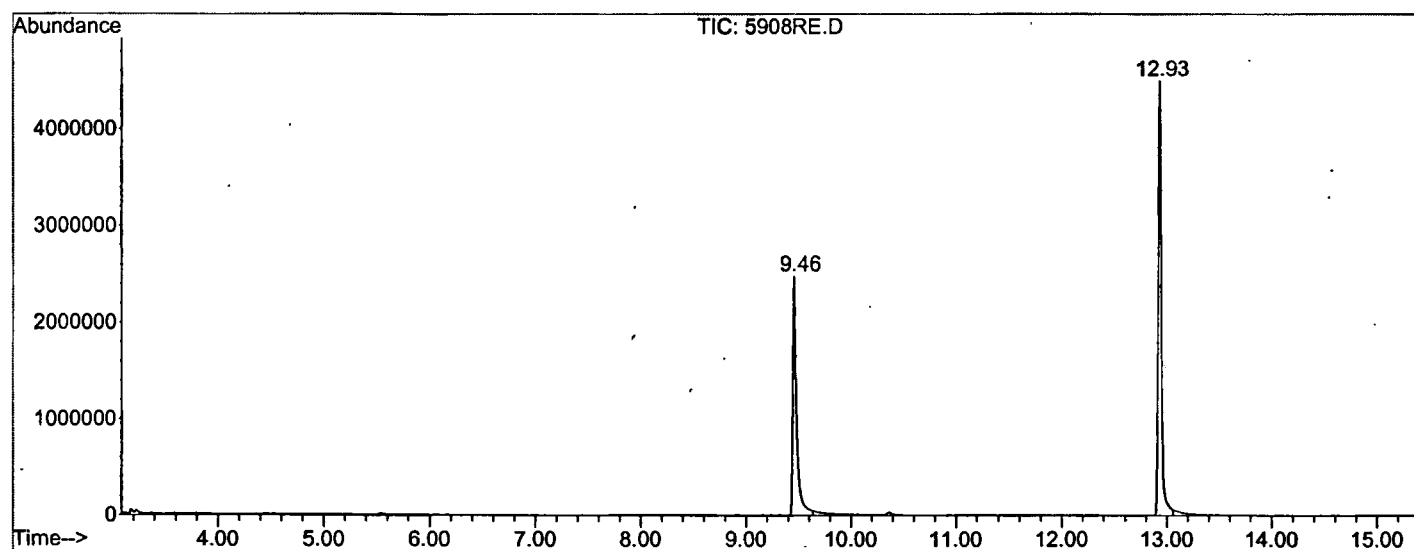

Tentatively Identified Compound (LSC) summary

Operator ID: Bohlk Date Acquired: 7 Apr 2002 12:00 pm
 Data File: C:\MSDCHEM\1\DATA\040502\5908RE.D
 Name: SAMPLE 5908 3/22/02 RE-EXT
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
