

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/11/2002 Time: 15:50:25

Sample: AE06800
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/11/02 15:50 Ended: 4/11/02 15:50 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds				
2	Surr_2,4-DDD		115		5.0

Comments for Sample AE06800 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-11-2002 Time: 15:51:37

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recoveries for 8 of the 43 compounds in the LCS Standard were high.

Quantitation Report

(QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\040502\6800.D

Vial: 42

Acq On : 7 Apr 2002 5:28 am

Operator: Bohlk

Sample : SAMPLE 6800 3/22/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 10 07:23:02 2002

Quant Results File: 5080402.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Apr 08 06:47:22 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.46	152	1002463	20.00	ug/L	-0.01
10) Naphthalene-d8	12.93	136	4853354	20.00	ug/L	-0.01
17) Acenaphthene-d10	18.05	164	2850556	20.00	ug/L	0.00
29) Phenanthrene-d10	22.41	188	4029760	20.00	ug/L	-0.01
38) Chrysene-d12	30.23	240	2947361	20.00	ug/L	-0.02
44) Perylene-d12	34.11	264	1798036	20.00	ug/L	-0.01

System Monitoring Compounds

37) 2,4-DDD (SURR)	27.36	235	229892	5.75	ug/L	0.00
Spiked Amount	5.000		Recovery	=	115.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	d
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
28) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
30) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
31) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
32) Hexachlorobenzene	0.00	284	0	N.D.	
33) Phenanthrene	0.00	178	0	N.D.	
34) Anthracene	0.00	178	0	N.D.	
35) Di-n-butylphthalate	0.00	149	0	N.D.	d
36) Fluoranthene	0.00	202	0	N.D.	
39) Pyrene	0.00	202	0	N.D.	
40) Butylbenzylphthalate	0.00	149	0	N.D.	
41) Benzo (a) anthracene	0.00	228	0	N.D.	d
42) Bis (2-ethylhexyl) phthala	30.86	149	4714	0.05	ug/L 89
43) Chrysene	0.00	228	0	N.D.	d
45) Di-n-Octylphthalate	0.00	149	0	N.D.	
46) Benzo (b) fluoranthene	0.00	252	0	N.D.	

(#)=qualifier out of range (m)=manual integration

6800.D 5080402.M Wed Apr 10 07:27:14 2002

Quantitation Report

(QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\040502\6800.D

Vial: 42

Acq On : 7 Apr 2002 5:28 am

Operator: Bohlk

Sample : SAMPLE 6800 3/22/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 10 07:23:02 2002

Quant Results File: 5080402.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Apr 08 06:47:22 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
47) Benzo (k) fluoranthene	0.00	252	0	N.D.		
48) Benzo (a) pyrene	0.00	252	0	N.D.	d	
49) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
50) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
51) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration
6800.D 5080402.M Wed Apr 10 07:27:14 2002

Data File : C:\MSDCHEM\1\DATA\040502\6800.D

Vial: 42

Acq On : 7 Apr 2002 5:28 am

Operator: Bohlk

Sample : SAMPLE 6800 3/22/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 10 10:27 2002


Quant Results File: 5080402.RES

Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Apr 08 06:47:22 2002

Response via : Initial Calibration

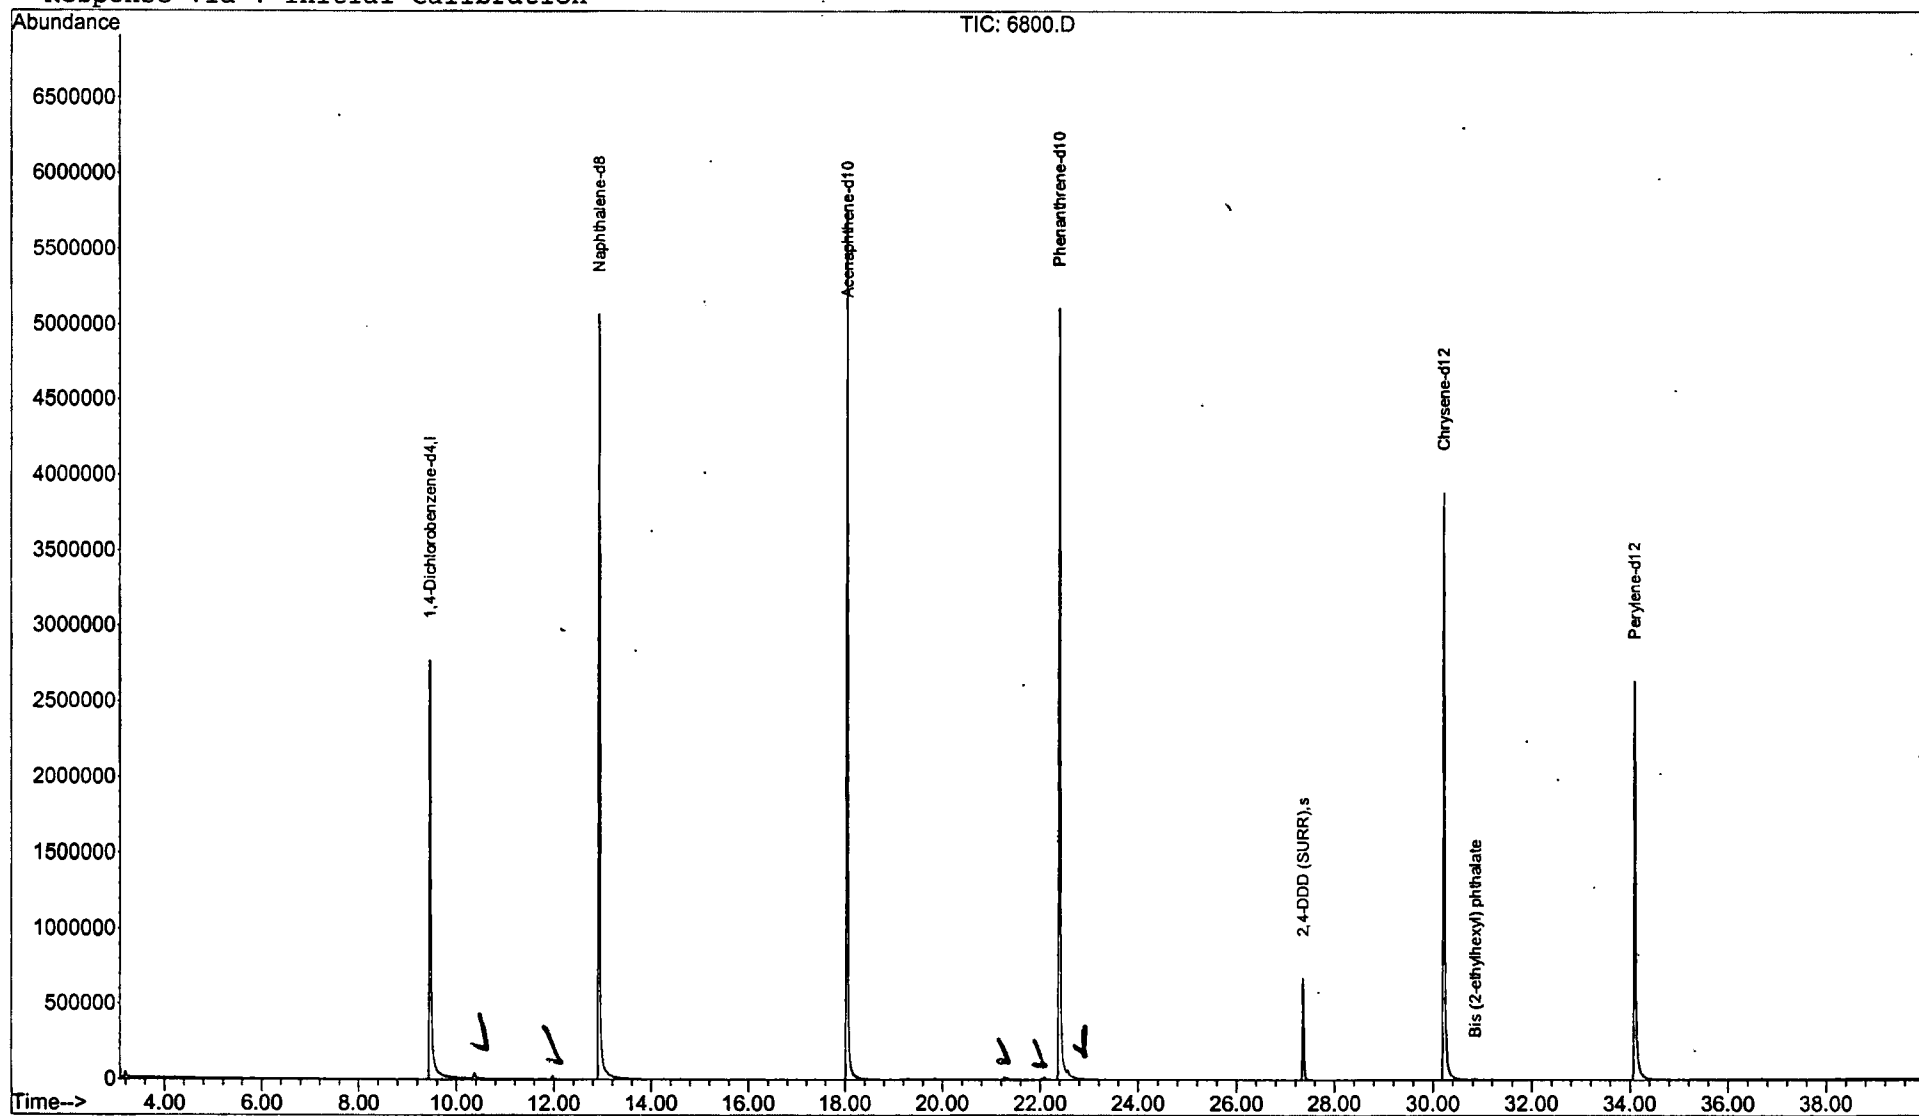

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\040502\6800.D
Acq On : 7 Apr 2002 5:28 am
Sample : SAMPLE 6800 3/22/02
Misc :
MS Integration Params: LSCINT.P

Vial: 42
Operator: Bohlk
Inst : Instrumen
Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)
Title : Quantitation For Method 508gcscan
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.460	1079	1086	1110	rBV	2767206	6764886	55.99%	11.472%
2	12.933	1670	1677	1703	rBV	5067172	10627624	87.96%	18.023%
3	18.050	2538	2548	2565	rBV	5756850	12081984	100.00%	20.489%
4	22.410	3280	3290	3311	rBV2	5111655	11734091	97.12%	19.899%
5	22.569	3313	3317	3333	rVB4	52180	172737	1.43%	0.293%
6	27.357	4123	4132	4143	rBV	670928	1324431	10.96%	2.246%
7	30.230	4610	4621	4648	rBV2	3885934	9472679	78.40%	16.064%
8	34.108	5270	5281	5309	rBV	2635578	6788376	56.19%	11.512%

Sum of corrected areas: 58966808

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\040502\6800.D
 Operator : Bohlk
 Acquired : 7 Apr 2002 5:28 am using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: SAMPLE 6800 3/22/02
 Misc Info :
 Vial Number: 42
 Quant File : 5080402.RES (RTE Integrator)

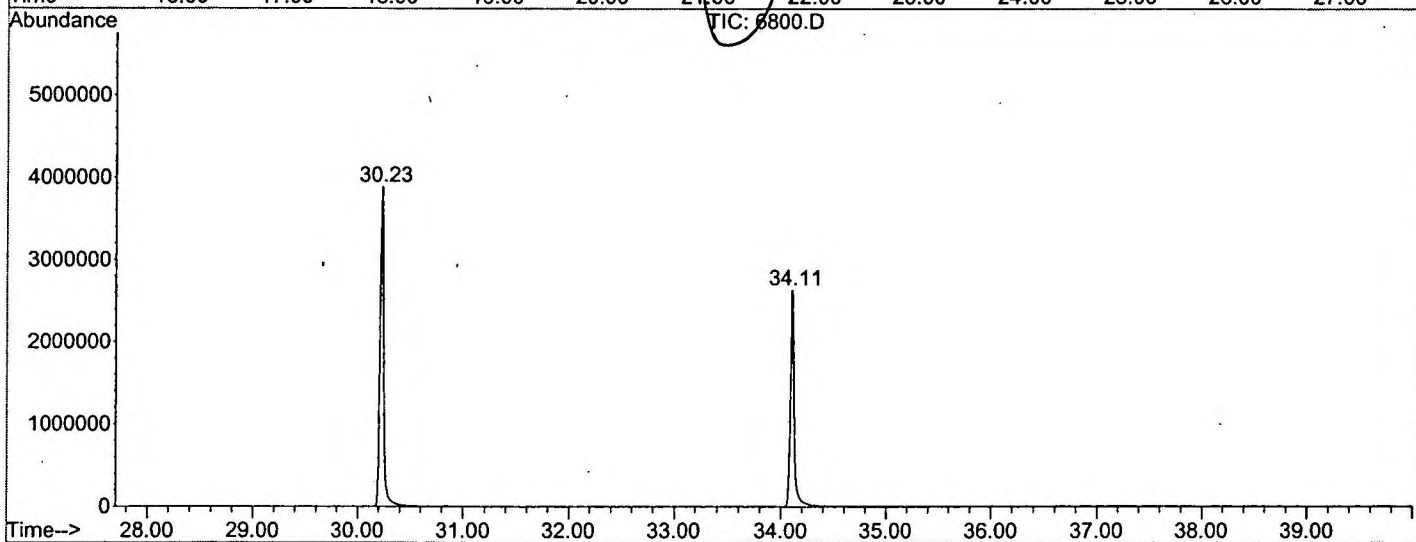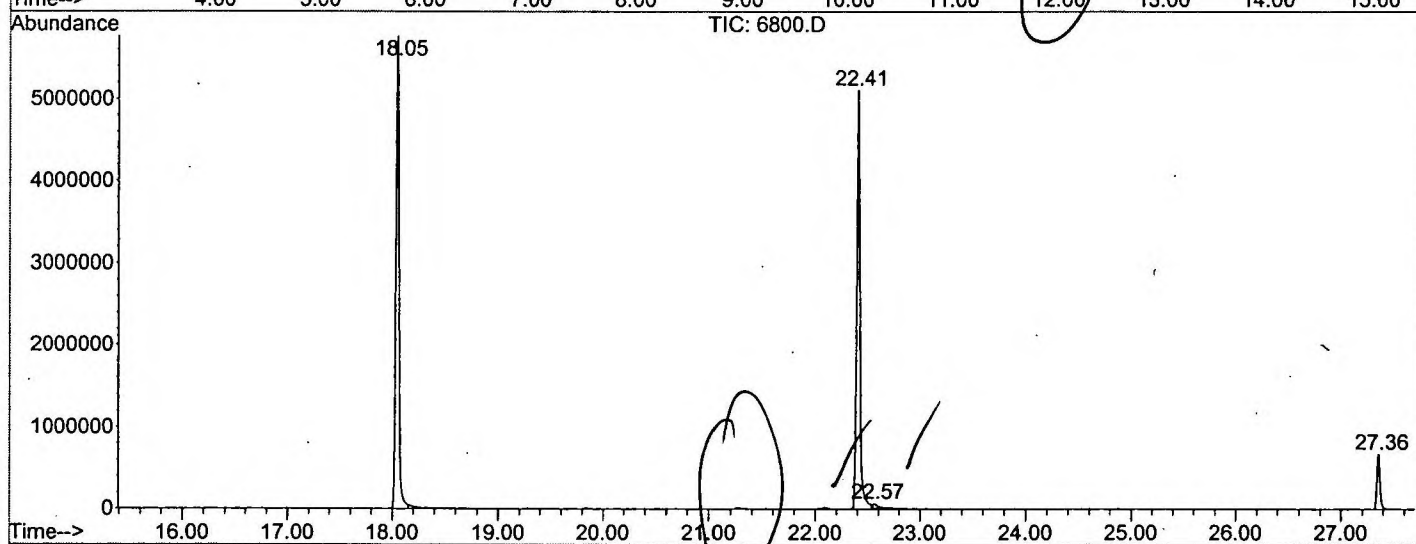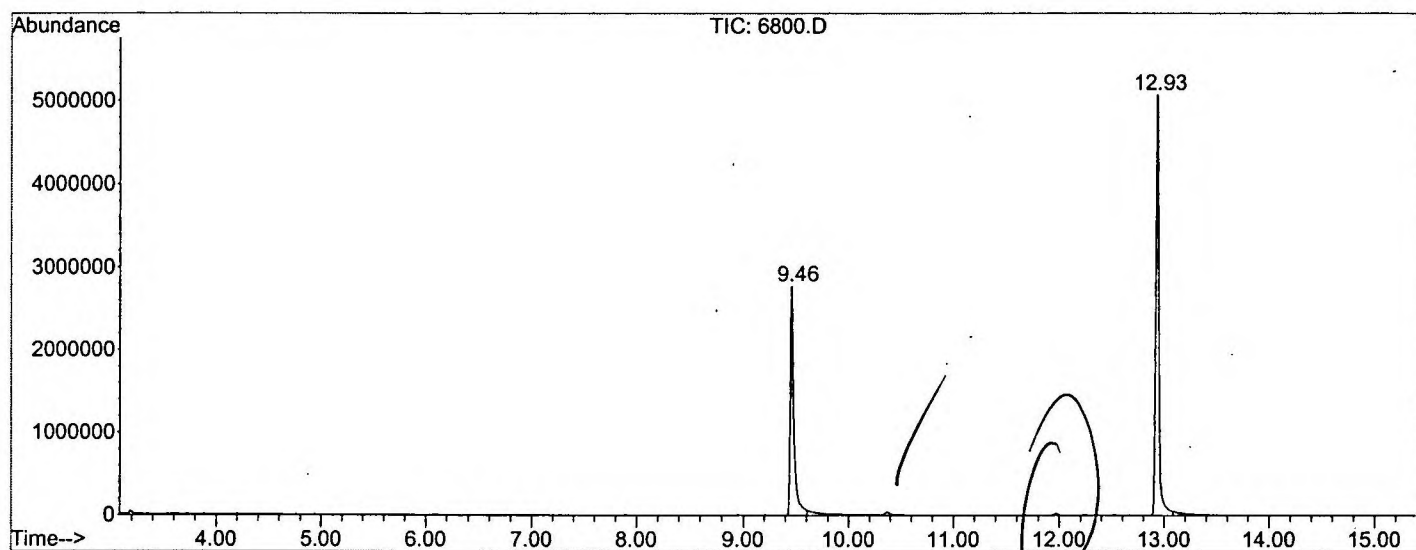

Tentatively Identified Compound (LSC) summary

Operator ID: Bohlk Date Acquired: 7 Apr 2002 5:28 am
 Data File: C:\MSDCHEM\1\DATA\040502\6800.D
 Name: SAMPLE 6800 3/22/02
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080402.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc