

Method 508 mod.

Date Extracted 3/25/02

Page 25

Ref

#GCM5-18078

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count		
LB		500ml		1ml			1ml	10A	7			
6981					1ml			10B				
6982								10C				
6983								9A				
6984	FB							1B				
6985								4A				
6986								6A				
6987								4B				
6988	FB							9B				
								1B				
								9A				

Remarks

Reviewed by [Signature] 3/25/02

drip rate must be between 5-15 ml/min for liq-liq extractors

Extraction type Sep Fun Solv. lot# X01E19 NaCl lot# V39618 Na2SO4 lot# V46625

STANDARD INT STD LOG#

CALIBRATION HPO 41022

REF SPIKE

IND/MDF

NO CHECK

INT STD 040802

SUBSTRATE

W/LPC

GEN/INDT


Verified by [Signature]

Reviewed by [Signature]
Date 4/22/02

DFTPP

Data File : C:\HPCHEM\1\DATA\APR1802\DFTPP.D
 Acq On : 18 Apr 2002 11:31 am
 Sample :
 Misc :
 MS Integration Params: GOOFY.P
 Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table

Vial: 1
 Operator:
 Inst : 209
 Multiplr: 1.00

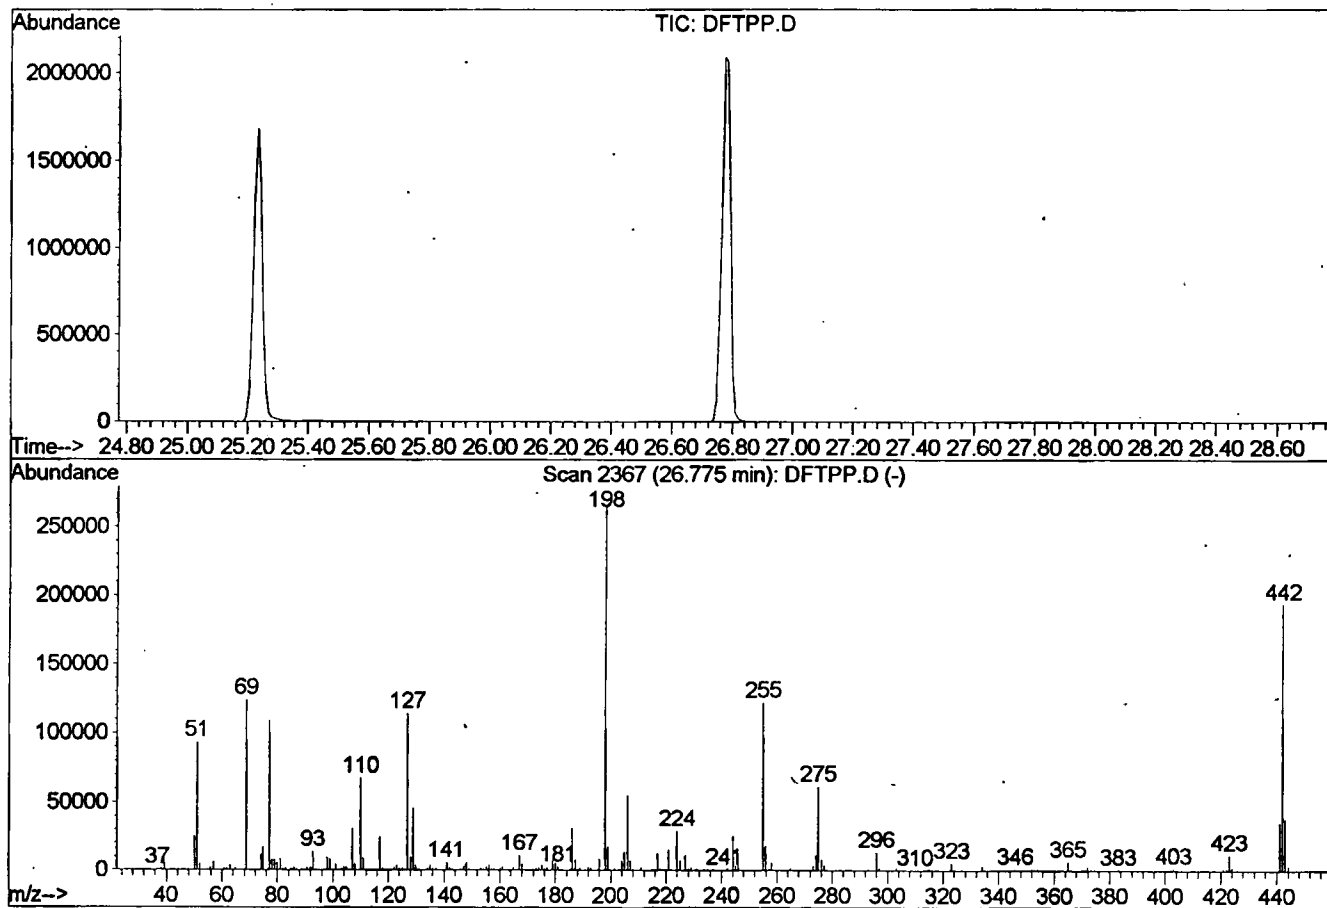

Spectrum Information: Scan 2367

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	35.1	93440	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.7	124192	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	42.9	114088	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	266048	PASS
199	198	5	9	6.6	17464	PASS
275	198	10	30	23.1	61480	PASS
365	198	1	100	2.3	6070	PASS
441	443	0.01	100	93.0	35192	PASS
442	198	40	110	72.9	193984	PASS
443	442	17	23	19.5	37840	PASS