

User: Galos, Marie
 Westchester Dept. of Labs & Research
 Date: 04/19/2002 Time: 09:27:48

Sample: AE06981
 Analysis: \$B1GCMS Blank for GCMS Scan
 Units: ug
 Started: 4/18/20 00:02 Ended: 4/18/20 00:02 Analyst: MG
 Result source: manual entry
 Page: 1

	Component Name	Viol ¹	Result	MDL
1	n-Nitrosodimethylamine		< MDL	2.0
2	bis(2-Chloroethyl)ether		< MDL	2.0
3	1,3-Dichlorobenzene		< MDL	2.0
4	1,4-Dichlorobenzene		< MDL	2.0
5	1,2-Dichlorobenzene		< MDL	2.0
6	2,2'-oxybis(1-Chloropropane)		< MDL	2.0
7	n-Nitrosodi-n-propylamine		< MDL	2.0
8	Hexachloroethane		< MDL	2.0
9	Nitrobenzene		< MDL	2.0
10	Isophorone		< MDL	2.0
11	bis(2-Chloroethoxy)methane		< MDL	2.0
12	1,2,4-Trichlorobenzene		< MDL	2.0
13	Naphthalene		< MDL	2.0
14	Hexachlorobutadiene		< MDL	2.0
15	2-Chloronaphthalene		< MDL	2.0
16	Dimethylphthalate		< MDL	2.0
17	2,6-Dinitrotoluene		< MDL	2.0
18	Acenaphthylene		< MDL	2.0
19	Acenaphthene		< MDL	2.0
20	2,4-Dinitrotoluene		< MDL	2.0
21	Diethylphthalate		< MDL	2.0
22	4-Chlorophenylphenylether		< MDL	2.0
23	Fluorene		< MDL	2.0
24	Azobenzene		< MDL	2.0
25	n-Nitrosodiphenylamine		< MDL	2.0
26	4-Bromophenylphenylether		< MDL	2.0
27	Hexachlorobenzene		< MDL	2.0
28	Phenanthrene		< MDL	2.0
29	Anthracene		< MDL	2.0
30	Di-n-butylphthalate		< MDL	2.0
31	Fluoranthene		< MDL	2.0
32	Pyrene		< MDL	2.0
33	Butylbenzylphthalate		< MDL	2.0
34	Benzo(a)anthracene		< MDL	2.0
35	bis(2-Ethylhexyl)phthalate		< MDL	2.0
36	Chrysene		< MDL	2.0
37	Di-n-octylphthalate		< MDL	2.0
38	Benzo(b)fluoranthene		< MDL	2.0
39	Benzo(k)fluoranthene		< MDL	2.0
40	Benzo(a)pyrene		< MDL	2.0
41	Indeno(1,2,3-cd)pyrene		< MDL	2.0
42	Dibenz(a,h)anthracene		< MDL	2.0
43	Benzo(g,h,i)perylene		< MDL	2.0

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR1802\LB.D
 Acq On : 18 Apr 2002 3:53 pm
 Sample : GC/MS SCAN 3/25
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 19 8:41 2002

Vial: 5
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Apr 17 11:48:30 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0412

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.21	152	508670	20.00	ug/l	-0.03
10) Naphthalene-d8	15.85	136	1820422	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.15	164	1022324	20.00	ug/l	-0.03
30) Phenanthrene-d10	25.59	188	1496164	20.00	ug/l	-0.03
39) Chrysene-d12	33.65	240	939947	20.00	ug/l	-0.03
45) Perylene-d12	37.87	264	591733	20.00	ug/l	-0.05

System Monitoring Compounds

28) TCMX	0.00	209	0	0.00	ug/L	
Spiked Amount	10.000		Recovery	=	0.00%	
38) 2,4-DDD	30.67	235	60852	3.49	ug/mL	0.17
Spiked Amount	5.000		Recovery	=	69.80%	

Target Compounds

				Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.
3) bis(2-Chloroethyl)ether	0.00	93	0	N.D.
4) 1,3-Dichlorobenzene	12.12	146	332	N.D.
5) 1,4-Dichlorobenzene	12.25	146	188	N.D.
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.
9) Hexachloroethane	0.00	117	0	N.D.
11) Nitrobenzene	0.00	77	0	N.D.
12) Isophorone	0.00	82	0	N.D.
13) bis(2-Chloroethoxy)methane	0.00	93	0	N.D.
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.
15) Naphthalene	15.89	128	372	N.D.
16) Hexachlorobutadiene	16.45	225	335	N.D.
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.
19) 2-Chloronaphthalene	0.00	162	0	N.D.
20) Dimethylphthalate	0.00	163	0	N.D.
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.
22) Acenaphthylene	0.00	152	0	N.D.
23) Acenaphthene	0.00	153	0	N.D.
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.
25) Diethylphthalate	0.00	149	0	N.D.
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.
27) Fluorene	0.00	166	0	N.D.
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.

(#) = qualifier out of range (m) = manual integration

LB.D GCMS0412.M Fri Apr 19 08:42:34 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR1802\LB.D
Acq On : 18 Apr 2002 3:53 pm
Sample : GC/MS SCAN 3/25
Misc :
MS Integration Params: GOOFY.P
Quant Time: Apr 19 8:41 2002

Vial: 5
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Apr 17 11:48:30 2002
Response via : Initial Calibration
DataAcq Meth : GCMS0412

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.59	178	351	N.D.	
35) Anthracene	25.59	178	351	N.D.	
36) Di-n-butylphthalate	27.55	149	551	N.D.	
37) Fluoranthene	0.00	202	0	N.D.	
40) Pyrene	0.00	202	0	N.D.	
41) Butylbenzylphthalate	0.00	149	0	N.D.	
42) Benzo(a)anthracene	33.65	228	2569	N.D.	
43) Bis(2-ethylhexyl)phthalate	33.86	149	37427	1.58 ug/l	99
44) Chrysene	33.73	228	275	N.D.	
46) Di-n-Octylphthalate	0.00	149	0	N.D.	
47) Benzo(b)fluoranthene	0.00	252	0	N.D.	
48) Benzo(k)fluoranthene	0.00	252	0	N.D.	
49) Benzo(a)pyrene	37.87	252	2340	N.D.	
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.	
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.	

(#) = qualifier out of range (m) = manual integration

LB.D GCMS0412.M

Fri Apr 19 08:42:35 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR1802\LB.D
Acq On : 18 Apr 2002 3:53 pm
Sample : GC/MS SCAN 3/25
Misc :
MS Integration Params: GOOFY.P
Quant Time: Apr 19 8:41 2002

Vial: 5
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0412.RES

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Apr 17 11:48:30 2002
Response via : Initial Calibration

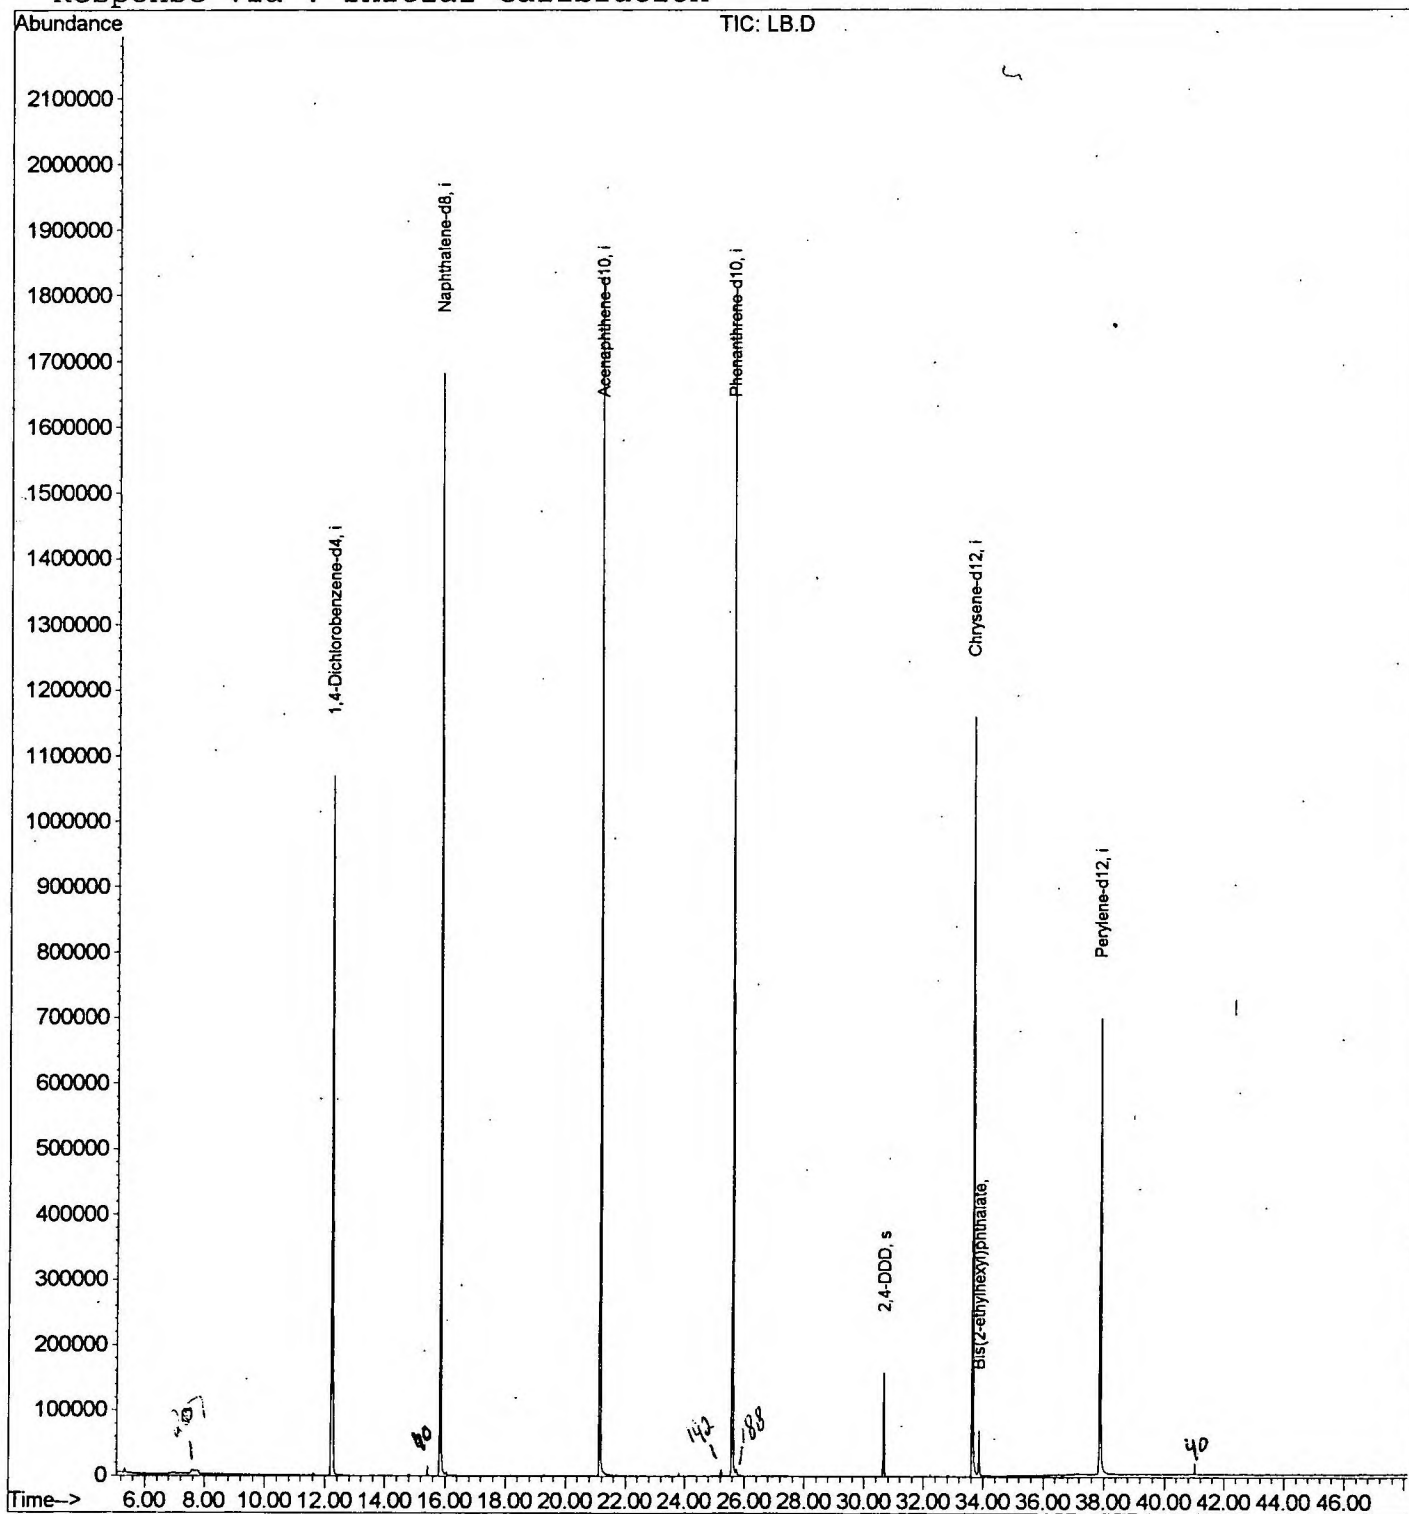

LSC Area Percent Report

• Data File : C:\HPCHEM\1\DATA\APR1802\LB.D
 Acq On : 18 Apr 2002 3:53 pm
 Sample : GC/MS SCAN 3/25
 Misc :
 MS Integration Params: LSCINT.P

Vial: 5
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	12.213	775	781	799	rBV	1068786	2723462	70.87%	14.509%
2	15.848	1171	1177	1193	rBV	1681356	3426450	89.16%	18.254%
3	21.145	1748	1754	1775	rBV	1828323	3843169	100.00%	20.474%
4	25.588	2231	2238	2250	rBV2	1808145	3699777	96.27%	19.710%
5	30.665	2786	2791	2796	rBV	158165	300641	7.82%	1.602%
6	33.640	3109	3115	3129	rBV2	1159236	2681736	69.78%	14.287%
7	33.860	3134	3139	3147	rVB	69166	135099	3.52%	0.720%
8	37.872	3568	3576	3592	rBV2	694876	1960718	51.02%	10.445%




Sum of corrected areas: 18771052

LB.D GCMS0412.M

Fri Apr 19 09:06:15 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR1802\LB.D
 Operator :
 Acquired : 18 Apr 2002 3:53 pm using AcqMethod GCMS0412
 Instrument : 209
 Sample Name: GC/MS SCAN 3/25
 Misc Info :
 Vial Number: 5
 Quant File :GCMS0412.RES (RTE Integrator)

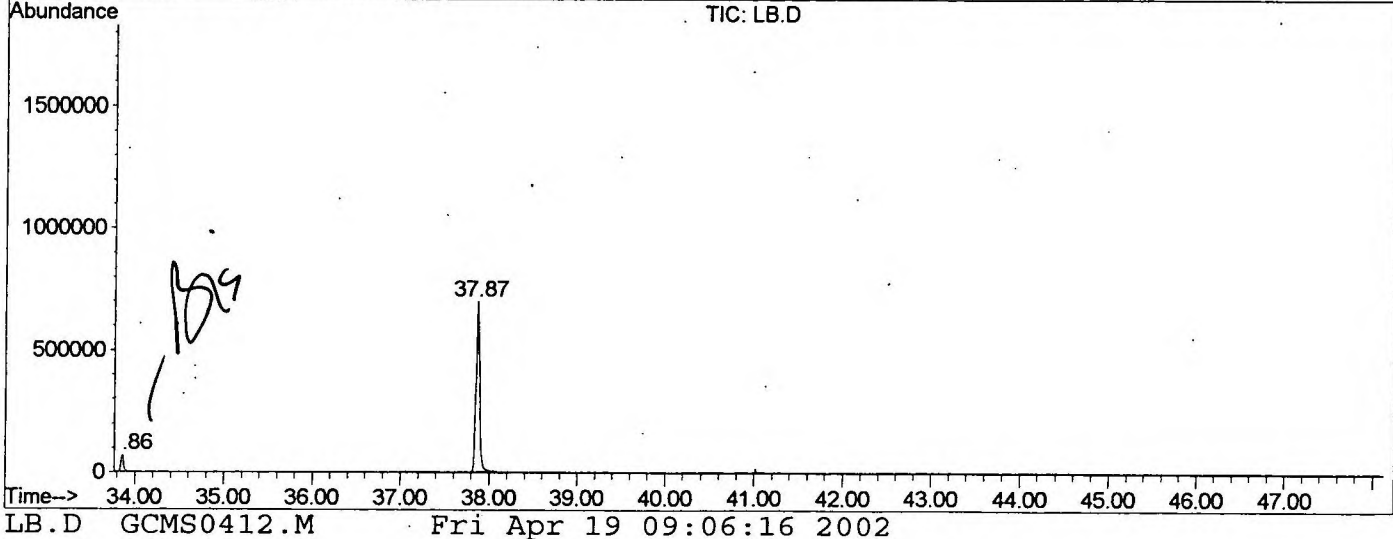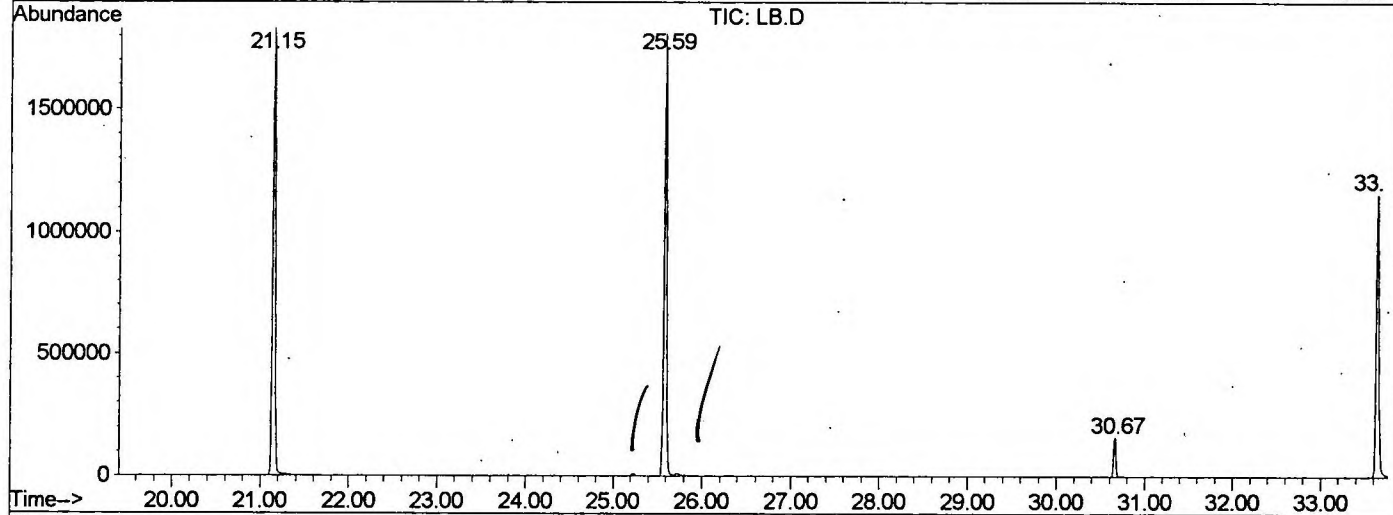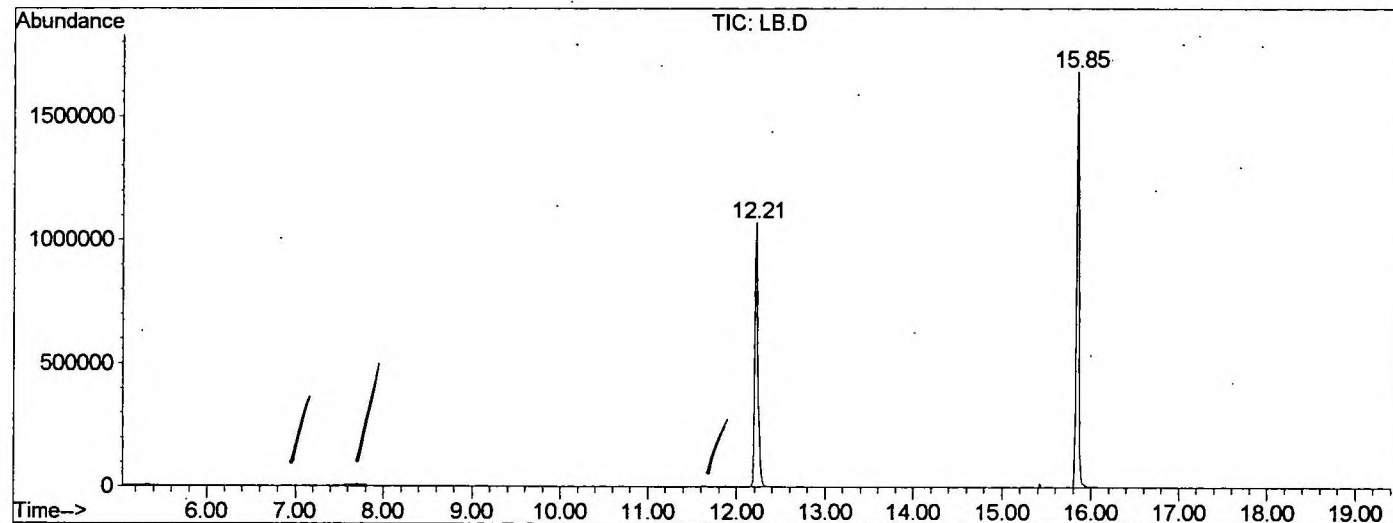

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 18 Apr 2002 3:53 pm
Data File: C:\HPCHEM\1\DATA\APR1802\LB.D
Name: GC/MS SCAN 3/25
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc

LB.D GCMS0412.M	Fri Apr 19	09:06:16	2002					