

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/22/2002 Time: 08:58:07

Sample: AE06984

Analysis: \$GCMS GCMS Scan For Unknowns

Units: ug

Started: 4/22/02 08:57 Ended: 4/22/02 08:57 Analyst: DLV

Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		80		10.0

Comments for Sample AE06984 - Analysis \$GCMS

Westchester Dept. of Labs & Research.

User: Vinci, David L

Date: 04-22-2002 Time: 08:58:33

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recovery for 7 of the 43 compounds in the LCS Standard were low.

Quantitation Report (QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR1802\6984.D
 Acq On : 18 Apr 2002 9:44 pm
 Sample : GC/MS SCAN 3/25 FB
 Misc :
 MS Integration Params: GOOFY.P
 Quant Time: Apr 19 8:53 2002

Vial: 11
 Operator:
 Inst : 209
 Multiplr: 1.00

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Last Update : Wed Apr 17 11:48:30 2002
 Response via : Initial Calibration
 DataAcq Meth : GCMS0412

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	12.21	152	583655	20.00	ug/l	-0.03
10) Naphthalene-d8	15.85	136	2107855	20.00	ug/l	-0.03
17) Acenaphthene-d10	21.15	164	1187808	20.00	ug/l	-0.03
30) Phenanthrene-d10	25.59	188	1726770	20.00	ug/l	-0.03
39) Chrysene-d12	33.64	240	1086990	20.00	ug/l	-0.04
45) Perylene-d12	37.87	264	703262	20.00	ug/l	-0.05

System Monitoring Compounds

28) TCMX	0.00	209	0	0.00	ug/L	
Spiked Amount	10.000		Recovery	=	0.00%	
38) 2,4-DDD	30.66	235	80561	4.01	ug/mL	0.16
Spiked Amount	5.000		Recovery	=	80.20%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-Chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3-Dichlorobenzene	0.00	146	0	N.D.	
5) 1,4-Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2-Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2'-oxybis(1-Chloropropan	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methane	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	15.89	128	269	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-Chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	21.45	165	276	N.D.	
25) Diethylphthalate	22.62	149	1284	N.D.	
26) 4-Chlorophenyl-phenylether	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	168	0	N.D.	
32) 4-Bromophenyl-phenylether	0.00	248	0	N.D.	

(#) = qualifier out of range (m) = manual integration

6984.D GCMS0412.M Fri Apr 19 08:53:58 2002

Page 1

Quantitation Report

(QT Reviewed)

Data File : C:\HPCHEM\1\DATA\APR1802\6984.D

Vial: 11

Acq On : 18 Apr 2002 9:44 pm

Operator:

Sample : GC/MS SCAN 3/25 FB

Inst : 209

Misc :

Multiplr: 1.00

MS Integration Params: GOOFY.P

Quant Time: Apr 19 8:53 2002

Quant Results File: GCMS0412.RES

Quant Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)

Title : 209 625/TCLP calibration table

Last Update : Wed Apr 17 11:48:30 2002

Response via : Initial Calibration

DataAcq Meth : GCMS0412

Compound	R.T.	QIon	Response	Conc Unit	Qvalue
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	25.60	178	538	N.D.	
35) Anthracene	25.60	178	538	N.D.	
36) Di-n-butylphthalate	27.55	149	2342	N.D.	
37) Fluoranthene	29.28	202	102	N.D.	
40) Pyrene	0.00	202	0	N.D.	
41) Butylbenzylphthalate	0.00	149	0	N.D.	
42) Benzo(a)anthracene	33.65	228	3109	N.D.	
43) Bis(2-ethylhexyl)phthalate	33.86	149	74224	2.72 ug/l	97
44) Chrysene	33.71	228	1741	N.D.	
46) Di-n-Octylphthalate	35.60	149	503	N.D.	
47) Benzo(b)fluoranthene	36.69	252	1159	N.D.	
48) Benzo(k)fluoranthene	36.75	252	1369	N.D.	
49) Benzo(a)pyrene	37.87	252	3037	N.D.	
50) Indeno(1,2,3-cd)pyrene	0.00	276	0	N.D.	
51) Dibenz(a,h)anthracene	0.00	278	0	N.D.	
52) Benzo(g,h,i)perylene	0.00	276	0	N.D.	

 (#) = qualifier out of range (m) = manual integration

6984.D GCMS0412.M

Fri Apr 19 08:53:59 2002

Page 2


Quantitation Report

Data File : C:\HPCHEM\1\DATA\APR1802\6984.D
Acq On : 18 Apr 2002 9:44 pm
Sample : GC/MS SCAN 3/25 FB
Misc :
MS Integration Params: GOOFY.P
Quant Time: Apr 19 8:53 2002

Vial: 11
Operator:
Inst : 209
Multiplr: 1.00

Quant Results File: GCMS0412.RES

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title : 209 625/TCLP calibration table
Last Update : Wed Apr 17 11:48:30 2002
Response via : Initial Calibration

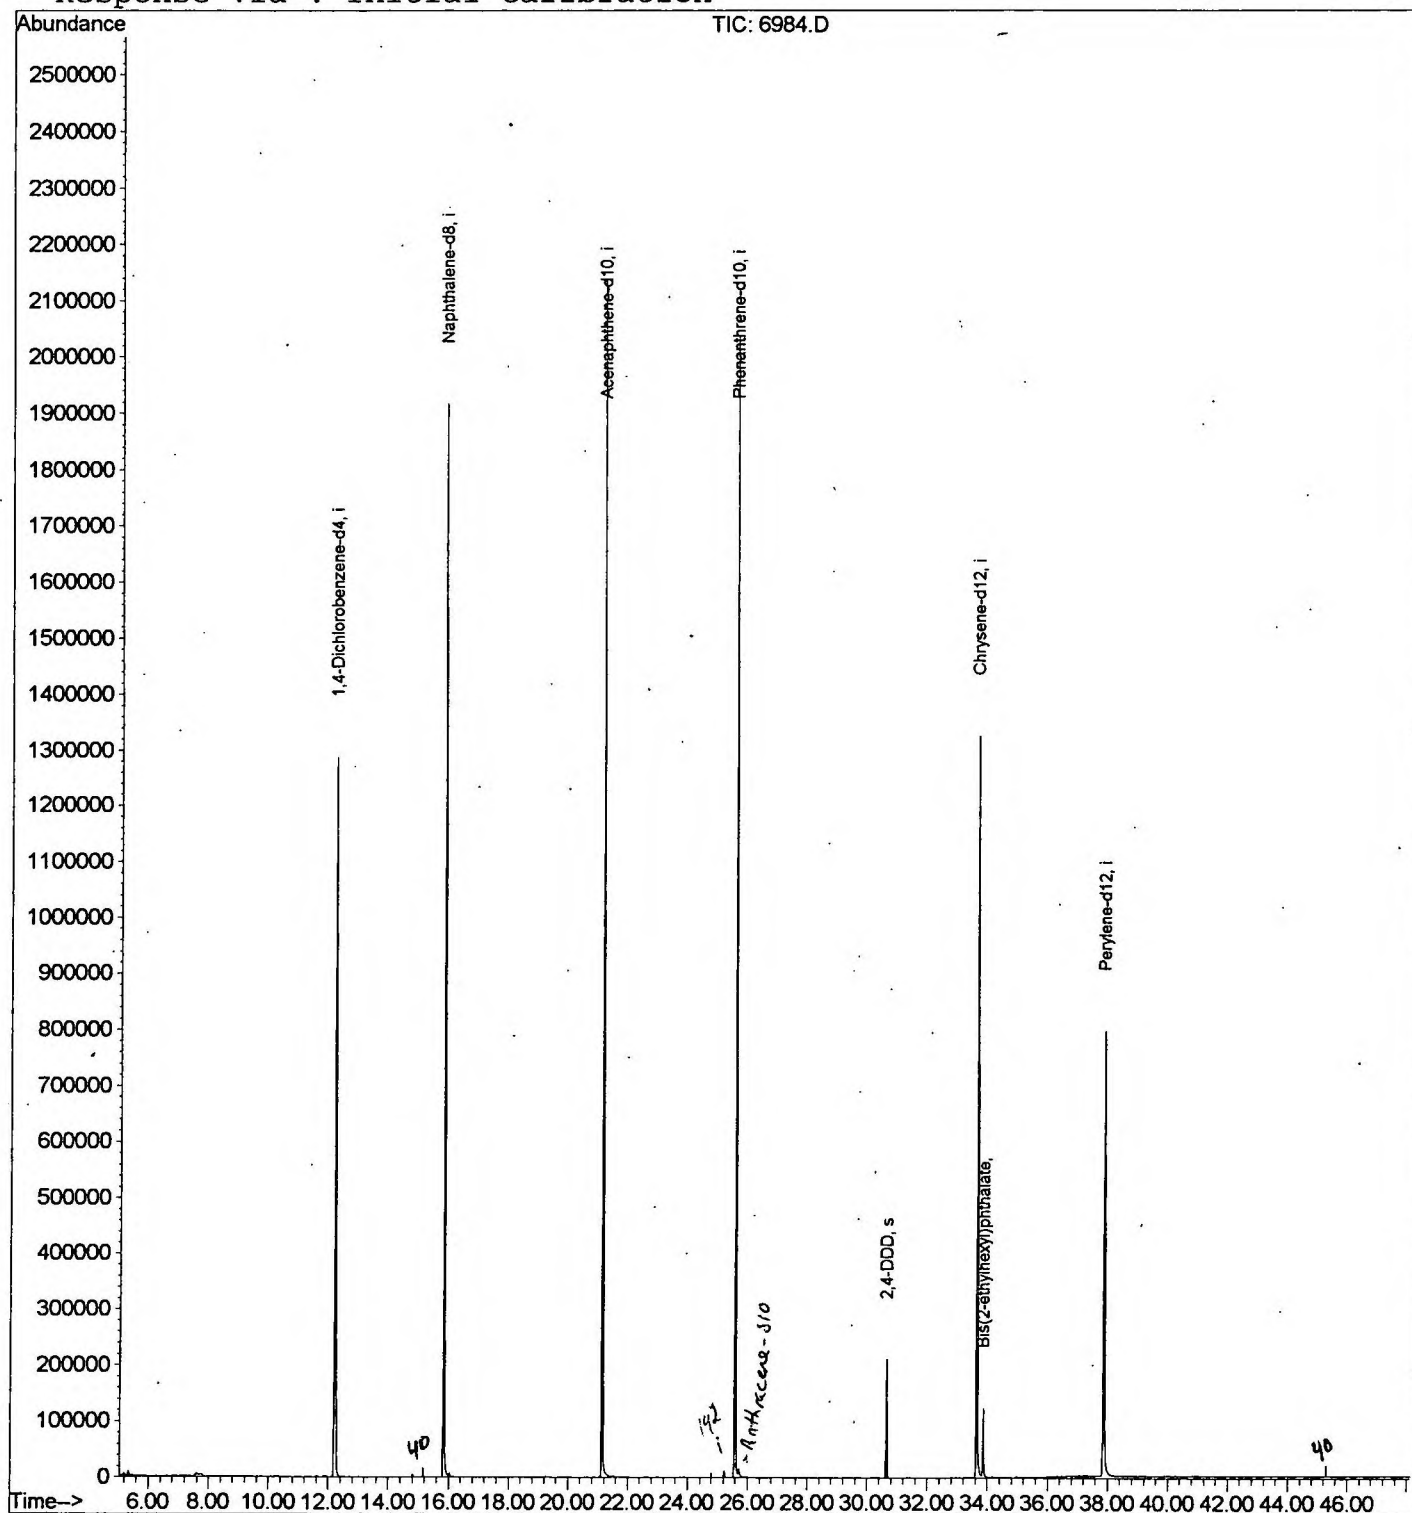

LSC Area Percent Report

Data File : C:\HPCHEM\1\DATA\APR1802\6984.D
 Acq On : 18 Apr 2002 9:44 pm
 Sample : GC/MS SCAN 3/25 FB
 Misc :
 MS Integration Params: LSCINT.P

Vial: 11
 Operator:
 Inst : 209
 Multiplr: 1.00

Method : C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
 Title : 209 625/TCLP calibration table
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Signal : TIC




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	peak area	peak % max.	% of total
1	12.213	775	781	800	rVB	1286521	3118050	69.81%	14.208%
2	15.849	1170	1177	1194	rBV	1917184	3970034	88.89%	18.091%
3	21.146	1748	1754	1771	rBV	2139555	4466426	100.00%	20.353%
4	25.589	2231	2238	2250	rBV2	2039216	4295147	96.17%	19.572%
5	30.656	2785	2790	2798	rVB	210453	392181	8.78%	1.787%
6	33.640	3108	3115	3131	rBV2	1326624	3098811	69.38%	14.121%
7	33.860	3134	3139	3149	rVB	121806	250376	5.61%	1.141%
8	37.872	3567	3576	3592	rBV	794157	2354197	52.71%	10.728%

Sum of corrected areas: 21945222

6984.D GCMS0412.M Fri Apr 19 09:05:40 2002

LSC Report - Integrated Chromatogram

File : C:\HPCHEM\1\DATA\APR1802\6984.D
 Operator :
 Acquired : 18 Apr 2002 9:44 pm using AcqMethod GCMS0412
 Instrument : 209
 Sample Name: GC/MS SCAN 3/25 FB
 Misc Info :
 Vial Number: 11
 Quant File :GCMS0412.RES (RTE Integrator)

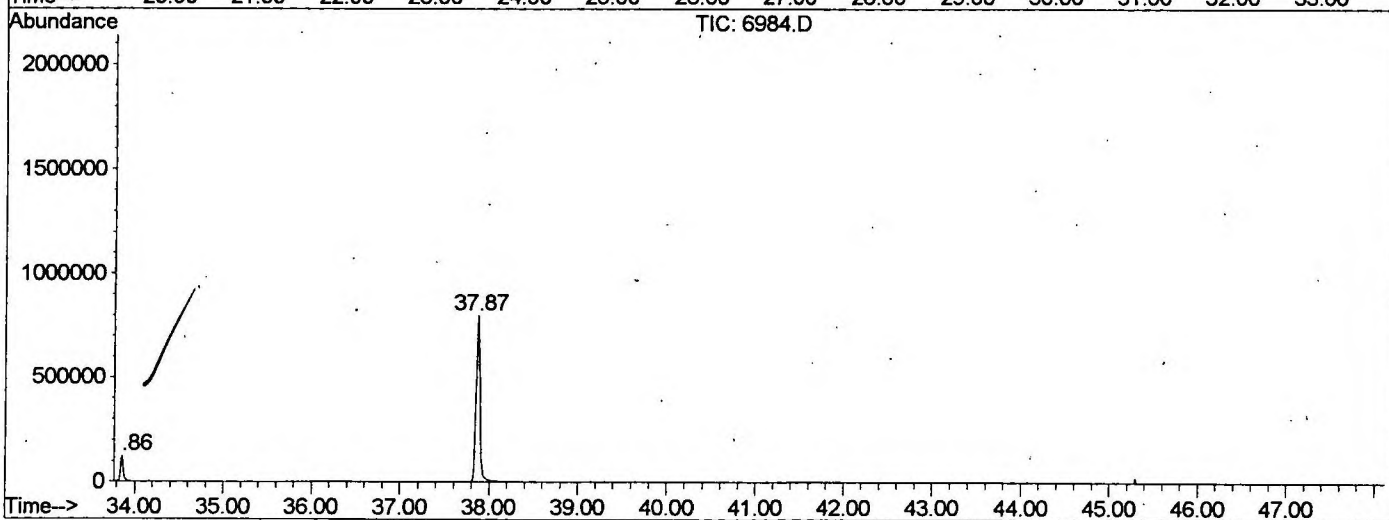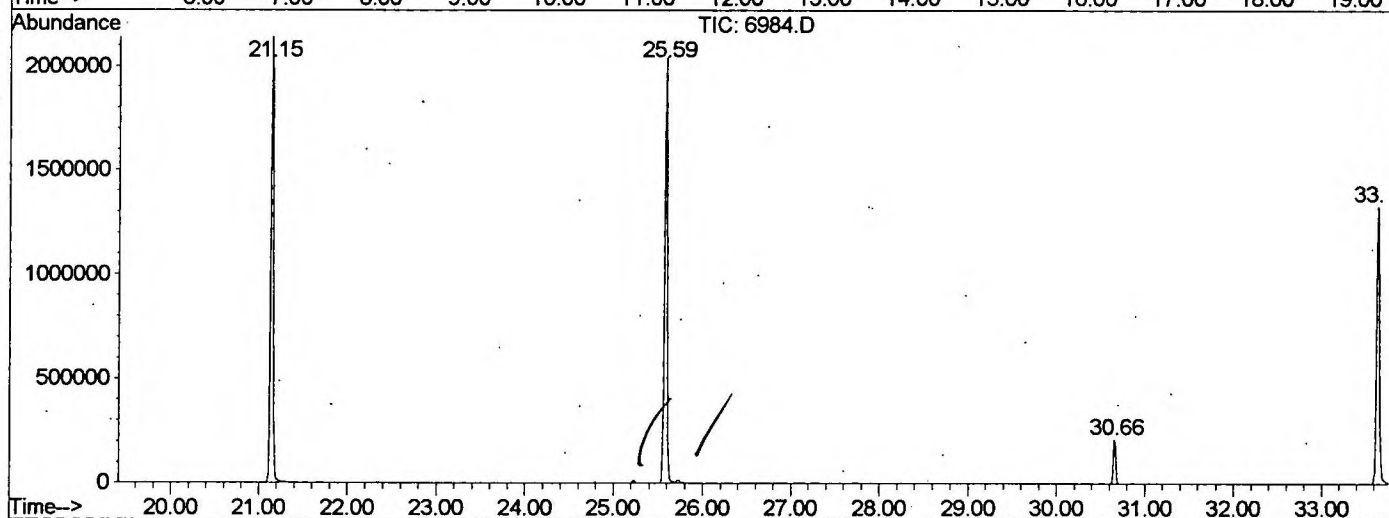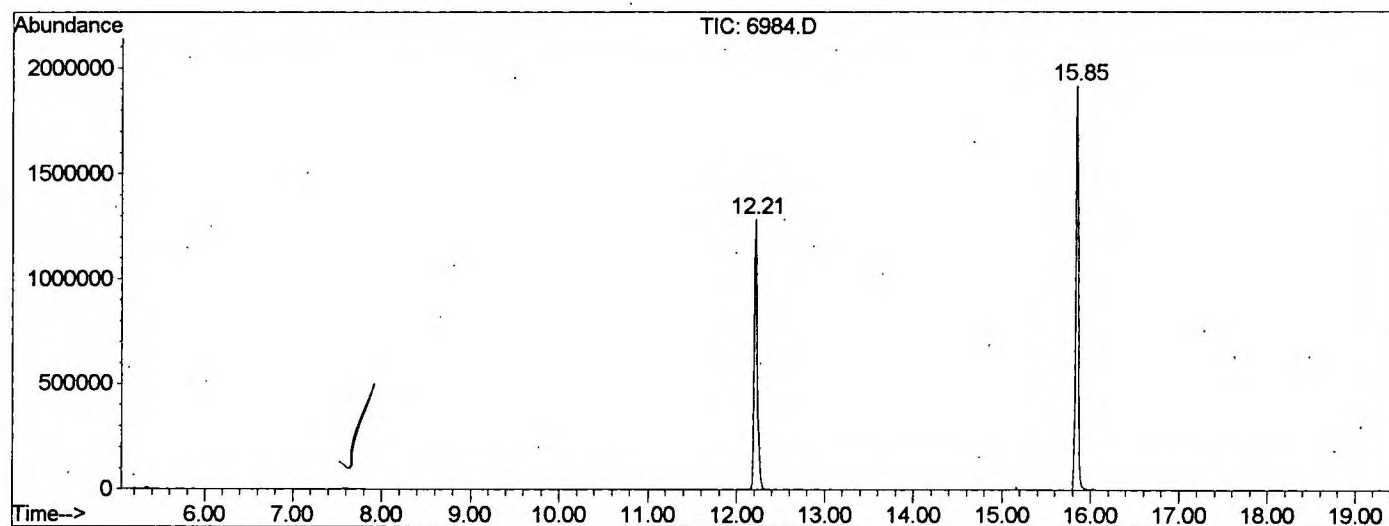

6984.D GCMS0412.M Fri Apr 19 09:05:40 2002

Tentatively Identified Compound (LSC) summary

Operator ID: Date Acquired: 18 Apr 2002 9:44 pm
Data File: C:\HPCHEM\1\DATA\APR1802\6984.D
Name: GC/MS SCAN 3/25 FB
Misc:
Method: C:\HPCHEM\1\METHODS\GCMS0412.M (RTE Integrator)
Title: 209 625/TCLP calibration table
Library Searched: C:\DATABASE\NBS75K.L

TIC Top	Hit name	RT	EstConc	Units	Area	IntStd	ISRT	ISArea	ISConc
6984.D	GCMS0412.M	Fri Apr 19 09:05:41 2002							