


File : C:\MSDCHEM\1\DATA\041702\DFTAA417.D
Operator : Bohlk
Acquired : 17 Apr 2002 8:29 am using AcqMethod 508SCAN
Instrument : Instrumen
Sample Name: DFTPP
Misc Info :
Vial Number: 1

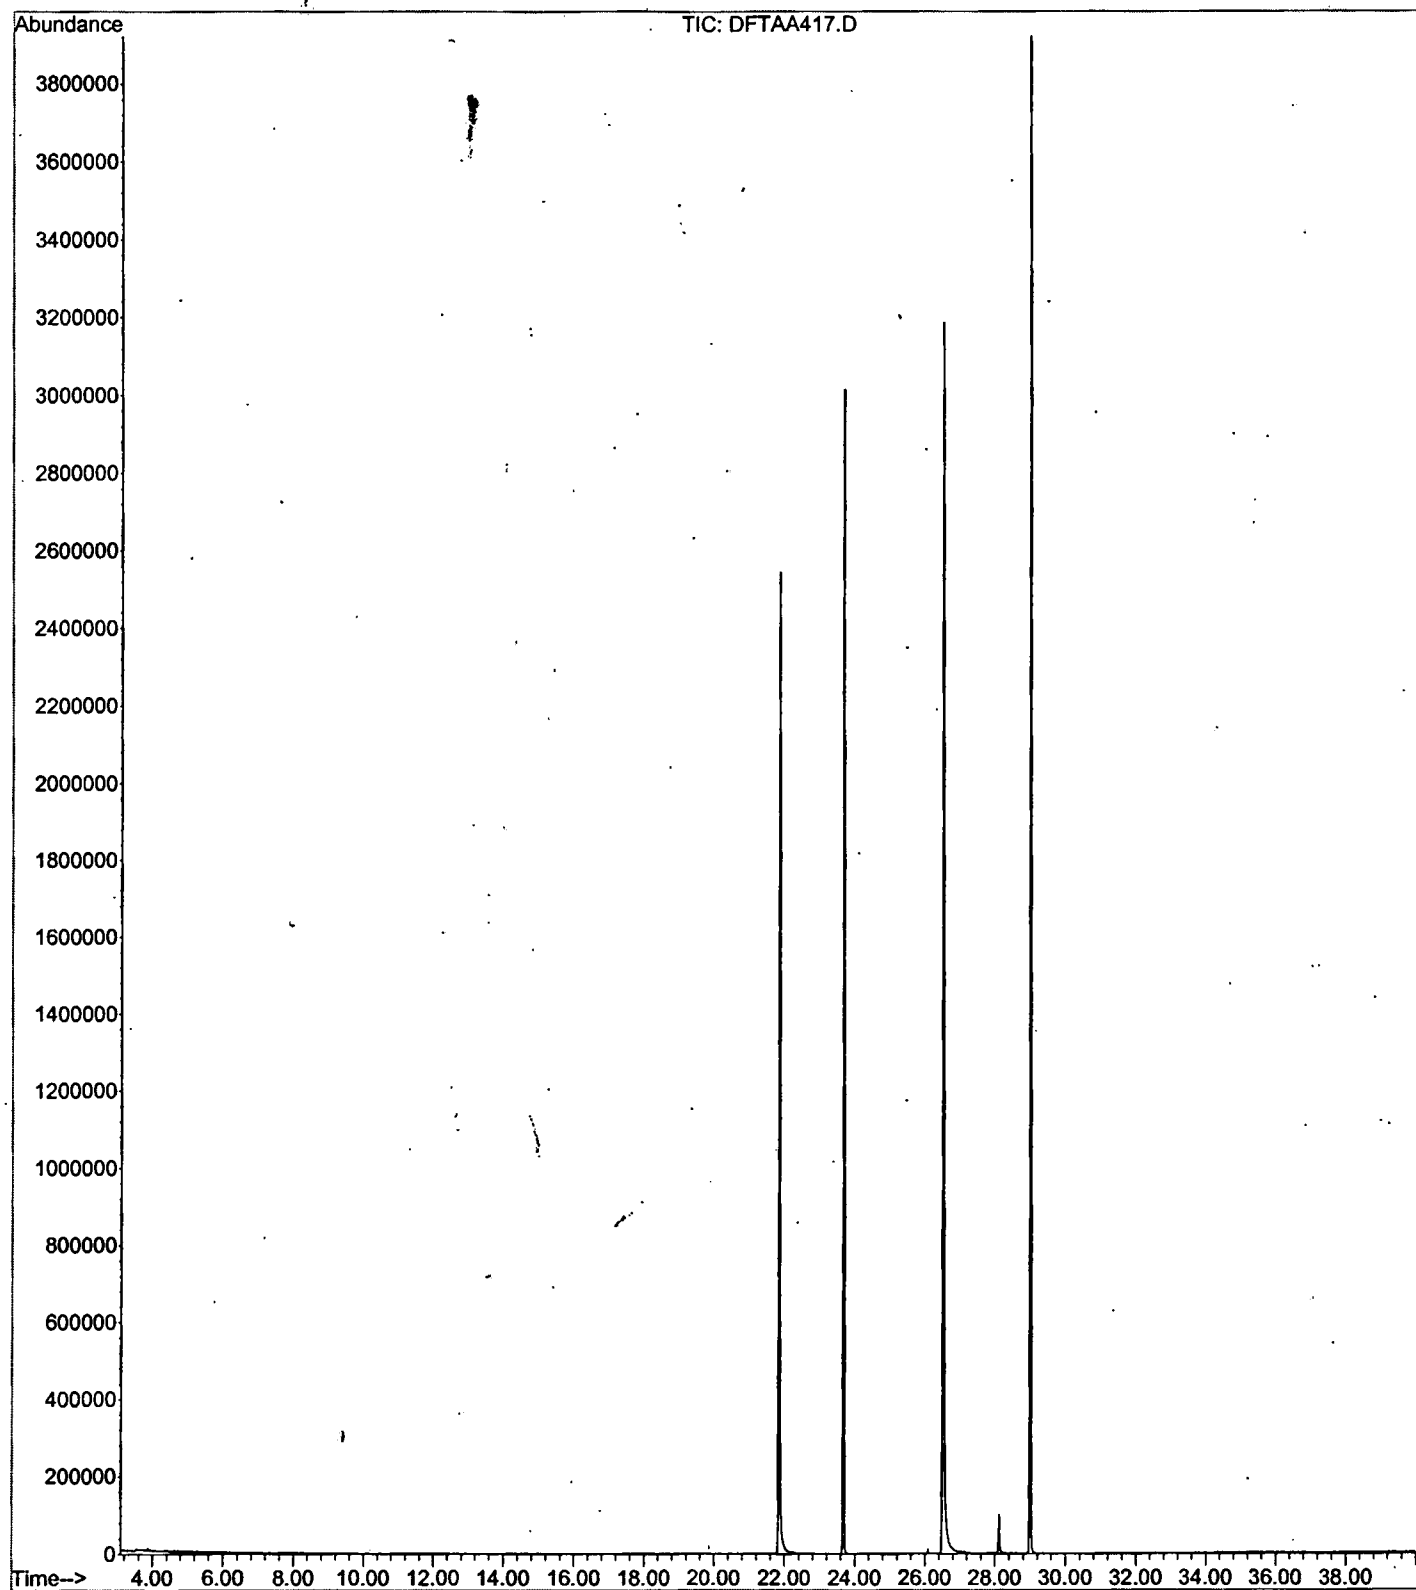

DFTPP

Data File : C:\MSDCHEM\1\DATA\041702\DFTAA417.D
Acq On : 17 Apr 2002 8:29 am
Sample : DFTPP
Misc :
MS Integration Params: BENZO.P

Vial: 1
Operator: Bohlk
Inst : Instrumen
Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
Title : Quantitation For Method 508gcscan

Spectrum Information: Scan 3506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	44.4	165184	PASS
68	69	0.00	2	1.4	2428	PASS
69	198	0.00	100	46.2	172032	PASS
70	69	0.00	2	0.3	598	PASS
127	198	40	60	49.3	183424	PASS
197	198	0.00	1	0.6	2175	PASS
198	198	100	100	100.0	372288	PASS
199	198	5	9	7.3	27080	PASS
275	198	10	30	18.8	69984	PASS
365	198	1	100	1.8	6692	PASS
441	443	0.01	100	82.4	31600	PASS
442	198	40	110	53.6	199488	PASS
443	442	17	23	19.2	38344	PASS

DFTAA417.D 5080402BBC.M

Wed Apr 17 09:12:45 2002