

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/23/2002 Time: 11:38:32

Sample: AE06958
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/23/02 11:37 Ended: 4/23/02 11:37 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		99		10.0

Comments for Sample AE06958 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-23-2002 Time: 11:39:43

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\041702\6958.D

Vial: 12

Acq On : 17 Apr 2002 5:46 pm

Operator: Bohlk

Sample : SAMPLE 6958 3/25/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 22 11:38:30 2002

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.41	152	499337	40.00	ug/L	0.00
10) Naphthalene-d8	12.89	136	2193270	40.00	ug/L	0.00
17) Acenaphthene-d10	17.99	164	1246438	40.00	ug/L	0.00
30) Phenanthrene-d10	22.34	188	1760892	40.00	ug/L	0.00
39) Chrysene-d12	30.14	240	1404533	40.00	ug/L	-0.01
45) Perylene-d12	34.01	264	841738	40.00	ug/L	0.00

System Monitoring Compounds

28) TCMX (SURR)	0.00	244	0	0.00	ug/L	
Spiked Amount	10.000		Recovery	=	0.00%	
38) 2,4-DDD (SURR)	27.28	235	129846	9.90	ug/L	0.01
Spiked Amount	10.000		Recovery	=	99.00%	

Target Compounds

						Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	d	
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.		
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.		
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	12.94	128	7262	0.14	ug/L	80
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
25) Diethylphthalate	0.00	149	0	N.D.		
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
31) N-Nitrosodiphenylamine	0.00	169	0	N.D.		
32) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.		
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	0.00	178	0	N.D.	d	
35) Anthracene	0.00	178	0	N.D.	d	
36) Di-n-butylphthalate	0.00	149	0	N.D.	d	
37) Fluoranthene	0.00	202	0	N.D.		
40) Pyrene	0.00	202	0	N.D.		
41) Butylbenzylphthalate	0.00	149	0	N.D.		
42) Benzo (a) anthracene	0.00	228	0	N.D.	d	
43) Bis (2-ethylhexyl) phthala	30.77	149	30305	0.87	ug/L	99
44) Chrysene	0.00	228	0	N.D.	d	

(#)= qualifier out of range (m) = manual integration

6958.D 5080402BBC.M Mon Apr 22 11:41:47 2002

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\041702\6958.D

Vial: 12

Acq On : 17 Apr 2002 5:46 pm

Operator: Bohlk

Sample : SAMPLE 6958 3/25/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 22 11:38:30 2002

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo (b) fluoranthene	0.00	252	0	N.D.		
48) Benzo (k) fluoranthene	0.00	252	0	N.D.		
49) Benzo (a) pyrene	0.00	252	0	N.D.	d	
50) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
51) Dibenzo (a,h) anthracene	0.00	278	0	N.D.		
52) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

6958.D 5080402BBC.M

Mon Apr 22 11:41:48 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\041702\6958.D

Vial: 12

Acq On : 17 Apr 2002 5:46 pm

Operator: Bohlk

Sample : SAMPLE 6958 3/25/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 22 11:41 2002


Quant Results File: 5080402BBC.RES

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

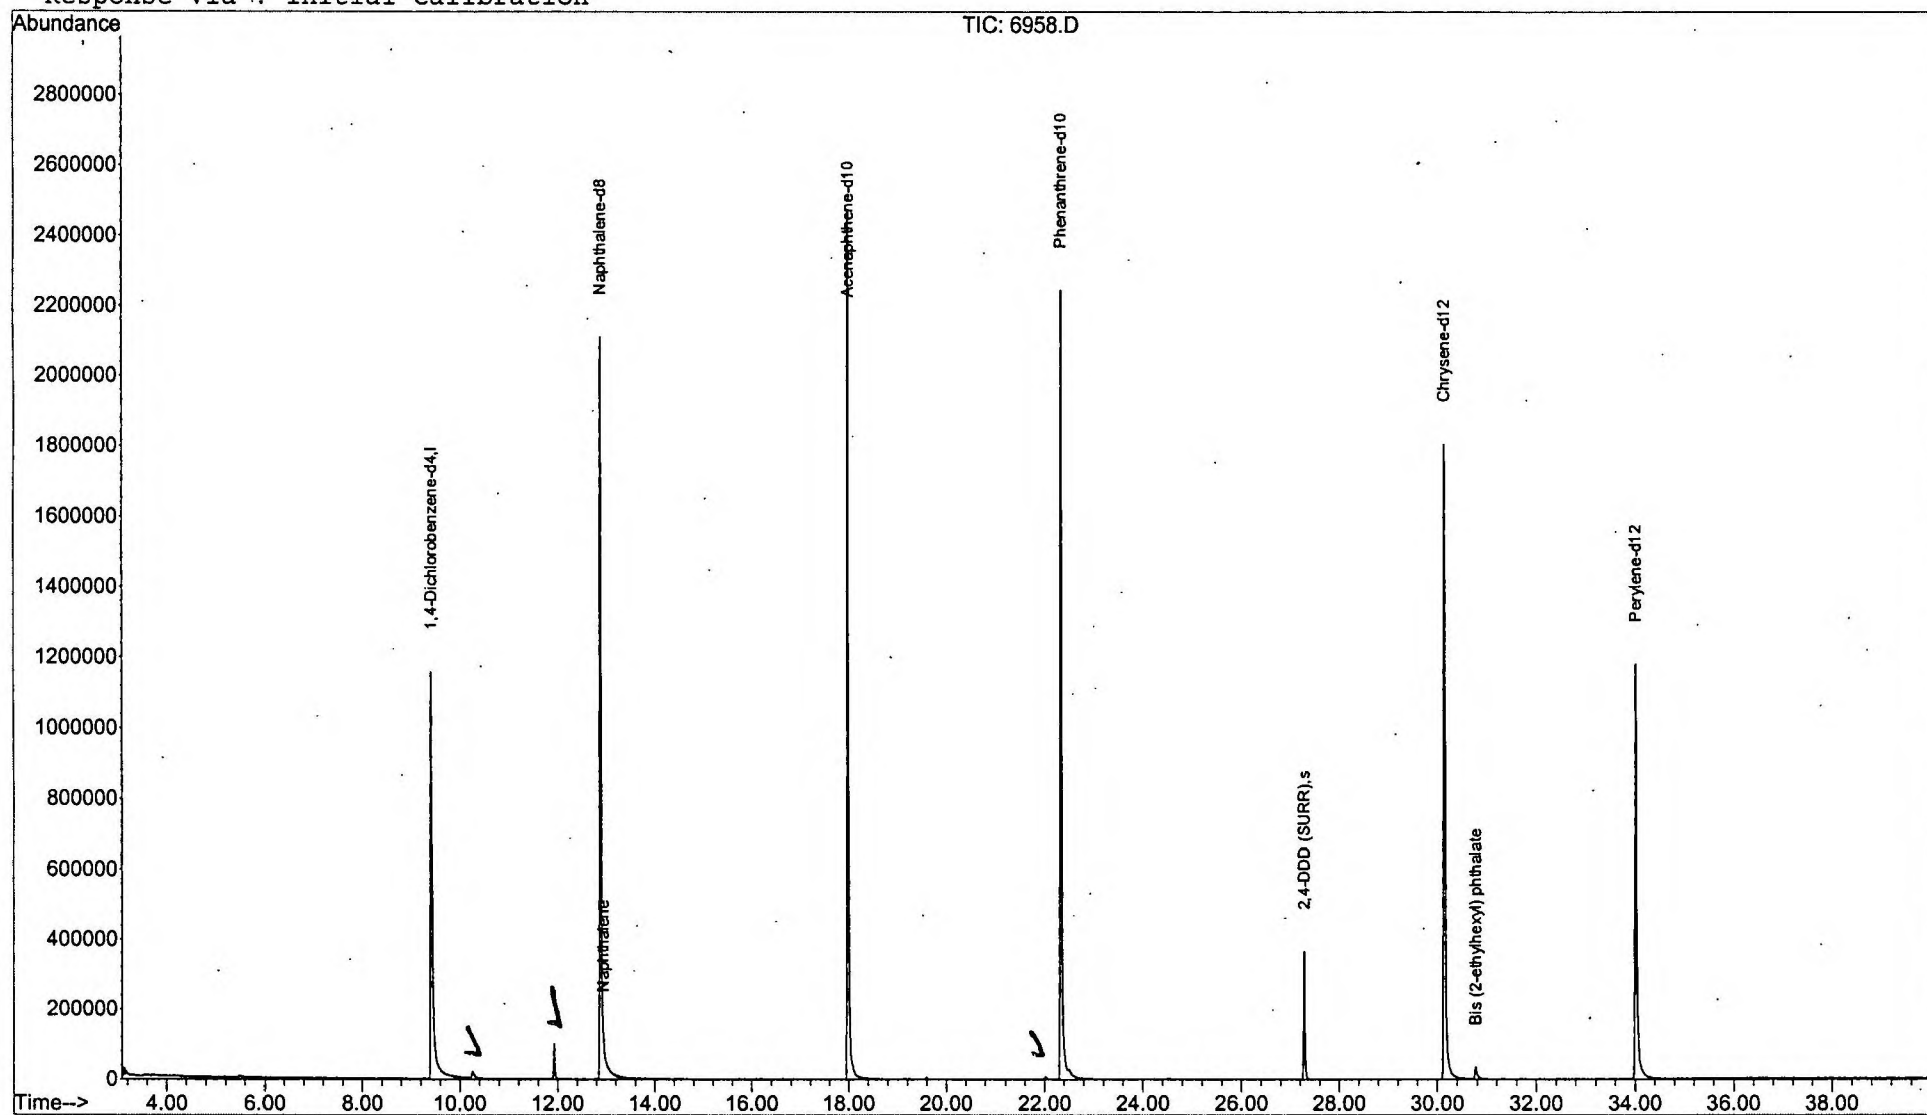

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\041702\6958.D

Acq On : 17 Apr 2002 5:46 pm

Sample : SAMPLE 6958 3/25/02

Misc :

MS Integration Params: LSCINT.P

Vial: 12

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.413	1072	1078	1103	rBV	1155226	3255544	61.05%	12.098%
2	11.928	1499	1506	1517	rBV	100862	183552	3.44%	0.682%
3	12.886	1661	1669	1693	rBV	2109080	4773323	89.52%	17.739%
4	17.991	2529	2538	2562	rBV	2470474	5332261	100.00%	19.816%
5	22.339	3268	3278	3299	rBV2	2244592	5097270	95.59%	18.943%
6	27.281	4112	4119	4131	rBV2	362715	692938	13.00%	2.575%
7	30.142	4596	4606	4628	rBV3	1804474	4366476	81.89%	16.227%
8	30.771	4706	4713	4723	rBV5	34304	94504	1.77%	0.351%
9	34.020	5254	5266	5297	rBV2	1177879	3113076	58.38%	11.569%

Sum of corrected areas: 26908944

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\041702\6958.D
Operator : Bohlk
Acquired : 17 Apr 2002 5:46 pm using AcqMethod 508SCAN
Instrument : Instrumen
Sample Name: SAMPLE 6958 3/25/02
Misc Info :
Vial Number: 12
Quant File : 5080402BBC.RES (RTE Integrator)

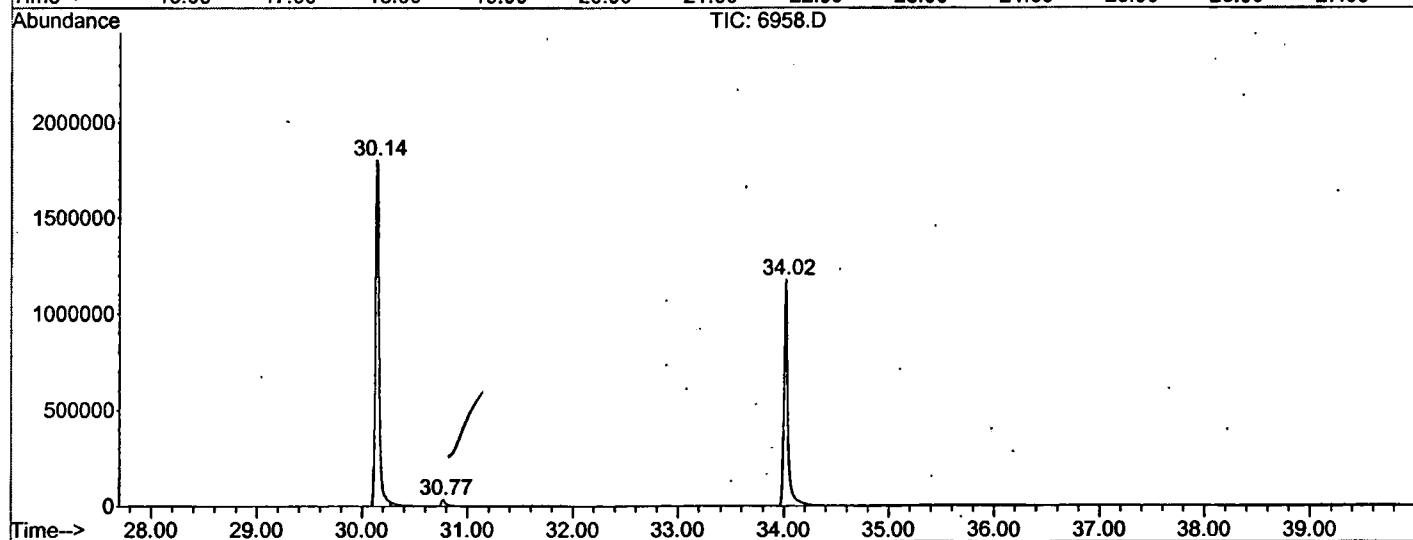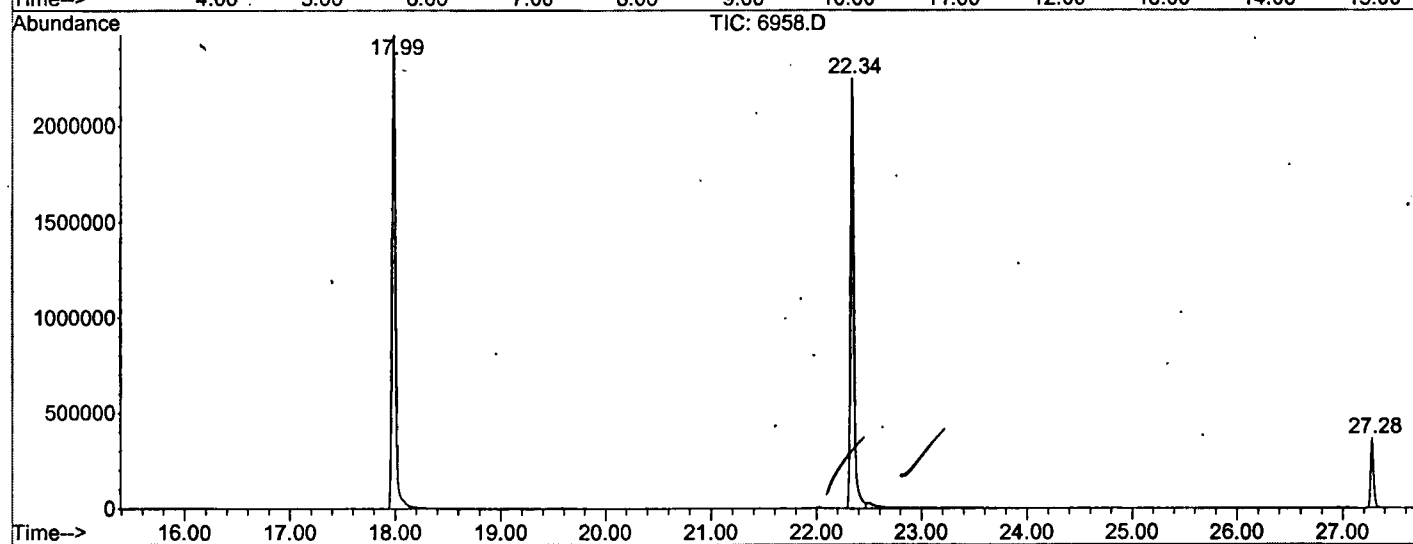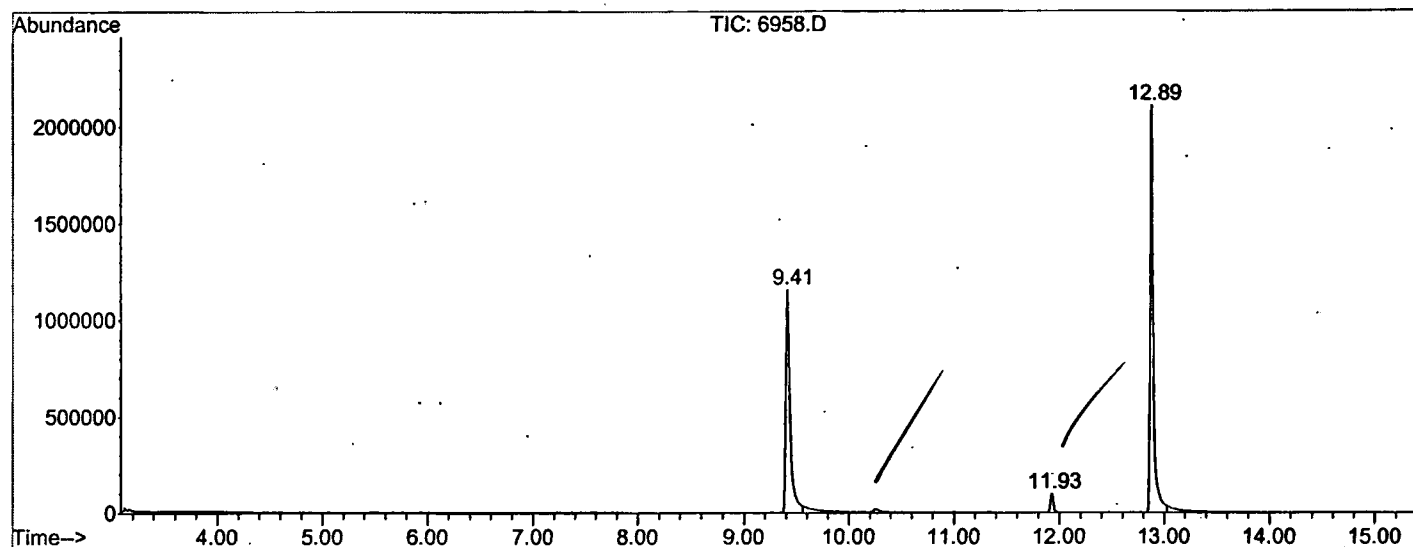

Library Search Compound Report

Data File : C:\MSDCHEM\1\DATA\041702\6958.D
 Acq On : 17 Apr 2002 5:46 pm
 Sample : SAMPLE 6958 3/25/02
 Misc :
 MS Integration Params: LSCINT.P










Vial: 12
 Operator: Bohlk
 Inst : Instrumen
 Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
 Title : Quantitation For Method 508gcscan
 Library : C:\DATABASE\WILEY7N.L

 Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.93	1.54 ug/L	183552	Naphthalene-d8	12.89

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	90
2			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	50
3			Benzeneethanamine, N-[(pentafluorophenyl)methyl]-	475	C21H26F5NO2Si2	055429-85-1	40
4			Benzoic acid, 2-[(trimethylsilyl)ethoxy]-	282	C13H22O3Si2	003789-85-3	40

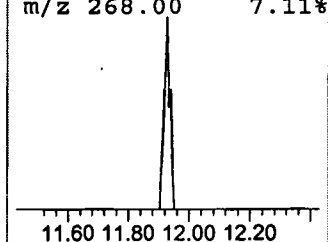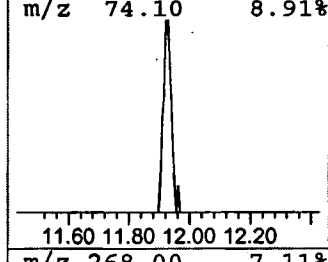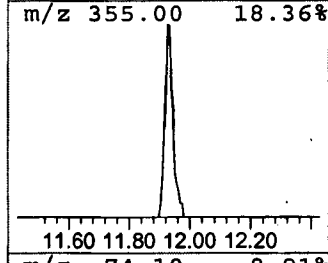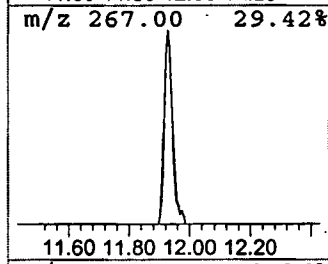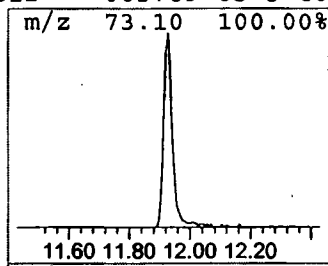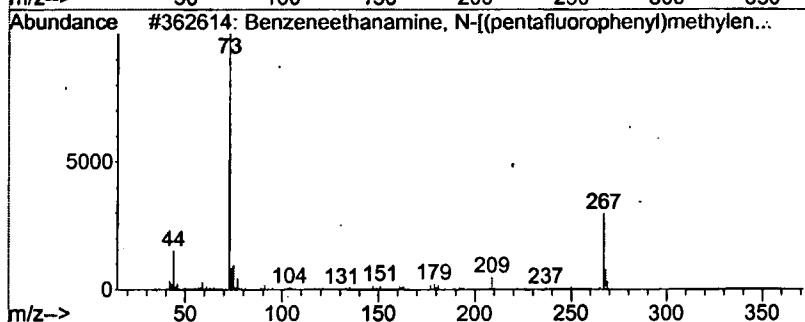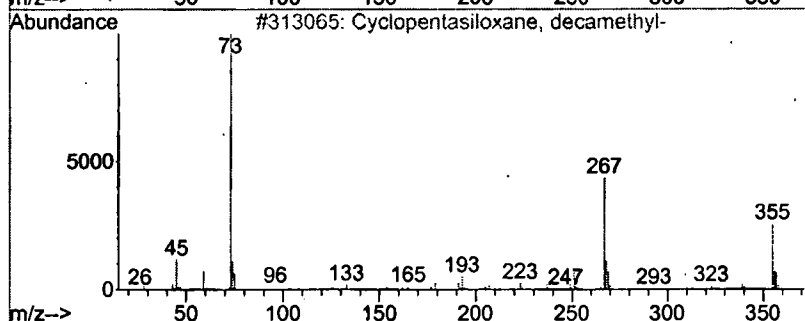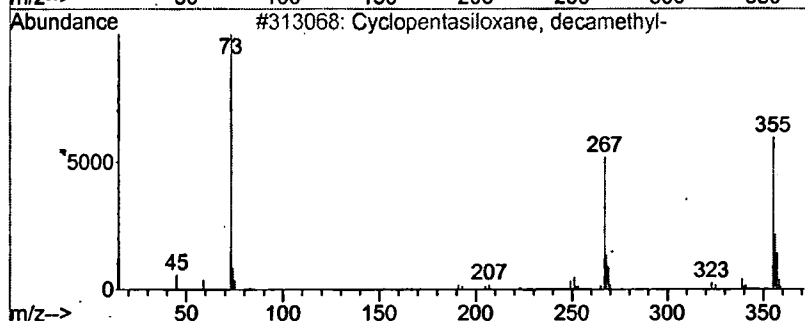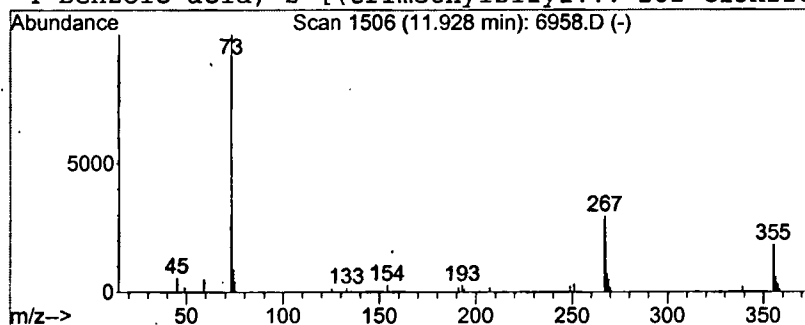

Tentatively Identified Compound (LSC) summary

Operator ID: Bohlk Date Acquired: 17 Apr 2002 5:46 pm
 Data File: C:\MSDCHEM\1\DATA\041702\6958.D
 Name: SAMPLE 6958 3/25/02
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentasiloxan...	11.93	1.5 ug/L		183552	2	12.89	4773320	40.0