

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/23/2002 Time: 11:41:52

Sample: AE06959

Analysis: \$GCMS GCMS Scan For Unknowns

Units: ug

Started: 4/23/02 11:41 Ended: 4/23/02 11:41 Analyst: DLV

Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds				
2	Surr_2,4-DDD		88		10.0

Comments for Sample AE06959 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-23-2002 Time: 11:42:19

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\041702\6959.D

Vial: 13

Acq On : 17 Apr 2002 6:36 pm

Operator: Bohlk

Sample : SAMPLE 6959 3/25/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 22 11:44:12 2002

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.41	152	479504	40.00	ug/L	0.00
10) Naphthalene-d8	12.89	136	2125237	40.00	ug/L	0.00
17) Acenaphthene-d10	17.99	164	1222940	40.00	ug/L	0.00
30) Phenanthrene-d10	22.34	188	1710113	40.00	ug/L	0.00
39) Chrysene-d12	30.15	240	1341960	40.00	ug/L	0.00
45) Perylene-d12	34.01	264	808959	40.00	ug/L	0.00

System Monitoring Compounds

28) TCMX (SURR)	0.00	244	0	0.00	ug/L	
Spiked Amount	10.000		Recovery	=	0.00%	
38) 2,4-DDD (SURR)	27.28	235	111793	8.78	ug/L	0.01
Spiked Amount	10.000		Recovery	=	87.80%	

Target Compounds

						Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	d	
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.		
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.		
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.		
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.		
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.		
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.		
9) Hexachloroethane	0.00	117	0	N.D.		
11) Nitrobenzene	0.00	77	0	N.D.		
12) Isophorone	0.00	82	0	N.D.		
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.		
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.		
15) Naphthalene	0.00	128	0	N.D.		
16) Hexachlorobutadiene	0.00	225	0	N.D.		
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.		
19) 2-chloronaphthalene	0.00	162	0	N.D.		
20) Dimethylphthalate	0.00	163	0	N.D.		
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d	
22) Acenaphthylene	0.00	152	0	N.D.		
23) Acenaphthene	0.00	153	0	N.D.		
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.		
25) Diethylphthalate	0.00	149	0	N.D.		
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.		
27) Fluorene	0.00	166	0	N.D.		
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.		
31) N-Nitrosodiphenylamine	0.00	169	0	N.D.		
32) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.		
33) Hexachlorobenzene	0.00	284	0	N.D.		
34) Phenanthrene	0.00	178	0	N.D.		
35) Anthracene	0.00	178	0	N.D.		
36) Di-n-butylphthalate	0.00	149	0	N.D.	d	
37) Fluoranthene	0.00	202	0	N.D.		
40) Pyrene	0.00	202	0	N.D.		
41) Butylbenzylphthalate	0.00	149	0	N.D.		
42) Benzo (a) anthracene	0.00	228	0	N.D.	d	
43) Bis (2-ethylhexyl) phthala	30:76	149	5433	0.16	ug/L	78
44) Chrysene	0.00	228	0	N.D.	d	

(#) = qualifier out of range (m) = manual integration

6959.D 5080402BBC.M Mon Apr 22 11:46:18 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\041702\6959.D

Vial: 13

Acq On : 17 Apr 2002 6:36 pm

Operator: Bohlk

Sample : SAMPLE 6959 3/25/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 22 11:44:12 2002

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo (b) fluoranthene	0.00	252	0	N.D.		
48) Benzo (k) fluoranthene	0.00	252	0	N.D.		
49) Benzo (a) pyrene	0.00	252	0	N.D.	d	
50) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
51) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
52) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

6959.D 5080402BBC.M

Mon Apr 22 11:46:19 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\041702\6959.D

Vial: 13

Acq On : 17 Apr 2002 6:36 pm

Operator: Bohlk

Sample : SAMPLE 6959 3/25/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 22 11:45 2002


Quant Results File: 5080402BBC.RES

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Tue Apr 16 18:27:45 2002

Response via : Initial Calibration

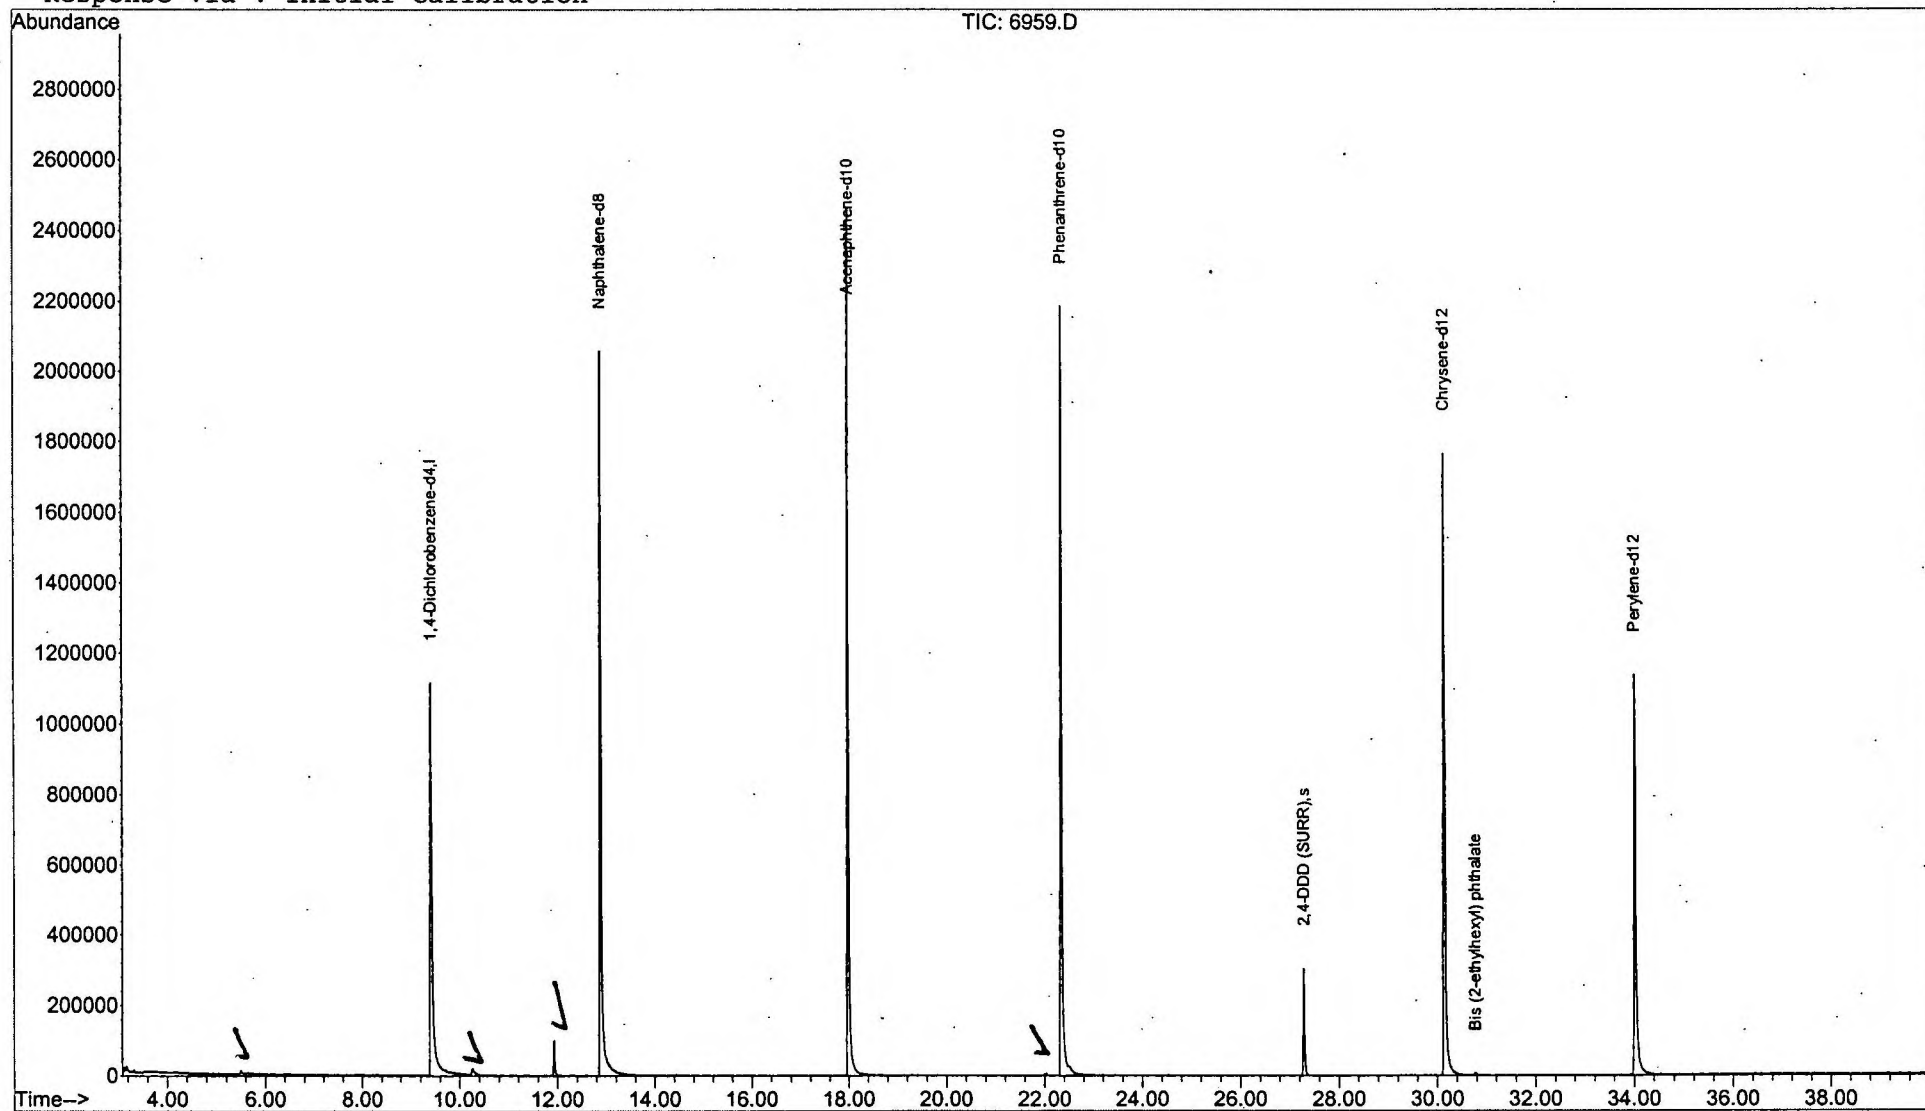

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\041702\6959.D
Acq On : 17 Apr 2002 6:36 pm
Sample : SAMPLE 6959 3/25/02
Misc :
MS Integration Params: LSCINT.P

Vial: 13
Operator: Bohlk
Inst : Instrumen
Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
Title : Quantitation For Method 508gcscan
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.413	1071	1078	1098	rBV	1115216	3127338	59.36%	12.012%
2	11.928	1500	1506	1514	rBV2	98518	178789	3.39%	0.687%
3	12.885	1661	1669	1693	rBV	2057079	4680729	88.85%	17.979%
4	17.991	2529	2538	2568	rBV	2463879	5268164	100.00%	20.235%
5	22.339	3269	3278	3301	rBV2	2186404	4999877	94.91%	19.205%
6	27.281	4112	4119	4132	rBV	304138	596305	11.32%	2.290%
7	30.148	4597	4607	4628	rBV2	1765341	4208126	79.88%	16.164%
8	34.014	5255	5265	5292	rBV2	1138263	2975407	56.48%	11.429%

Sum of corrected areas: 26034735

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\041702\6959.D
 Operator : Bohlk
 Acquired : 17 Apr 2002 6:36 pm using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: SAMPLE 6959 3/25/02
 Misc Info :
 Vial Number: 13
 Quant File :5080402BBC.RES (RTE Integrator)

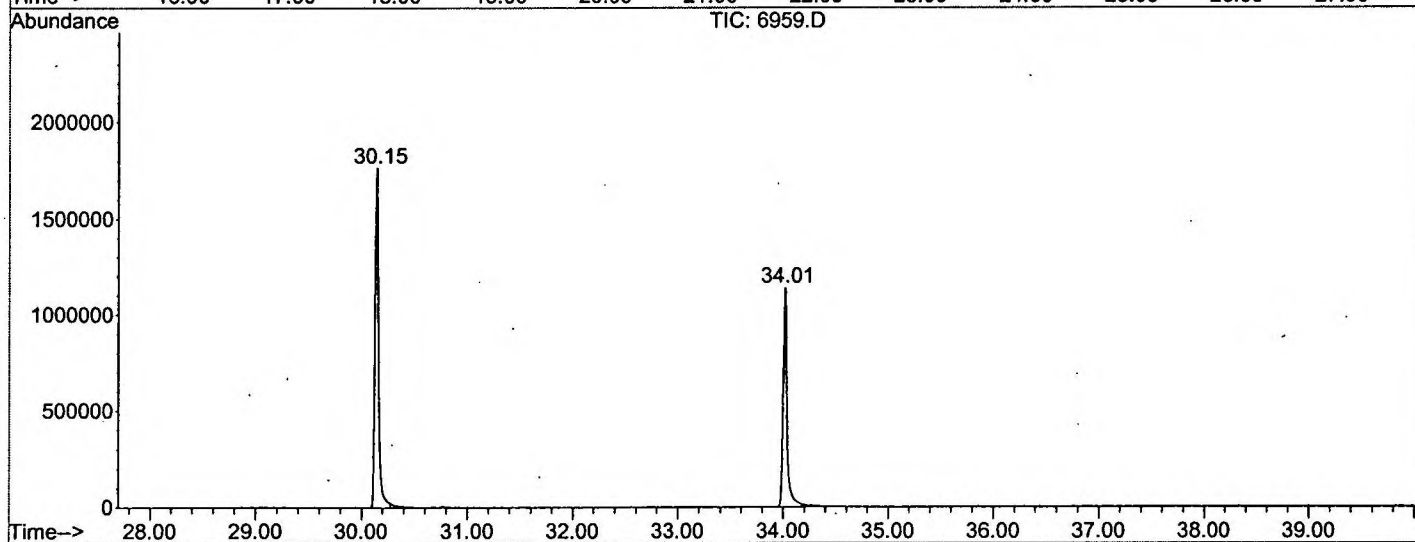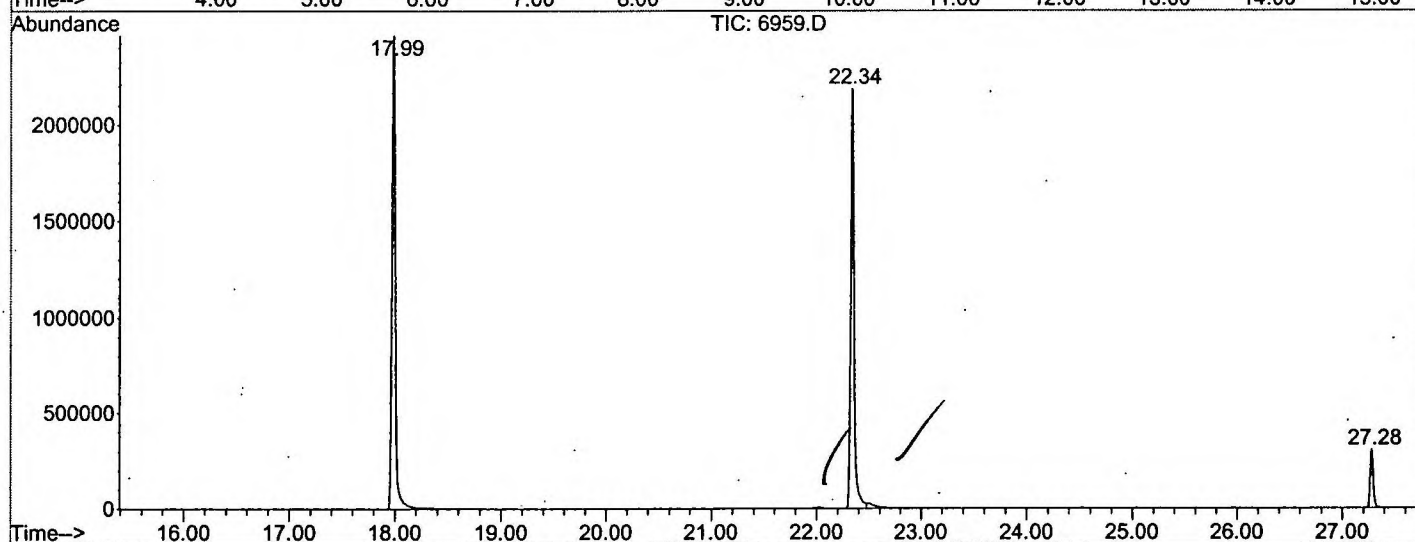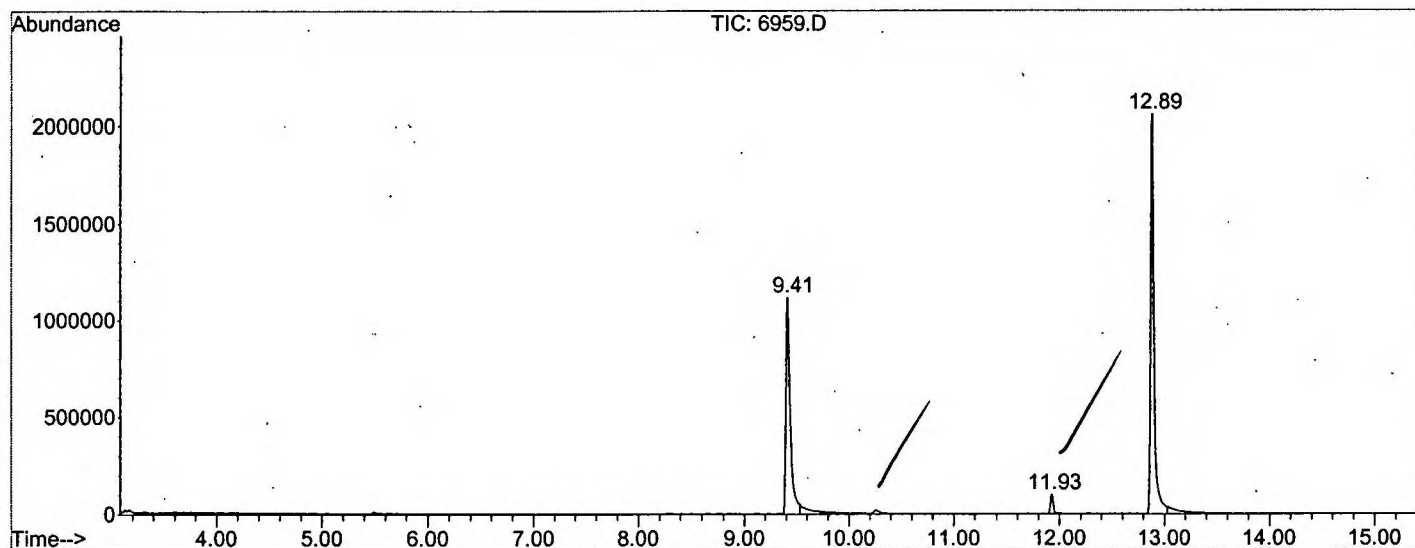

Library Search Compound Report

Data File : C:\MSDCHEM\1\DATA\041702\6959.D

Acq On : 17 Apr 2002 6:36 pm

Sample : SAMPLE 6959 3/25/02

Misc :

MS Integration Params: LSCINT.P

Vial: 13

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)










Title : Quantitation For Method 508gcscan

Library : C:\DATABASE\WILEY7N.L

Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.93	1.53 ug/L	178789	Naphthalene-d8	12.89

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	90
2			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	72
3			Pentasiloxane, 1,1,3,3,5,5,7,7,9...	356	C10H32O4Si5	000995-83-5	40
4			Benzeneethanamine, N-[(pentafluoro...	475	C21H26F5NO2Si2	055429-85-1	33

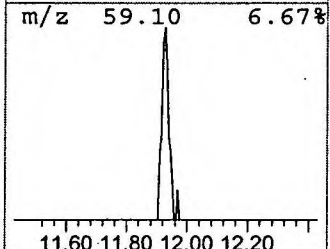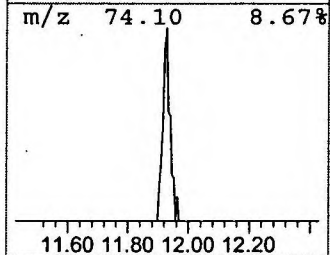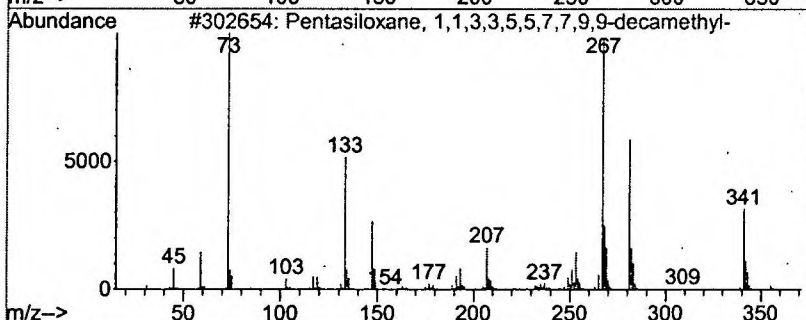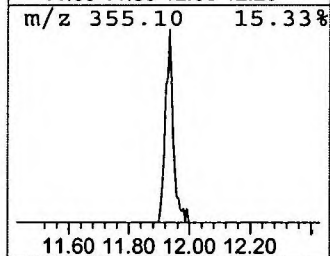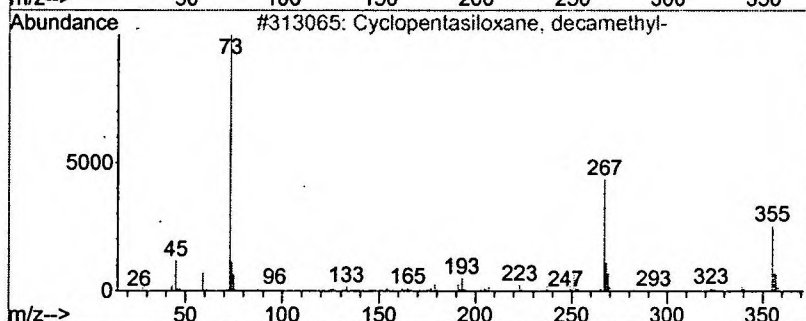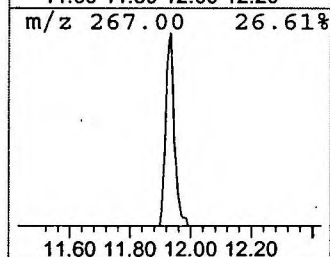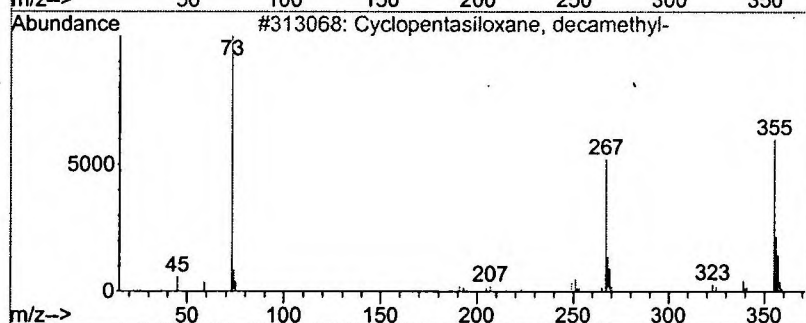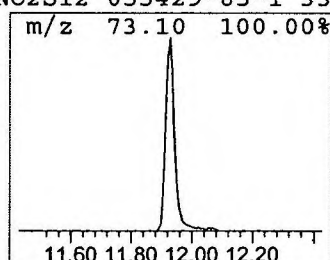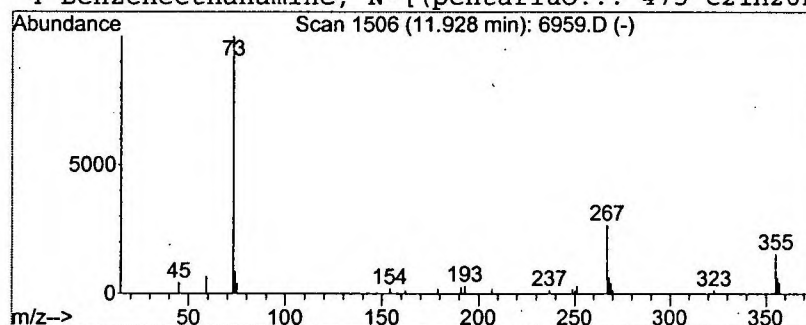

Tentatively Identified Compound (LSC) summary

Operator ID: Bohlk Date Acquired: 17 Apr 2002 6:36 pm
 Data File: C:\MSDCHEM\1\DATA\041702\6959.D
 Name: SAMPLE 6959 3/25/02
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentasiloxan...	11.93	1.5	ug/L	178789	2	12.89	4680730	40.0