

User: Bohlk, Ted
 Westchester Dept. of Labs & Research
 Date: 04/24/2002 Time: 09:33:07

Sample: AE07173
 Analysis: \$B1GCMS Blank for GCMS Scan
 Units: ug
 Started: 3/27/02 09:27 Ended: 4/18/02 09:27 Analyst: TB
 Result source: manual entry
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	n-Nitrosodimethylamine		< MDL		2.0
2	bis(2-Chloroethyl)ether		< MDL		2.0
3	1,3-Dichlorobenzene		< MDL		2.0
4	1,4-Dichlorobenzene		< MDL		2.0
5	1,2-Dichlorobenzene		< MDL		2.0
6	2,2'-oxybis(1-Chloropropane)		< MDL		2.0
7	n-Nitrosodi-n-propylamine		< MDL		2.0
8	Hexachloroethane		< MDL		2.0
9	Nitrobenzene		< MDL		2.0
10	Isophorone		< MDL		2.0
11	bis(2-Chloroethoxy)methane		< MDL		2.0
12	1,2,4-Trichlorobenzene		< MDL		2.0
13	Naphthalene		< MDL		2.0
14	Hexachlorobutadiene		< MDL		2.0
15	2-Chloronaphthalene		< MDL		2.0
16	Dimethylphthalate		< MDL		2.0
17	2,6-Dinitrotoluene		< MDL		2.0
18	Acenaphthylene		< MDL		2.0
19	Acenaphthene		< MDL		2.0
20	2,4-Dinitrotoluene		< MDL		2.0
21	Diethylphthalate		< MDL		2.0
22	4-Chlorophenylphenylether		< MDL		2.0
23	Fluorene		< MDL		2.0
24	Azobenzene		< MDL		2.0
25	n-Nitrosodiphenylamine		< MDL		2.0
26	4-Bromophenylphenylether		< MDL		2.0
27	Hexachlorobenzene		< MDL		2.0
28	Phenanthrene		< MDL		2.0
29	Anthracene		< MDL		2.0
30	Di-n-butylphthalate		< MDL		2.0
31	Fluoranthene		< MDL		2.0
32	Pyrene		< MDL		2.0
33	Butylbenzylphthalate		< MDL		2.0
34	Benzo(a)anthracene		< MDL		2.0
35	bis(2-Ethylhexyl)phthalate		< MDL		2.0
36	Chrysene		< MDL		2.0
37	Di-n-octylphthalate		< MDL		2.0
38	Benzo(b)fluoranthene		< MDL		2.0
39	Benzo(k)fluoranthene		< MDL		2.0
40	Benzo(a)pyrene		< MDL		2.0
41	Indeno(1,2,3-cd)pyrene		< MDL		2.0
42	Dibenz(a,h)anthracene		< MDL		2.0
43	Benzo(g,h,i)perylene		< MDL		2.0

Quantitation Report

(QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\041802\LBA0418.D

Acq On : 18 Apr 2002 11:54 am

Sample : LB 3/27/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 24 08:10:04 2002

Vial: 5

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Wed Apr 24 08:08:47 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.41	152	489783	40.00	ug/L	0.00
10) Naphthalene-d8	12.89	136	2288708	40.00	ug/L	0.00
17) Acenaphthene-d10	17.99	164	1285750	40.00	ug/L	0.00
30) Phenanthrene-d10	22.34	188	1818542	40.00	ug/L	0.00
39) Chrysene-d12	30.15	240	1419478	40.00	ug/L	0.00
45) Perylene-d12	34.02	264	835406	40.00	ug/L	0.00

System Monitoring Compounds

28) TCMX (SURR)	19.95	244	20098	3.92	ug/L	0.00
Spiked Amount	4.000		Recovery	=	98.00%	
38) 2,4-DDD (SURR)	0.00	235	0	0.00	ug/L	
Spiked Amount	10.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D. d	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzene/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
32) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	0.00	178	0	N.D.	
35) Anthracene	0.00	178	0	N.D.	
36) Di-n-butylphthalate	0.00	149	0	N.D.	
37) Fluoranthene	0.00	202	0	N.D.	
40) Pyrene	0.00	202	0	N.D.	
41) Butylbenzylphthalate	0.00	149	0	N.D.	
42) Benzo (a) anthracene	0.00	228	0	N.D. d	
43) Bis (2-ethylhexyl) phthala	30.77	149	61531	1.75	ug/L 91
44) Chrysene	0.00	228	0	N.D. d	

(#)=qualifier out of range (m)=manual integration

LBA0418.D 5080402BBC.M

Wed Apr 24 08:24:09 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\041802\LBA0418.D

Acq On : 18 Apr 2002 11:54 am

Sample : LB 3/27/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 24 08:10:04 2002

Vial: 5

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Wed Apr 24 08:08:47 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo (b) fluoranthene	0.00	252	0	N.D.		
48) Benzo (k) fluoranthene	0.00	252	0	N.D.		
49) Benzo (a) pyrene	0.00	252	0	N.D.	d	
50) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
51) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
52) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

LBA0418.D 5080402BBC.M

Wed Apr 24 08:24:09 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\041802\LBA0418.D

Vial: 5

Acq On : 18 Apr 2002 11:54 am

Operator: Bohlk

Sample : LB 3/27/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 24 8:11 2002


Quant Results File: 5080402BBC.RES

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Wed Apr 24 08:08:47 2002

Response via : Initial Calibration

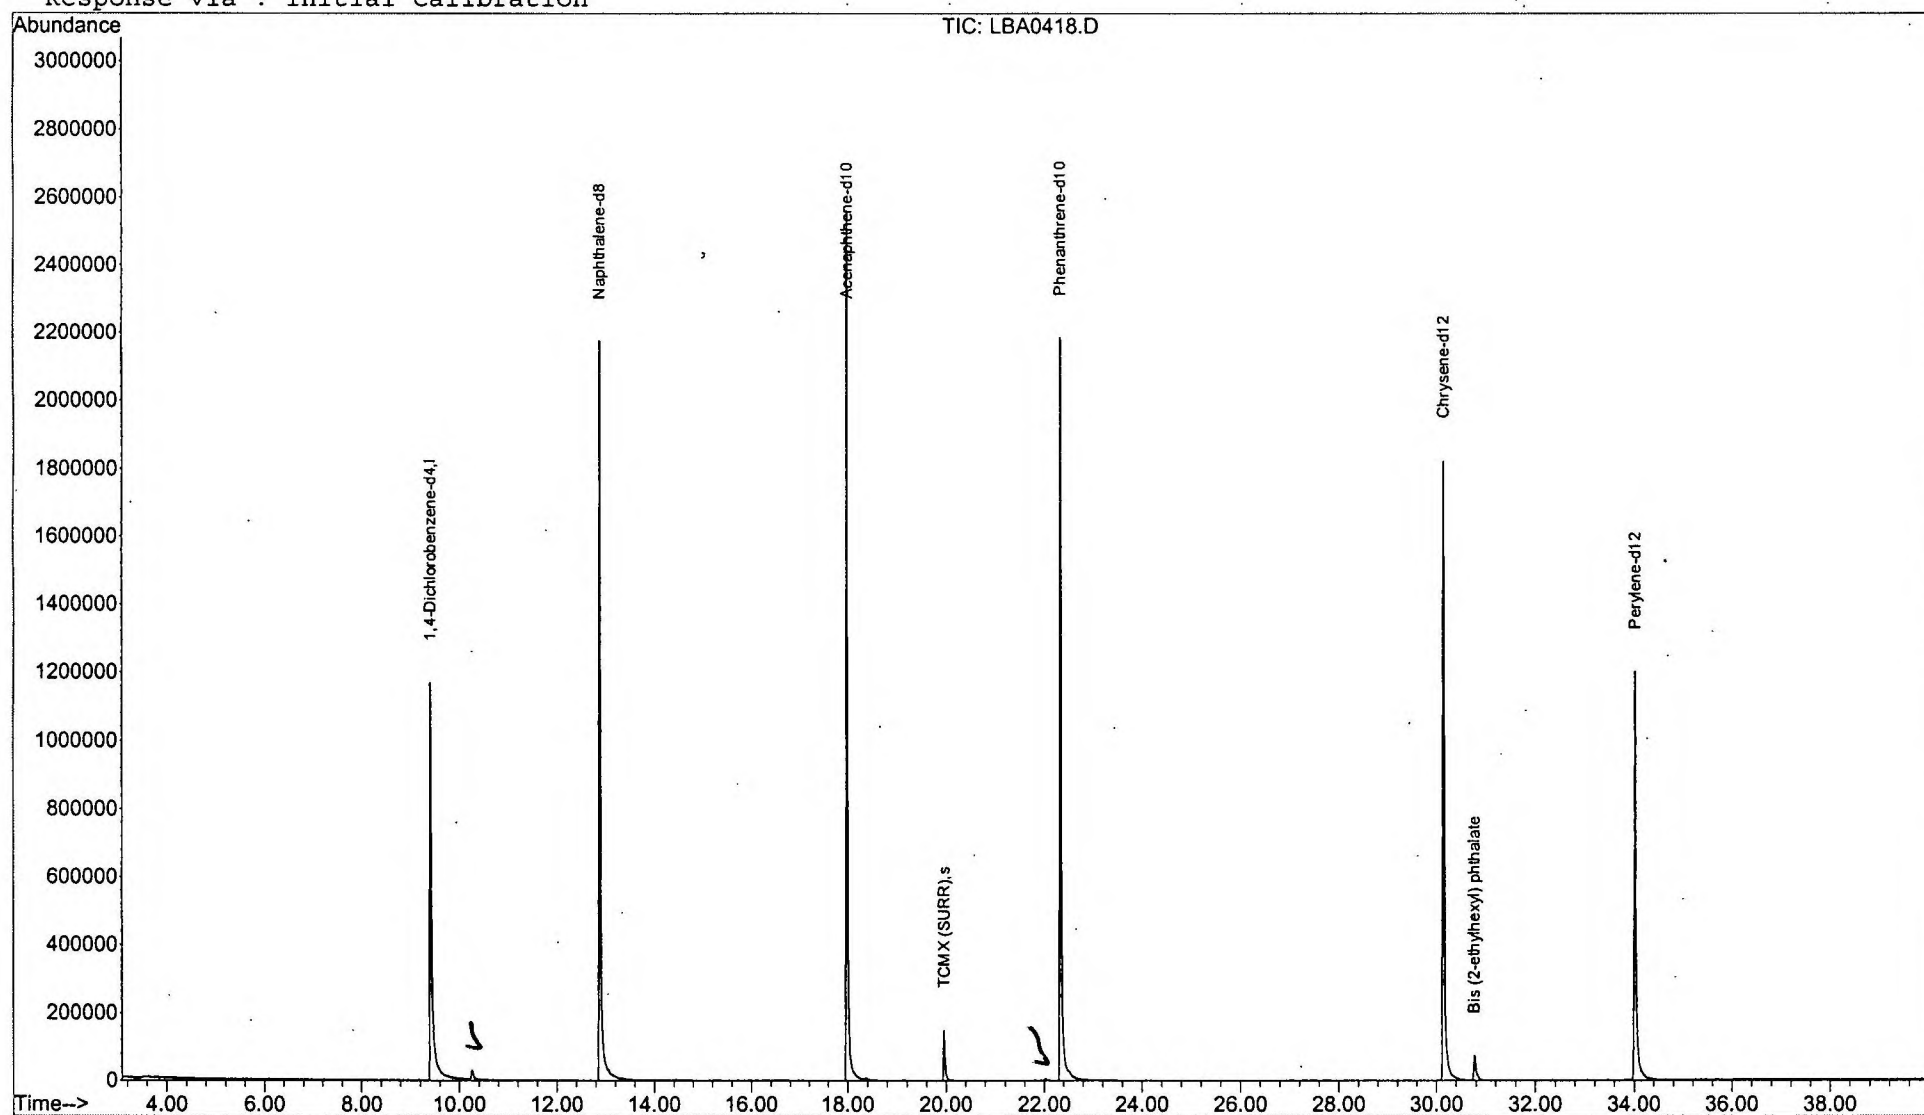

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\041802\LBA0418.D

Acq On : 18 Apr 2002 11:54 am

Sample : LB 3/27/02

Misc :

MS Integration Params: LSCINT.P

Vial: 5

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.407	1071	1077	1101	rBV	1167906	3239282	59.89%	12.106%
2	10.259	1212	1222	1230	rBV2	26593	75767	1.40%	0.283%
3	12.886	1661	1669	1693	rBV	2175386	4874955	90.13%	18.220%
4	17.991	2529	2538	2557	rBV	2556971	5408816	100.00%	20.215%
5	19.954	2866	2872	2884	rBV2	147345	316343	5.85%	1.182%
6	22.339	3270	3278	3303	rBV2	2185368	5207276	96.27%	19.462%
7	30.148	4597	4607	4630	rBV2	1822164	4381020	81.00%	16.374%
8	30.765	4706	4712	4728	rBV2	72926	224342	4.15%	0.838%
9	34.020	5256	5266	5284	rBV	1201107	3028856	56.00%	11.320%

Sum of corrected areas: 26756657

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\041802\LBA0418.D
 Operator : Bohlk
 Acquired : 18 Apr 2002 11:54 am using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: LB 3/27/02
 Misc Info :
 Vial Number: 5
 Quant File :5080402BBC.RES (RTE Integrator)

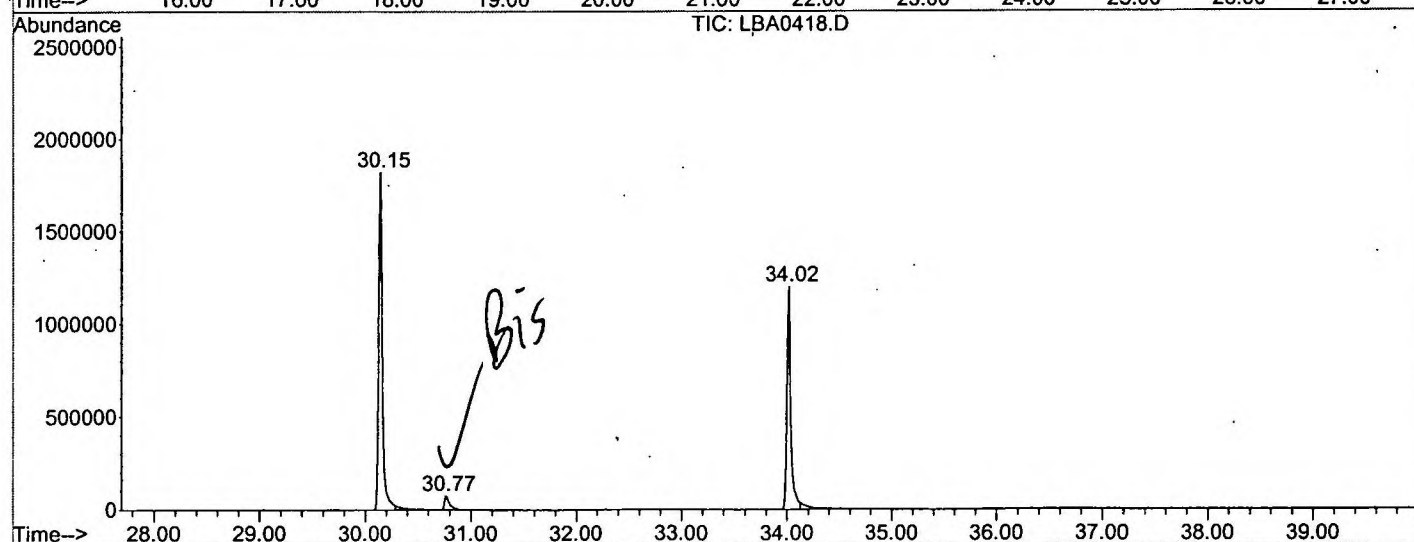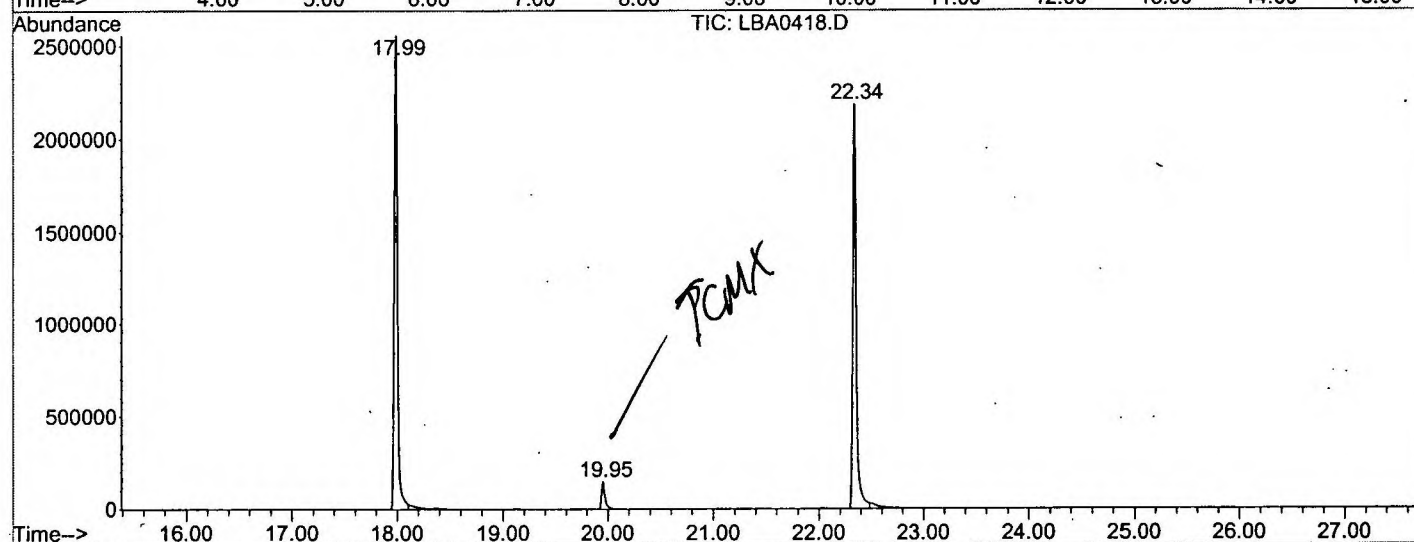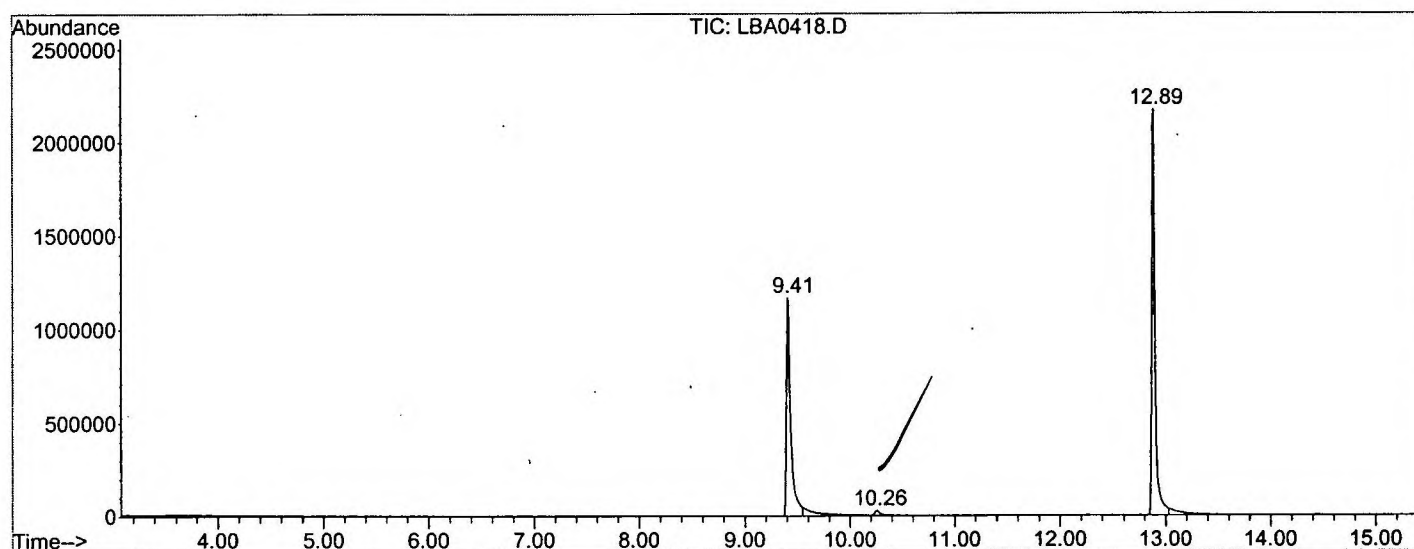

Library Search Compound Report

Data File : C:\MSDCHEM\1\DATA\041802\LBA0418.D

Acq On : 18 Apr 2002 11:54 am

Sample : LB 3/27/02

Misc :

MS Integration Params: LSCINT.P

Vial: 5

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)










Title : Quantitation For Method 508gcscan

Library : C:\DATABASE\WILEY7N.L

Peak Number 1 1,4-Dichlorobenzene-d4 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.26	0.94 ug/L	75767	1,4-Dichlorobenzene-d4	9.41

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,4-Dichlorobenzene-d4	150	C6D4Cl2	003855-82-1	91
2		1,4-Dichlorobenzene-d4	150	C6D4Cl2	003855-82-1	91
3		1,2-Dichlorobenzene-d4 \$\$ Benzen...	150	C6D4Cl2	002199-69-1	91
4		Benzene-1,2,3,4-d4-, 5,6-dichlor...	150	C6D4Cl2	002199-69-1	72

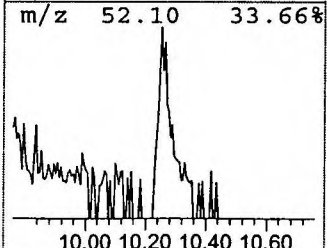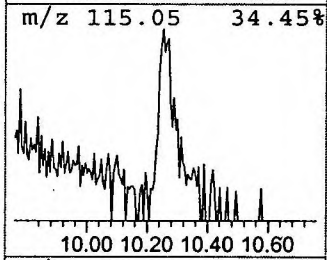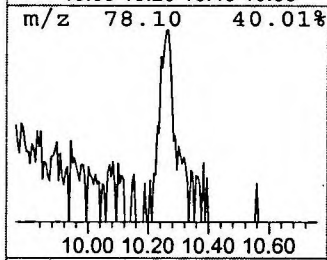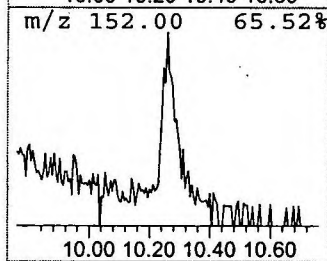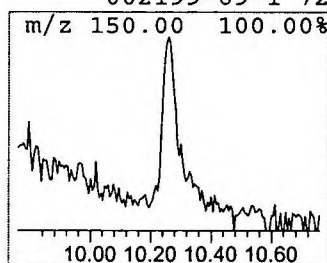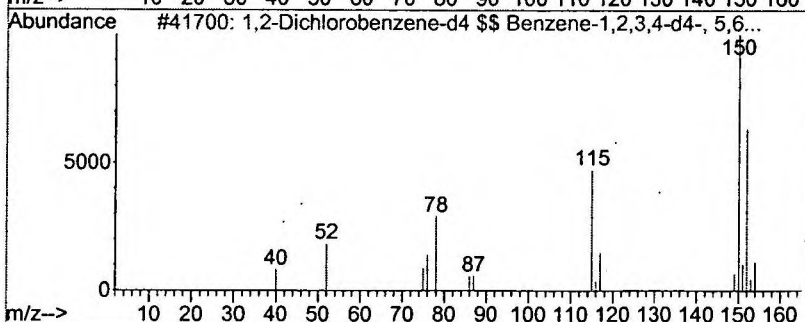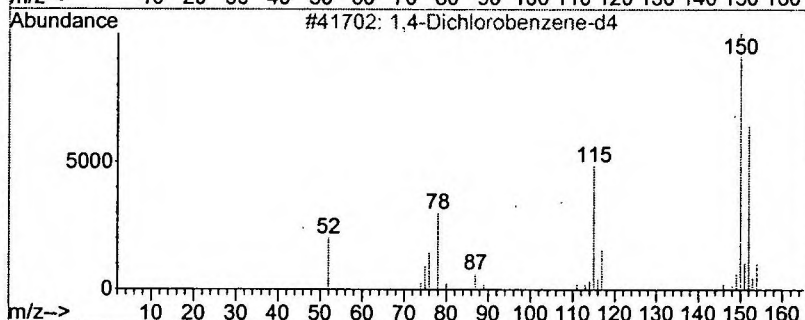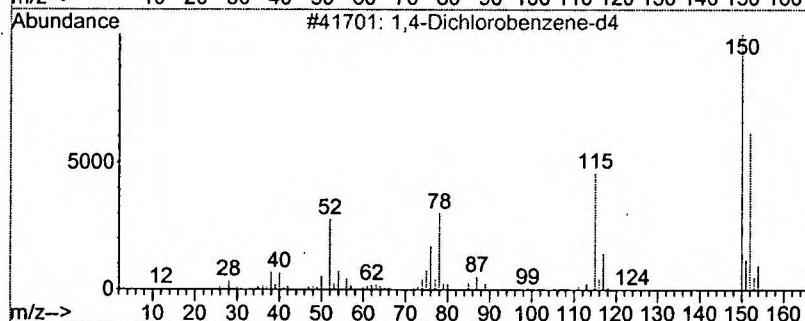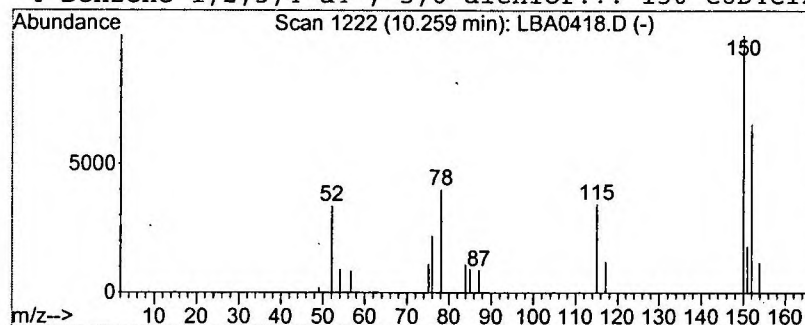

Tentatively Identified Compound (LSC) summary

Operator ID: Bohlk Date Acquired: 18 Apr 2002 11:54 am
 Data File: C:\MSDCHEM\1\DATA\041802\LBA0418.D
 Name: LB 3/27/02
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1,4-Dichlorobenze...	10.26	0.9	ug/L	75767	1	9.41	3239280	40.0