

User: Vinci, David L
Westchester Dept. of Labs & Research
Date: 04/25/2002 Time: 12:15:38

Sample: AE07176
Analysis: \$GCMS GCMS Scan For Unknowns
Units: ug
Started: 4/25/02 12:15 Ended: 4/25/02 12:15 Analyst: DLV
Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds				
2	Surr_2,4-DDD		114		10.0

Comments for Sample AE07176 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-25-2002 Time: 12:16:42

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds.

Quantitation Report

(QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\041802\7176.D

Acq On : 18 Apr 2002 6:40 pm

Sample : SAMPLE 7176 3/27/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 24 08:41:33 2002

Vial: 13

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Wed Apr 24 08:08:47 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.41	152	587937	40.00	ug/L	0.00
10) Naphthalene-d8	12.89	136	2533730	40.00	ug/L	0.00
17) Acenaphthene-d10	17.99	164	1404612	40.00	ug/L	0.00
30) Phenanthrene-d10	22.34	188	1989998	40.00	ug/L	0.00
39) Chrysene-d12	30.15	240	1627904	40.00	ug/L	0.00
45) Perylene-d12	34.02	264	988068	40.00	ug/L	0.00

System Monitoring Compounds

28) TCMX (SURR)	19.95	244	25444	4.54	ug/L	0.00
Spiked Amount	4.000		Recovery	=	113.50%	
38) 2,4-DDD (SURR)	0.00	235	0	0.00	ug/L	
Spiked Amount	10.000		Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	d
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D.	d
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
32) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	0.00	178	0	N.D.	
35) Anthracene	0.00	178	0	N.D.	
36) Di-n-butylphthalate	0.00	149	0	N.D.	
37) Fluoranthene	0.00	202	0	N.D.	
40) Pyrene	0.00	202	0	N.D.	
41) Butylbenzylphthalate	0.00	149	0	N.D.	
42) Benzo (a) anthracene	0.00	228	0	N.D.	d
43) Bis (2-ethylhexyl) phthala	30.76	149	100379	2.49	ug/L 96
44) Chrysene	0.00	228	0	N.D.	d

(#)=qualifier out of range (m)=manual integration

7176.D 5080402BBC.M Wed Apr 24 08:42:18 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\041802\7176.D

Acq On : 18 Apr 2002 6:40 pm

Sample : SAMPLE 7176 3/27/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 24 08:41:33 2002

Vial: 13

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080402BBC.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Wed Apr 24 08:08:47 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo (b) fluoranthene	0.00	252	0	N.D.		
48) Benzo (k) fluoranthene	0.00	252	0	N.D.		
49) Benzo (a) pyrene	0.00	252	0	N.D.	d	
50) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
51) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
52) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

7176.D 5080402BBC.M Wed Apr 24 08:42:18 2002

Data File : C:\MSDCHEM\1\DATA\041802\7176.D

Vial: 13

Acq On : 18 Apr 2002 6:40 pm

Operator: Bohlk

Sample : SAMPLE 7176 3/27/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 24 8:42 2002


Quant Results File: 5080402BBC.RES

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Wed Apr 24 08:08:47 2002

Response via : Initial Calibration

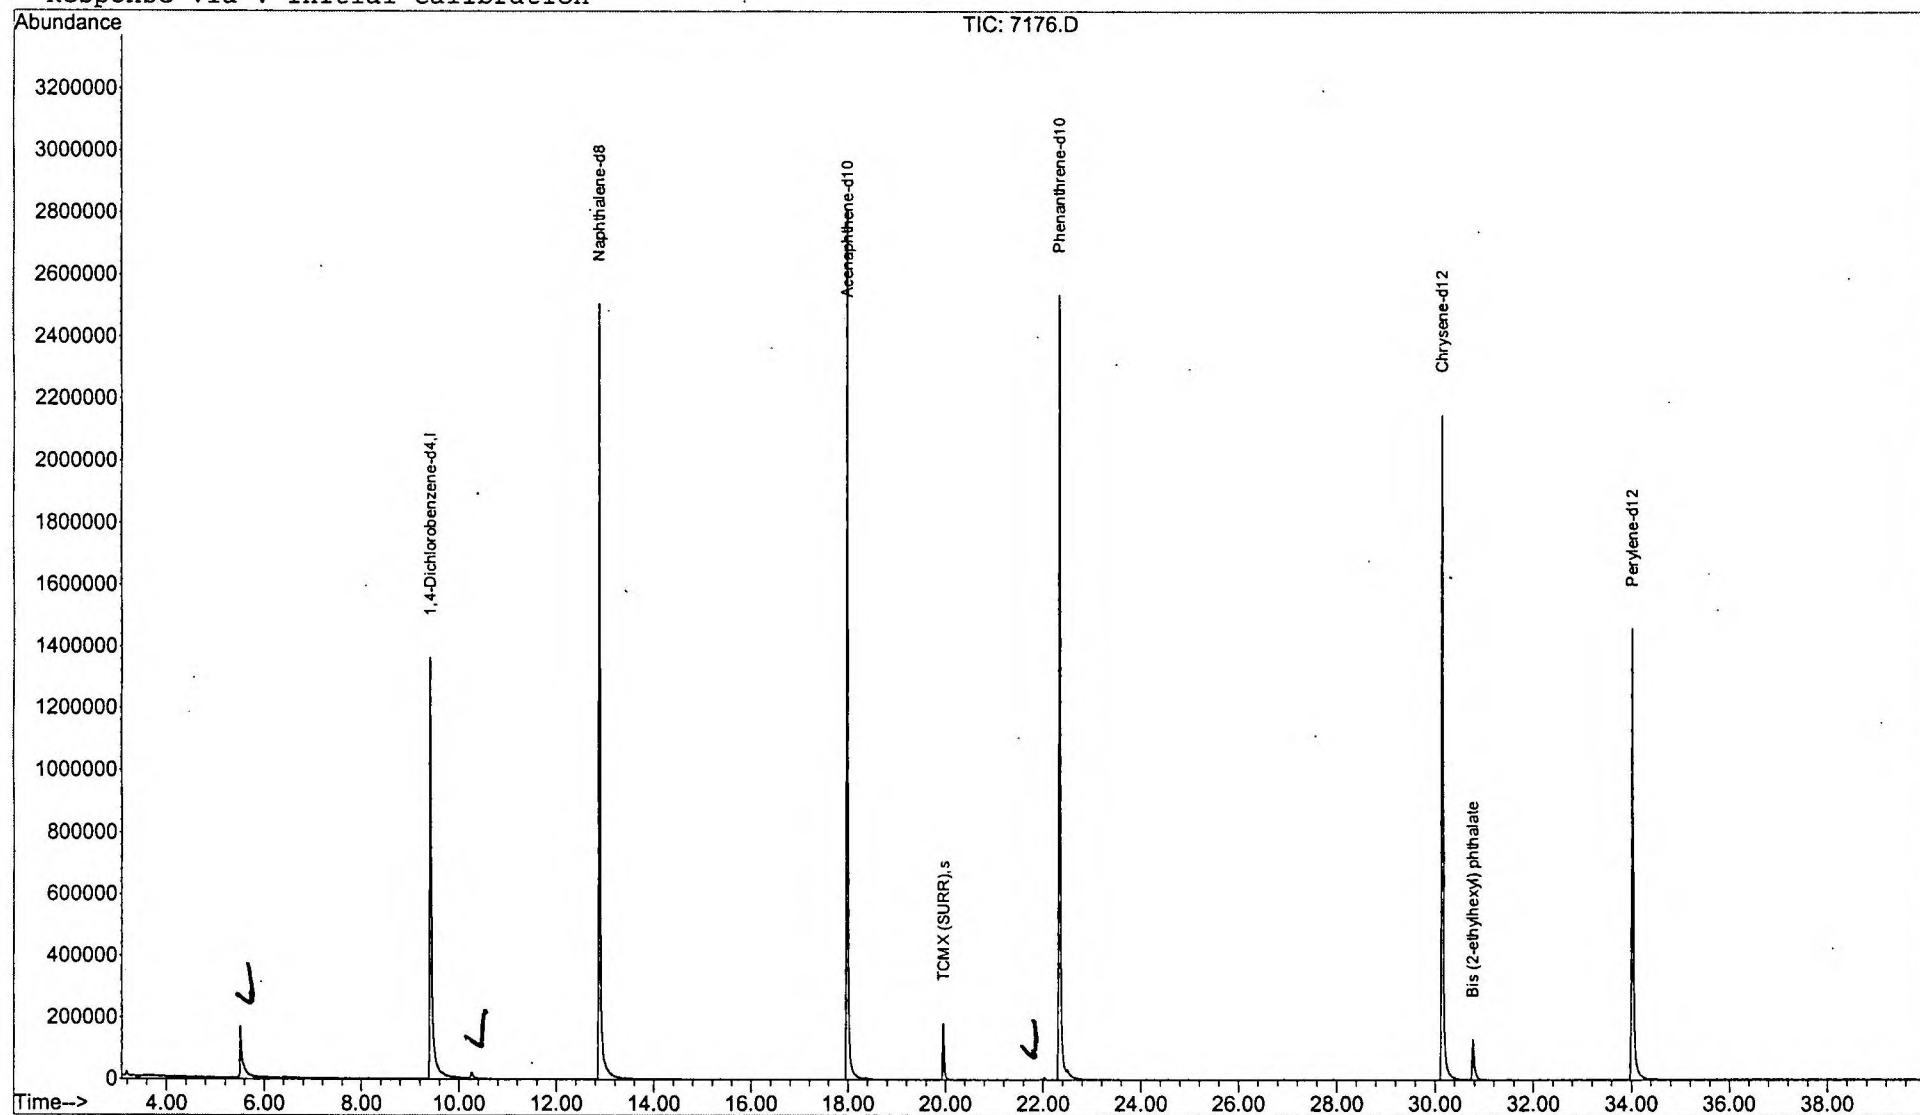

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\041802\7176.D

Acq On : 18 Apr 2002 6:40 pm

Sample : SAMPLE 7176 3/27/02

Misc :

MS Integration Params: LSCINT.P

Vial: 13

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.512	411	414	441	rBV	158873	474488	7.86%	1.521%
2	9.413	1072	1078	1104	rBV	1362444	3737393	61.90%	11.977%
3	10.259	1215	1222	1234	rBV4	20732	65573	1.09%	0.210%
4	12.885	1661	1669	1691	rBV	2506241	5402453	89.48%	17.313%
5	17.991	2529	2538	2569	rBV	2809155	6037865	100.00%	19.350%
6	19.954	2865	2872	2883	rBV2	181532	400828	6.64%	1.285%
7	22.339	3269	3278	3301	rBV2	2536384	5769436	95.55%	18.489%
8	30.148	4597	4607	4640	rBV2	2147441	5190586	85.97%	16.634%
9	30.765	4705	4712	4734	rBV2	131066	401742	6.65%	1.287%
10	34.020	5252	5266	5287	rBV2	1461069	3723601	61.67%	11.933%

Sum of corrected areas: 31203965

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\041802\7176.D
 Operator : Bohlk
 Acquired : 18 Apr 2002 6:40 pm using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: SAMPLE 7176 3/27/02
 Misc Info :
 Vial Number: 13
 Quant File :5080402BBC.RES (RTE Integrator)

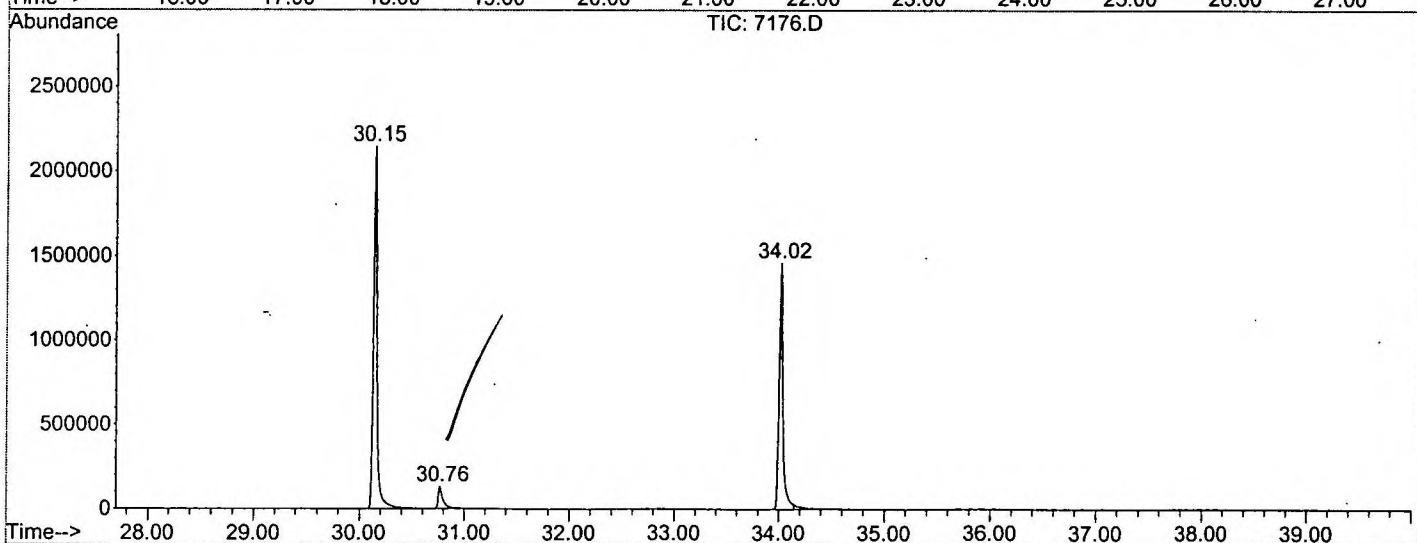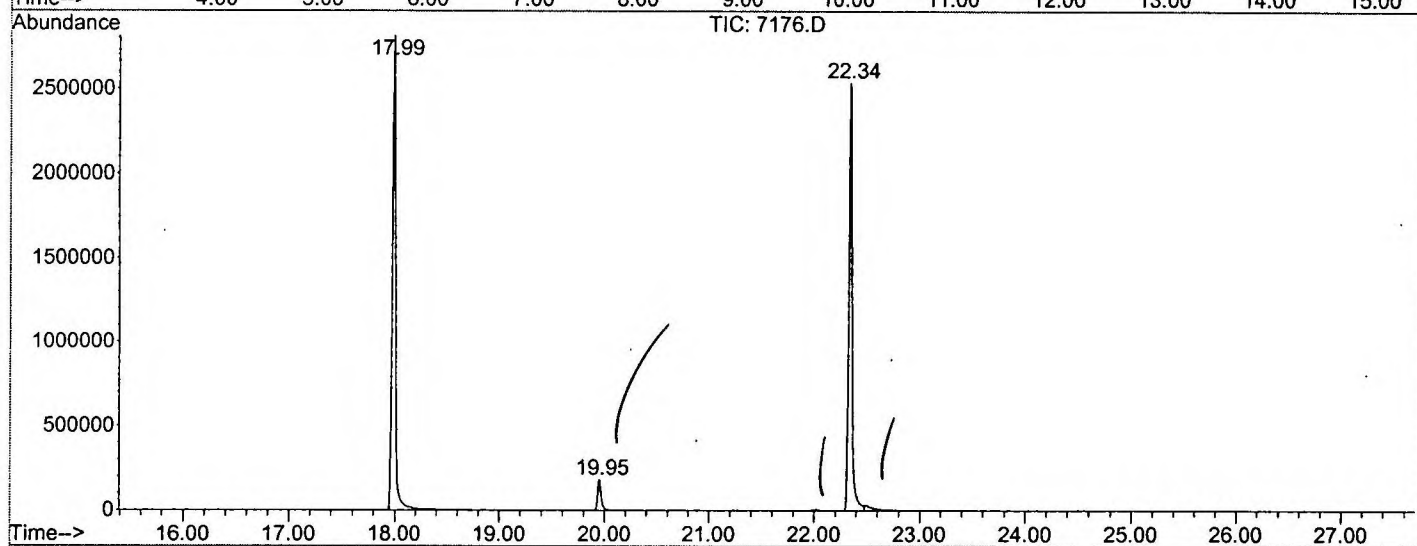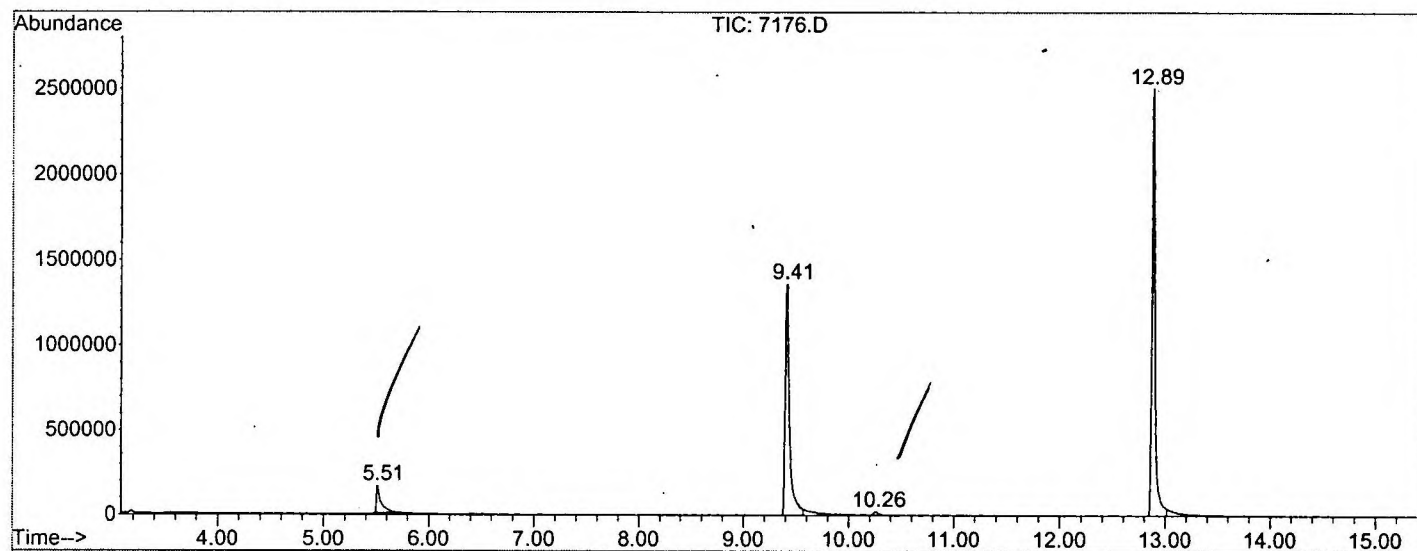

Library Search Compound Report

Data File : C:\MSDCHEM\1\DATA\041802\7176.D
Acq On : 18 Apr 2002 6:40 pm
Sample : SAMPLE 7176 3/27/02
Misc :
MS Integration Params: LSCINT.P

Vial: 13
Operator: Bohlk
Inst : Instrumen
Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)










Title : Quantitation For Method 508gcscan

Library : C:\DATABASE\WILEY7N.L

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.51	5.08 ug/L	474488	1,4-Dichlorobenzene-d4	9.41

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-...	116	C6H12O2	000123-42-2	83
2			2-Pentanone, 4-hydroxy-4-methyl-...	116	C6H12O2	000123-42-2	83
3			2-Pentanone, 4-hydroxy-4-methyl-...	116	C6H12O2	000123-42-2	64
4			2-Pentanone, 4-hydroxy-4-methyl-...	116	C6H12O2	000123-42-2	64

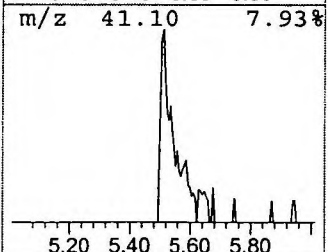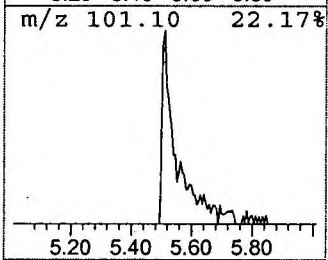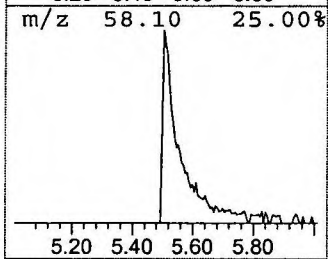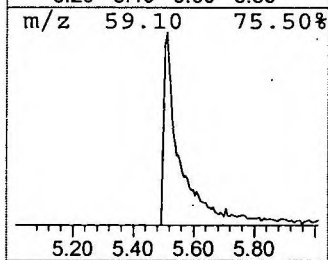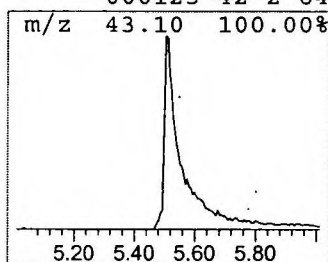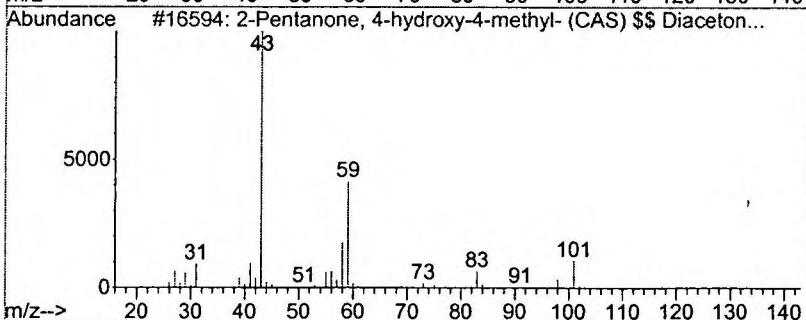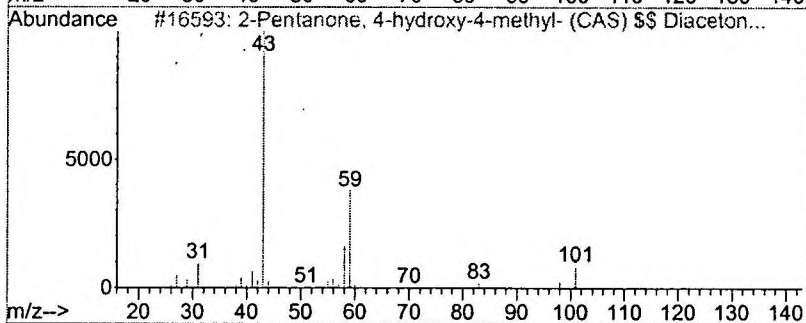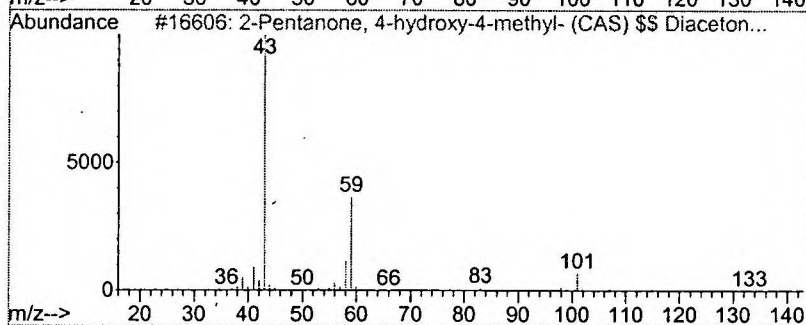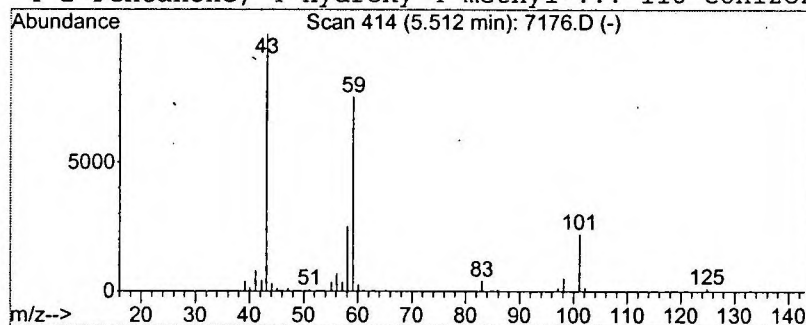

Tentatively Identified Compound (LSC) summary

Operator ID: Bohlk Date Acquired: 18 Apr 2002 6:40 pm
 Data File: C:\MSDCHEM\1\DATA\041802\7176.D
 Name: SAMPLE 7176 3/27/02
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080402BBC.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.51	5.1	ug/L	474488	1	9.41	3737390	40.0