

User: Vinci, David L
 Westchester Dept. of Labs & Research
 Date: 04/16/2002 Time: 15:48:03

Sample: AE07114
 Analysis: \$GCMS GCMS Scan For Unknowns
 Units: ug
 Started: 4/16/02 15:47 Ended: 4/16/02 15:47 Analyst: DLV
 Page: 1

	Component Name	Viol	Result	Qualifier	MDL
1	Other unknown compounds		.		
2	Surr_2,4-DDD		91		5.0

Comments for Sample AE07114 - Analysis \$GCMS

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 04-16-2002 Time: 15:48:46

The GCMS scan, from 35 to 550 amu, does not reveal the presence of unusual compounds. The recoveries for 2 of the 43 compounds in the LCS Standard were high.

Quantitation Report

(QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\041002\7114.D

Acq On : 11 Apr 2002 6:26 am

Sample : SAMPLE 7114 3/27/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 15 18:06:50 2002

Vial: 21

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Results File: 5080402BB.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BB.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Apr 15 15:56:12 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.41	152	487389	40.00	ug/L	0.00
10) Naphthalene-d8	12.88	136	2233192	40.00	ug/L	-0.01
17) Acenaphthene-d10	17.99	164	1262391	40.00	ug/L	-0.01
30) Phenanthrene-d10	22.34	188	1788565	40.00	ug/L	-0.01
39) Chrysene-d12	30.14	240	1370145	40.00	ug/L	-0.02
45) Perylene-d12	34.01	264	860083	40.00	ug/L	-0.01

System Monitoring Compounds

28) TCMX (SURR)	19.95	244	24269	9.08	ug/L	0.00
Spiked Amount 10.000			Recovery	=	90.80%	
38) 2,4-DDD (SURR)	0.00	235	0	0.00	ug/L	
Spiked Amount 5.000			Recovery	=	0.00%	

Target Compounds

					Qvalue
2) N-nitroso-dimethyl amine	0.00	74	0	N.D.	
3) bis(2-chloroethyl) ether	0.00	93	0	N.D.	
4) 1,3 - Dichlorobenze	0.00	146	0	N.D.	
5) 1,4 - Dichlorobenzene	0.00	146	0	N.D.	
6) 1,2 - Dichlorobenzene	0.00	146	0	N.D.	
7) 2,2' - oxybis (1-Chloropr	0.00	45	0	N.D.	
8) N-Nitroso-di-n-propylamine	0.00	70	0	N.D.	
9) Hexachloroethane	0.00	117	0	N.D.	
11) Nitrobenzene	0.00	77	0	N.D.	
12) Isophorone	0.00	82	0	N.D.	
13) bis(2-Chloroethoxy) methan	0.00	93	0	N.D.	
14) 1,2,4-Trichlorobenzene	0.00	180	0	N.D.	
15) Naphthalene	0.00	128	0	N.D.	
16) Hexachlorobutadiene	0.00	225	0	N.D.	
18) Hexachlorocyclopentadiene	0.00	237	0	N.D.	
19) 2-chloronaphthalene	0.00	162	0	N.D.	
20) Dimethylphthalate	0.00	163	0	N.D.	
21) 2,6-Dinitrotoluene	0.00	165	0	N.D. d	
22) Acenaphthylene	0.00	152	0	N.D.	
23) Acenaphthene	0.00	153	0	N.D.	
24) 2,4-Dinitrotoluene	0.00	165	0	N.D.	
25) Diethylphthalate	0.00	149	0	N.D.	
26) 4-Chlorophenyl-phenyl ethe	0.00	204	0	N.D.	
27) Fluorene	0.00	166	0	N.D.	
29) Azobenzen/ 1,2-Diphenylhyd	0.00	77	0	N.D.	
31) N-Nitrosodiphenylamine	0.00	169	0	N.D.	
32) 4-Bromophenyl-phenyl ether	0.00	248	0	N.D.	
33) Hexachlorobenzene	0.00	284	0	N.D.	
34) Phenanthrene	0.00	178	0	N.D.	
35) Anthracene	0.00	178	0	N.D.	
36) Di-n-butylphthalate	0.00	149	0	N.D.	
37) Fluoranthene	0.00	202	0	N.D.	
40) Pyrene	0.00	202	0	N.D.	
41) Butylbenzylphthalate	0.00	149	0	N.D.	
42) Benzo (a) anthracene	0.00	228	0	N.D. d	
43) Bis (2-ethylhexyl) phthala	30.76	149	84974	3.45	ug/L 97
44) Chrysene	0.00	228	0	N.D. d	

(#)=qualifier out of range (m)=manual integration

7114.D 5080402BB.M Mon Apr 15 18:08:10 2002

Page 1

Quantitation Report (QT Reviewed)

Data File : C:\MSDCHEM\1\DATA\041002\7114.D

Vial: 21

Acq On : 11 Apr 2002 6:26 am

Operator: Bohlk

Sample : SAMPLE 7114 3/27/02

Inst : Instrumen

Misc :

Multiplr: 1.00

MS Integration Params: BENZO.P

Quant Time: Apr 15 18:06:50 2002

Quant Results File: 5080402BB.RES

Quant Method : C:\MSDCHEM\1\5973N\5080402BB.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Apr 15 15:56:12 2002

Response via : Initial Calibration

DataAcq Meth : 508SCAN

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
46) Di-n-Octylphthalate	0.00	149	0	N.D.		
47) Benzo (b) fluoranthene	0.00	252	0	N.D.		
48) Benzo (k) fluoranthene	0.00	252	0	N.D.		
49) Benzo (a) pyrene	0.00	252	0	N.D.	d	
50) Indeno (1,2,3-cd) pyrene	0.00	276	0	N.D.		
51) Dibenz (a,h) anthracene	0.00	278	0	N.D.		
52) Benzo (g,h,i) perylene	0.00	276	0	N.D.		

(#) = qualifier out of range (m) = manual integration

7114.D 5080402BB.M Mon Apr 15 18:08:11 2002

Page 2

Data File : C:\MSDCHEM\1\DATA\041002\7114.D

Acq On : 11 Apr 2002 6:26 am

Sample : SAMPLE 7114 3/27/02

Misc :

MS Integration Params: BENZO.P

Quant Time: Apr 15 18:08 2002

Vial: 21

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00


Quant Results File: 5080402BB.RES

Method : C:\MSDCHEM\1\5973N\5080402BB.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Last Update : Mon Apr 15 15:56:12 2002

Response via : Initial Calibration

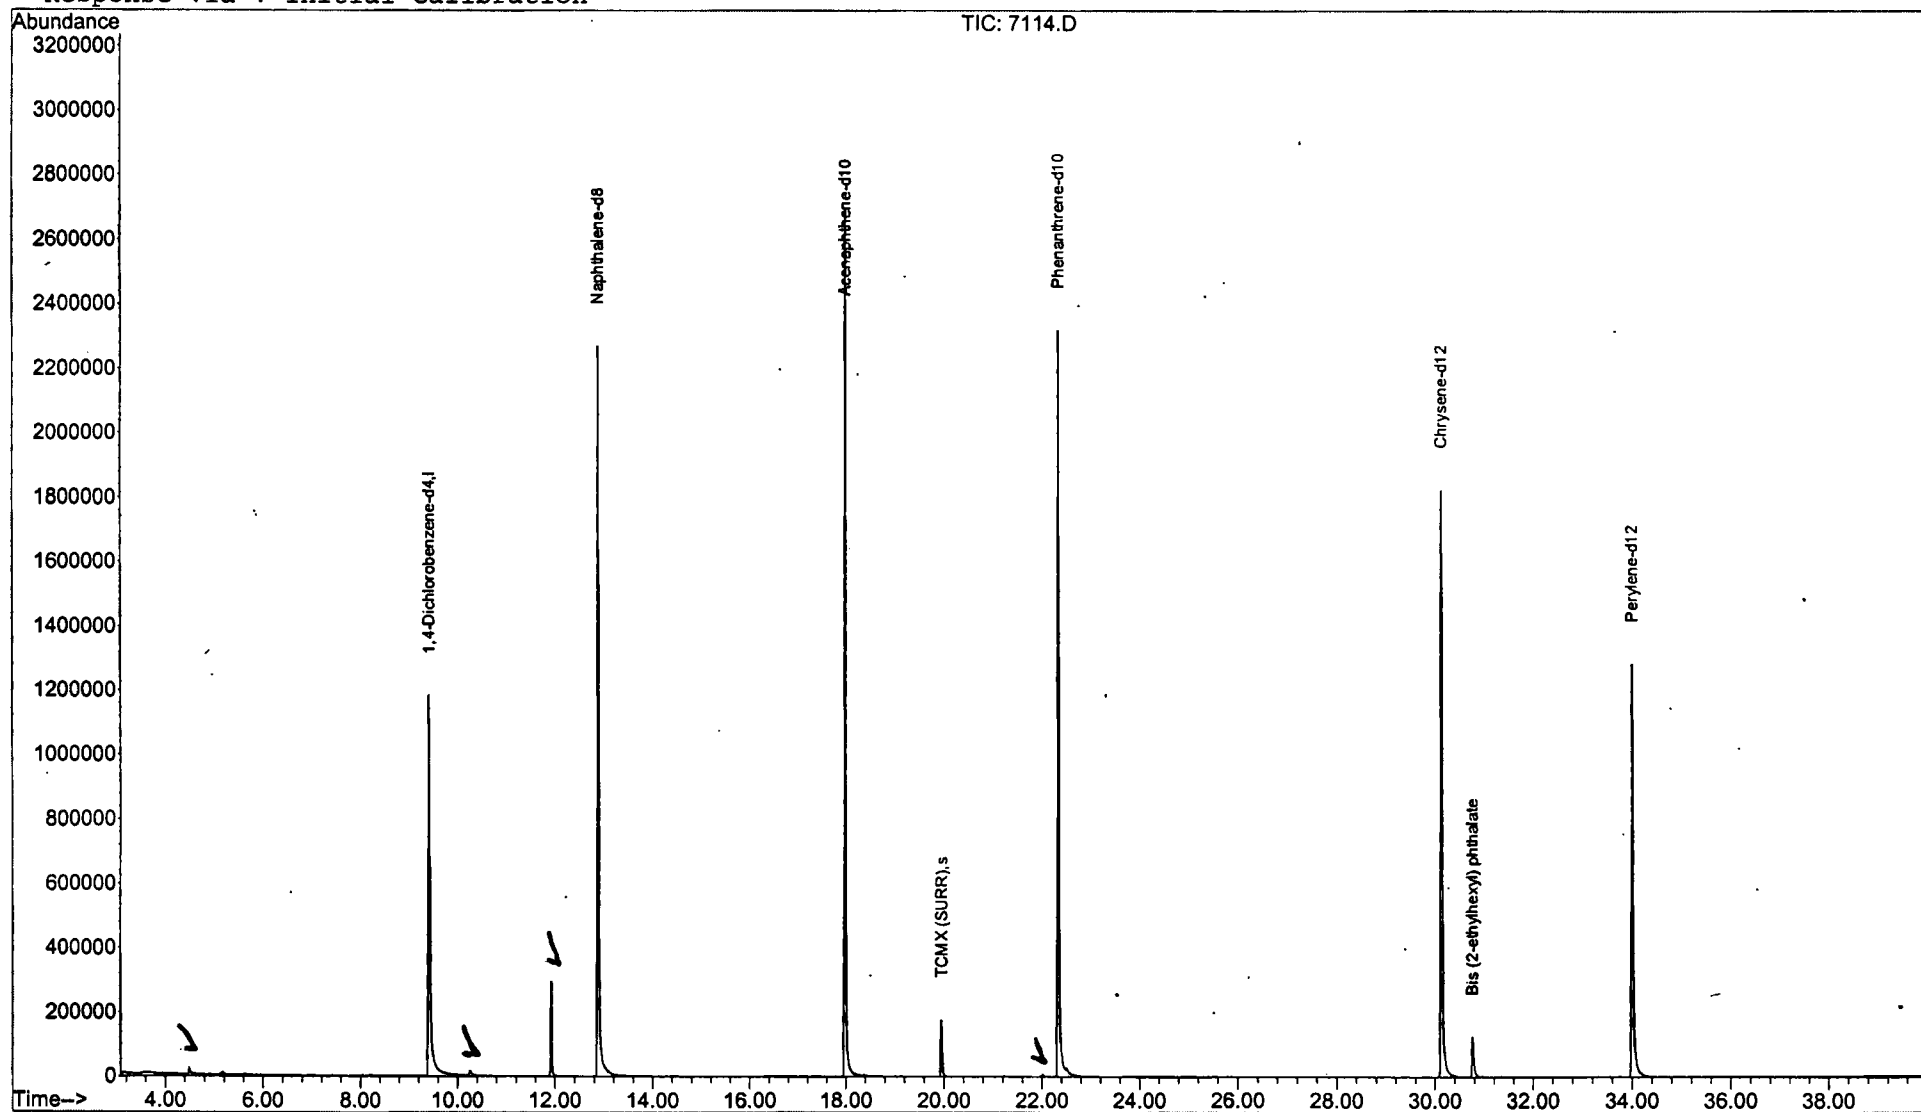

LSC Area Percent Report

Data File : C:\MSDCHEM\1\DATA\041002\7114.D

Acq On : 11 Apr 2002 6:26 am

Sample : SAMPLE 7114 3/27/02

Misc :

MS Integration Params: LSCINT.P

Vial: 21

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Method : C:\MSDCHEM\1\5973N\5080402BB.M (RTE Integrator)

Title : Quantitation For Method 508gcscan

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5




Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.407	1071	1077	1096	rBV	1182626	3087008	57.46%	11.387%
2	11.922	1499	1505	1514	rBV	296206	523591	9.75%	1.931%
3	12.879	1660	1668	1691	rBV	2269231	4781931	89.01%	17.639%
4	17.985	2528	2537	2562	rBV	2695128	5372219	100.00%	19.816%
5	19.948	2864	2871	2882	rBV3	176013	360687	6.71%	1.330%
6	22.339	3269	3278	3296	rBV2	2318240	5113386	95.18%	18.862%
7	30.142	4596	4606	4631	rBV2	1823292	4349084	80.96%	16.042%
8	30.765	4702	4712	4727	rBV3	124227	318433	5.93%	1.175%
9	34.014	5255	5265	5288	rBV2	1283110	3203667	59.63%	11.817%

Sum of corrected areas: 27110006

LSC Report - Integrated Chromatogram

File : C:\MSDCHEM\1\DATA\041002\7114.D
 Operator : Bohlk
 Acquired : 11 Apr 2002 6:26 am using AcqMethod 508SCAN
 Instrument : Instrumen
 Sample Name: SAMPLE 7114 3/27/02
 Misc Info :
 Vial Number: 21
 Quant File :5080402BB.RES (RTE Integrator)

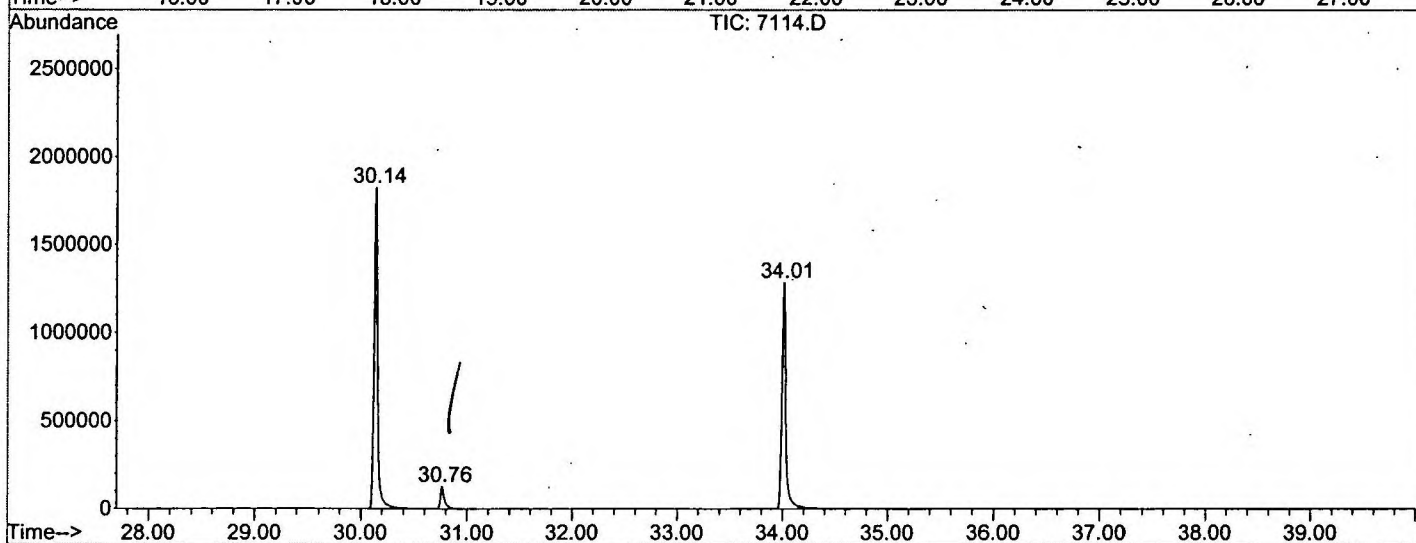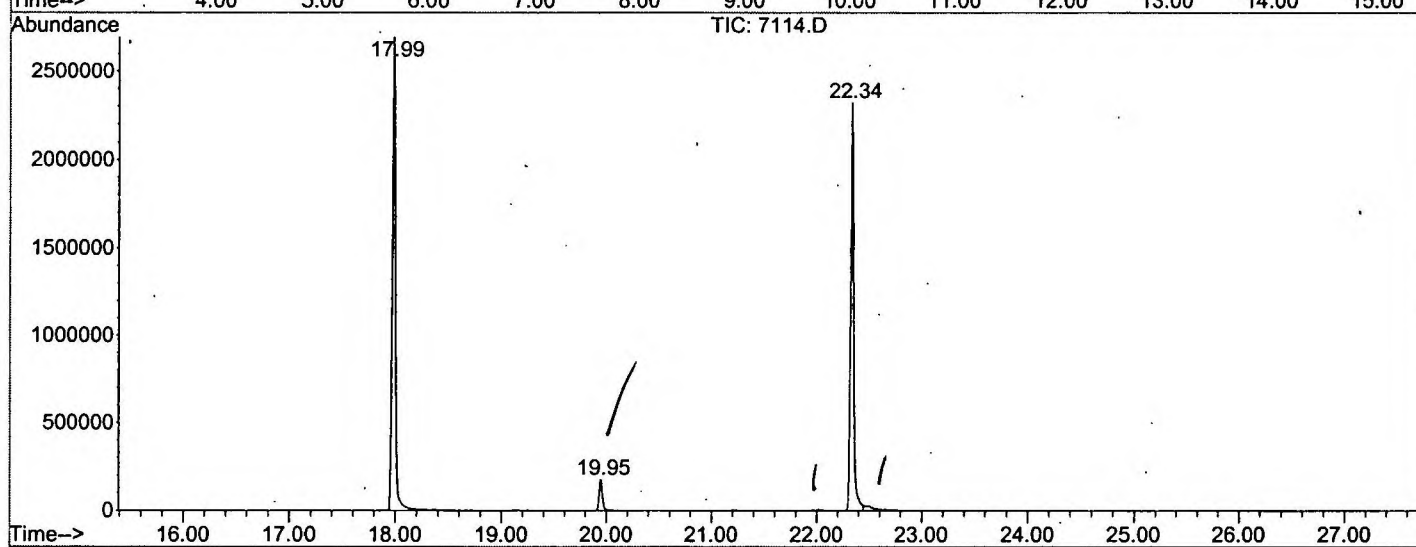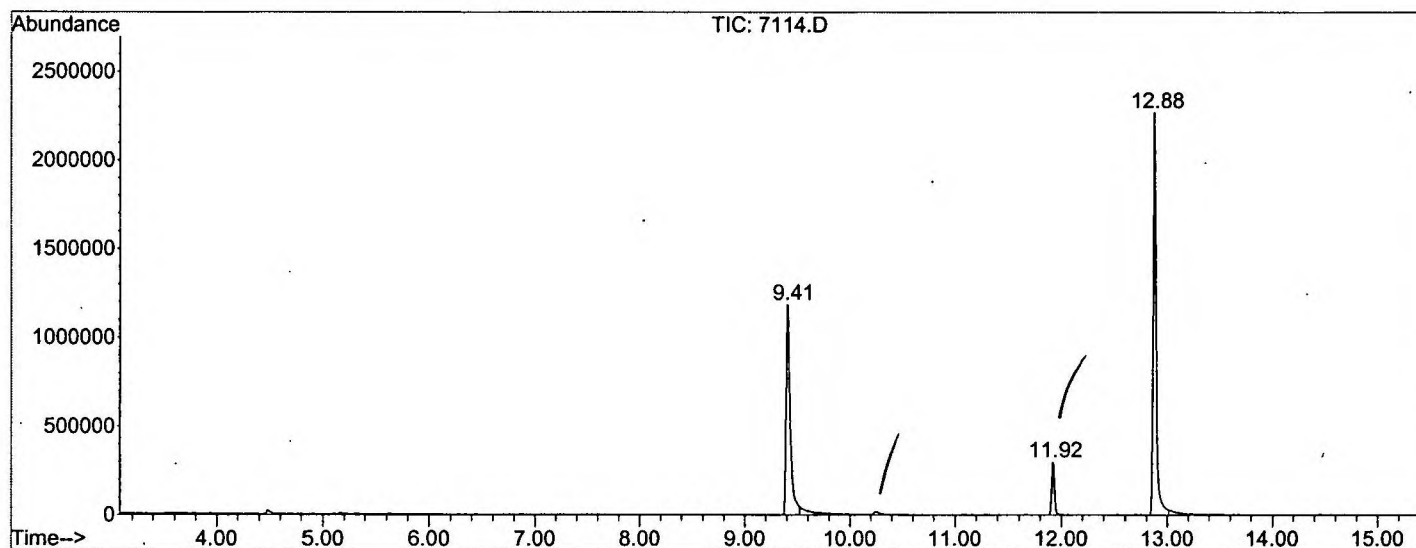

Library Search Compound Report

Data File : C:\MSDCHEM\1\DATA\041002\7114.D

Acq On : 11 Apr 2002 6:26 am

Sample : SAMPLE 7114 3/27/02

Misc :

MS Integration Params: LSCINT.P

Vial: 21

Operator: Bohlk

Inst : Instrumen

Multiplr: 1.00

Quant Method : C:\MSDCHEM\1\5973N\5080402BB.M (RTE Integrator)










Title : Quantitation For Method 508gcscan

Library : C:\DATABASE\WILEY7N.L

Peak Number 1 Cyclopentasiloxane, decamet... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.92	4.38 ug/L	523591	Naphthalene-d8	12.88

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	72
2			Cyclopentasiloxane, decamethyl-	370	C10H30O5Si5	000541-02-6	53
3			Benzeneethanamine, N-[(pentafluorophenyl)methyl]-	475	C21H26F5NO2Si2	055429-85-1	40
4			M-HYDROXYPHENETHANOL 2TMS	282	C14H26O2Si2	000000-00-0	40

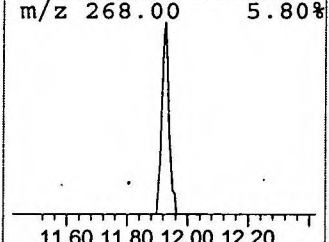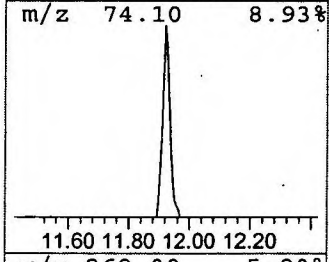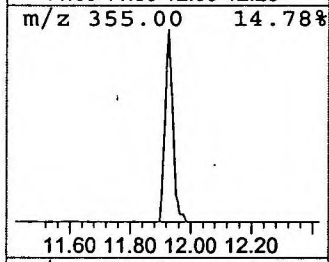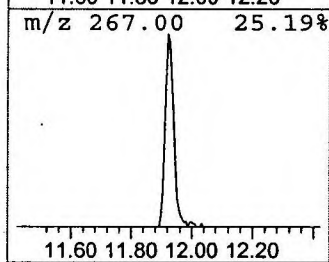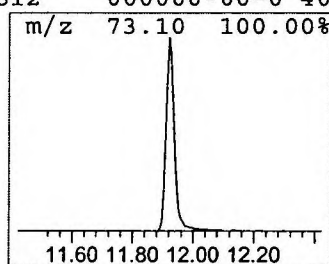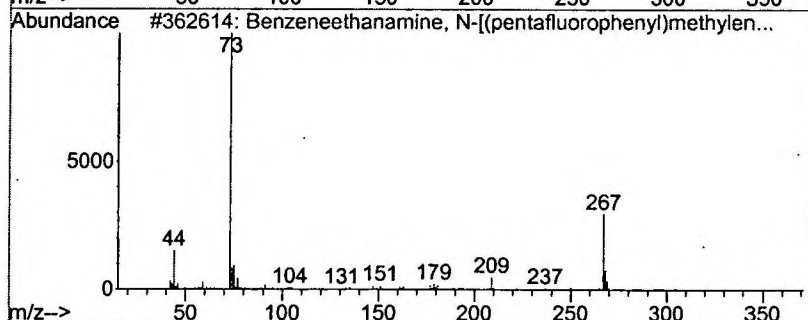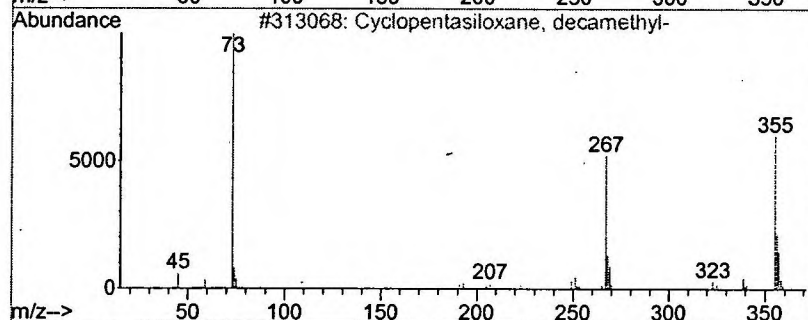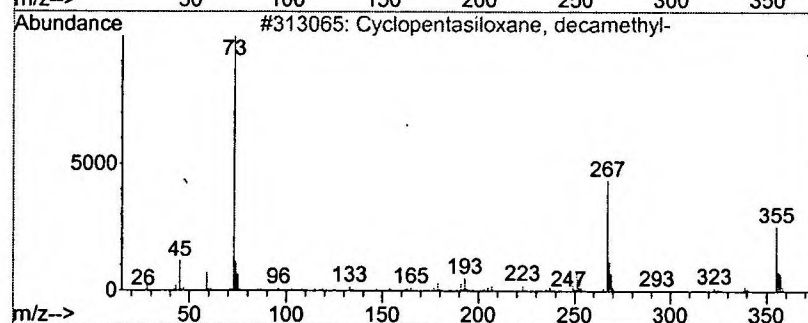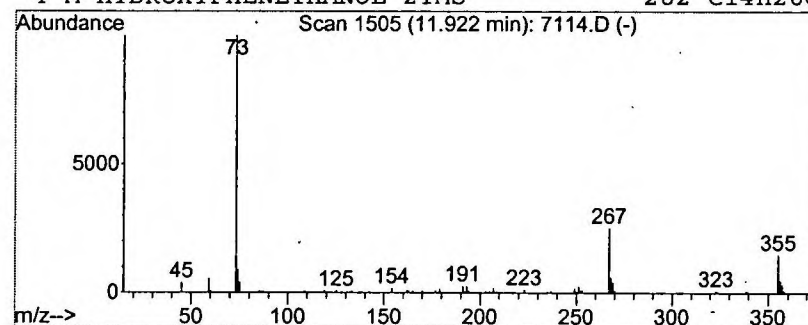

Tentatively Identified Compound (LSC) summary

Operator ID: Bohlk Date Acquired: 11 Apr 2002 6:26 am
 Data File: C:\MSDCHEM\1\DATA\041002\7114.D
 Name: SAMPLE 7114 3/27/02
 Misc:
 Method: C:\MSDCHEM\1\5973N\5080402BB.M (RTE Integrator)
 Title: Quantitation For Method 508gcscan
 Library Searched: C:\DATABASE\WILEY7N.L

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentasiloxan...	11.92	4.4	ug/L	523591	2	12.88	4781930	40.0