

User: Bohlk, Ted
Westchester Dept. of Labs & Research
Date: 09/22/2001 Time: 10:48:56

Sample: AD22486
Analysis: \$525 Organic Chemicals - 525.2
Units: ug
Started: 9/18/01 10:46 Ended: 9/19/95 10:46 Analyst: TB
Result source: manual entry
Page: 1

not our bottles

	Component Name	Viol	Result	Qualifier	MDL
1	Hexachlorocyclopentadiene		< MDL		0.10
2	Hexachlorobenzene		< MDL		0.10
3	Simazine		< MDL		0.07
4	Atrazine		< MDL		0.10
5	Alachlor		< MDL		0.20
6	bis(2-Ethylhexyl)adipate		< MDL		0.60
7	bis(2-Ethylhexyl)phthalate		0.62		0.60
8	Benzo(a)pyrene		< MDL		0.20
9	EPTC		< MDL		1.0
10	2,6-Dinitrotoluene		< MDL		2.0
11	2,4-Dinitrotoluene		< MDL		2.0
12	Molinate		< MDL		0.90
13	Terbacil		< MDL		2.0
14	Acetochlor		< MDL		2.0
15	Metribuzin		< MDL		0.15
16	Metolachlor		< MDL		0.75
17	Butachlor		< MDL		0.40
18	4,4-DDE		< MDL		0.80
19	Surr_1,3-Dimethyl-2-nitrobenzen		5.3		1.0
20	Surr_Triphenyl phosphate		6.0		1.0
21	Surr_Perylene-d12		4.7		1.0

Chromatogram Plot

File: E:\22486A

Date: Sep-19-1991 20:27:58

Comment: BOHLK; METHOD 525; INST 204; 09/19/01; SAMPLE 22486

Scan No: 1

Retention Time: 0:01


RIC: 0

Mass Range: 0 - 0

Plotted: 1 to 1860

Range: 1 to 1860

100% = 3691706

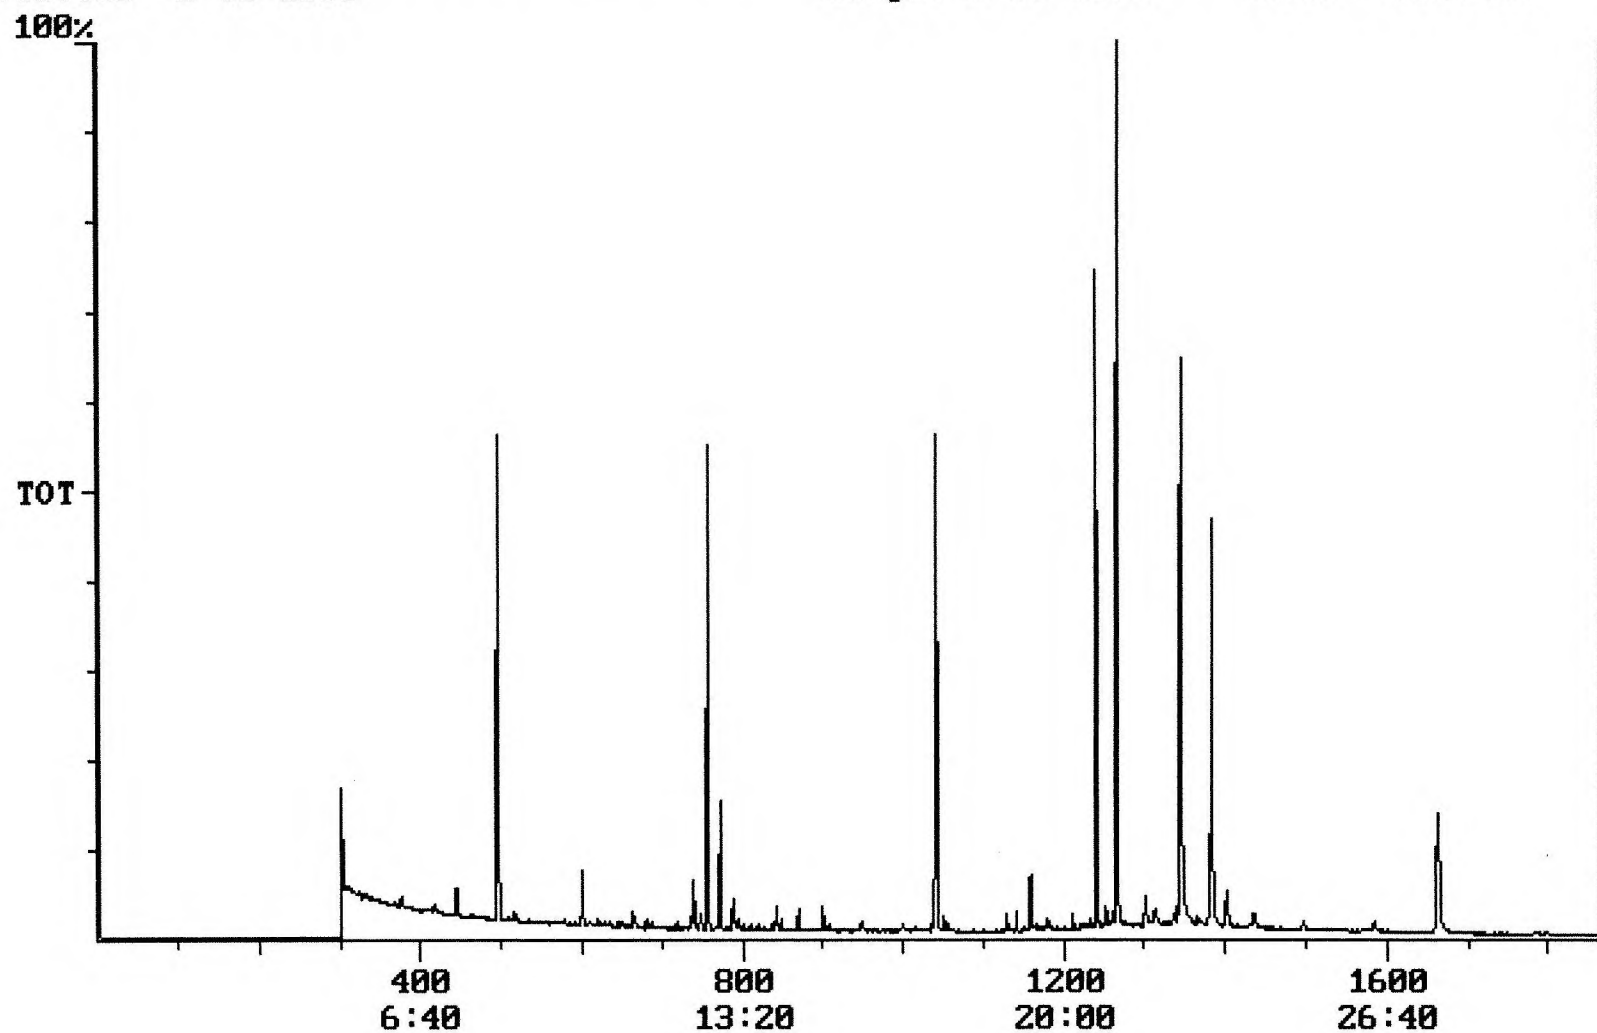

Integration Report Quanfile: 22486A Quan Entries: 15
 Comment: BOHLK; METHOD 525; INST 204; 09/19/01; SAMPLE 22486
 Sorted via: Entry Number ↑

No	Name of Compound	R Time	Scan#	Mode	Peak Area	Pk Height
1	acenaphthene d-10(IS)	12:37	757	Auto	909,404	456,761
2	phenanthrene d-10 (IS)	17:22	1042	Auto	1,536,614	664,939
3	chrysene d-12(IS)	23:03	1383	Auto	1,078,989	488,461
4	p-terphenyl d-14(IS)	21:06	1266	Auto	1,723,832	1,210,511
5	acenaphthene d-10(SURR)	12:37	757	Auto	909,404	456,761
6	phenanthrene d-10(SURR)	17:22	1042	Auto	1,536,614	664,939
7	chrysene d-12 (SURR)	23:03	1383	Auto	1,078,989	488,461
8	1,3-dimethyl-2-nitrobenzene	8:15	495	Auto	589,750	312,957
9	triphenyl phosphate (S)	22:25	1345	Auto	904,474	348,324
10	perylene d-12 (SURR)	27:43	1663	Auto	648,318	124,862
11	bis(2-ethylhexyl)adipate	22:25	1345	Auto	17,583	3,212
12	bis(2-ethylhexyl)phthalate	23:21	1401	Auto	154,275	42,838
13	2,6-dinitrotoluene	12:15	735	Auto	14,279	9,146
14	2,4-dinitrotoluene	13:23	803	Auto	2,216	1,241
15	4,4'-dichlorodiphenyl ether	21:01	1261	Auto	1,165	1,165

Quantitation Report

Quanfile: 22486A

Quan Entries: 15

Comment: BOHLK; METHOD 525; INST 204; 09/19/01; SAMPLE 22486

Sorted via: Entry Number ↑

(S) = Standard

Cal	Name of Compound	S	Scan#	R Time	Me	Calc Amt(A)	Units
1	acenaphthene d-10(IS)	I	757	12:37	BB	5.000	UG/L
2	phenanthrene d-10 (IS)	I	1042	17:22	BV	5.000	UG/L
3	chrysene d-12(IS)	I	1383	23:03	BB	5.000	UG/L
4	p-terphenyl d-14(IS)	I	1266	21:06	BB	5.000	UG/L
5	acenaphthene d-10(SURR	A	757	12:37	BB	3.650	UG/L
6	phenanthrene d-10(SURR	A	1042	17:22	BV	4.153	UG/L
7	chrysene d-12 (SURR)	A	1383	23:03	BB	4.075	UG/L
8	1,3-dimethyl-2-nitrobe	A	495	8:15	BB	5.295	UG/L
9	triphenyl phosphate (S	A	1345	22:25	BB	5.990	UG/L
10	perylene d-12 (SURR)	A	1663	27:43	BB	4.682	UG/L
16	bis(2-ethylhexyl)adipa	A	1345	22:25	MM	0.147	UG/L
17	bis(2-ethylhexyl)phtha	A	1401	23:21	MM	0.618	UG/L
20	2,6-dinitrotoluene	A	735	12:15	BB	0.253	UG/L
21	2,4-dinitrotoluene	A	803	13:23	BB	0.031	UG/L
28	4,4'-dde	A	1261	21:01	BB	0.009	UG/L

• **Comments for Sample AD22486 - Analysis \$525**

Westchester Dept. of Labs & Research

User: Vinci, David L

Date: 09-24-2001 Time: 13:15:03

Bis(2-Ethylhexyl)phthalate was presnet in the Labortatory Blank at 0.37 ug/L. The recovery for bis(2-Ethylhexyl)phthalate in the MDL Standard was above its acceptance range. The recoveries for Terbacil in the LCS Standard and the Spiked Sample were above their acceptance ranges. This sample was submitted to our laboratory using NYCDEP bottles.

Comments for Sample AD22486 - Analysis \$525

Westchester Dept. of Labs & Research
User: Vinci, David L
Date: 10-04-2001 Time: 14:28:36

Bis(2-Ethylhexyl)phthalate was present in the Laboratory Blank at 0.37 ug/L. The recovery for bis(2-Ethylhexyl)phthalate in the MDL Standard was above its acceptance range. The recoveries for Terbacil in the LCS Standard and the Spiked Sample were above their acceptance ranges. This sample was submitted to our laboratory using NYCDEP bottles.