

User: Bohlk, Ted
Westchester Dept. of Labs & Research
Date: 10/02/2001 Time: 11:43:50


Sample: AD22582
Analysis: \$LP525 Organic Extractables
Units: ug
Started: 9/29/01 11:40 Ended: 9/29/01 11:40 Analyst: TB
Result source: manual entry
Page: 1

	Component Name	Viol	Result
1	DFTPP		PASSED
2	ENDRIN *		54
3	DDT		1.6


flag

Instrument serviced prior to injection

Chromatogram Plot File: C:\DFTA0929 Date: Sep-29-1991 10:37:42
Comment: BOHLK; METHOD 525; INST 204; 09/28/01; DFTPP
Scan No: 1 Retention Time: 0:01 RIC: 0 Mass Range: 0 - 0
Plotted: 1 to 1860 Range: 1 to 1860 100% = 6129435

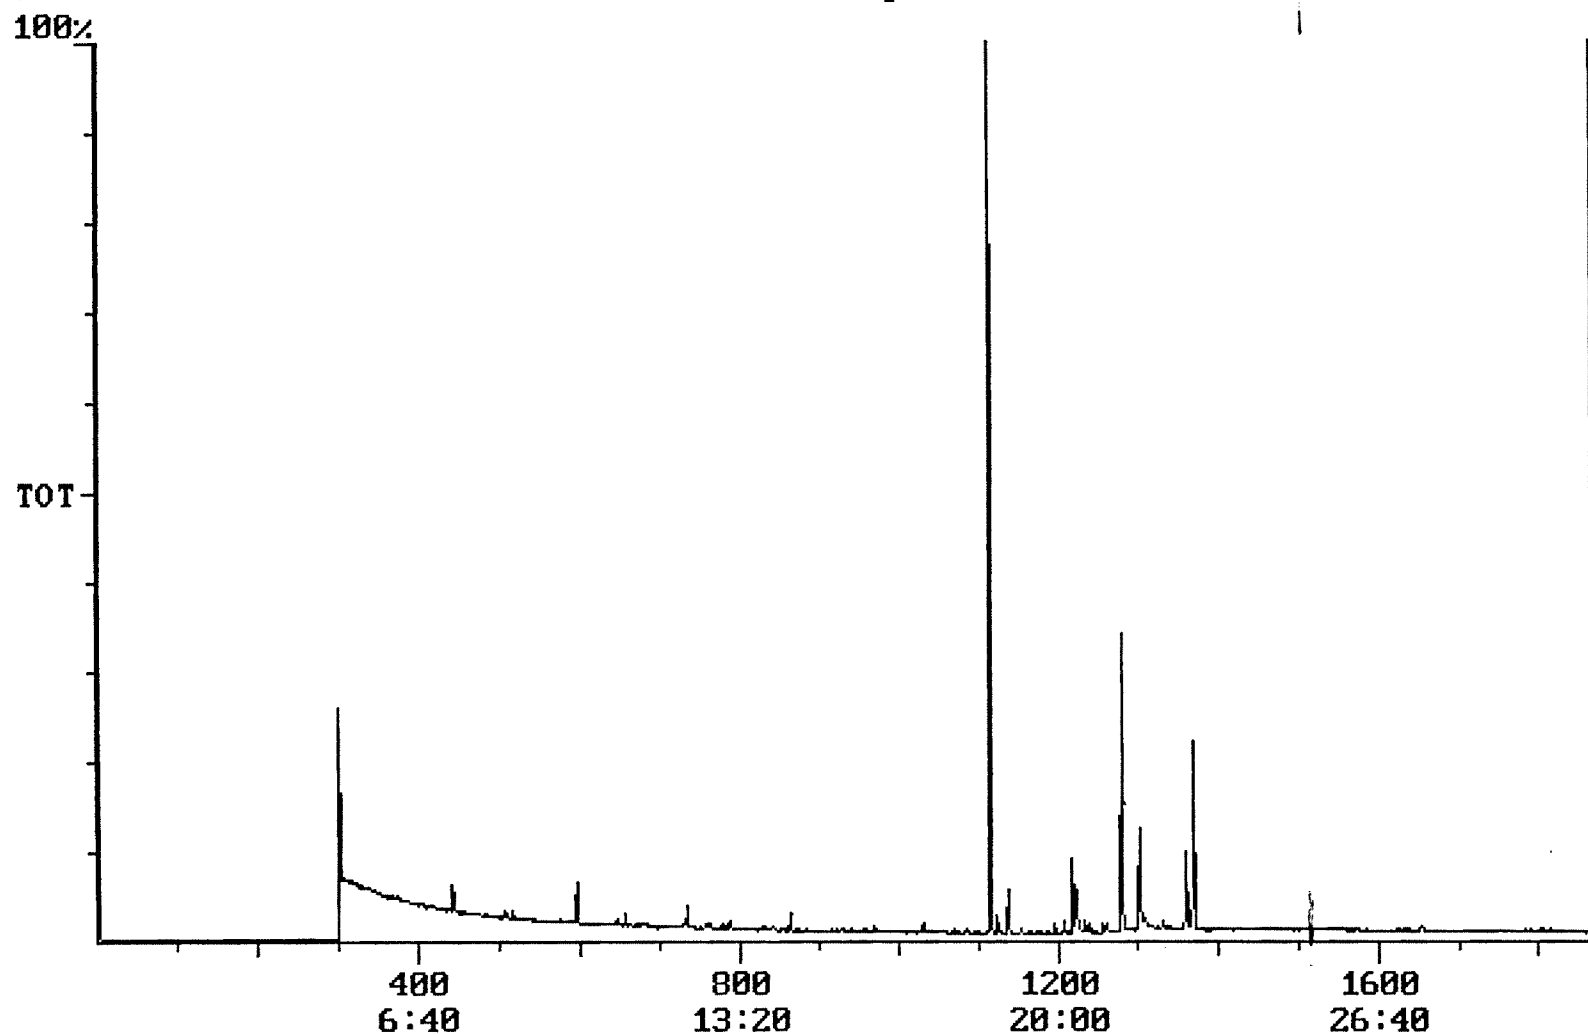

Chromatogram Plot File: C:\DFTA0929 Date: Sep-29-1991 10:37:42
Comment: BOHLK; METHOD 525; INST 204; 09/28/01; DFIPP
Scan No: 1100 Retention Time: 18:20 RIC: 54613 Mass Range: 47 - 147
Plotted: 1100 to 1140 Range: 1 to 1860 100% = 6129435

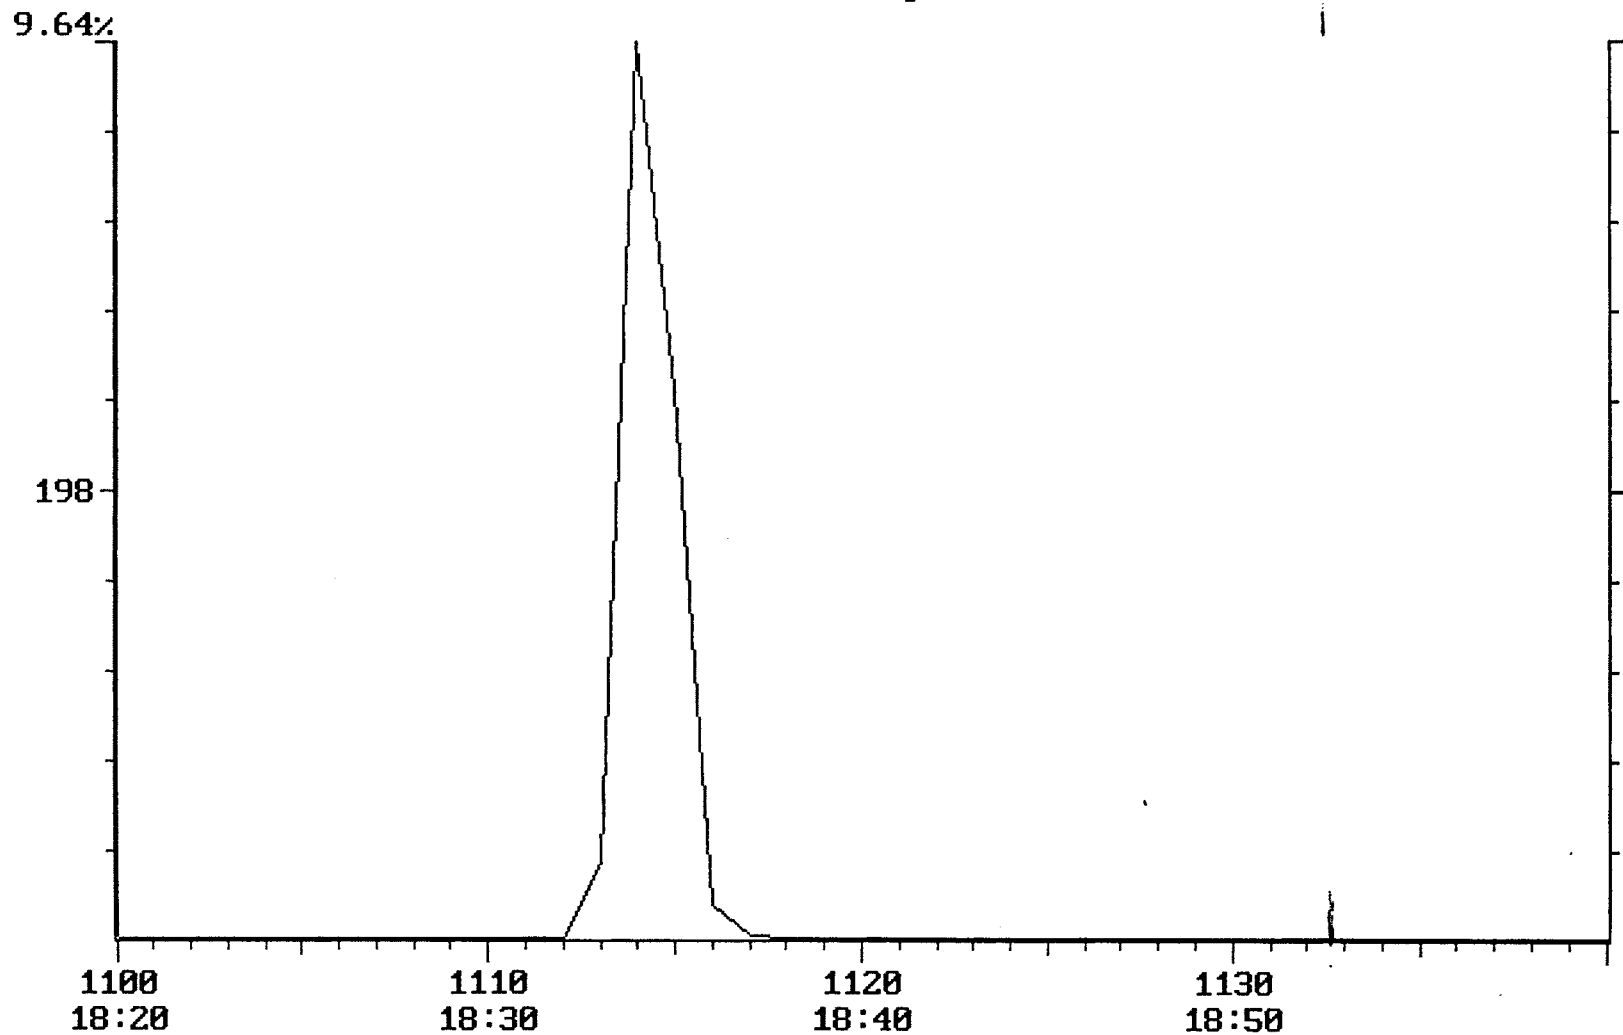

Mass List

File: C:\DFTA0929 Date: Sep-29-1991 10:37:42

Comment: BOHLK; METHOD 525; INST 204; 09/28/01; DFTPP

Scan No: 1114 Retention Time: 18:34 RIC: 6129435 Mass Range: 45 - 444

Peaks: 172 Mass of Base Peak: 442 Int: 1116867 Threshold: 0 %

Mass	Intensity	% Base	Mass	Intensity	% Base	Mass	Intensity	% Base
45	3,313	0.30	81	18,072	1.62	112	2,409	0.22
47	5,722	0.51	82	4,216	0.38	116	4,819	0.43
49	26,506	2.37	83	4,518	0.40	117	110,542	9.90
50	125,903	11.27	84	4,819	0.43	118	7,228	0.65
51	356,325	31.90	85	6,626	0.59	122	5,421	0.49
52	13,253	1.19	86	11,144	1.00	123	10,240	0.92
55	8,433	0.76	87	3,012	0.27	124	4,819	0.43
56	9,939	0.89	88	3,012	0.27	127	183,433	16.42
57	17,469	1.56	91	3,614	0.32	128	12,650	1.13
61	4,819	0.43	92	5,120	0.46	129	75,000	6.72
62	4,819	0.43	93	37,951	3.40	130	8,132	0.73
63	7,530	0.67	96	1,807	0.16	134	2,710	0.24
65	3,313	0.30	98	37,349	3.34	135	6,927	0.62
67	2,108	0.19	99	14,156	1.27	136	3,915	0.35
68	7,228	0.65	100	3,614	0.32	137	6,626	0.59
69	265,662	23.79	101	8,433	0.76	141	12,048	1.08
70	2,409	0.22	103	6,024	0.54	142	4,819	0.43
73	5,421	0.49	104	5,722	0.51	143	2,710	0.24
74	38,554	3.45	105	6,927	0.62	146	4,216	0.38
75	38,855	3.48	106	3,915	0.35	147	7,530	0.67
76	12,650	1.13	107	81,927	7.34	148	15,662	1.40
77	255,421	22.87	108	12,349	1.11	149	4,819	0.43
78	13,253	1.19	109	3,614	0.32	151	2,409	0.22
79	35,843	3.21	110	171,686	15.37	154	4,216	0.38
80	20,180	1.81	111	18,674	1.67	155	6,024	0.54

Mass List

File: C:\DFTA0929 Date: Sep-29-1991 10:37:42

Comment: BOHLK; METHOD 525; INST 204; 09/28/01; DFTPP

Scan No: 1114 Retention Time: 18:34 RIC: 6129435 Mass Range: 45 - 444

Peaks: 172 Mass of Base Peak: 442 Int: 1116867 Threshold: 0 %

Mass	Intensity	% Base	Mass	Intensity	% Base	Mass	Intensity	% Base
156	9,337	0.84	200	3,614	0.32	255	379,819	34.01
157	3,915	0.35	203	4,518	0.40	256	51,506	4.61
160	3,614	0.32	204	15,662	1.40	257	5,120	0.46
161	4,518	0.40	205	21,084	1.89	258	19,578	1.75
165	5,120	0.46	206	90,361	8.09	259	3,915	0.35
166	4,216	0.38	207	14,457	1.29	265	5,722	0.51
167	25,602	2.29	208	3,614	0.32	273	12,349	1.11
168	14,759	1.32	210	2,108	0.19	274	40,060	3.59
173	2,710	0.24	211	3,915	0.35	275	203,614	18.23
174	4,216	0.38	217	24,096	2.16	276	20,180	1.81
175	9,337	0.84	218	6,325	0.57	277	17,168	1.54
177	4,518	0.40	221	9,638	0.86	278	4,518	0.40
179	14,156	1.27	223	5,722	0.51	293	4,518	0.40
180	7,831	0.70	224	57,831	5.18	296	45,783	4.10
181	7,831	0.70	225	13,554	1.21	297	4,819	0.43
185	7,831	0.70	227	26,807	2.40	303	5,421	0.49
186	68,975	6.18	228	3,012	0.27	304	2,108	0.19
187	21,686	1.94	229	3,313	0.30	315	9,638	0.86
189	4,216	0.38	235	2,108	0.19	316	3,012	0.27
192	5,722	0.51	239	3,313	0.30	317	2,710	0.24
193	4,518	0.40	240	2,710	0.24	323	19,879	1.78
196	12,048	1.08	244	35,843	3.21	324	4,216	0.38
197	7,228	0.65	245	6,927	0.62	327	3,012	0.27
198	590,662	52.89	246	11,144	1.00	333	2,710	0.24
199	39,457	3.53	249	3,614	0.32	334	12,048	1.08

Mass List

File: C:\DFTA0929 Date: Sep-29-1991 10:37:42

Comment: BOHLK; METHOD 525; INST 204; 09/28/01; DFTPP

Scan No: 1114 Retention Time: 18:34 RIC: 6129435 Mass Range: 45 - 444

Peaks: 172 Mass of Base Peak: 442 Int: 1116867 Threshold: 0 %

Mass	Intensity	% Base	Mass	Intensity	% Base	Mass	Intensity	% Base
197	7,228	0.65	245	6,927	0.62	327	3,012	0.27
198	590,662	52.89	246	11,144	1.00	333	2,710	0.24
199	39,457	3.53	249	3,614	0.32	334	12,048	1.08
200	3,614	0.32	255	379,819	34.01	335	4,216	0.38
203	4,518	0.40	256	51,506	4.61	341	2,710	0.24
204	15,662	1.40	257	5,120	0.46	352	4,518	0.40
205	21,084	1.89	258	19,578	1.75	353	3,915	0.35
206	90,361	8.09	259	3,915	0.35	354	13,554	1.21
207	14,457	1.29	265	5,722	0.51	365	62,650	5.61
208	3,614	0.32	273	12,349	1.11	366	9,638	0.86
210	2,108	0.19	274	40,060	3.59	371	3,614	0.32
211	3,915	0.35	275	203,614	18.23	372	10,542	0.94
217	24,096	2.16	276	20,180	1.81	373	3,915	0.35
218	6,325	0.57	277	17,168	1.54	383	2,710	0.24
221	9,638	0.86	278	4,518	0.40	402	4,216	0.38
223	5,722	0.51	293	4,518	0.40	403	7,530	0.67
224	57,831	5.18	296	45,783	4.10	404	6,024	0.54
225	13,554	1.21	297	4,819	0.43	421	7,228	0.65
227	26,807	2.40	303	5,421	0.49	422	5,421	0.49
228	3,012	0.27	304	2,108	0.19	423	50,602	4.53
229	3,313	0.30	315	9,638	0.86	424	13,253	1.19
235	2,108	0.19	316	3,012	0.27	441	159,638	14.29
239	3,313	0.30	317	2,710	0.24	442	1,116,867	100.00
240	2,710	0.24	323	19,879	1.78	443	209,036	18.72
244	35,843	3.21	324	4,216	0.38	444	12,349	1.11

Chromatogram Plot

File: C:\DFTA0929

Date: Sep-29-1991 10:37:42

Comment: BOHLK; METHOD 525; INST 204; 09/28/01; DFTPP

Scan No: 1290

Retention Time: 21:30


RIC: 74603

Mass Range: 45 - 281

Plotted: 1270 to 1290

Range: 1 to 1860

100% = 6129435

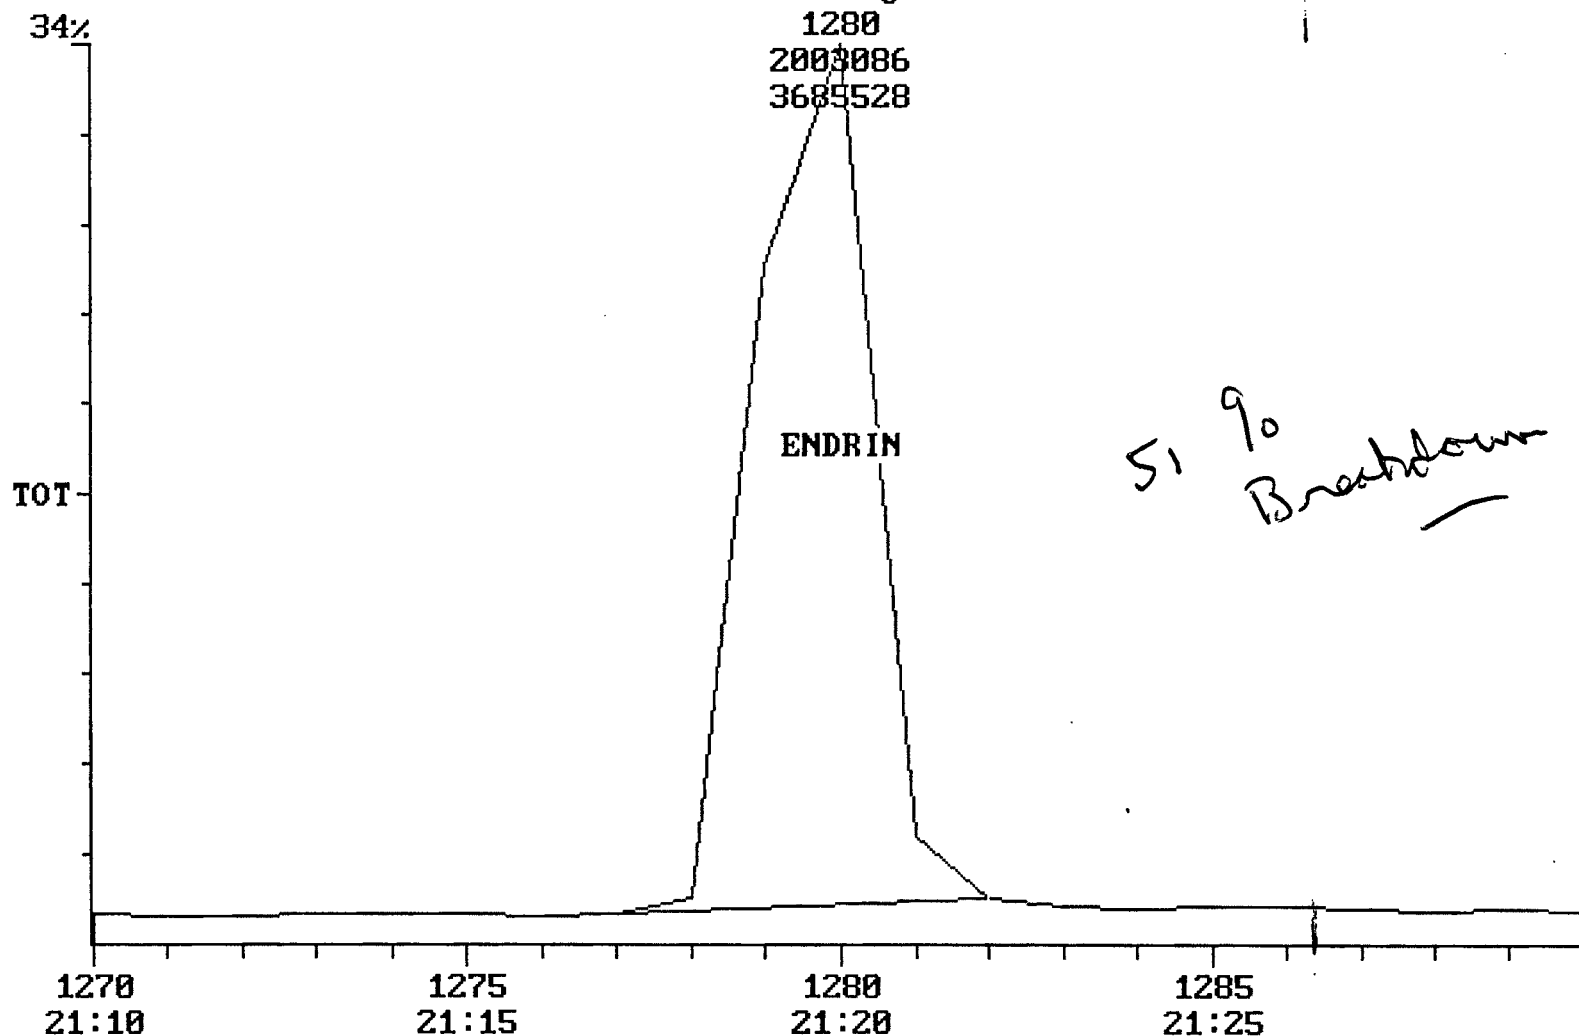

Chromatogram Plot

File: C:\DFTA0929

Date: Sep-29-1991 10:37:42

Comment: BOHLK; METHOD 525; INST 204; 09/28/01; DFTPP

Scan No: 1315

Retention Time: 21:55


RIC: 95197

Mass Range: 45 - 355

Plotted: 1290 to 1315

Range: 1 to 1860

100% = 6129435

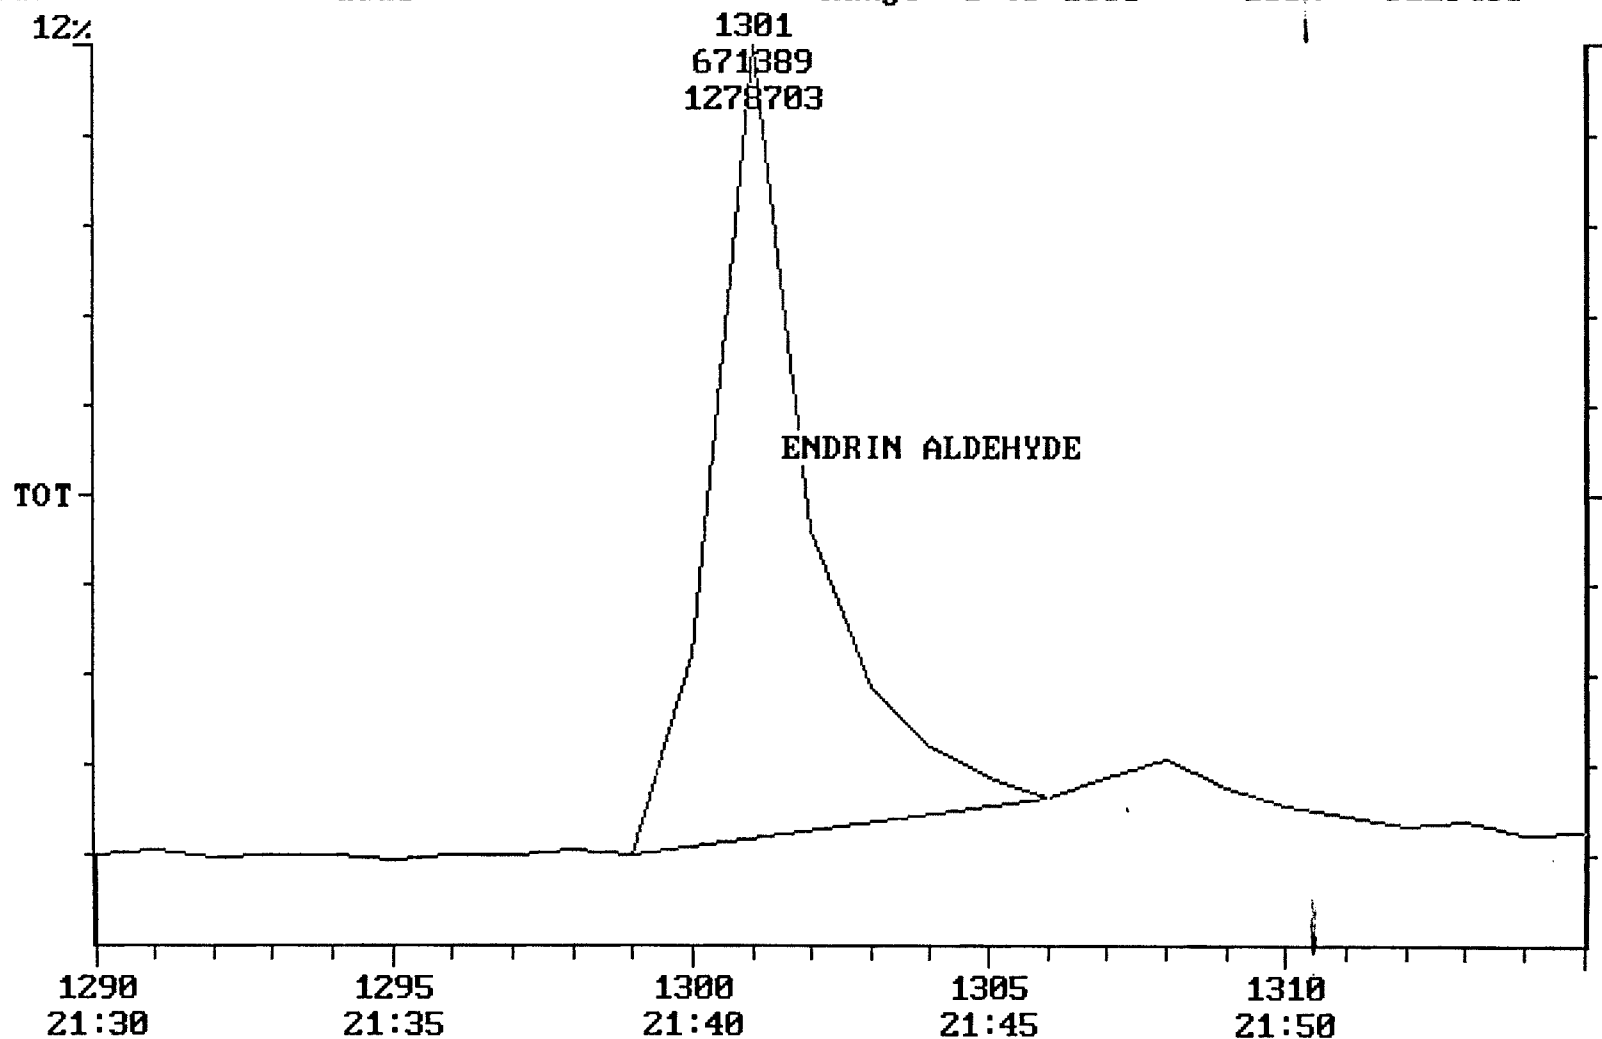

Chromatogram Plot

File: C:\DFTA0929

Date: Sep-29-1991 10:37:42

Comment: BOHLK; METHOD 525; INST 204; 09/28/01; DFIPP

Scan No: 1380

Retention Time: 23:00


RIC: 71157

Mass Range: 45 - 355

Plotted: 1360 to 1380

Range: 1 to 1860

100% = 6129435

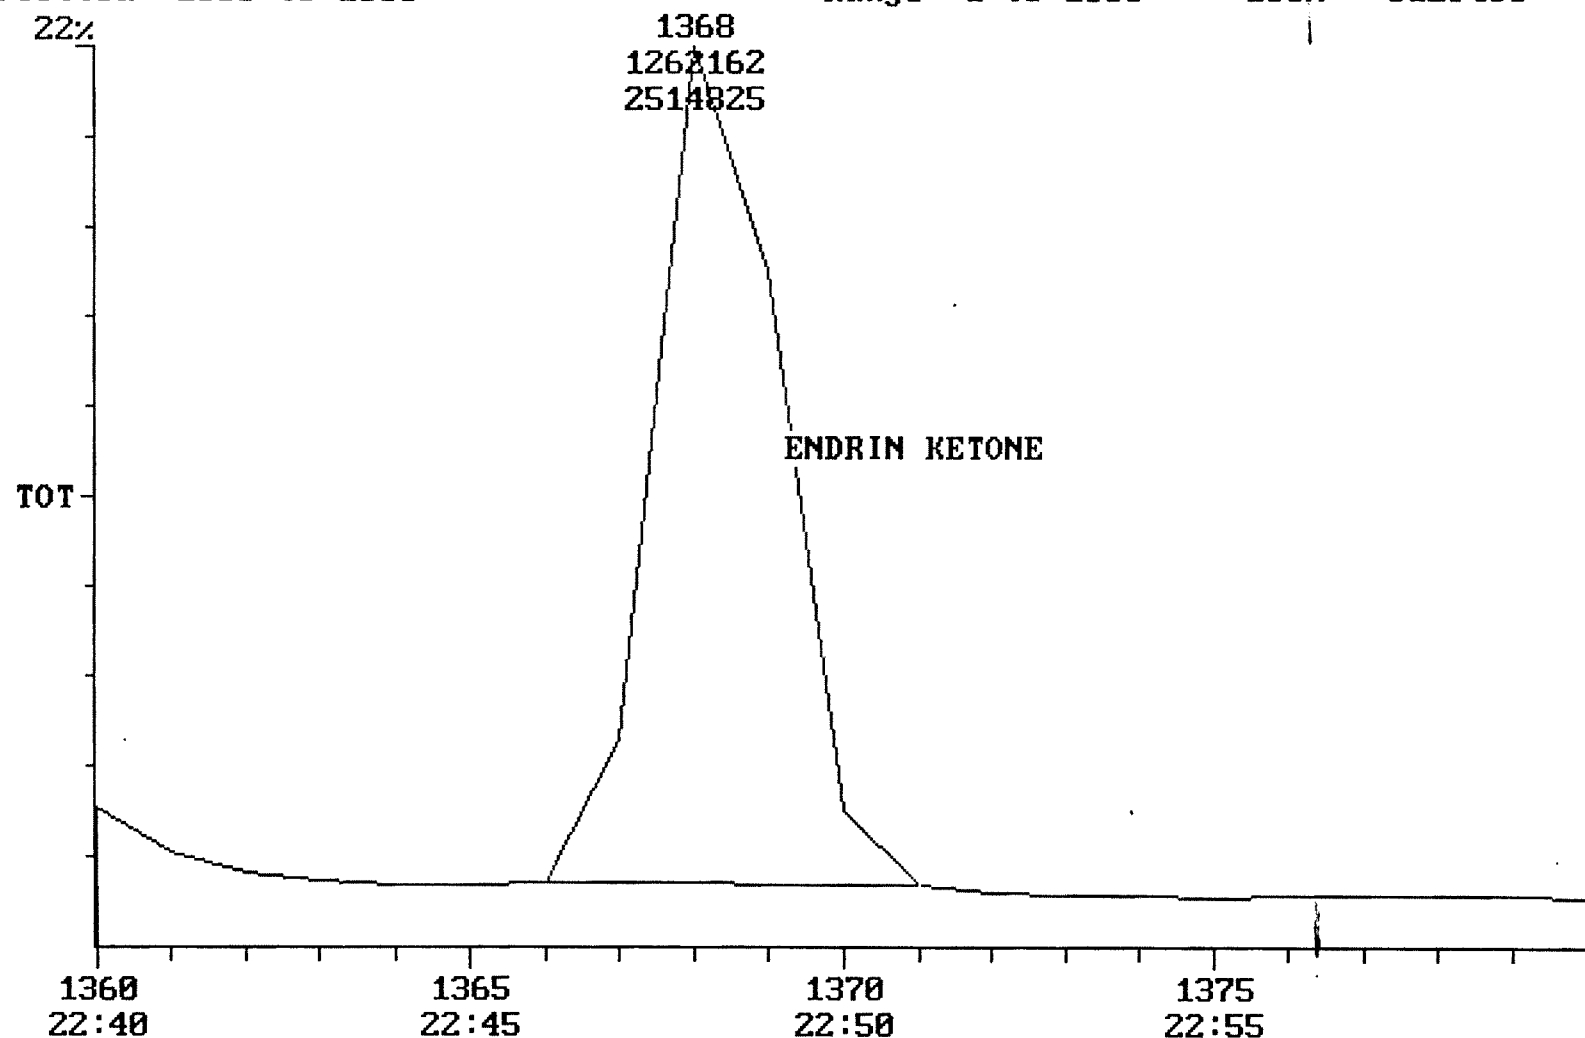

Chromatogram Plot

File: C:\DDTA0929

Date: Sep-29-1991 11:28:53

Comment: BOHLK; METHOD 525; INST 204; 09/28/01; DT

Scan No: 1

Retention Time: 0:01


RIC: 0

Mass Range: 0 - 0

Plotted: 1 to 1860

Range: 1 to 1860

100% = 4986039

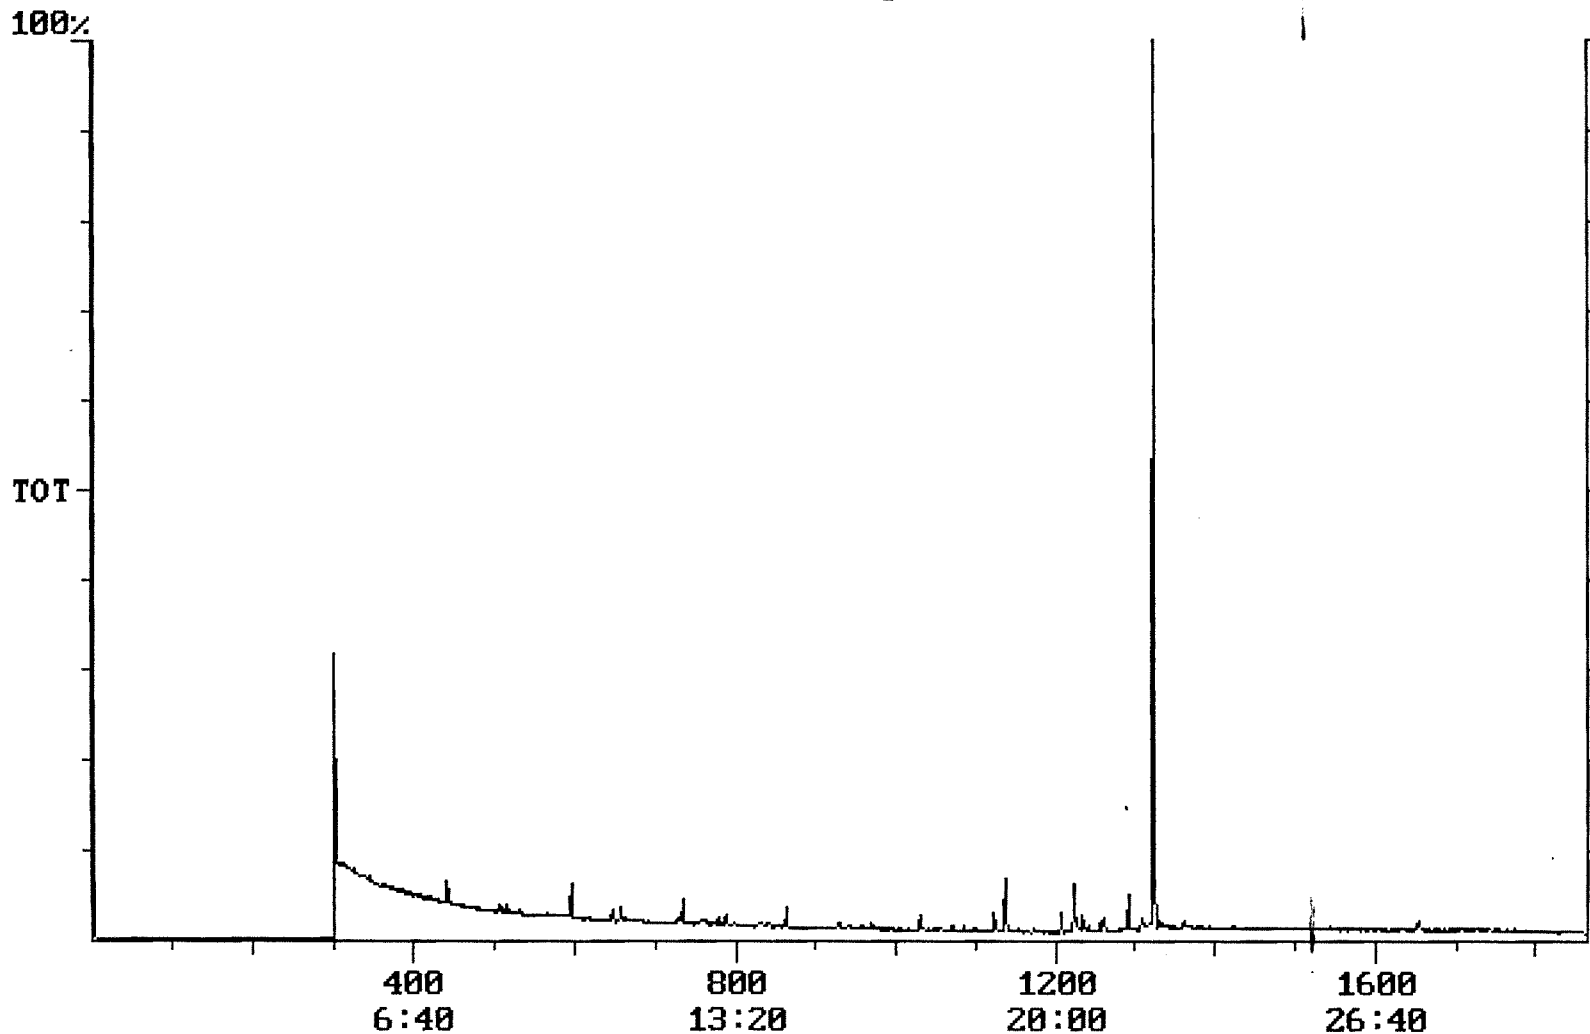

Chromatogram Plot

File: C:\DDTA0929

Date: Sep-29-1991 11:28:53

Comment: BOHLK; METHOD 525; INST 204; 09/28/01; DT

Scan No: 1270

Retention Time: 21:10


RIC: 52228

Mass Range: 45 - 207


Plotted: 1250 to 1270

Range: 1 to 1860

100% = 4986039

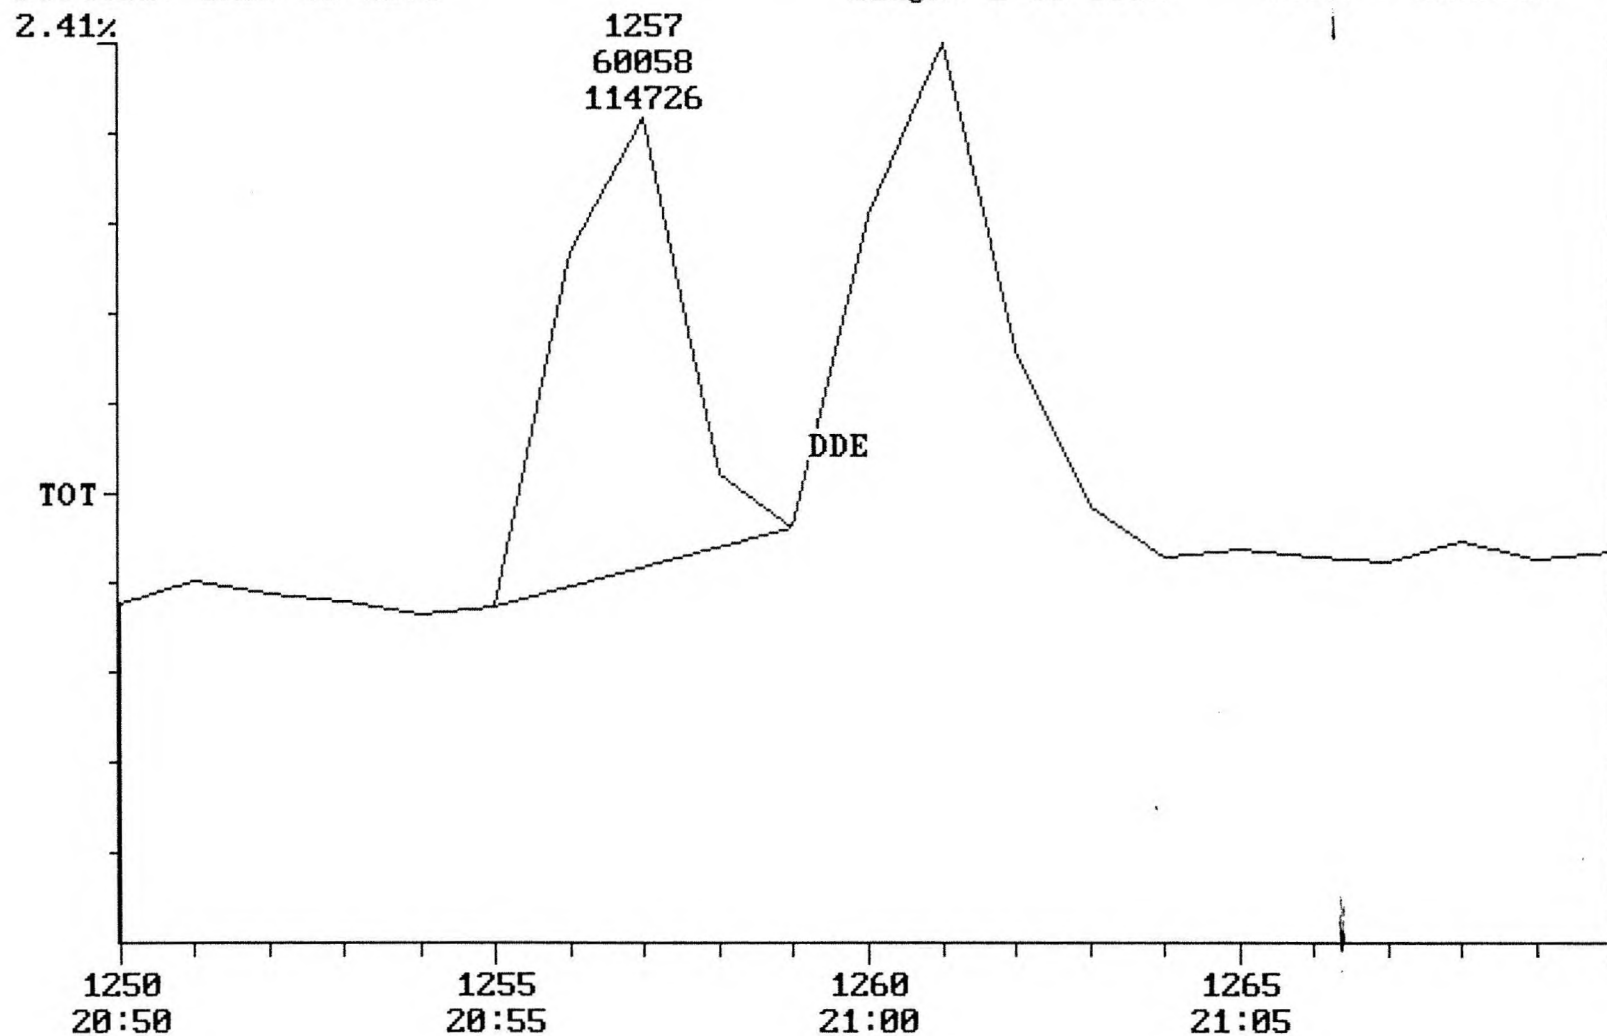

Chromatogram Plot File: C:\DDTA0929 Date: Sep-29-1991 11:28:53
Comment: BOHLK; METHOD 525; INST 204; 09/28/01; DT
Scan No: 1310 Retention Time: 21:50 RIC: 87692 Mass Range: 45 - 429
Plotted: 1280 to 1310 Range: 1 to 1860 100% = 4986039

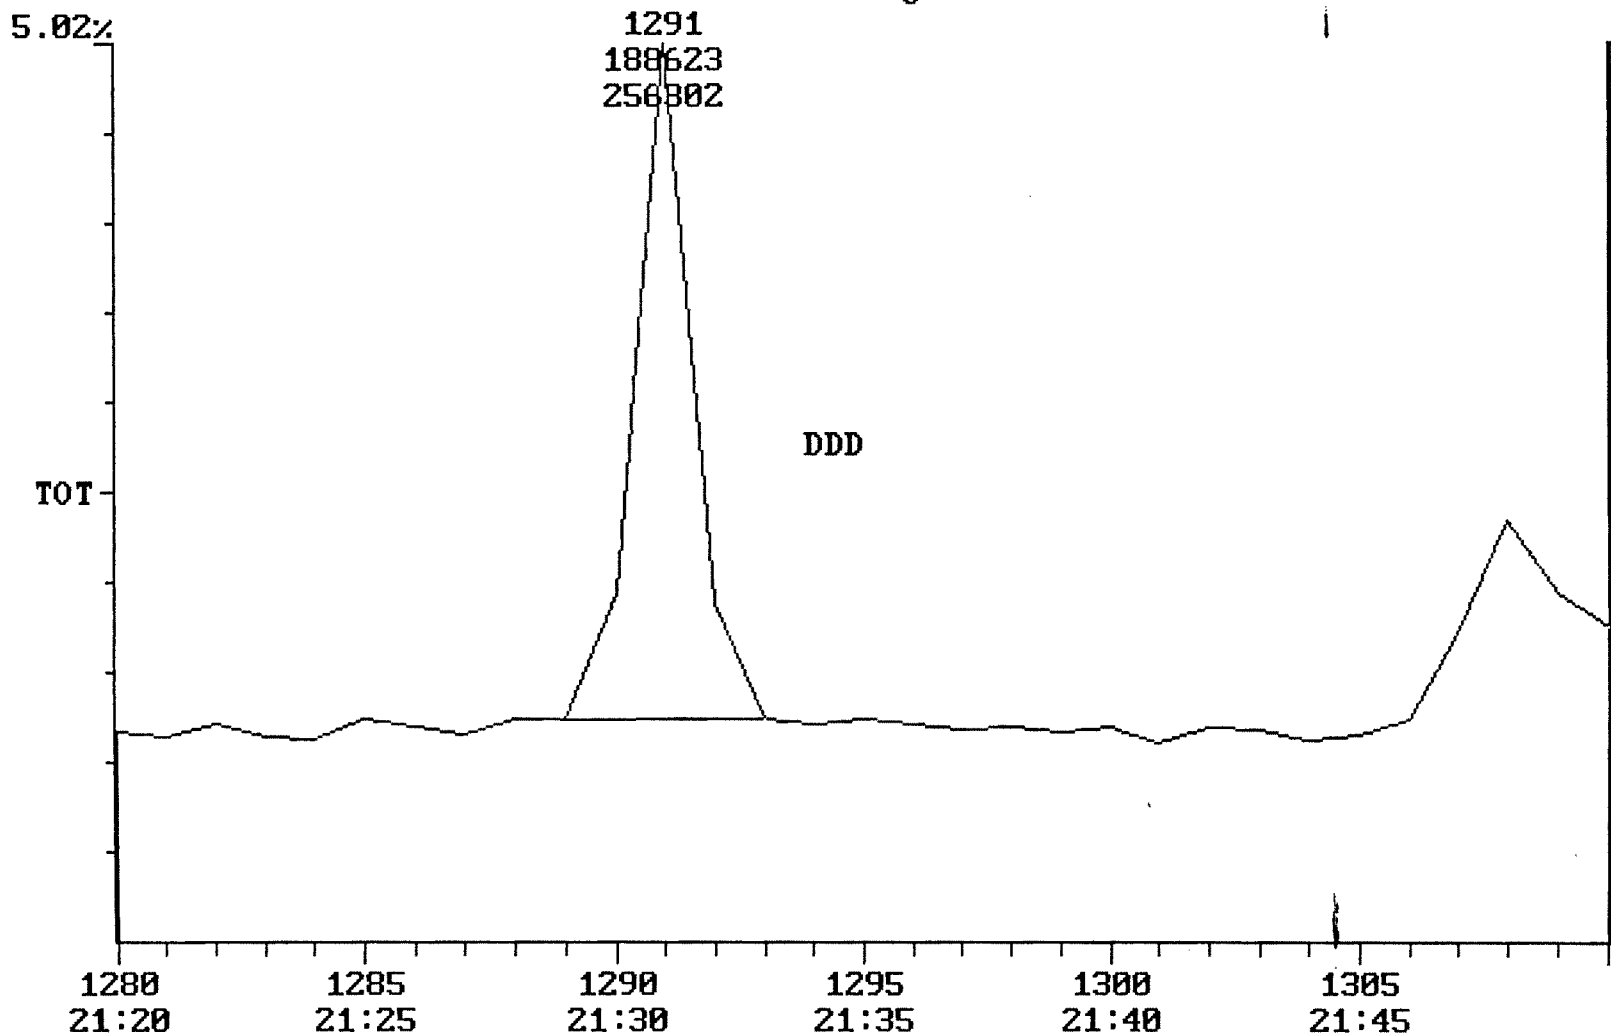

Chromatogram Plot

File: C:\DDTA0929

Date: Sep-29-1991 11:28:53

Comment: BOHLK; METHOD 525; INST 204; 09/28/01; DT

Scan No: 1349

Retention Time: 22:29


RIC: 71218

Mass Range: 45 - 281

Plotted: 1310 to 1349

Range: 1 to 1860

100% = 4986039

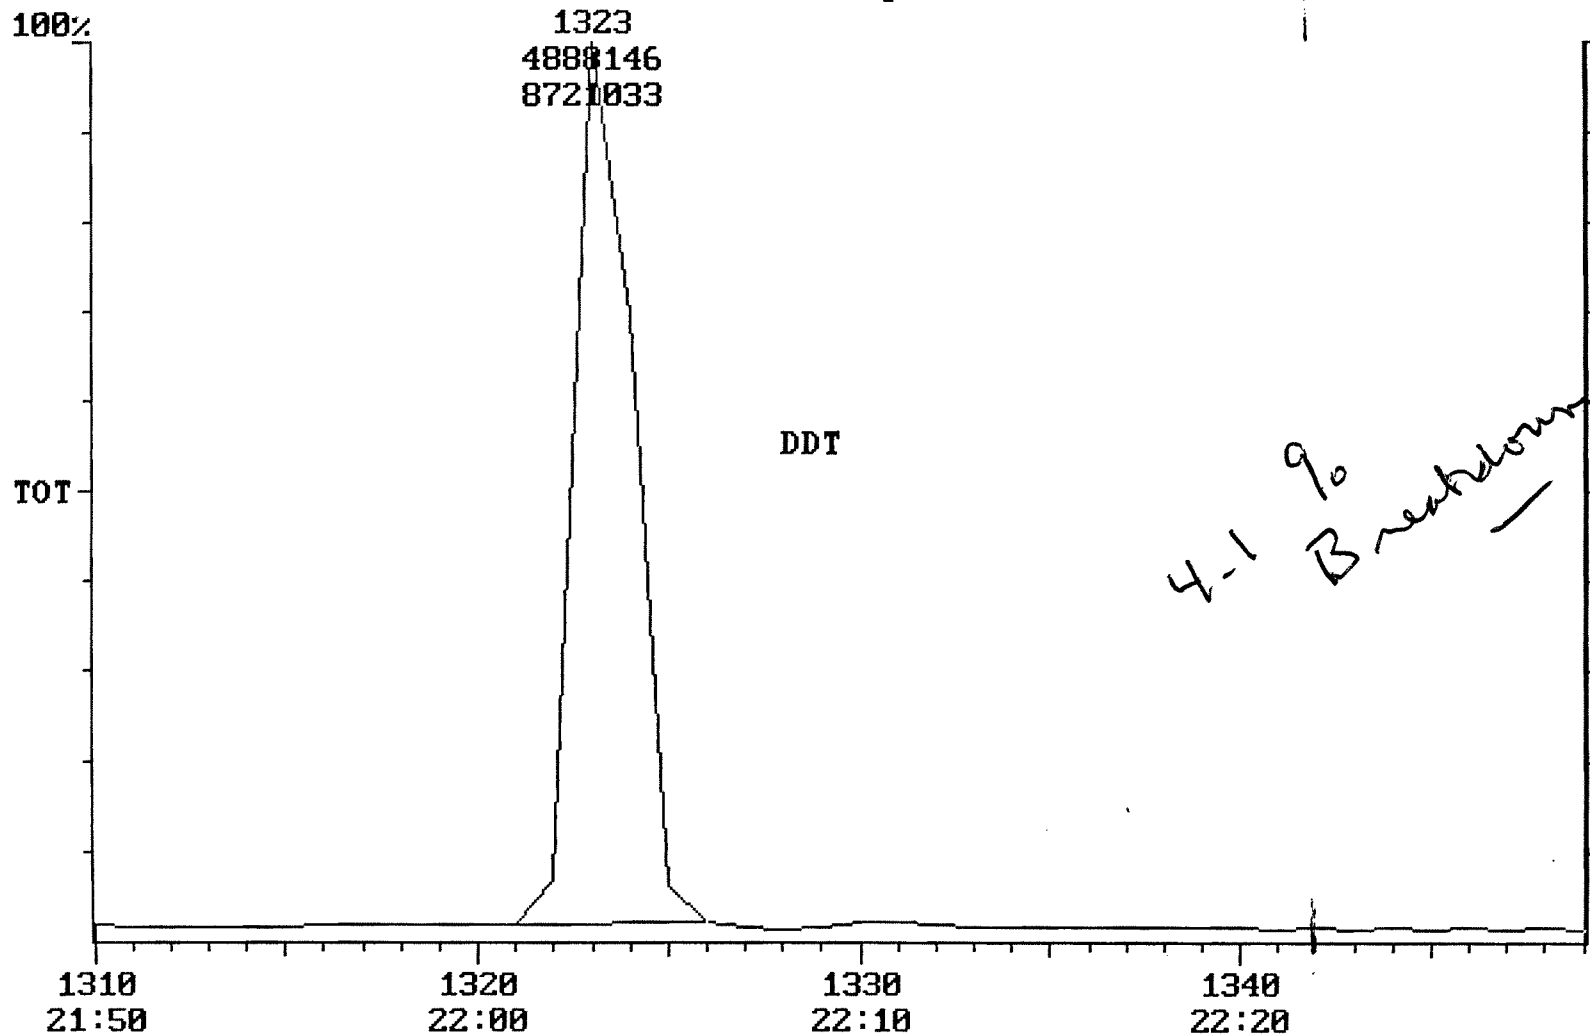

Chromatogram Plot

File: E:\DFTB0929

Date: Sep-29-1991 17:46:39

Comment: BOHLK; METHOD 525; INST 204; 09/29/01; DFTPP/ENDRIN

Scan No: 1

Retention Time: 0:01


RIC: 0

Mass Range: 0 - 0


Plotted: 1 to 1859

Range: 1 to 1859

100% = 7765938

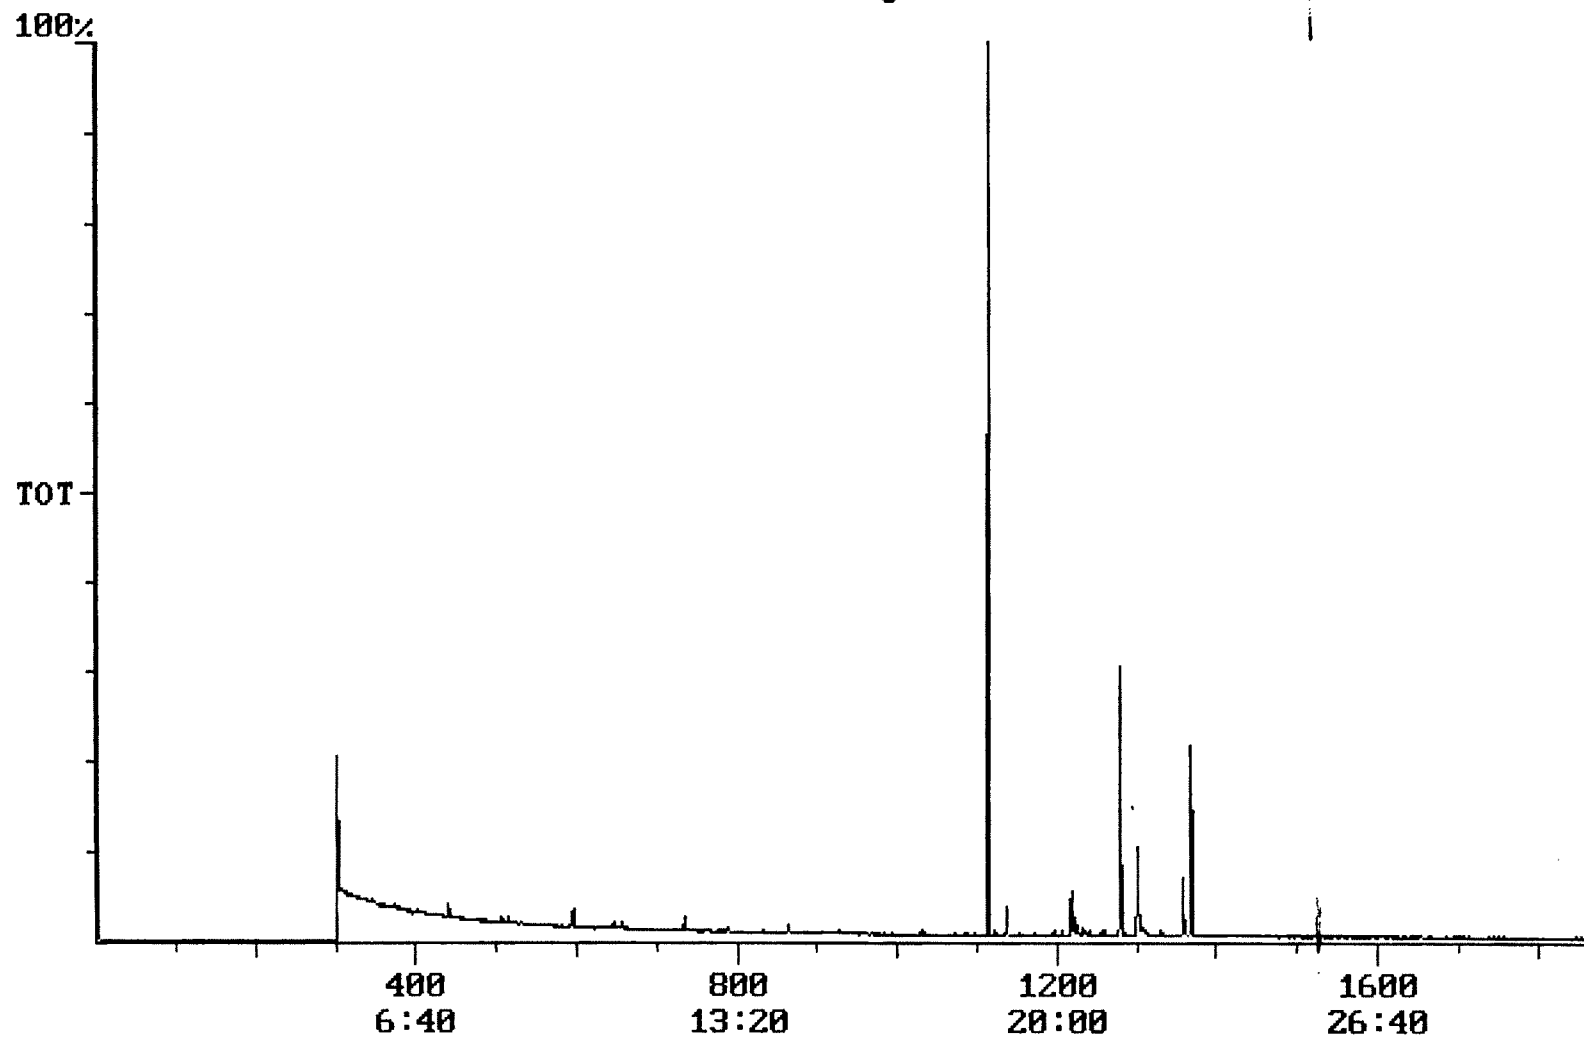

Chromatogram Plot File: E:\DFTB0929 Date: Sep-29-1991 17:46:39
Comment: BOHLK; METHOD 525; INST 204; 09/29/01; DFTPP/ENDRIN
Scan No: 1100 Retention Time: 18:20 RIC: 55031 Mass Range: 47 - 88
Plotted: 1100 to 1140 Range: 1 to 1859 100% = 7765938

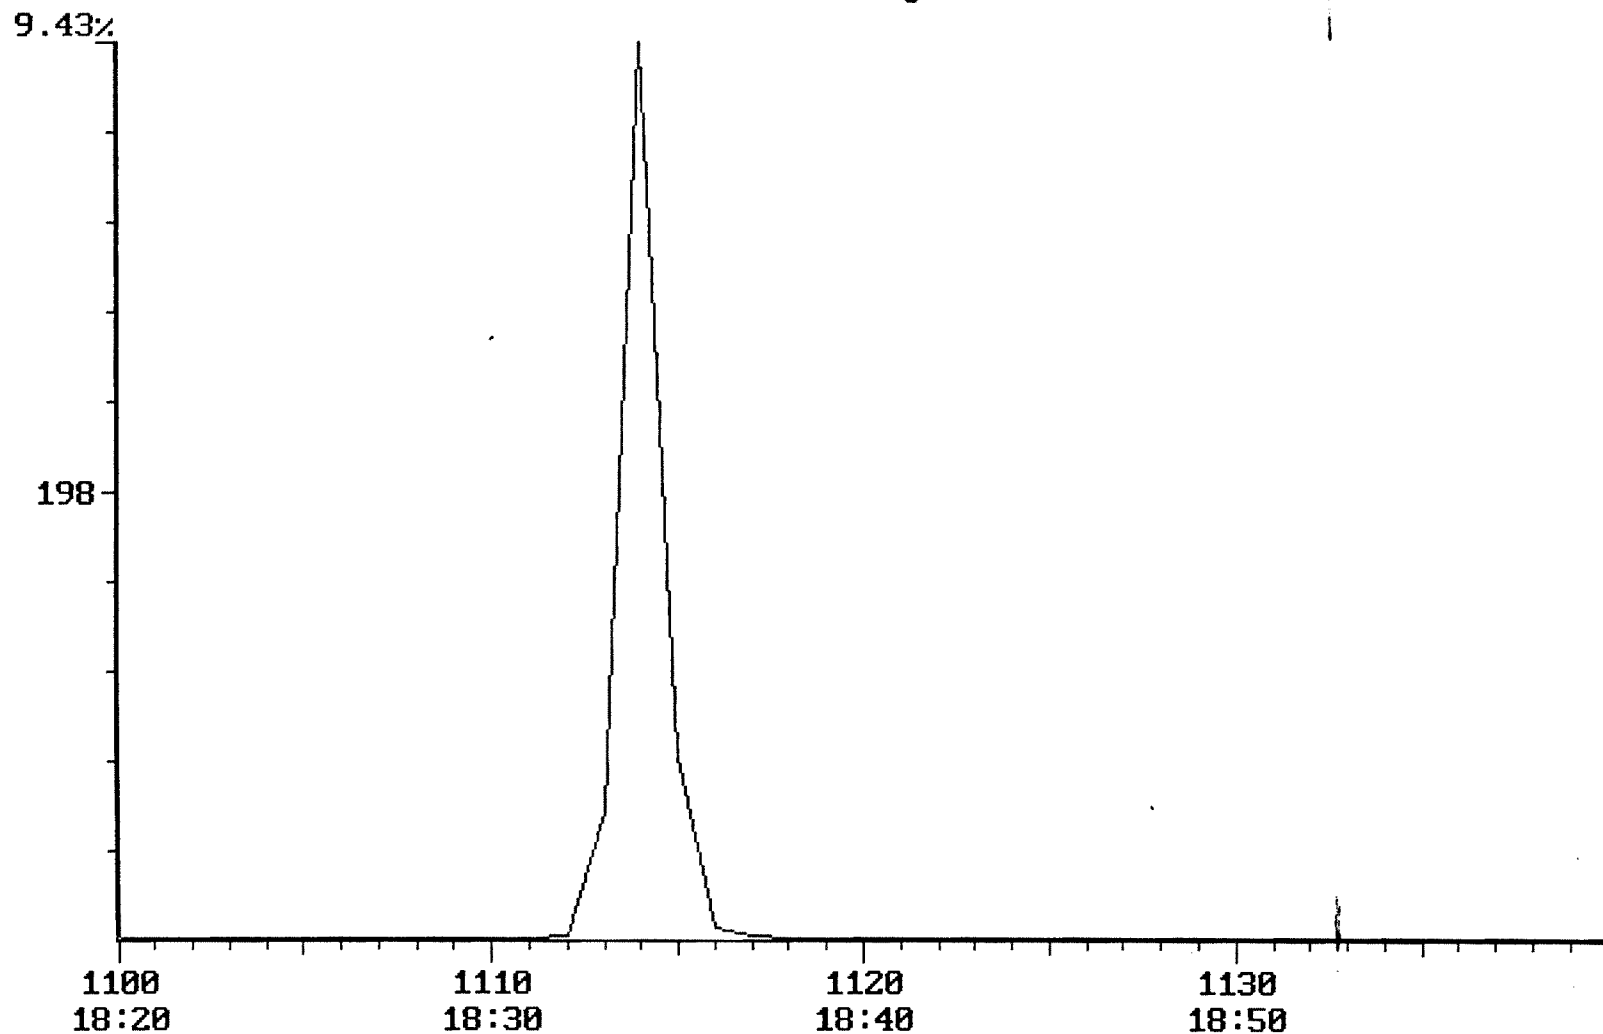

Mass List

File: E:\DFTB0929 Date: Sep-29-1991 17:46:39

Comment: BOHLK; METHOD 525; INST 204; 09/29/01; DFTPP/ENDRIN

Scan No: 1114 Retention Time: 18:34 RIC: 7765938 Mass Range: 49 - 445

Peaks: 171 Mass of Base Peak: 442 Int: 1254296 Threshold: 0 %

Mass	Intensity	% Base	Mass	Intensity	% Base	Mass	Intensity	% Base
49	26,171	2.09	84	7,421	0.59	124	3,515	0.28
50	185,937	14.82	85	7,031	0.56	125	6,250	0.50
51	485,937	38.74	86	12,890	1.03	127	239,843	19.12
52	24,609	1.96	87	4,687	0.37	128	20,312	1.62
55	8,593	0.69	91	4,687	0.37	129	103,906	8.28
56	14,453	1.15	92	5,078	0.40	130	8,593	0.69
57	20,703	1.65	93	56,640	4.52	131	3,125	0.25
58	2,343	0.19	96	5,078	0.40	134	6,250	0.50
61	6,640	0.53	98	51,171	4.08	135	9,765	0.78
62	8,984	0.72	99	24,218	1.93	136	5,078	0.40
63	13,671	1.09	101	9,765	0.78	137	6,640	0.53
65	5,078	0.40	103	7,812	0.62	140	3,906	0.31
67	2,343	0.19	104	9,375	0.75	141	17,187	1.37
68	7,421	0.59	105	7,031	0.56	142	6,640	0.53
69	343,750	27.41	107	117,578	9.37	143	3,515	0.28
73	7,421	0.59	108	15,625	1.25	147	9,765	0.78
74	59,765	4.76	109	5,468	0.44	148	24,218	1.93
75	53,125	4.24	110	199,218	15.88	149	5,078	0.40
76	25,000	1.99	111	25,390	2.02	153	5,468	0.44
77	364,453	29.06	112	3,906	0.31	154	6,250	0.50
78	26,171	2.09	116	7,421	0.59	155	10,546	0.84
79	44,921	3.58	117	149,218	11.90	156	12,500	1.00
80	21,484	1.71	118	5,859	0.47	157	4,296	0.34
81	30,468	2.43	122	7,031	0.56	158	5,078	0.40
82	3,906	0.31	123	8,593	0.69	159	2,734	0.22

Mass List

File: E:\DFTB0929 Date: Sep-29-1991 17:46:39

Comment: BOHLK; METHOD 525; INST 204; 09/29/01; DFTPP/ENDRIN

Scan No: 1114 Retention Time: 18:34 RIC: 7765938 Mass Range: 49 - 445

Peaks: 171 Mass of Base Peak: 442 Int: 1254296 Threshold: 0 %

Mass	Intensity	% Base	Mass	Intensity	% Base	Mass	Intensity	% Base
160	4,687	0.37	200	2,734	0.22	257	5,468	0.44
161	4,687	0.37	204	13,671	1.09	258	23,046	1.84
165	8,593	0.69	205	26,953	2.15	259	3,906	0.31
166	5,859	0.47	206	123,828	9.87	265	8,984	0.72
167	39,453	3.15	207	18,359	1.46	273	13,671	1.09
168	14,843	1.18	208	7,421	0.59	274	53,515	4.27
169	3,125	0.25	211	5,078	0.40	275	267,578	21.33
173	5,078	0.40	217	39,453	3.15	276	33,593	2.68
174	7,421	0.59	218	7,421	0.59	277	21,875	1.74
175	17,968	1.43	221	12,890	1.03	278	5,859	0.47
177	6,250	0.50	222	5,859	0.47	284	2,734	0.22
178	3,515	0.28	223	4,687	0.37	285	5,078	0.40
179	16,796	1.34	224	63,281	5.05	293	7,812	0.62
180	7,812	0.62	225	20,312	1.62	296	49,218	3.92
181	6,250	0.50	227	33,593	2.68	297	8,984	0.72
185	12,109	0.97	228	4,687	0.37	301	4,296	0.34
186	85,156	6.79	229	11,328	0.90	303	8,203	0.65
187	25,781	2.06	243	6,250	0.50	304	3,125	0.25
189	9,375	0.75	244	47,265	3.77	315	10,937	0.87
191	4,296	0.34	245	8,593	0.69	316	7,421	0.59
192	7,421	0.59	246	16,796	1.34	323	23,828	1.90
196	10,937	0.87	249	3,906	0.31	324	5,468	0.44
197	8,593	0.69	254	5,078	0.40	334	14,453	1.15
198	732,031	58.36	255	464,062	37.00	335	8,203	0.65
199	38,281	3.05	256	70,312	5.61	352	7,421	0.59

Mass List

File: E:\DFTB0929 Date: Sep-29-1991 17:46:39

Comment: BOHLK; METHOD 525; INST 204; 09/29/01; DFTPP/ENDRIN

Scan No: 1114 Retention Time: 18:34 RIC: 7765938 Mass Range: 49 - 445

Peaks: 171 Mass of Base Peak: 442 Int: 1254296 Threshold: 0 %

Mass	Intensity	% Base	Mass	Intensity	% Base	Mass	Intensity	% Base
196	10,937	0.87	249	3,906	0.31	324	5,468	0.44
197	8,593	0.69	254	5,078	0.40	334	14,453	1.15
198	732,031	58.36	255	464,062	37.00	335	8,203	0.65
199	38,281	3.05	256	70,312	5.61	352	7,421	0.59
200	2,734	0.22	257	5,468	0.44	353	9,375	0.75
204	13,671	1.09	258	23,046	1.84	354	12,890	1.03
205	26,953	2.15	259	3,906	0.31	355	4,687	0.37
206	123,828	9.87	265	8,984	0.72	364	2,734	0.22
207	18,359	1.46	273	13,671	1.09	365	75,781	6.04
208	7,421	0.59	274	53,515	4.27	366	8,203	0.65
211	5,078	0.40	275	267,578	21.33	372	19,531	1.56
217	39,453	3.15	276	33,593	2.68	373	6,640	0.53
218	7,421	0.59	277	21,875	1.74	402	4,687	0.37
221	12,890	1.03	278	5,859	0.47	403	10,156	0.81
222	5,859	0.47	284	2,734	0.22	404	4,687	0.37
223	4,687	0.37	285	5,078	0.40	421	7,812	0.62
224	63,281	5.05	293	7,812	0.62	422	10,546	0.84
225	20,312	1.62	296	49,218	3.92	423	61,718	4.92
227	33,593	2.68	297	8,984	0.72	424	8,984	0.72
228	4,687	0.37	301	4,296	0.34	425	2,734	0.22
229	11,328	0.90	303	8,203	0.65	441	193,750	15.45
243	6,250	0.50	304	3,125	0.25	442	1,254,296	100.00
244	47,265	3.77	315	10,937	0.87	443	243,359	19.40
245	8,593	0.69	316	7,421	0.59	444	23,437	1.87
246	16,796	1.34	323	23,828	1.90	445	3,125	0.25

Chromatogram Plot

File: E:\DFTB0929

Date: Sep-29-1991 17:46:39


Comment: BOHLK; METHOD 525; INST 204; 09/29/01; DFTPP/ENDRIN

Scan No: 1290 Retention Time: 21:30 RIC: 55532 Mass Range: 45 - 281

Plotted: 1270 to 1290

Range: 1 to 1859

100% = 7765938

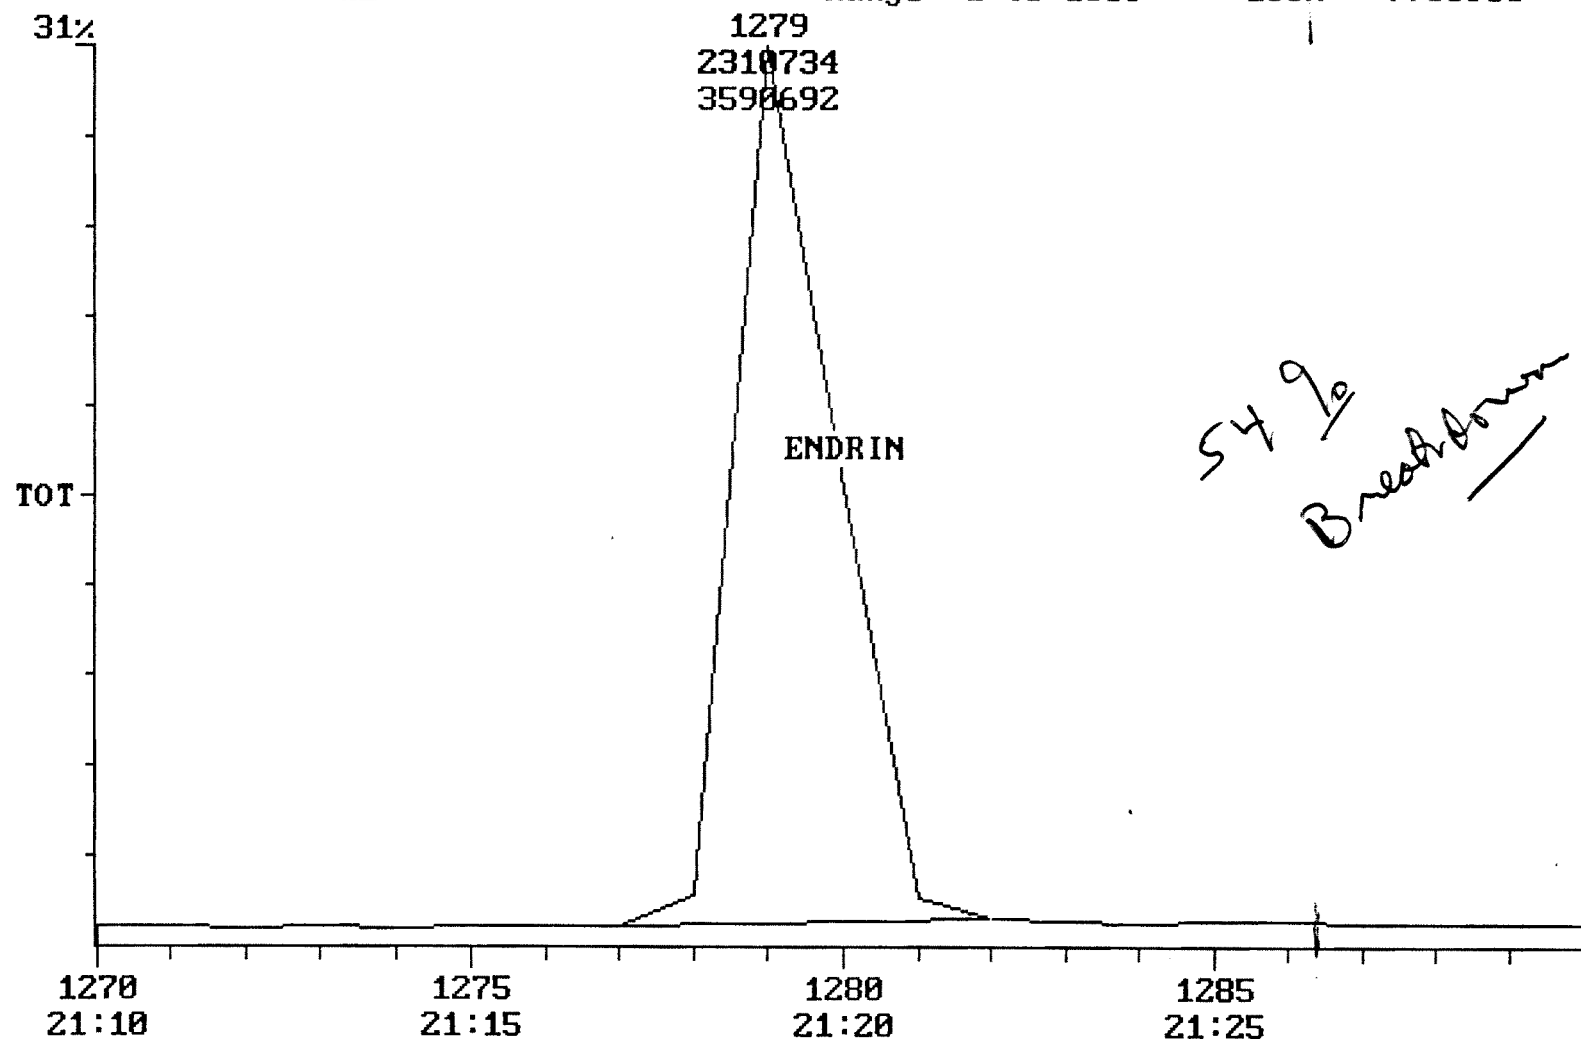

Chromatogram Plot

File: E:\DFTB0929

Date: Sep-29-1991 17:46:39


Comment: BOHLK; METHOD 525; INST 204; 09/29/01; DFTPP/ENDRIN

Scan No: 1315 Retention Time: 21:55 RIC: 64146 Mass Range: 45 - 281


Plotted: 1290 to 1315

Range: 1 to 1859

100% = 7765938

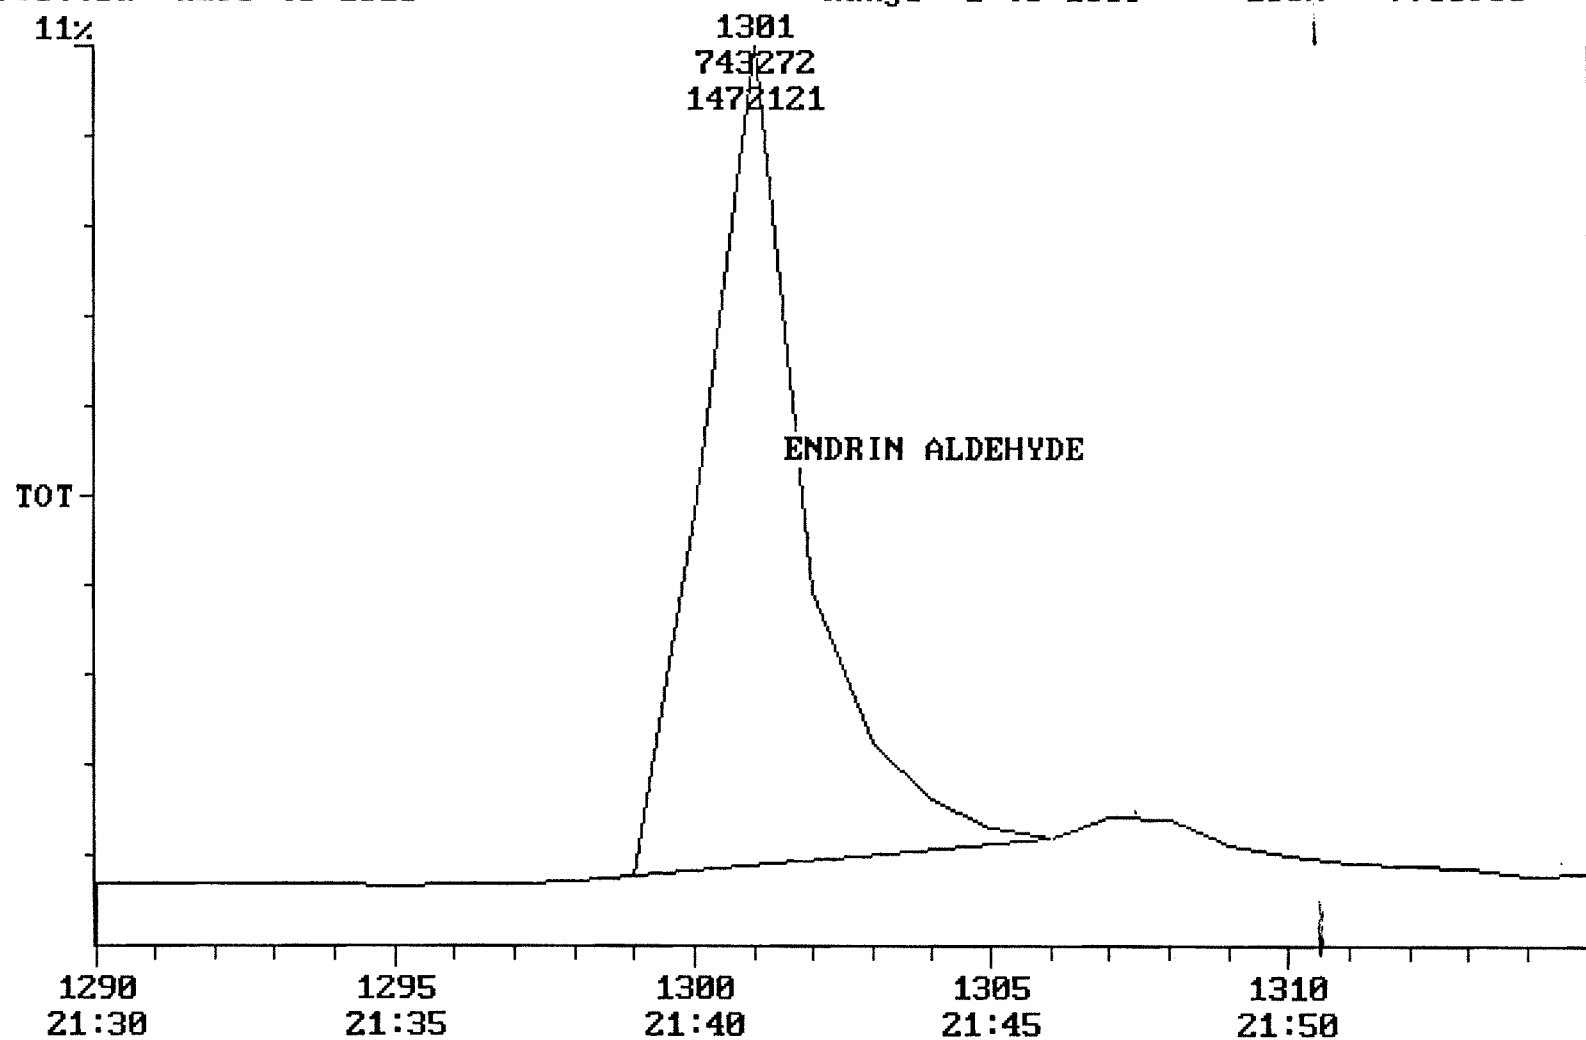

Chromatogram Plot File: E:\DFTB0929 Date: Sep-29-1991 17:46:39
Comment: BOHLK; METHOD 525; INST 204; 09/29/01; DFTPP/ENDRIN
Scan No: 1375 Retention Time: 22:55 RIC: 55825 Mass Range: 45 - 355
Plotted: 1362 to 1375 Range: 1 to 1859 100% = 7765938

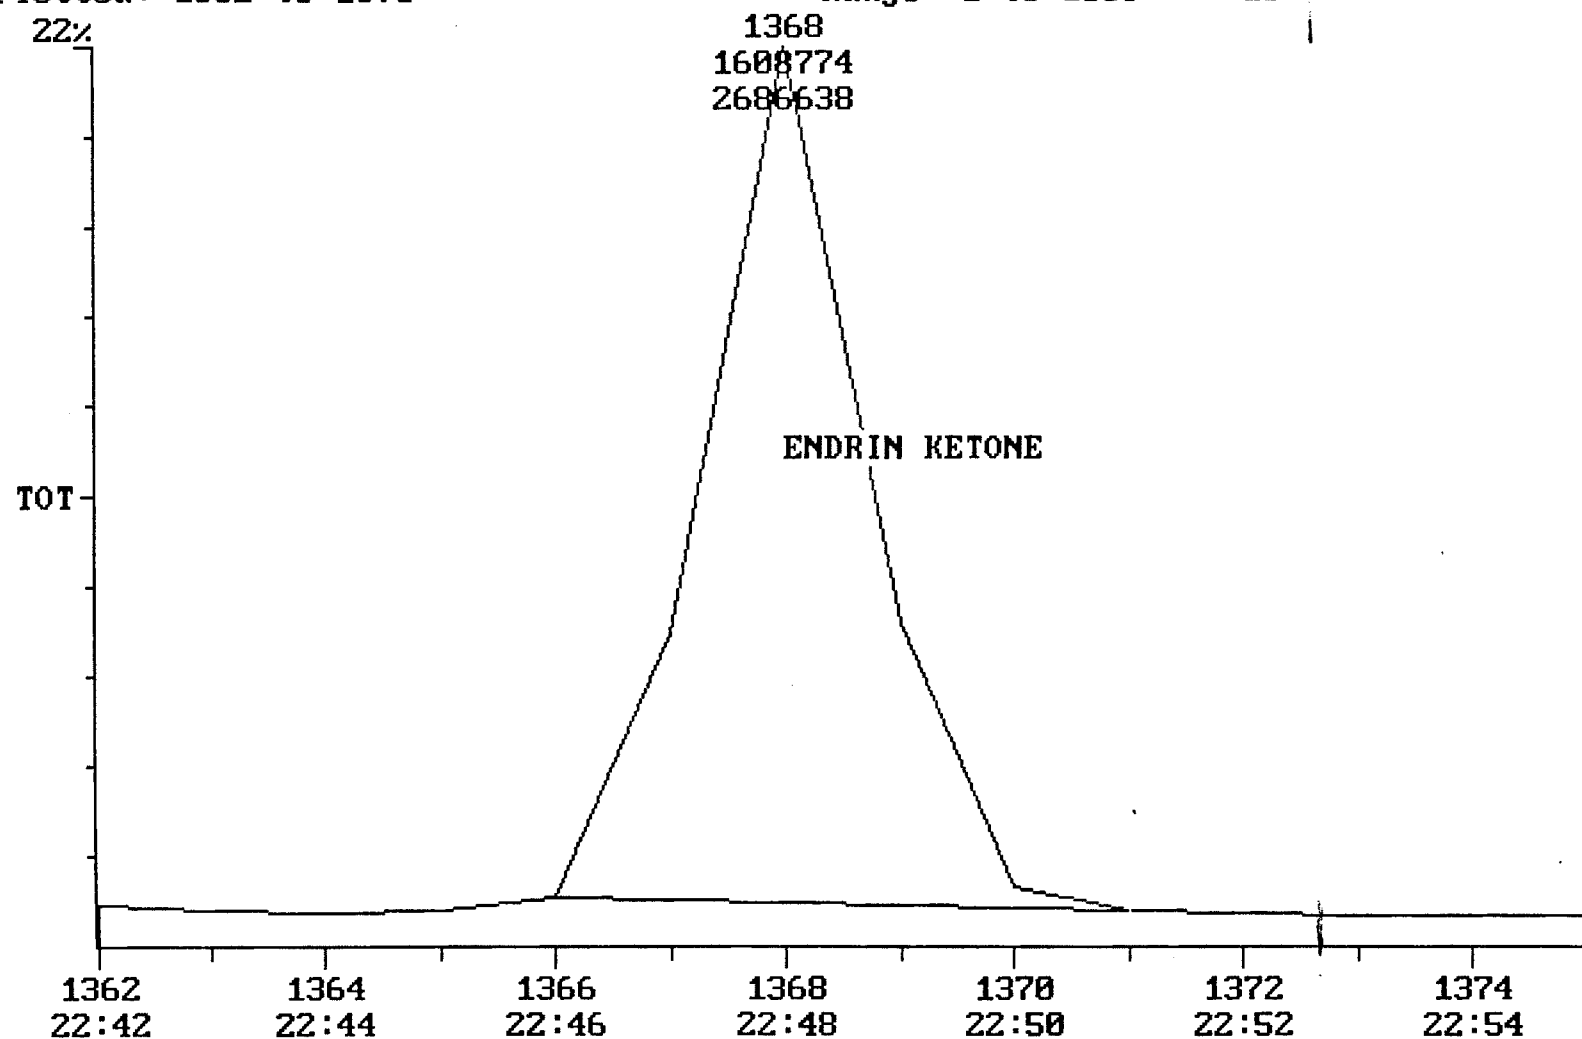

Chromatogram Plot

File: E:\DDTB0929

Date: Sep-29-1991 18:21:00

Comment: BOHLK; METHOD 525; INST 204; 09/29/01; DDT

Scan No: 1

Retention Time: 0:01


RIC: 0

Mass Range: 0 - 0

Plotted: 1 to 1860

Range: 1 to 1860

100% = 4418073

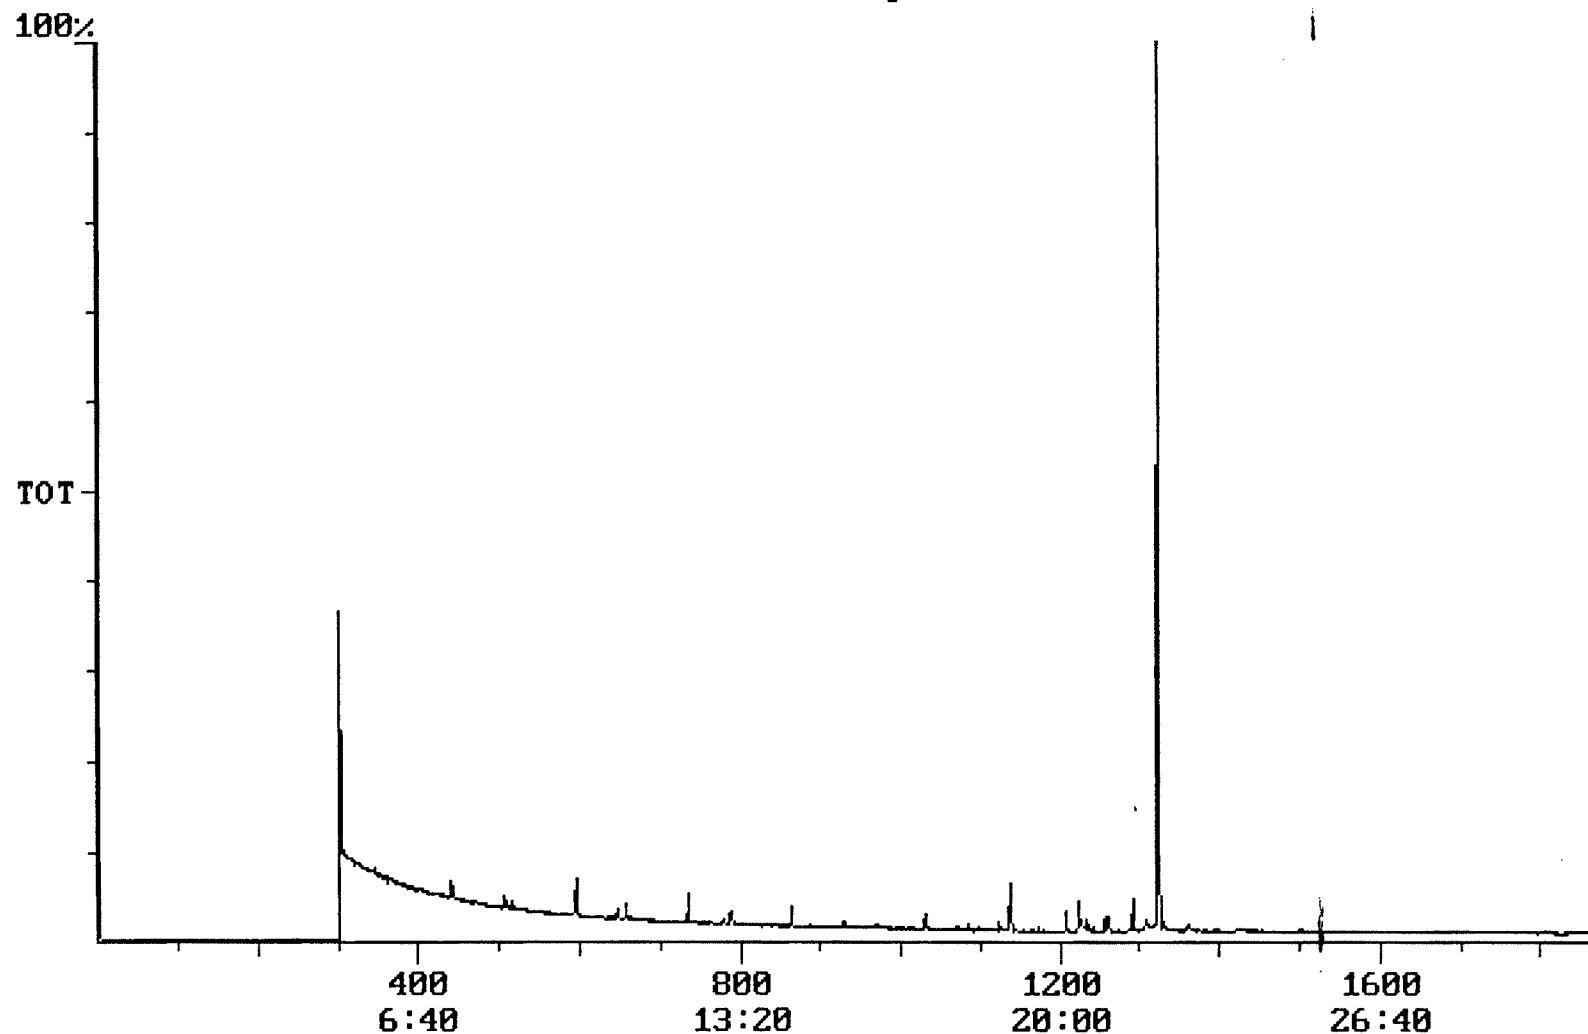

Chromatogram Plot

File: E:\DDTB0929

Date: Sep-29-1991 18:21:00

Comment: BOHLK; METHOD 525; INST 204; 09/29/01; DDT

Scan No: 1270

Retention Time: 21:10

RIC: 47297


Mass Range: 45 - 207

Plotted: 1240 to 1270

Range: 1 to 1860

100% = 4418073

2.85%

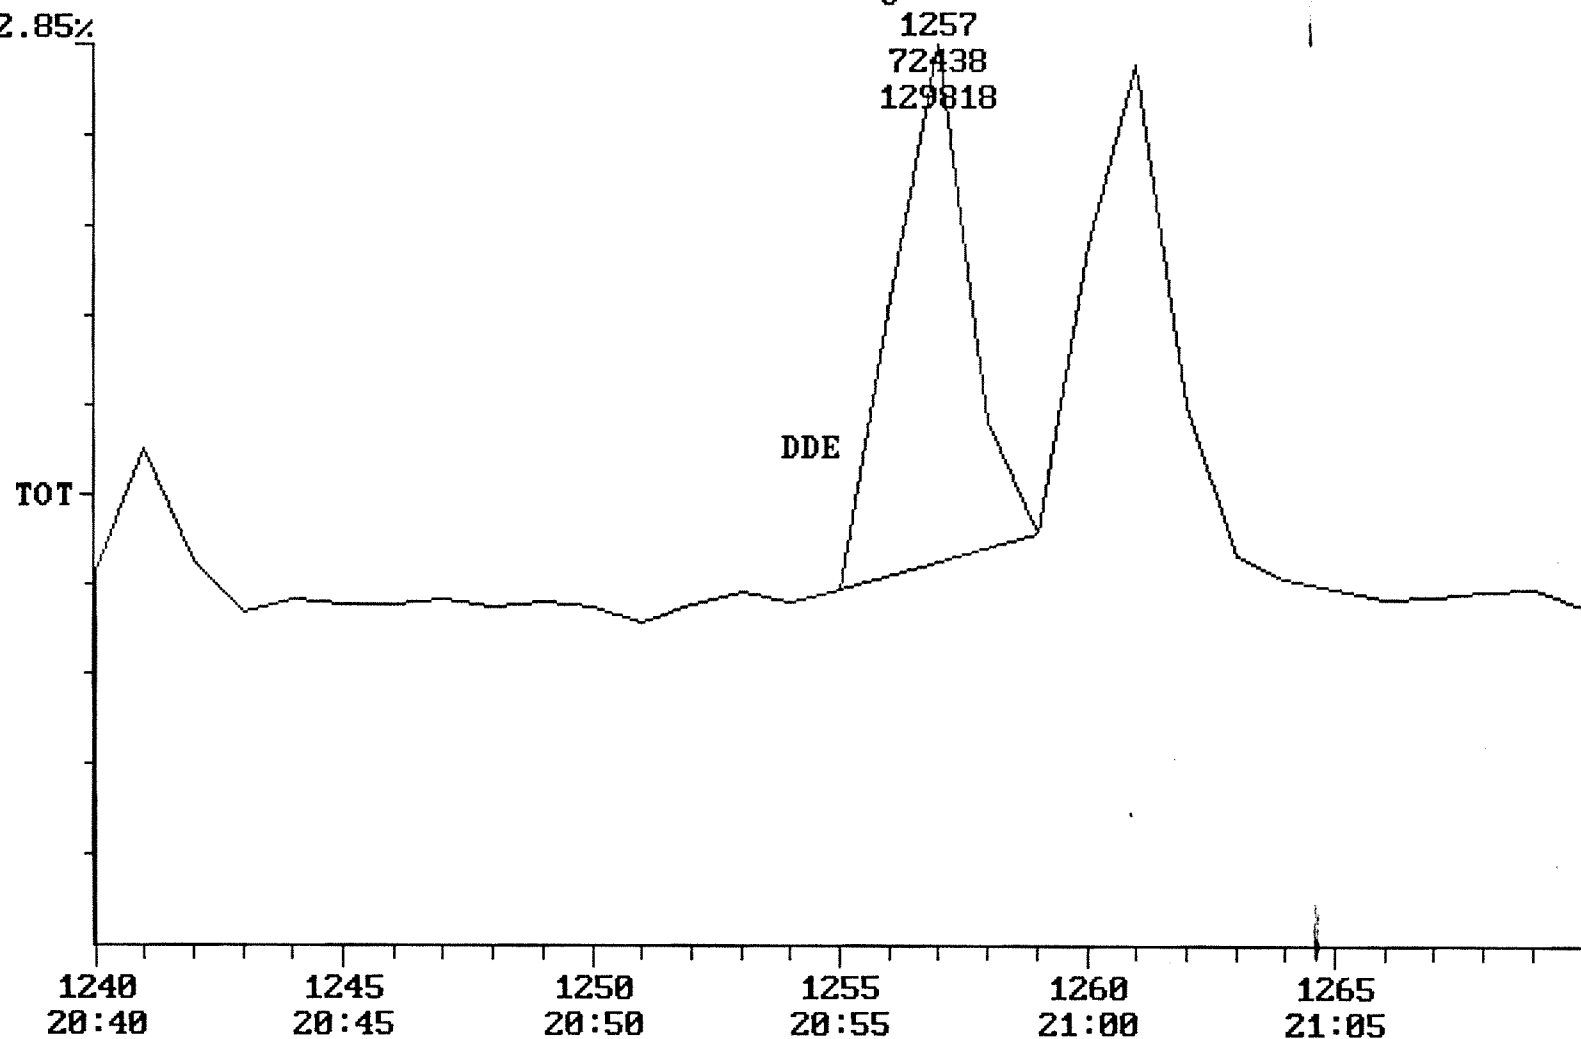

Chromatogram Plot

File: E:\DDTB0929

Date: Sep-29-1991 18:21:00

Comment: BOHLK; METHOD 525; INST 204; 09/29/01; DDT

Scan No: 1300

Retention Time: 21:40

RIC: 50419


Mass Range: 45 - 281

Plotted: 1280 to 1300

Range: 1 to 1860

100% = 4418073

4.69%

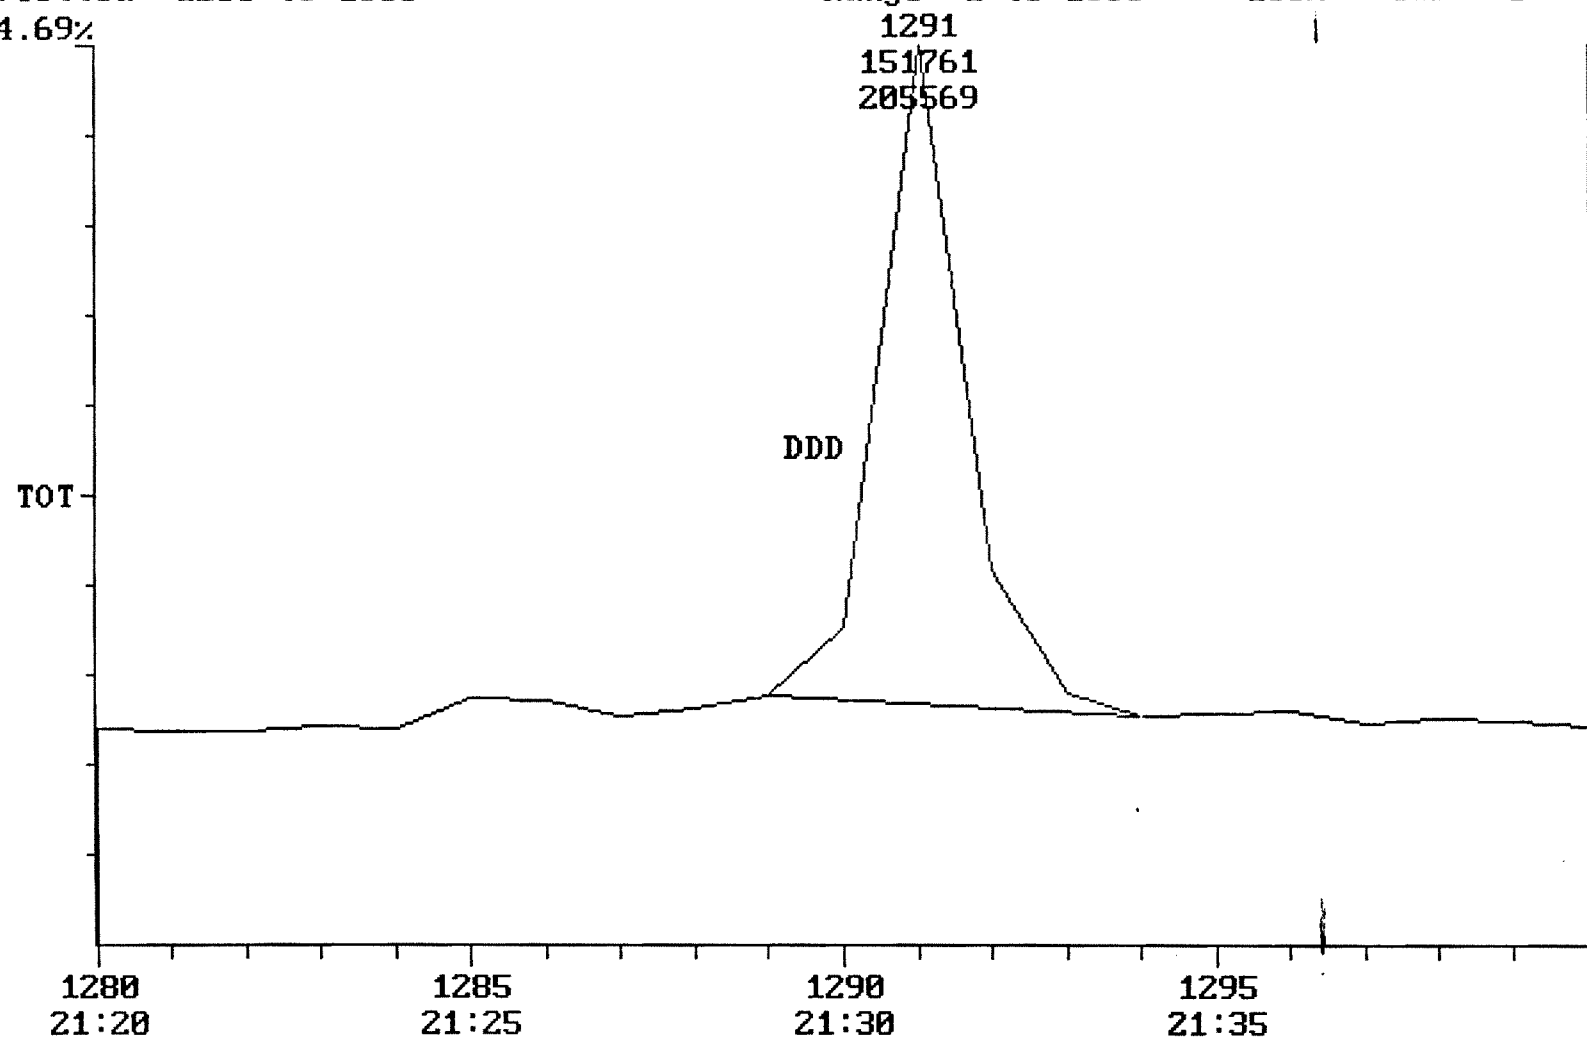

Chromatogram Plot

File: E:\DDTB0929

Date: Sep-29-1991 18:21:00

Comment: BOHLK; METHOD 525; INST 204; 09/29/01; DDT

Scan No: 1350

Retention Time: 22:30

RIC: 49696

Mass Range: 45 - 281

Plotted: 1300 to 1350

Range: 1 to 1860

100% = 4418073

