

Method 508

Date Extracted

10/2/01

Page

1196cms

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH =7	Count
	Lab. cell	500ml		✓			2ml			
	Ref Chloroform									
	MDL Chloroform									
	PRL 1016									
2390	Spike pest				✓					
2390	Spike chlopest				✓					
23844	Spike chloroform				✓					
23844	Spike chloroform				✓					
	23844 ✓									9
	2390 ✓									10
	23901 ✓									11
	23902 ✓									12
	23903 ✓									13
	23904 ✓									14
	23905 ✓									15
	23906 ✓									16
	23909 ✓									17
	23910 ✓									18
	23913 ✓									19
	22558 ✓	450ml		↓			↓			20
Reviewed by <u>JB 1/22/02</u>										
Remarks										
22558 re-extracted 450 ml										
PRL went to depress										
MDL went to depress										
drip rate must be between 5-15 ml/min for liq-liq extractors										
Extraction type - <u>Syft.</u>										
Solv. lot#										
NaCl lot# <u>T12617</u>										
Na2SO4 lot# <u>V18617</u>										
STANDARD	INT STD LOG#									
CALIBRATION										
REF/SPIKE	PRL 1500u	pest 200u	chlon 175u							
MDL/MDRF										
Q. CHECK										
INT. STD.										
SURROGATE	2064C									
LPC										
ENDRIN/DDT										

Analyst

my/AD

revision 4/12/01

Verified by

Reviewed by

Date

DW
10/27/1

Sequence Name: C:\HPCHEM\1\SEQUENCE\OCT1801.S
Comment: INST 209; 30Mx0.25umX0.50
Operator: 209 GALOS
Data Path: C:\HPCHEM\1\data\oct1801\
Pre-Seq Cmd:
Post-Seq Cmd:

Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP	NP091101	
2 Sample	2	LB	NP091101	lab blk 10/15
3 Sample	3	23906	NP091101	gc/ms unknown
4 Sample	4	23909	NP091101	gc/ms unknown
5 Sample	5	23910	NP091101	gc/ms unknown
6 Sample	6	23913	NP091101	gc/ms unknown
7 Sample	7	23340	NP091101	gc/ms unknown re extracted
8 Sample	8	23359	NP091101	gc/ms unknown re extracted
9 Sample	9	23341	NP091101	gc/ms unknown re extracted
10 Sample	10	23472	NP091101	gc/ms unknown re extracted
11 Sample	11	23342	NP091101	gc/ms unknown re extracted
12 Sample	12	23344	NP091101	gc/ms unknown re extracted

DFTPP

Data File : C:\HPCHEM\1\DATA\OCT1801\DFTPP.D

Acq On : 18 Oct 2001 4:10 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP091101.M (RTE Integrator)


Title : 209 625/TCLP calibration table 7/16/01

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

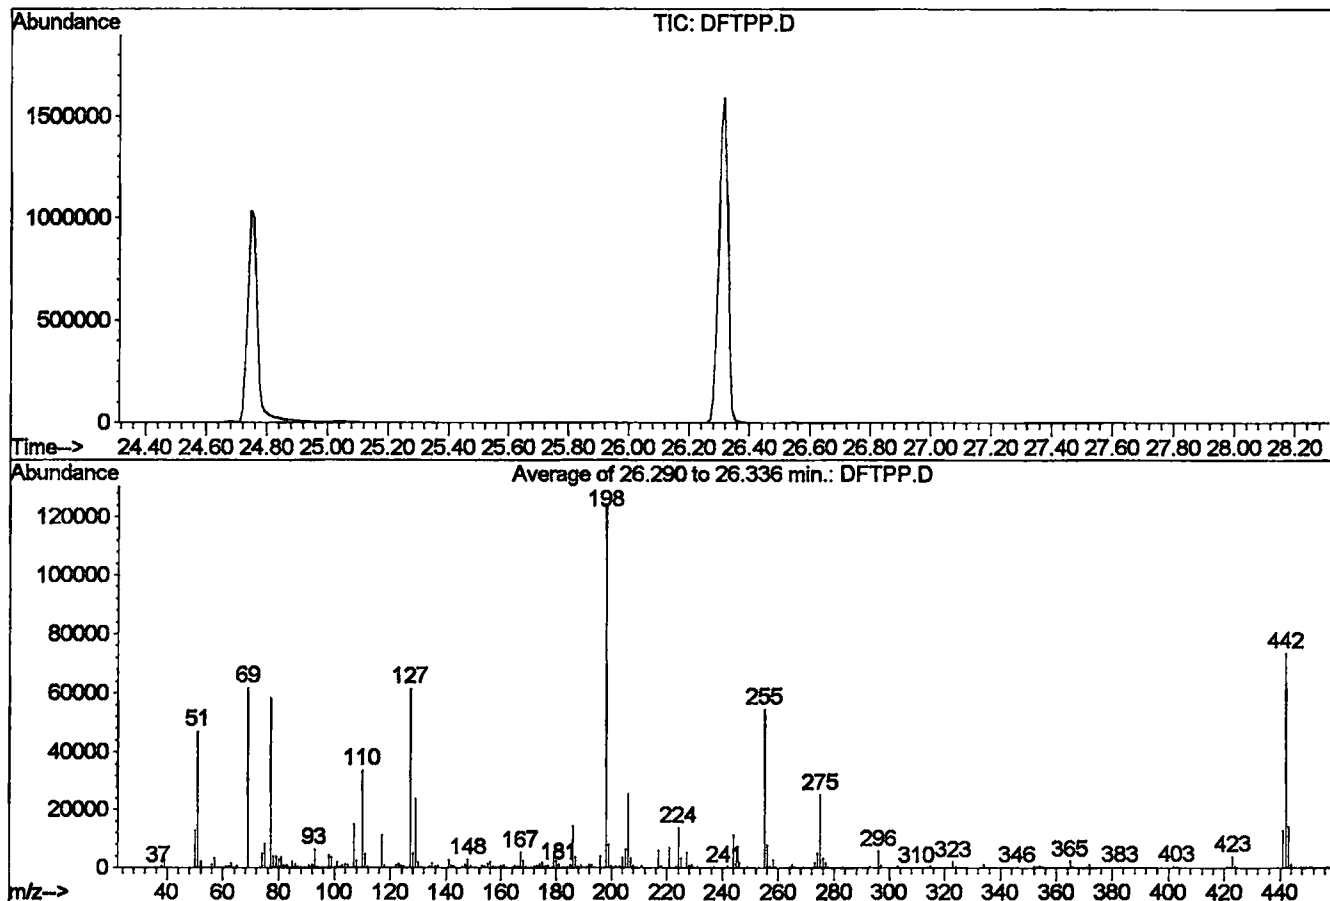

Spectrum Information: Average of 26.290 to 26.336 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	37.9 ✓	47047	PASS
68	69	0.00	2	0.0 ✓	0	PASS
69	198	0.00	100	49.7 ✓	61758	PASS
70	69	0.00	2	0.0 ✓	0	PASS
127	198	40	60	49.5 ✓	61541	PASS
197	198	0.00	1	0.0 ✓	0	PASS
198	198	100	100	100.0 ✓	124239	PASS
199	198	5	9	6.5 ✓	8094	PASS
275	198	10	30	20.4 ✓	25340	PASS
365	198	1	100	1.9 ✓	2329	PASS
441	443	0.01	100	90.9 ✓	12851	PASS
442	198	40	110	59.2 ✓	73570	PASS
443	442	17	23	19.2 ✓	14141	PASS