

GCMs

Reviewed by  
JB 1/20/02

Reviewed by \_\_\_\_\_  
Date \_\_\_\_\_

Sequence Name: C:\HPCHEM\1\SEQUENCE\OCT1701.S  
Comment: INST 209; 30Mx0.25umX0.50  
Operator: 209 GALOS  
Data Path: C:\HPCHEM\1\data\oct1701\  
Pre-Seq Cmd:  
Post-Seq Cmd:

|                        |                       |
|------------------------|-----------------------|
| Method Sections To Run | On A Barcode Mismatch |
| (X) Full Method        | (X) Inject Anyway     |
| ( ) Reprocessing Only  | ( ) Don't Inject      |

| Line | Type   | Vial | DataFile | Method   | Sample Name                |
|------|--------|------|----------|----------|----------------------------|
| 1    | Sample | 1    | DFTPP    | NP091101 |                            |
| 2    | Sample | 2    | LB       | NP091101 | lab blk 10/2               |
| 3    | Sample | 3    | 22558    | NP091101 | gc/ms unknown re extracted |
| 4    | Sample | 4    | 23844    | NP091101 | gc/ms unknown              |
| 5    | Sample | 5    | 23900    | NP091101 | gc/ms unknown              |
| 6    | Sample | 6    | 23901    | NP091101 | gc/ms unknown              |
| 7    | Sample | 7    | 23902    | NP091101 | gc/ms unknown              |
| 8    | Sample | 8    | 23903    | NP091101 | gc/ms unknown              |
| 9    | Sample | 9    | 23904    | NP091101 | gc/ms unknown              |
| 10   | Sample | 10   | 23905    | NP091101 | gc/ms unknown              |
| 11   | Sample | 11   | LBA      | NP091101 | lab blk 10/4               |
| 12   | Sample | 12   | 23914    | NP091101 | gc/ms unknown              |
| 13   | Sample | 13   | 23915    | NP091101 | gc/ms unknown              |
| 14   | Sample | 14   | 23947    | NP091101 | gc/ms unknown              |
| 15   | Sample | 15   | 23948    | NP091101 | gc/ms unknown              |
| 16   | Sample | 16   | 23994    | NP091101 | gc/ms unknown              |
| 17   | Sample | 17   | 23993    | NP091101 | gc/ms unknown              |
| 18   |        |      |          |          |                            |

DFTPP

Data File : C:\HPCHEM\1\DATA\OCT1701\DFTPP.D

Acq On : 17 Oct 2001 1:10 pm

Sample :

Misc :

MS Integration Params: RTEINT.P

Method : C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)


Title : 209 625/TCLP calibration table 7/16/01

Vial: 1

Operator: 209 GALOS

Inst : GC/MS 209

Multiplr: 1.00

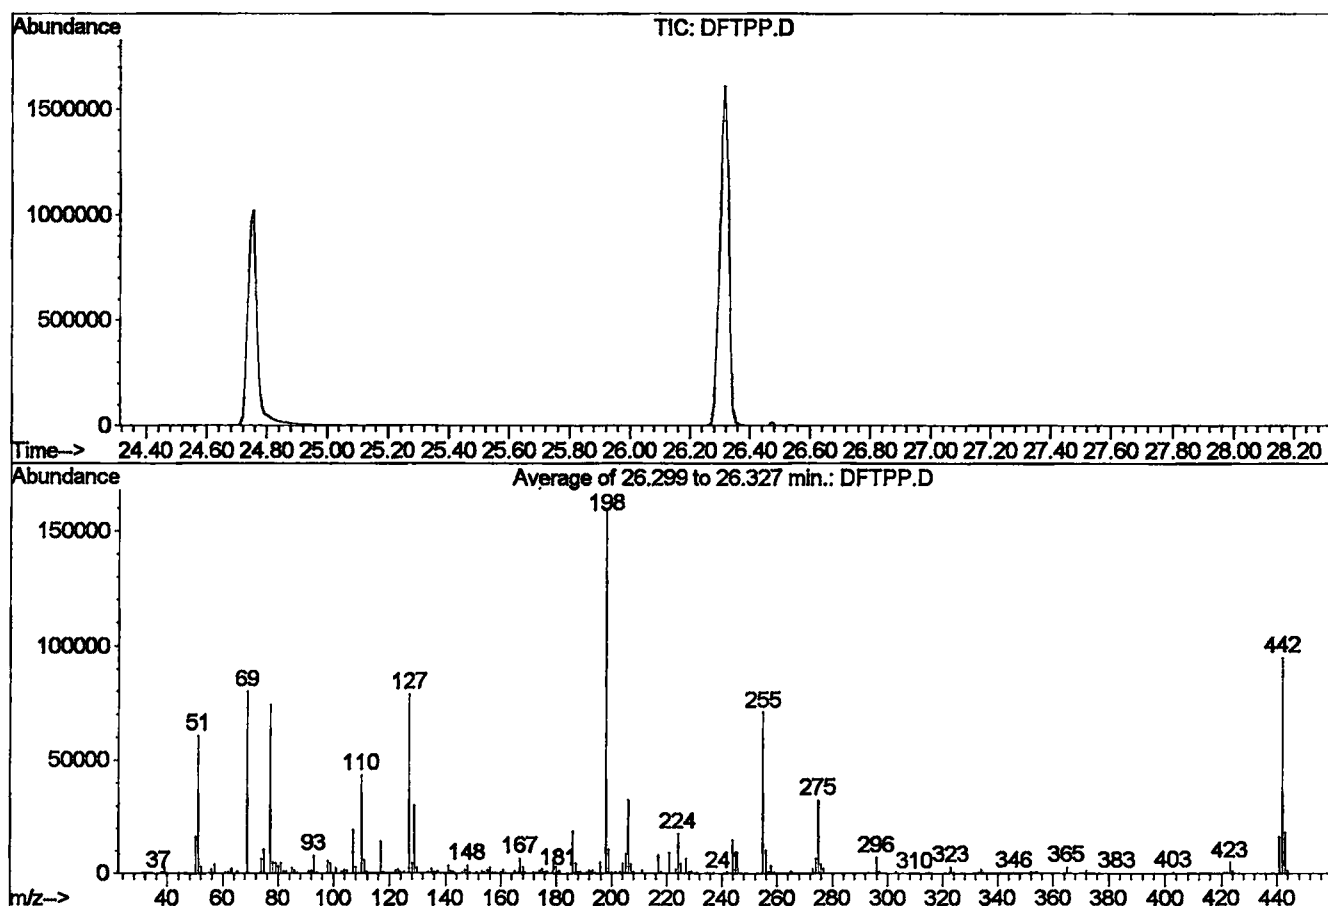

Spectrum Information: Average of 26.299 to 26.327 min.

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 30           | 60           | 38.0      | 60764   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 50.2      | 80322   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.1       | 77      | PASS             |
| 127         | 198          | 40           | 60           | 49.4      | 78978   | PASS             |
| 197         | 198          | 0.00         | 1            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 159976  | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 10785   | PASS             |
| 275         | 198          | 10           | 30           | 20.6      | 32982   | PASS             |
| 365         | 198          | 1            | 100          | 1.9       | 3008    | PASS             |
| 441         | 443          | 0.01         | 100          | 89.1      | 16317   | PASS             |
| 442         | 198          | 40           | 110          | 59.6      | 95304   | PASS             |
| 443         | 442          | 17           | 23           | 19.2      | 18318   | PASS             |

DFTPP.D NP101901.M

Thu Oct 25 12:12:49 2001