

Method S08

Date Extracted 10/5/01

Page 20

GCM8

Lab #	Description	Sample vol/wt	Drip rate ml/min	Surr add	Spk add	IS add	Final vol.	T.V. pos.	pH	Count
	Lab 6 with Stone	50ml	—	✓		—	2ml		7	
	100 Post									
	MDL Post									
	PRL 1232									
	24052									7
	24057									8
	24134									9
	24133									10
	24048									11
	24046									12
	24050									13
	24049									14
	24047									15
	23995									16
	23996									17
	23997									18
	23998									19
										20
	74134									
Reviewed by: <u>[Signature]</u> 10/20/02										
Remarks										
drip rate must be between 5-15 ml/min for liq-liq extractors drip rate - Extraction type <u>Supernatant</u> Solv.lot# NaCl lot# <u>12617</u> Na2SO4 lot# <u>8024 V32624</u>										
STANDARD	INT STD LOG#									
CALIBRATION										
REF/SPIKE	<u>post 24622</u>	<u>1502 PRL 1232</u>								
MDL/MDRF										
Q. CHECK										
INT. STD.										
SURROGATE	<u>20646</u>									
LPC										
ENDRIN/DDT										

Analyst CMAD/MC
revision 4/12/01

Verified by _____

Reviewed by [Signature]
Date 11/2/1

Sequence Name: C:\HPCHEM\1\SEQUENCE\OCT2501.S
 Comment: INST 209; 30Mx0.25umX0.50
 Operator: 209 GALOS
 Data Path: C:\HPCHEM\1\data\oct2501\
 Pre-Seq Cmd:
 Post-Seq Cmd:


Method Sections To Run	On A Barcode Mismatch
(X) Full Method	(X) Inject Anyway
() Reprocessing Only	() Don't Inject

Line Type	Vial	DataFile	Method	Sample Name
1 Sample	1	DFTPP	NP101901	
2 Sample	2	LB --	NP101901	lab blk 10/5
3 Sample	3	23995	NP101901	gc/ms unknown
4 Sample	4	23996	NP101901	gc/ms unknown
5 Sample	5	23997	NP101901	gc/ms unknown
6 Sample	6	23998	NP101901	gc/ms unknown
7 Sample	7	24046	NP101901	gc/ms unknown
8 Sample	8	24047	NP101901	gc/ms unknown
9 Sample	9	24048	NP101901	gc/ms unknown
10 Sample	10	24049	NP101901	gc/ms unknown
11 Sample	11	24050	NP101901	gc/ms unknown
12 Sample	12	24051	NP101901	gc/ms unknown
13 Sample	13	24052	NP101901	gc/ms unknown
14 Sample	14	24133	NP101901	gc/ms unknown
15 Sample	15	24134	NP101901	gc/ms unknown
16 Sample	16	LBB	NP101901	10/9
17 Sample	17	24135	NP101901	gc/ms unknown
18 Sample	18	24214	NP101901	gc/ms unknown
19 Sample	19	LBA	NP101901	10/1
20 Sample	20	23837	NP101901	gc/ms unknown
21 Sample	21	23838	NP101901	gc/ms unknown
22 Sample	1	DFTPP1	NP101901	
23 Sample	22	23839	NP101901	gc/ms unknown
24 Sample	23	23842	NP101901	gc/ms unknown
25 Sample	24	23843	NP101901	gc/ms unknown
26 Sample	25	23799	NP101901	gc/ms unknown
27 Sample	26	23798	NP101901	gc/ms unknown
28				

DFTPP

Data File : C:\HPCHEM\1\DATA\OCT2501\DFTPP.D
 Acq On : 25 Oct 2001 10:59 am
 Sample :
 Misc :
 MS Integration Params: RTEINT.P
 Method : C:\HPCHEM\1\METHODS\NP101901.M (RTE Integrator)
 Title : 209 625/TCLP calibration table 7/16/01

Vial: 1
 Operator: 209 GALOS
 Inst : GC/MS 209
 Multiplr: 1.00

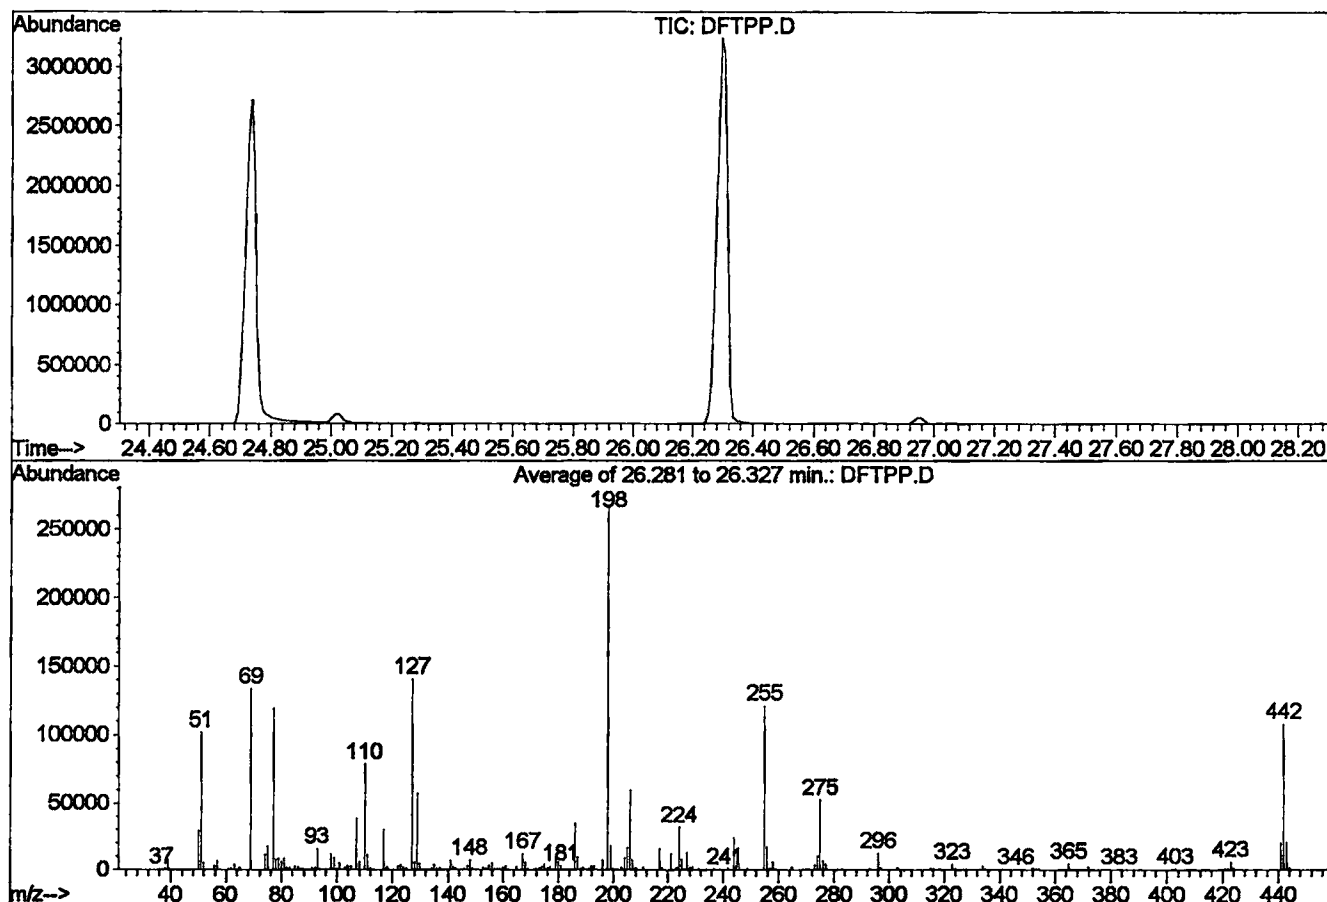

Spectrum Information: Average of 26.281 to 26.327 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	38.1	102023	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	50.0	133940	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	52.6	140811	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	267639	PASS
199	198	5	9	6.7	17850	PASS
275	198	10	30	19.4	52040	PASS
365	198	1	100	1.9	5060	PASS
441	443	0.01	100	97.2	20048	PASS
442	198	40	110	40.5	108365	PASS
443	442	17	23	19.0	20619	PASS

DFTPP.D NP101901.M Fri Oct 26 08:58:53 2001